

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031407.D
 Acq On : 06 May 2024 19:58
 Operator : MA/JU
 Sample : P2368-22
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43X6

Quant Time: May 06 23:13:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 14:17:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	108085	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	461344	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.245	164	314496	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	683162	20.000	ng/ul	0.00
79) Chrysene-d12	21.233	240	658467	20.000	ng/ul	0.00
88) Perylene-d12	24.110	264	653157	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	9338	3.739	ng/uL	0.00
4) Pyridine-d5	3.522	84	121981	18.792	ng/ul	0.00
7) Phenol-d5	6.775	99	157673	19.132	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	92203	19.812	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	137740	20.041	ng/ul	0.00
15) 4-Methylphenol-d8	8.304	113	127185	18.611	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	67419	19.396	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	72673	18.919	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.998	165	133860	19.389	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	200160	20.823	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	469727	20.757	ng/ul	0.00
49) Acenaphthylene-d8	13.939	160	508973	20.437	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	67276	16.723	ng/ul	0.00
60) Fluorene-d10	15.245	176	386418	20.894	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	68571	16.410	ng/ul	0.00
73) Anthracene-d10	17.098	188	615940	20.703	ng/ul	0.00
81) Pyrene-d10	19.404	212	734548	19.645	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.915	264	641639	20.594	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.651	266	18057	3.457	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031407.D
Acq On : 06 May 2024 19:58
Operator : MA/JU
Sample : P2368-22
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43X6

Quant Time: May 06 23:13:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 14:17:04 2024
Response via : Initial Calibration

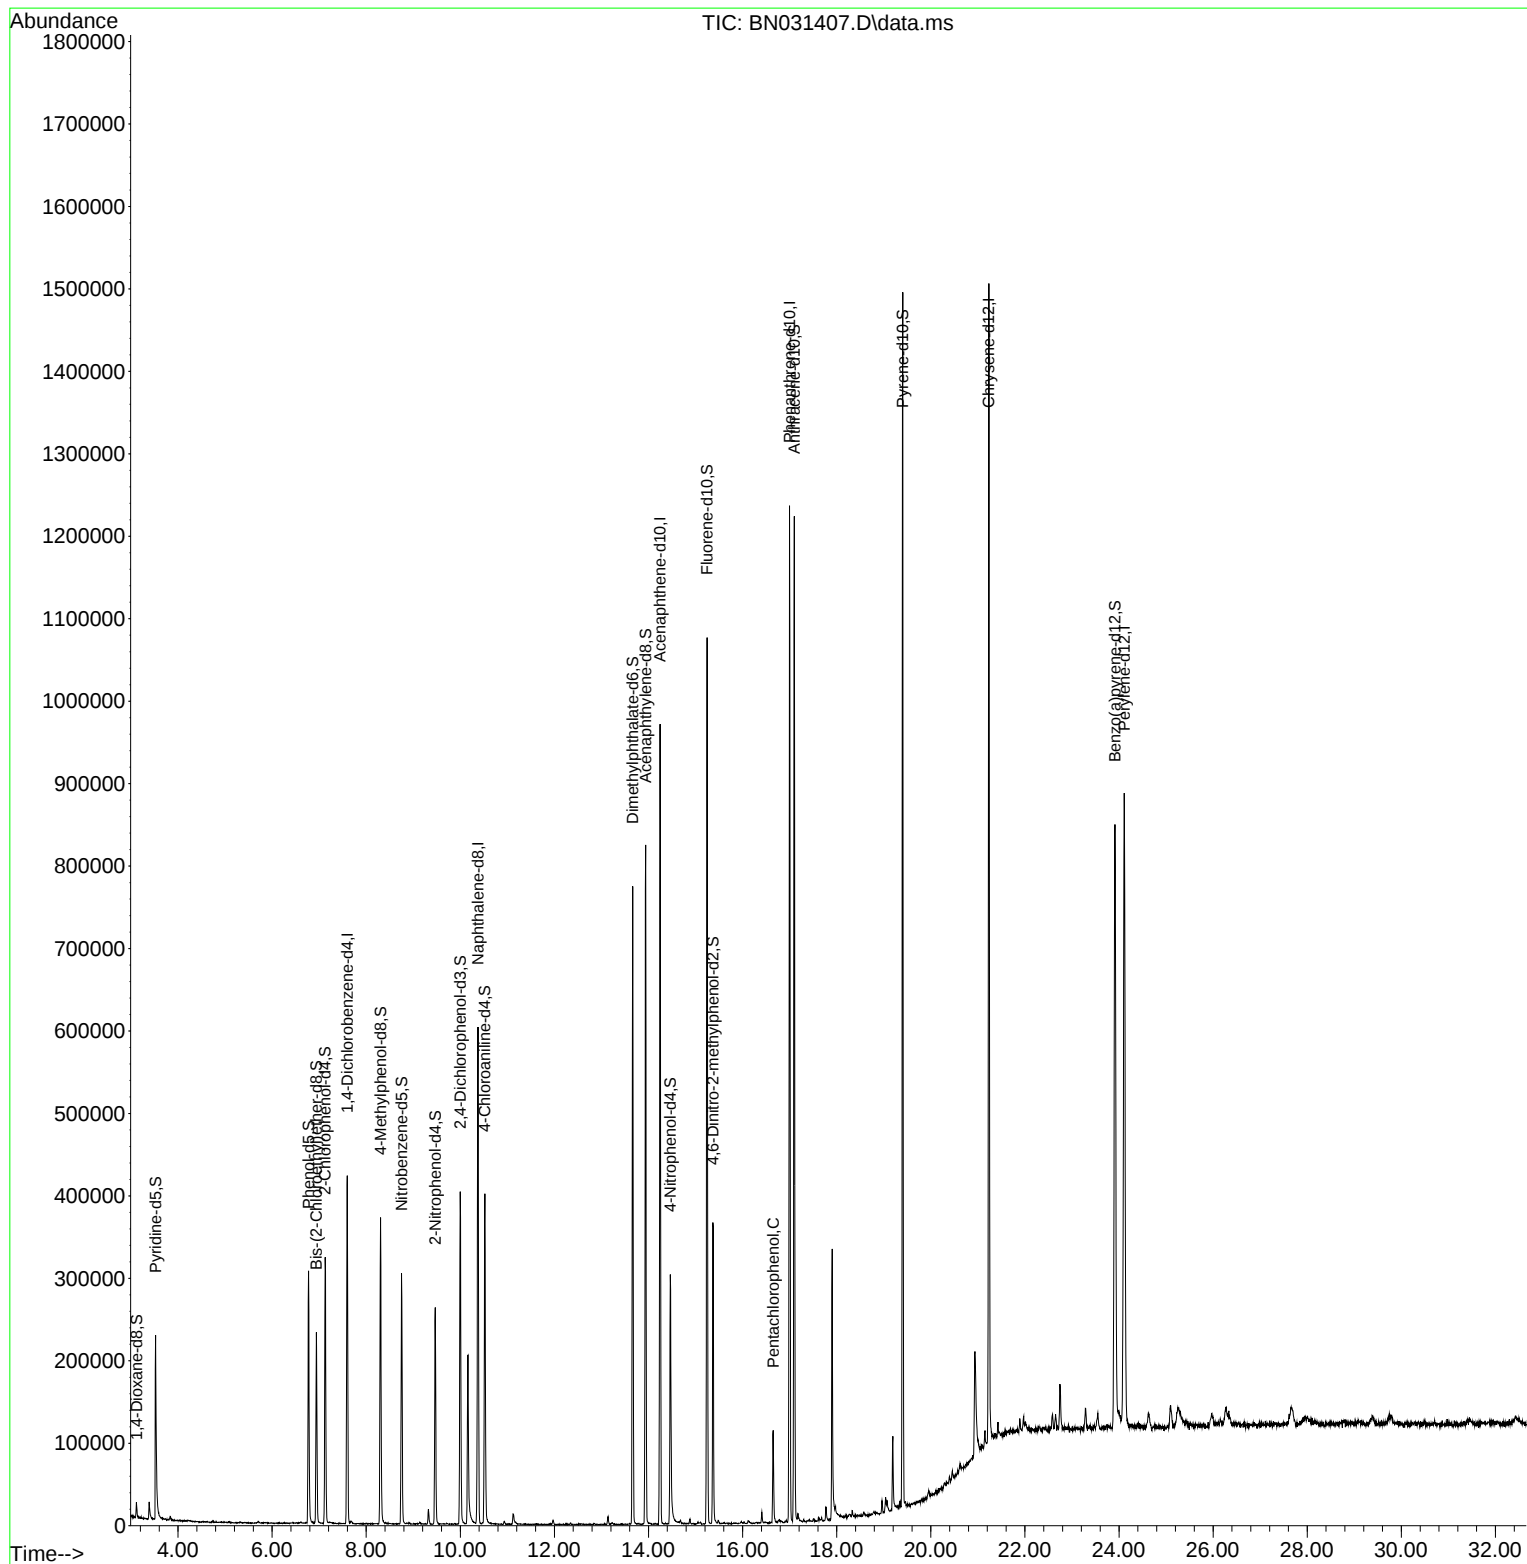

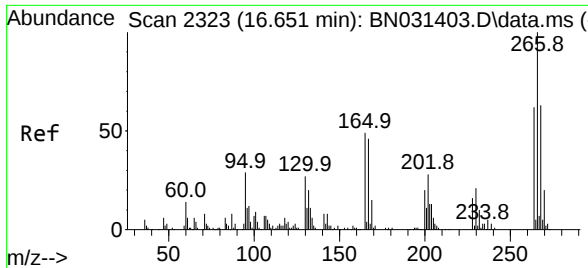

#71
 Pentachlorophenol
 Concen: 3.457 ng/ul
 RT: 16.651 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN031407.D
 Acq: 06 May 2024 19:58

Instrument :
 BNA_N
 ClientSampleId :
 A43X6

Tgt Ion:	266	Resp:	18057
Ion	Ratio	Lower	Upper
266	100		
264	63.0	49.6	74.4
268	58.5	47.8	71.6

