

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031394.D
 Acq On : 06 May 2024 11:12
 Operator : MA/JU
 Sample : PB160580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK580

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	18	22	29	rVB	32985	42103	1.45%	0.124%
2	3.522	87	91	109	rBV	399968	639453	22.02%	1.885%
3	3.834	140	144	148	rVB	10628	13349	0.46%	0.039%
4	6.775	637	644	655	rBV	517193	793083	27.31%	2.337%
5	6.940	667	672	681	rVB	383054	589483	20.30%	1.737%
6	7.128	696	704	716	rBV	542791	843938	29.06%	2.487%
7	7.599	777	784	792	rBV	569567	907142	31.23%	2.674%
8	8.305	897	904	916	rBV	647238	1018280	35.06%	3.001%
9	8.752	973	980	990	rBV	503463	811010	27.92%	2.390%
10	9.469	1094	1102	1119	rVB	438833	714140	24.59%	2.105%
11	9.999	1185	1192	1205	rBV	637777	1053141	36.26%	3.104%
12	10.375	1248	1256	1266	rBV	806670	1303950	44.90%	3.843%
13	10.522	1274	1281	1293	rBV	656511	1091987	37.60%	3.218%
14	11.975	1523	1528	1533	rVB	8231	12208	0.42%	0.036%
15	13.140	1720	1726	1732	rBV3	7403	11790	0.41%	0.035%
16	13.663	1809	1815	1827	rBV	1300453	1753508	60.37%	5.168%
17	13.940	1854	1862	1877	rBV	1349150	1953126	67.25%	5.756%
18	14.245	1906	1914	1923	rBV	1250435	1827726	62.93%	5.387%
19	14.463	1945	1951	1970	rBV	494391	812373	27.97%	2.394%
20	14.657	1981	1984	1990	rVB6	2555	4602	0.16%	0.014%
21	15.245	2077	2084	2093	rBV	1686468	2365644	81.45%	6.972%
22	15.375	2100	2106	2120	rBV	589198	795672	27.40%	2.345%
23	15.487	2121	2125	2129	rVB3	6621	9247	0.32%	0.027%
24	16.034	2214	2218	2221	rVB4	3175	4058	0.14%	0.012%
25	16.792	2342	2347	2349	rBV3	2552	3541	0.12%	0.010%
26	16.998	2376	2382	2393	rBV	1575547	2195195	75.58%	6.470%
27	17.098	2393	2399	2417	rVB2	1876001	2603501	89.64%	7.673%
28	17.904	2532	2536	2542	rBV6	3736	7344	0.25%	0.022%
29	18.928	2705	2710	2712	rBV5	2451	3861	0.13%	0.011%
30	18.963	2712	2716	2721	rVV2	20857	27991	0.96%	0.082%
31	19.033	2724	2728	2735	rVV	17659	24663	0.85%	0.073%
32	19.192	2753	2755	2761	rBV6	4178	6532	0.22%	0.019%
33	19.404	2785	2791	2800	rBV	2139033	2904437	100.00%	8.560%
34	21.233	3096	3102	3111	rBV	1609425	2260209	77.82%	6.661%
35	23.916	3549	3558	3574	rVB2	1052131	2421940	83.39%	7.138%
36	24.110	3583	3591	3604	rVB	884581	2099900	72.30%	6.189%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031394.D
Acq On : 06 May 2024 11:12
Operator : MA/JU
Sample : PB160580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 33930127

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031394.D
Acq On : 06 May 2024 11:12
Operator : MA/JU
Sample : PB160580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

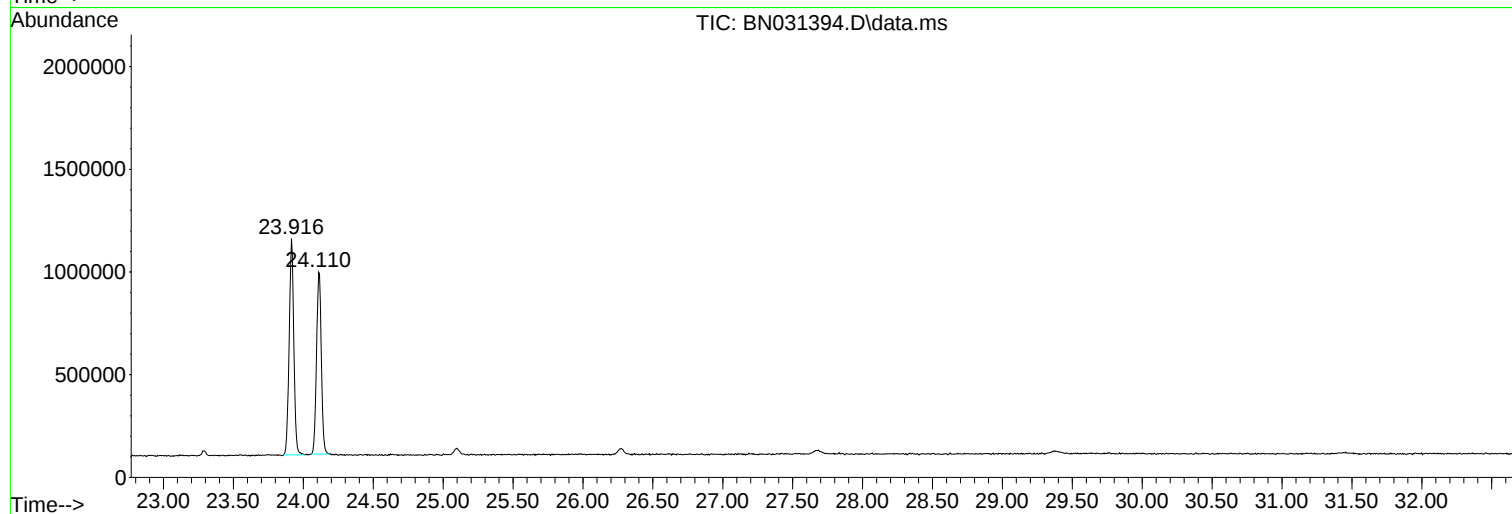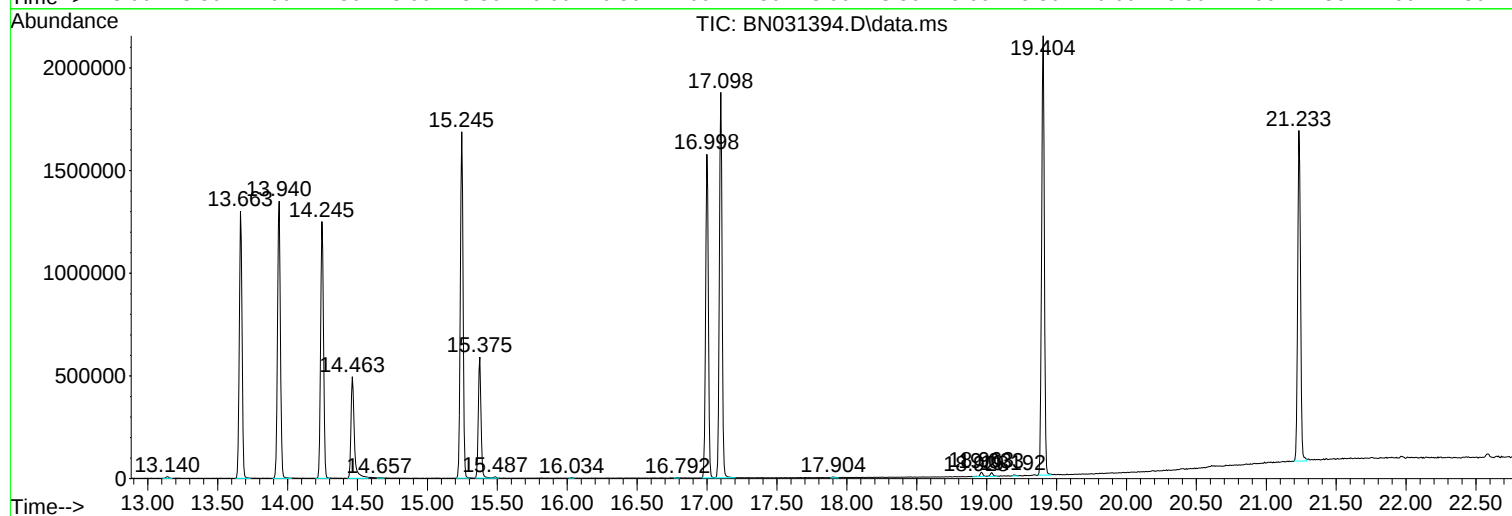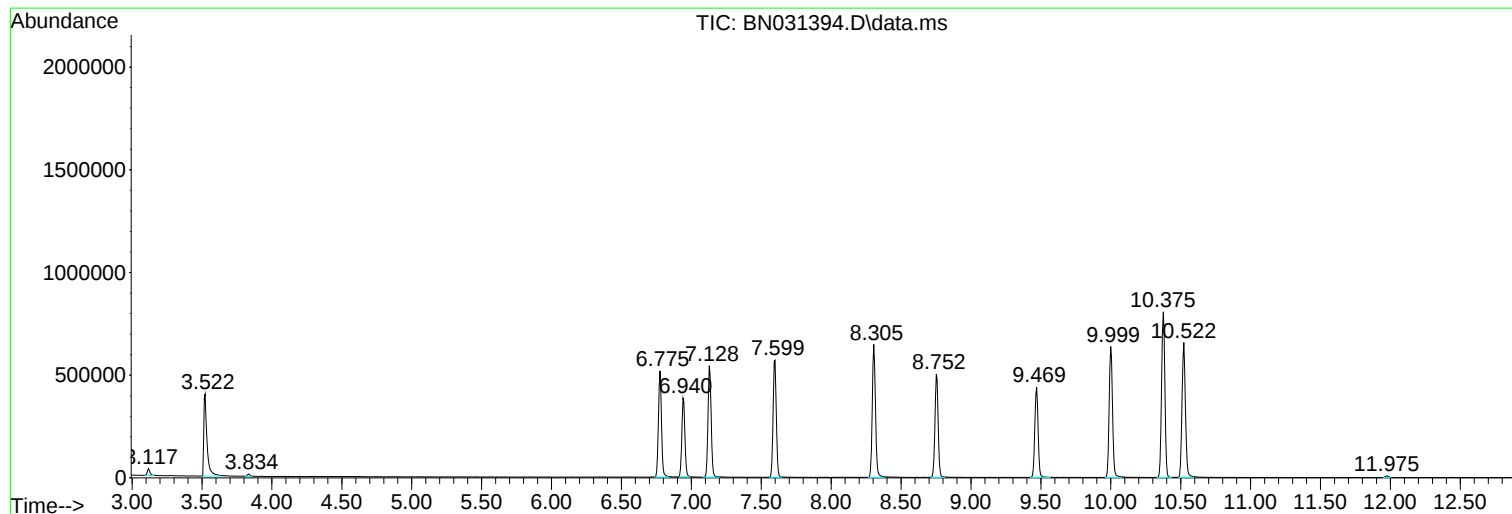

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031394.D
Acq On : 06 May 2024 11:12
Operator : MA/JU
Sample : PB160580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031394.D
Acq On : 06 May 2024 11:12
Operator : MA/JU
Sample : PB160580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------