

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031398.D
 Acq On : 06 May 2024 14:04
 Operator : MA/JU
 Sample : P2279-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	19	22	28	rVB2	19175	24563	0.58%	0.069%
2	3.528	89	92	110	rBV	86353	148707	3.52%	0.419%
3	3.834	141	144	152	rVB3	6451	9537	0.23%	0.027%
4	6.775	638	644	658	rVB	107943	170188	4.03%	0.479%
5	6.940	666	672	686	rBV	442905	671199	15.90%	1.889%
6	7.128	697	704	715	rBV	458611	713398	16.90%	2.008%
7	7.593	777	783	793	rBV	440800	701039	16.61%	1.973%
8	8.305	897	904	917	rBV	350065	547397	12.97%	1.541%
9	8.752	973	980	998	rBV	597717	949678	22.50%	2.673%
10	9.146	1041	1047	1054	rVB2	9975	15175	0.36%	0.043%
11	9.469	1092	1102	1115	rBV	502290	797449	18.89%	2.245%
12	9.999	1185	1192	1208	rBV	677962	1107128	26.23%	3.116%
13	10.375	1248	1256	1264	rBV	624366	1015103	24.05%	2.857%
14	10.522	1273	1281	1299	rBV	605598	1020434	24.18%	2.872%
15	11.634	1464	1470	1477	rVB2	7932	11904	0.28%	0.034%
16	11.975	1523	1528	1535	rVB2	10696	17112	0.41%	0.048%
17	13.057	1704	1712	1718	rBV4	9561	17477	0.41%	0.049%
18	13.140	1721	1726	1731	rBV	11344	16045	0.38%	0.045%
19	13.257	1741	1746	1751	rVB2	4128	6278	0.15%	0.018%
20	13.663	1809	1815	1827	rBV	1549797	2122568	50.29%	5.975%
21	13.940	1854	1862	1871	rBV	1631266	2340752	55.46%	6.589%
22	14.245	1908	1914	1929	rVB	1002779	1434406	33.99%	4.038%
23	14.469	1946	1952	1962	rBV	93968	176496	4.18%	0.497%
24	14.563	1964	1968	1974	rVB5	8754	13521	0.32%	0.038%
25	14.663	1982	1985	1992	rVB5	2446	4367	0.10%	0.012%
26	15.245	2077	2084	2099	rBV	2189823	3003686	71.17%	8.455%
27	15.375	2099	2106	2116	rVV	860705	1185163	28.08%	3.336%
28	15.487	2120	2125	2129	rVB4	9073	12959	0.31%	0.036%
29	16.034	2214	2218	2221	rVB3	3613	5629	0.13%	0.016%
30	16.998	2376	2382	2389	rBV	1282745	1763943	41.79%	4.965%
31	17.098	2392	2399	2417	rVB2	2645484	3703523	87.75%	10.425%
32	17.898	2531	2535	2545	rBV	99869	142100	3.37%	0.400%
33	17.986	2547	2550	2556	rVB5	4901	8469	0.20%	0.024%
34	18.333	2606	2609	2614	rVB3	5385	5656	0.13%	0.016%
35	18.963	2711	2716	2721	rBV2	32857	45503	1.08%	0.128%
36	19.033	2724	2728	2732	rBV	30784	42080	1.00%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Title : SVOA CALIBRATION

37	19.192	2750	2755	2761	rBV2	59601	83314	1.97%	0.235%
38	19.345	2777	2781	2784	rBV6	8789	11714	0.28%	0.033%
39	19.404	2785	2791	2798	rVV	3215374	4220557	100.00%	11.880%
40	20.933	3047	3051	3061	rBV6	47442	120539	2.86%	0.339%
41	21.233	3096	3102	3114	rBV	1344900	1851311	43.86%	5.211%
42	23.916	3549	3558	3579	rVB2	1508782	3578440	84.79%	10.072%
43	24.110	3583	3591	3605	rVB	709154	1690385	40.05%	4.758%




Sum of corrected areas: 35526892

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

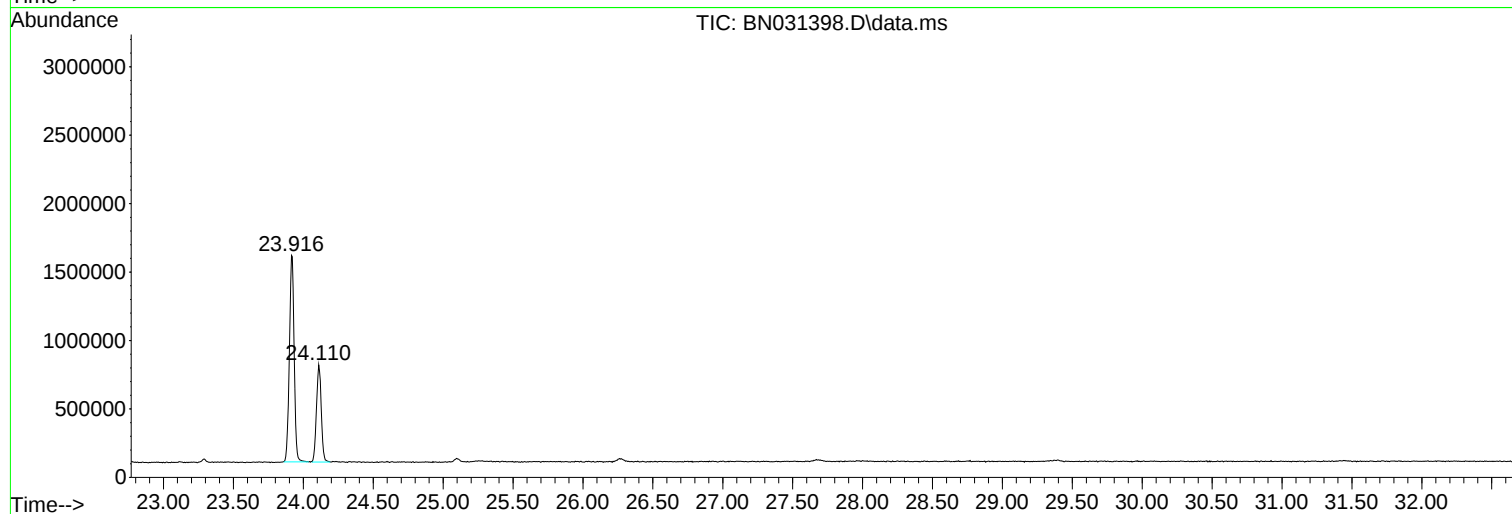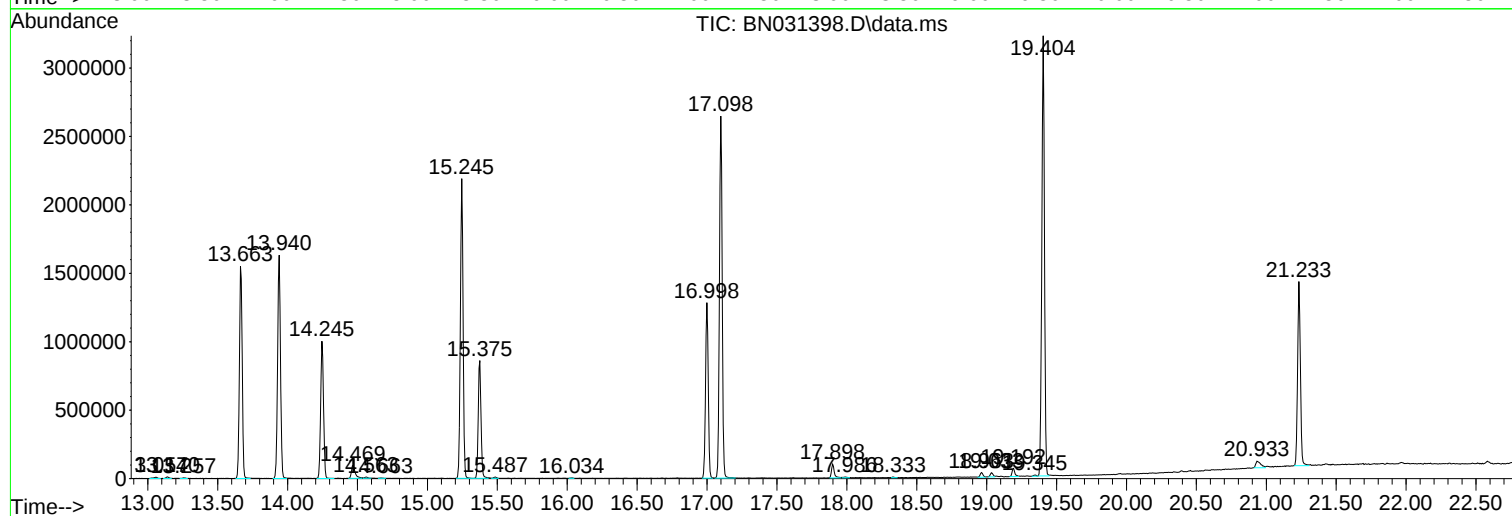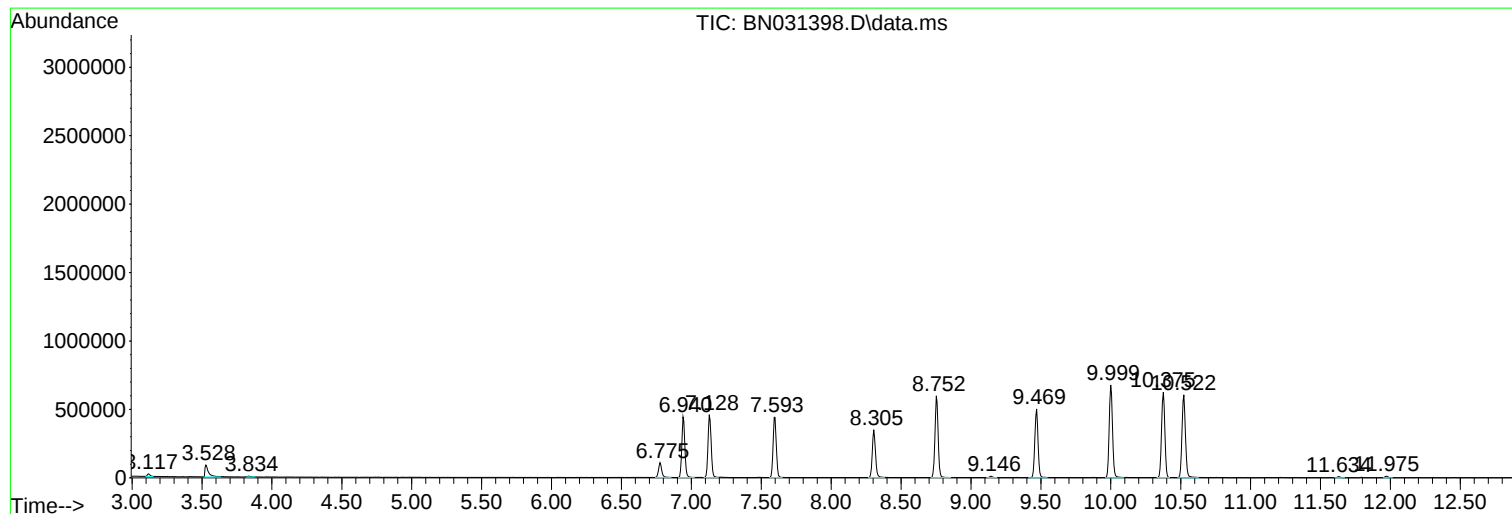

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031398.D
Acq On : 06 May 2024 14:04
Operator : MA/JU
Sample : P2279-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RR3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
