

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031406.D
 Acq On : 06 May 2024 19:19
 Operator : MA/JU
 Sample : P2368-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.029	3	7	12	rVB5	6851	12395	0.48%	0.046%
2	3.117	18	22	27	rBV	20630	27268	1.06%	0.101%
3	3.387	65	68	80	rBV	20184	35208	1.37%	0.131%
4	3.523	89	91	110	rBV	128609	219858	8.55%	0.818%
5	3.834	141	144	149	rVB5	5141	8175	0.32%	0.030%
6	5.705	457	462	467	rBV7	2732	4377	0.17%	0.016%
7	6.775	638	644	653	rBV	349276	540976	21.03%	2.012%
8	6.940	667	672	687	rVB	287399	444654	17.28%	1.654%
9	7.128	698	704	716	rBV	367520	571539	22.22%	2.126%
10	7.599	777	784	791	rBV	379246	606009	23.56%	2.254%
11	7.681	793	798	804	rVB6	3575	7246	0.28%	0.027%
12	8.305	897	904	917	rBV	422382	670213	26.05%	2.493%
13	8.752	973	980	989	rBV	387576	621778	24.17%	2.313%
14	8.922	1005	1009	1012	rVB4	2075	2774	0.11%	0.010%
15	9.140	1042	1046	1051	rVB3	3115	4459	0.17%	0.017%
16	9.322	1072	1077	1085	rVB3	19256	31230	1.21%	0.116%
17	9.469	1094	1102	1112	rBV	292894	472901	18.38%	1.759%
18	9.999	1185	1192	1206	rBV	455929	737554	28.67%	2.744%
19	10.169	1219	1221	1229	rVB5	2119	3252	0.13%	0.012%
20	10.375	1248	1256	1264	rBV	539775	880302	34.22%	3.275%
21	10.522	1274	1281	1294	rBV	444378	745248	28.97%	2.772%
22	10.934	1346	1351	1355	rBV4	4628	7656	0.30%	0.028%
23	11.128	1375	1384	1391	rBV2	28775	59504	2.31%	0.221%
24	11.975	1522	1528	1533	rBV2	6852	11439	0.44%	0.043%
25	13.140	1718	1726	1732	rBV3	7112	12014	0.47%	0.045%
26	13.663	1808	1815	1828	rBV	996706	1353360	52.61%	5.034%
27	13.940	1852	1862	1874	rBV	1079365	1585769	61.64%	5.899%
28	14.246	1908	1914	1922	rBV	855169	1221701	47.49%	4.545%
29	14.463	1945	1951	1969	rBV	262034	494072	19.20%	1.838%
30	15.098	2054	2059	2063	rVB5	1804	2983	0.12%	0.011%
31	15.246	2077	2084	2092	rBV	1473138	2006504	77.99%	7.464%
32	15.375	2098	2106	2116	rBV	284318	405857	15.78%	1.510%
33	15.481	2120	2124	2128	rBV4	4364	6612	0.26%	0.025%
34	15.810	2177	2180	2185	rBV4	1897	3186	0.12%	0.012%
35	15.969	2203	2207	2211	rBV5	2850	3994	0.16%	0.015%
36	16.034	2214	2218	2220	rBV5	3108	3958	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
 Data File : BN031406.D
 Acq On : 06 May 2024 19:19
 Operator : MA/JU
 Sample : P2368-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43K8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
 Title : SVOA CALIBRATION

37	16.145	2234	2237	2242	rVB3	1676	2740	0.11%	0.010%
38	16.763	2338	2342	2343	rBV3	2986	3333	0.13%	0.012%
39	16.922	2365	2369	2373	rBV5	2239	3574	0.14%	0.013%
40	16.998	2376	2382	2388	rVV	1090849	1525242	59.29%	5.674%
41	17.098	2392	2399	2412	rVV	1589822	2220741	86.32%	8.261%
42	17.204	2412	2417	2421	rVB6	6875	10180	0.40%	0.038%
43	17.398	2446	2450	2457	rBV7	4374	9444	0.37%	0.035%
44	17.504	2465	2468	2473	rVB5	2389	2621	0.10%	0.010%
45	17.675	2494	2497	2502	rVB3	7054	9650	0.38%	0.036%
46	17.898	2529	2535	2544	rBV	97890	137736	5.35%	0.512%
47	17.981	2544	2549	2553	rVB2	4242	7447	0.29%	0.028%
48	18.198	2583	2586	2590	rVB4	3446	3187	0.12%	0.012%
49	18.328	2605	2608	2612	rBV3	10513	12728	0.49%	0.047%
50	18.392	2616	2619	2623	rBV5	2079	2919	0.11%	0.011%
51	18.834	2690	2694	2698	rBV5	7493	10781	0.42%	0.040%
52	18.963	2712	2716	2722	rBV2	22061	29800	1.16%	0.111%
53	19.039	2725	2729	2732	rBV2	20617	31929	1.24%	0.119%
54	19.192	2750	2755	2758	rBV3	40874	51792	2.01%	0.193%
55	19.334	2775	2779	2784	rBV	24312	32940	1.28%	0.123%
56	19.404	2785	2791	2797	rVV	1958411	2572655	100.00%	9.570%
57	19.457	2797	2800	2805	rVB2	29299	36860	1.43%	0.137%
58	19.957	2882	2885	2889	rVB	47719	51972	2.02%	0.193%
59	20.457	2966	2970	2973	rBV	84760	89143	3.47%	0.332%
60	20.933	3046	3051	3069	rBV2	195728	476859	18.54%	1.774%
61	21.233	3096	3102	3115	rBV	1102598	1639932	63.74%	6.100%
62	21.422	3131	3134	3140	rBV2	81392	114060	4.43%	0.424%
63	21.969	3223	3227	3232	rBV	77463	110332	4.29%	0.410%
64	22.586	3328	3332	3337	rVB	65261	96714	3.76%	0.360%
65	23.292	3448	3452	3461	rVB3	61008	107636	4.18%	0.400%
66	23.916	3550	3558	3571	rBV2	866164	2081424	80.91%	7.743%
67	24.110	3583	3591	3607	rVB	646026	1570012	61.03%	5.840%




Sum of corrected areas: 26882408

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031406.D
Acq On : 06 May 2024 19:19
Operator : MA/JU
Sample : P2368-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

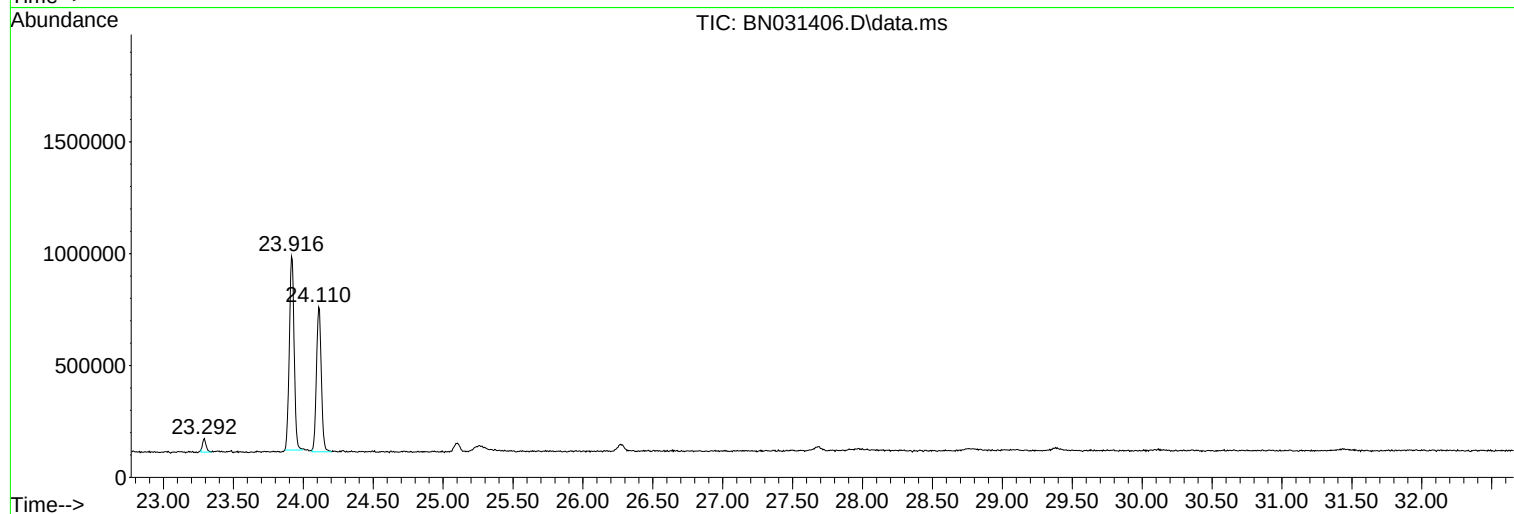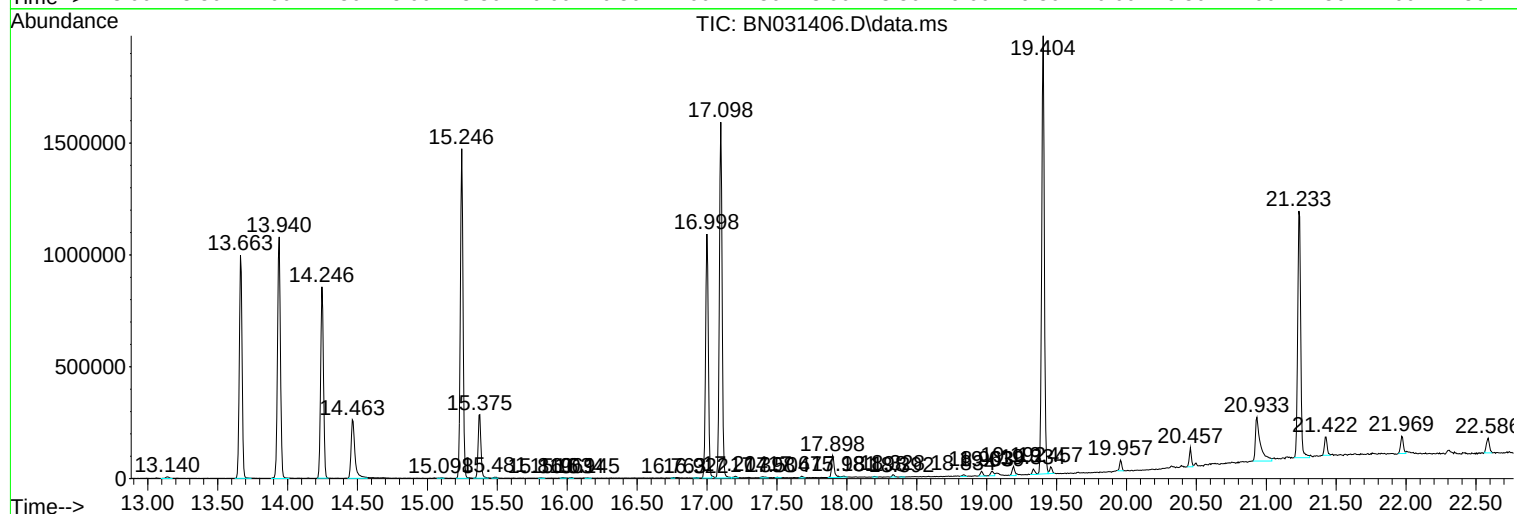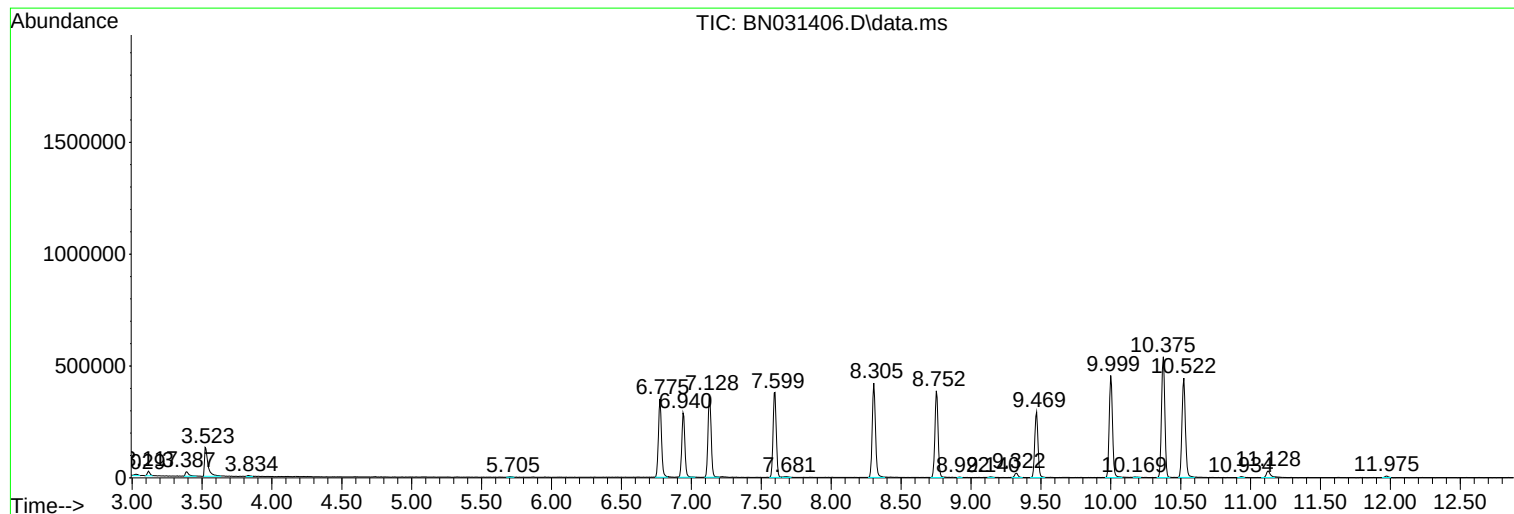

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031406.D
Acq On : 06 May 2024 19:19
Operator : MA/JU
Sample : P2368-03
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
A43K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
20.933	5.82 ng/ul	476859	Chrysene-d12	21.233	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
2	Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	91
3	Isobutyl tetracosyl ether	410	C28H58O	1000406-33-2	91
4	Cyclohexadecane	224	C16H32	000295-65-8	87
5	1-Dodecanol, 2-hexyl-	270	C18H38O	110225-00-8	81

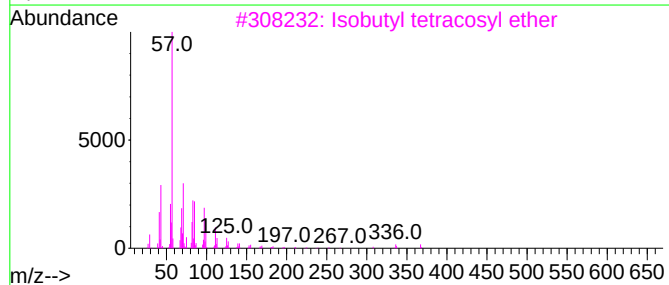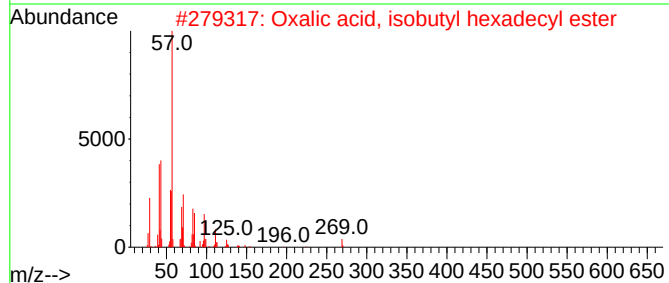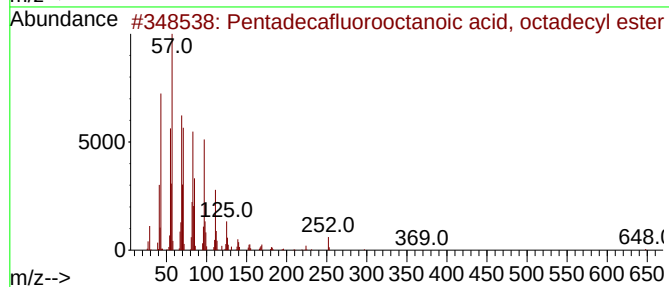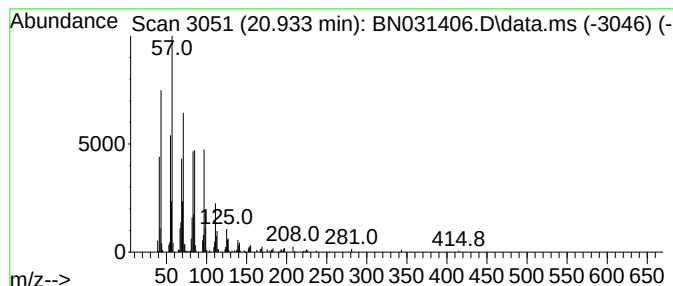

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050624\
Data File : BN031406.D
Acq On : 06 May 2024 19:19
Operator : MA/JU
Sample : P2368-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43K8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN050324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	20.933	5.8	ng/u1	476859	5	21.233	1639930	20.0