
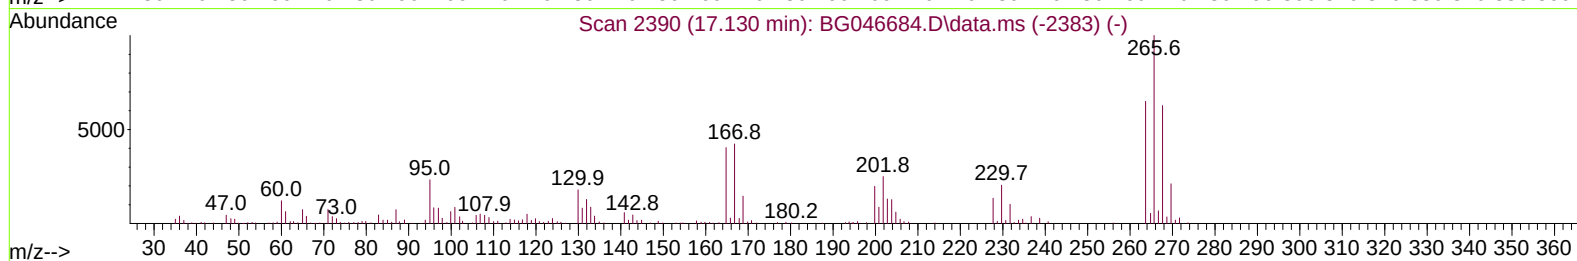
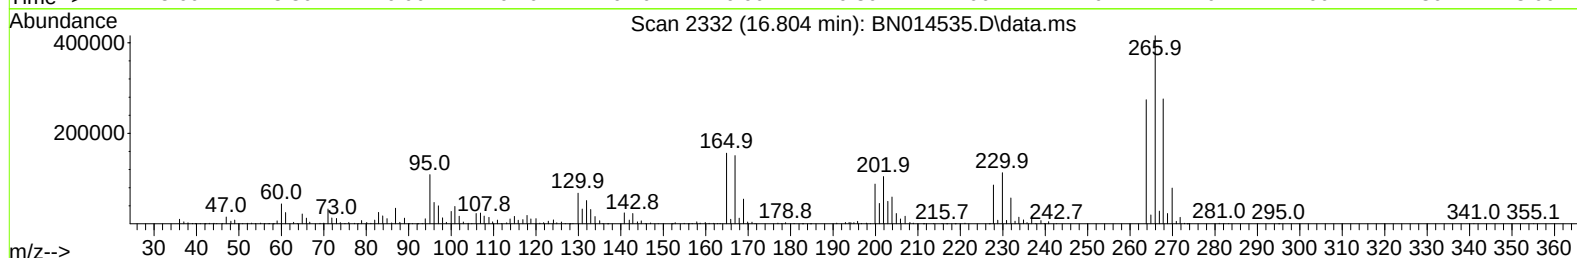


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050721\
 Data File : BN014535.D
 Acq On : 07 May 2021 12:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:11:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

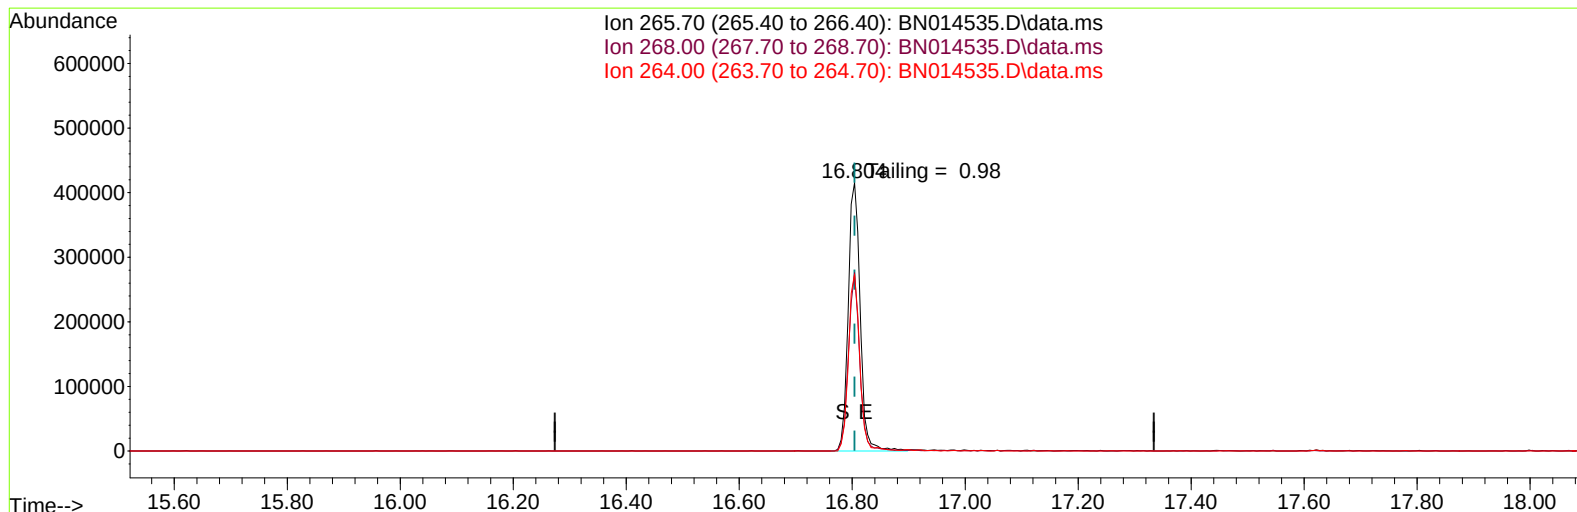

TIC: BN014535.D\data.ms

(70) Pentachlorophenol (C)




16.804min (0.000) 18680.46 ng

response 611760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.39
264.00	61.60	65.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050721\
 Data File : BN014535.D
 Acq On : 07 May 2021 12:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 04:11:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

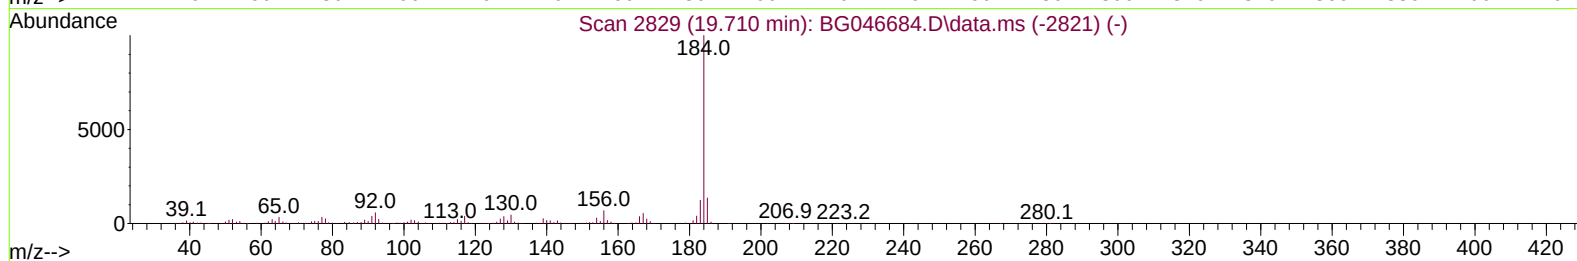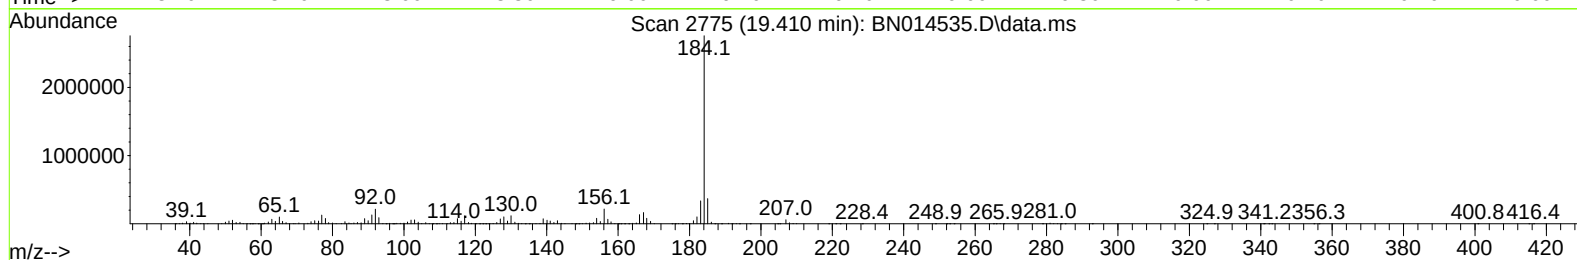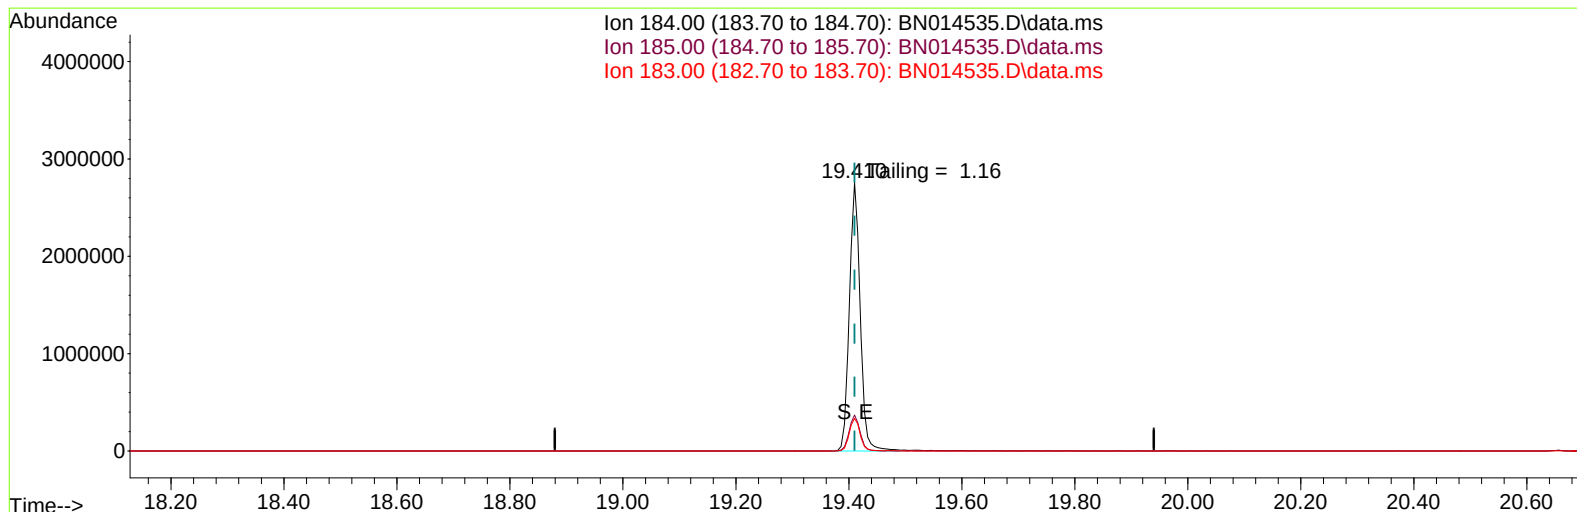

TIC: BN014535.D\data.ms

(77) Benzidine**19.410min (0.000) 819682.15 ng****response 3688983**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.40
183.00	13.20	12.17
0.00	0.00	0.00