
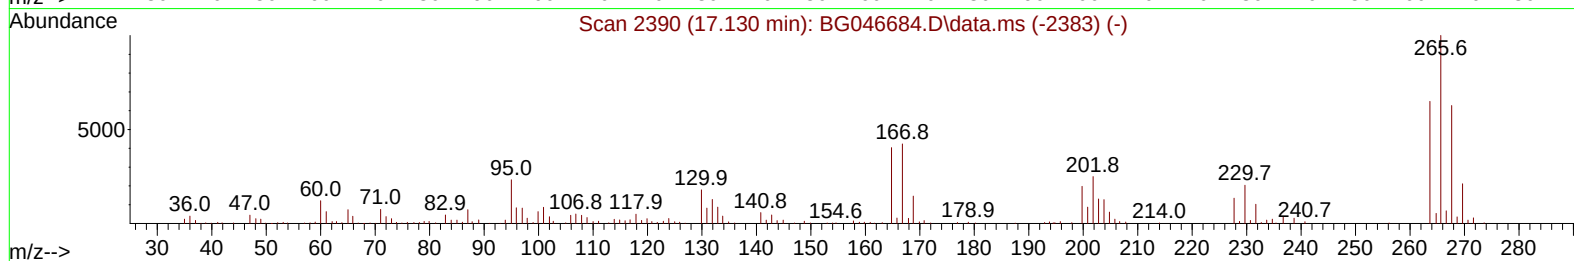
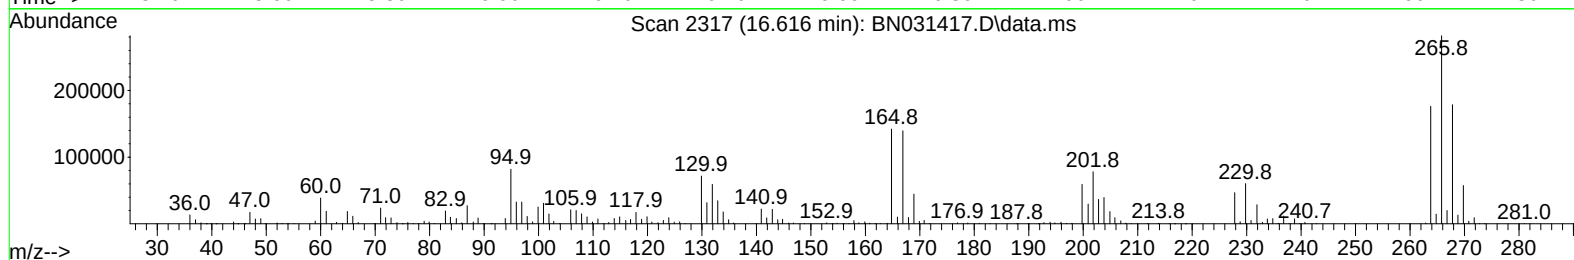


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050724\
Data File : BN031417.D
Acq On : 07 May 2024 11:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 13:01:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

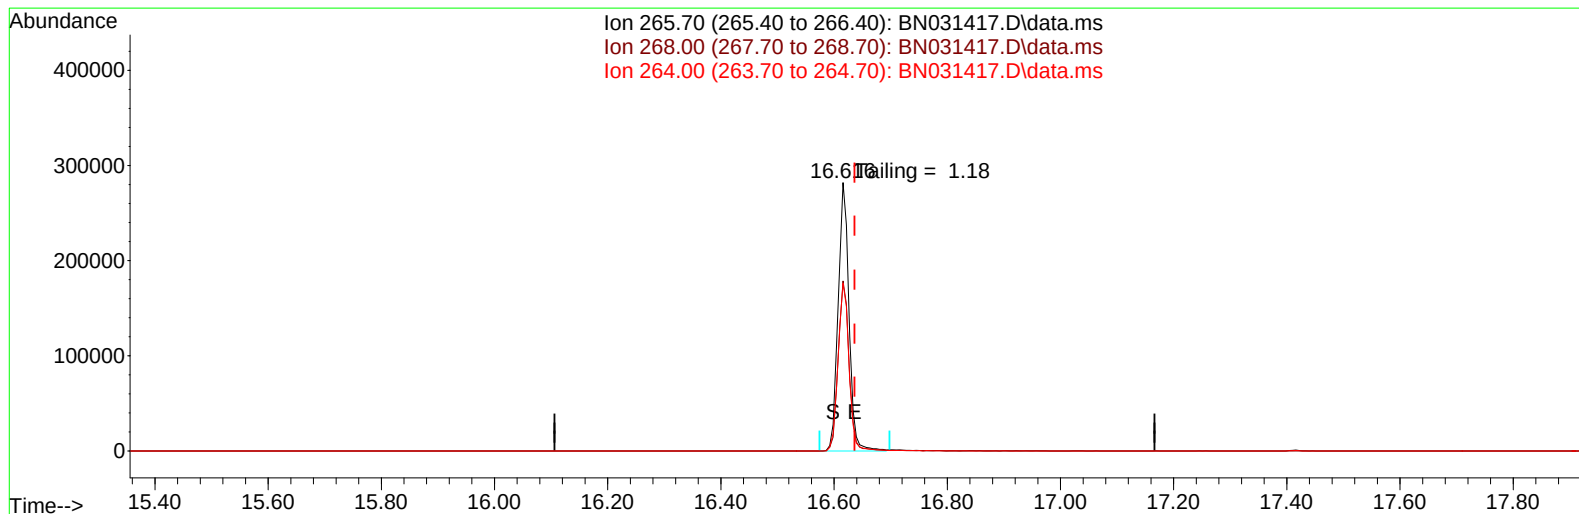

TIC: BN031417.D\data.ms

(70) Pentachlorophenol (C)




16.616min (-0.020) 19990.96 ng

response 377306

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.32
264.00	61.60	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050724\
Data File : BN031417.D
Acq On : 07 May 2024 11:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 13:01:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

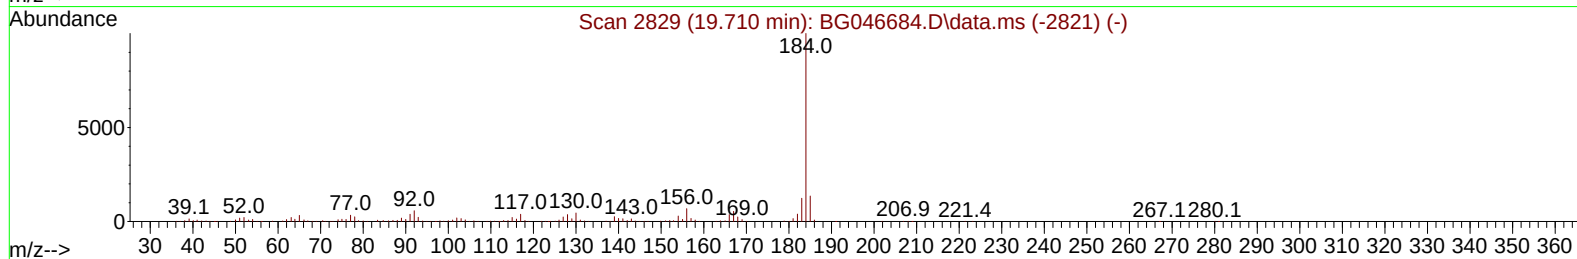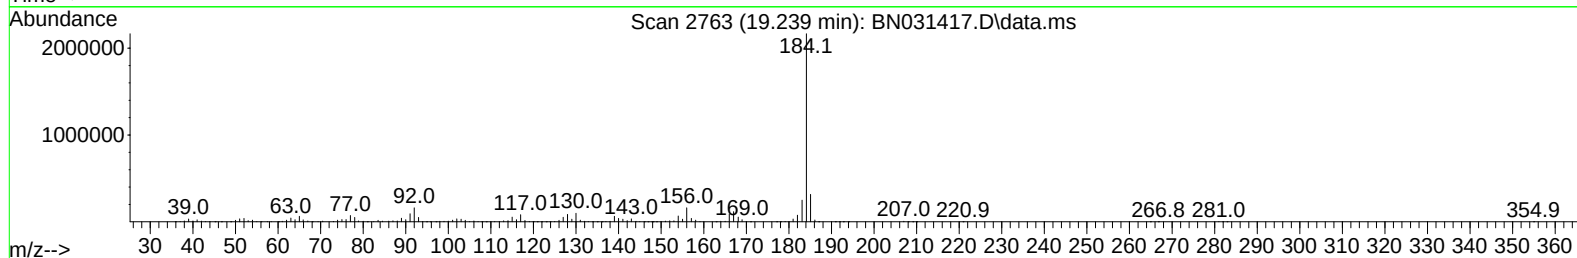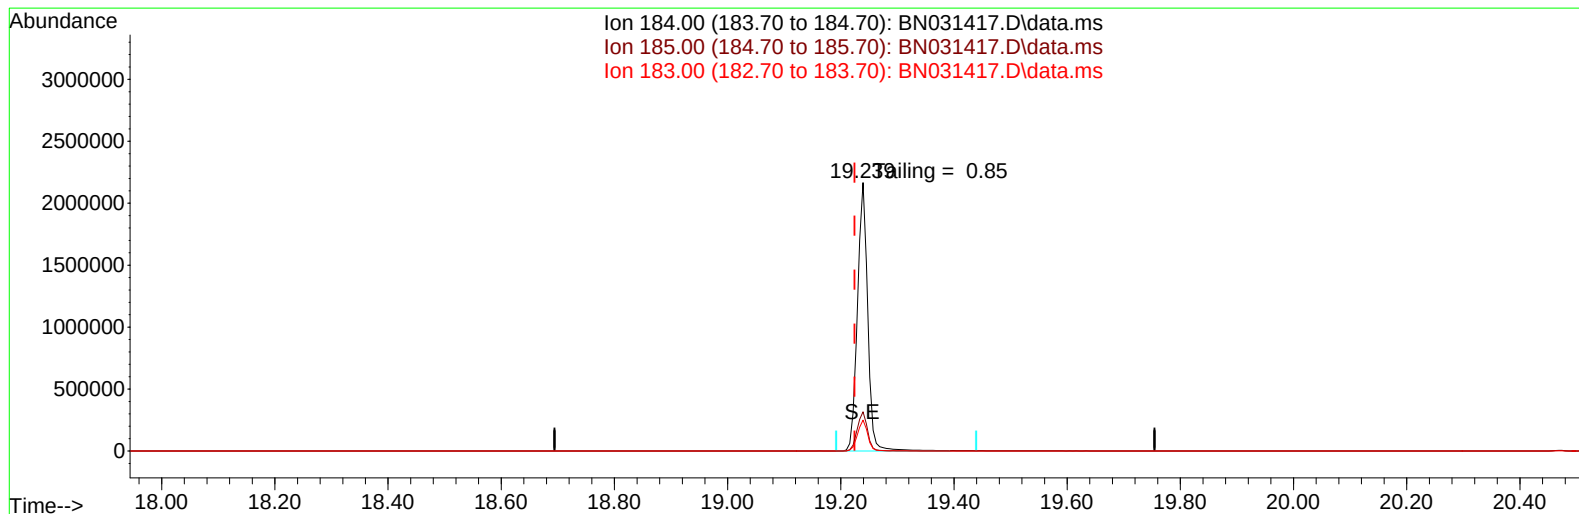

TIC: BN031417.D\data.ms

(77) Benzidine

19.239min (+ 0.015) 0.00 ng

response 2733936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	11.53
0.00	0.00	0.00