


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050724\
Data File : BN031417.D
Acq On : 07 May 2024 11:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 07 17:14:43 2024

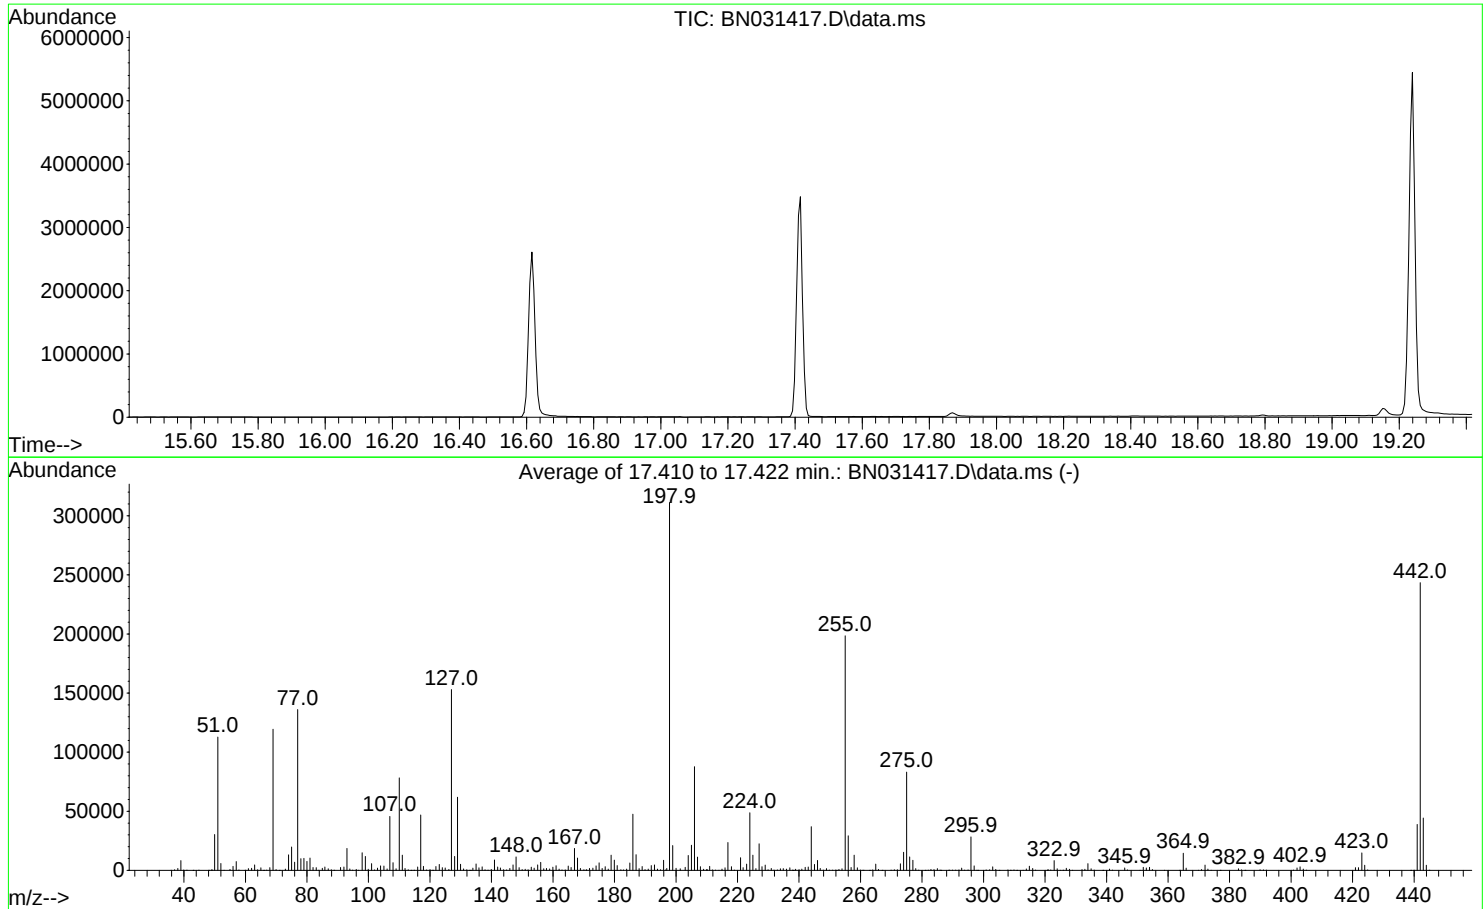




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	36.2	112789	PASS
68	69	0.00	2	1.9	2305	PASS
69	198	0.00	100	38.4	119392	PASS
70	69	0.00	2	0.5	646	PASS
127	198	10	80	49.2	153051	PASS
197	198	0.00	2	0.5	1639	PASS
198	198	100	100	100.0	311253	PASS
199	198	5	9	6.8	21031	PASS
275	198	10	60	26.7	83133	PASS
365	198	1	100	4.6	14459	PASS
441	198	0.01	100	12.5	38811	PASS
442	442	50	100	100.0	243392	PASS
443	442	15	24	18.2	44291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050724\
Data File : BN031417.D
Acq On : 07 May 2024 11:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 13:01:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

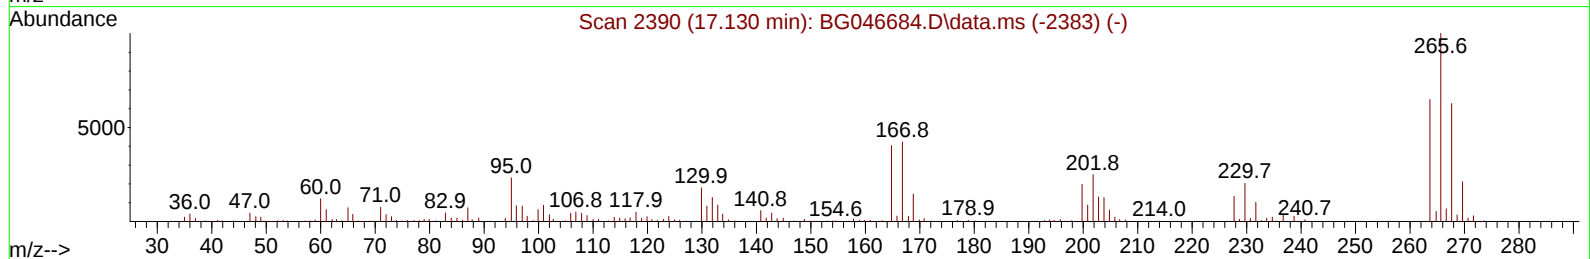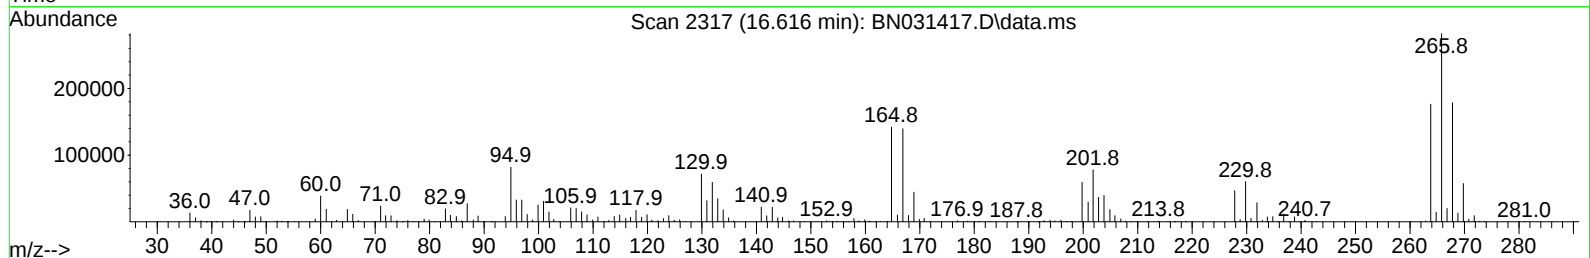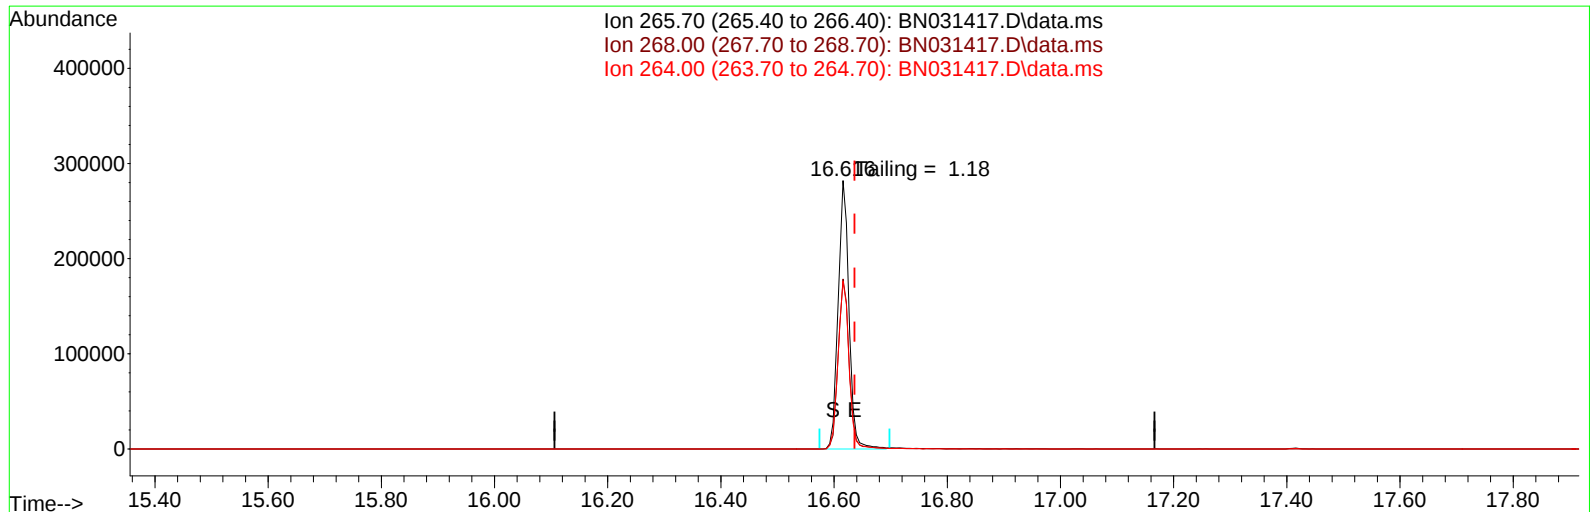

TIC: BN031417.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.020) 19990.96 ng




response 377306

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.32
264.00	61.60	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050724\
Data File : BN031417.D
Acq On : 07 May 2024 11:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 13:01:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

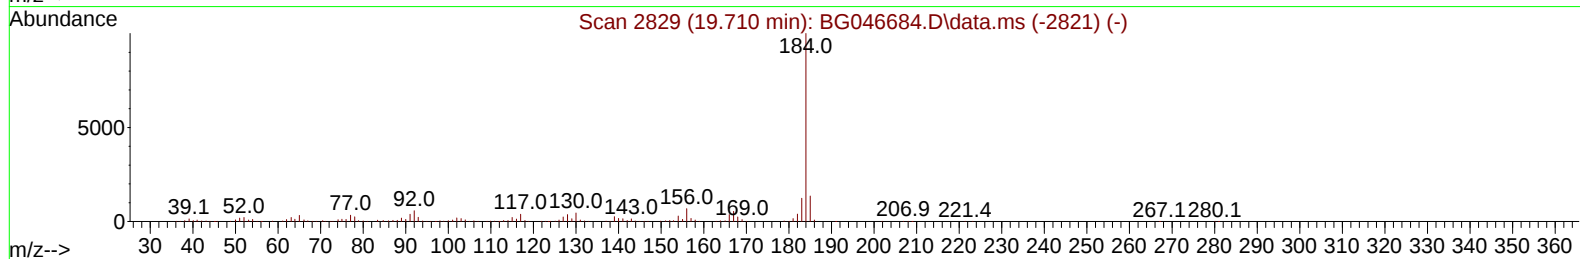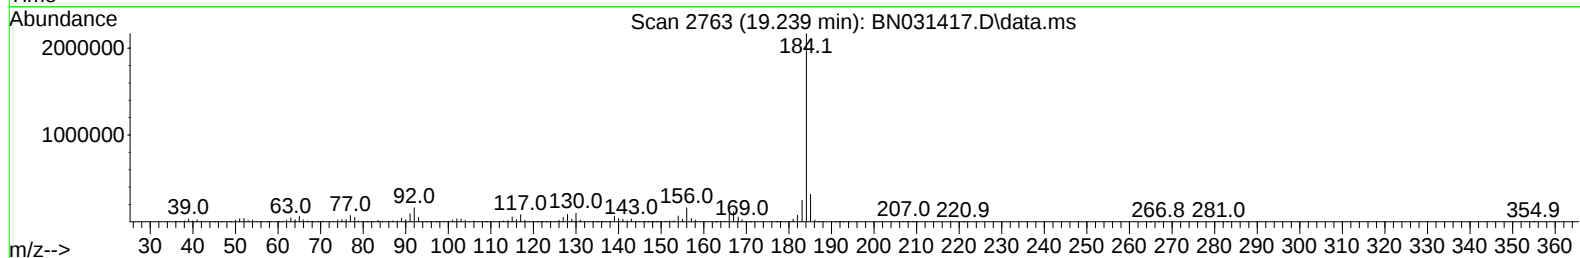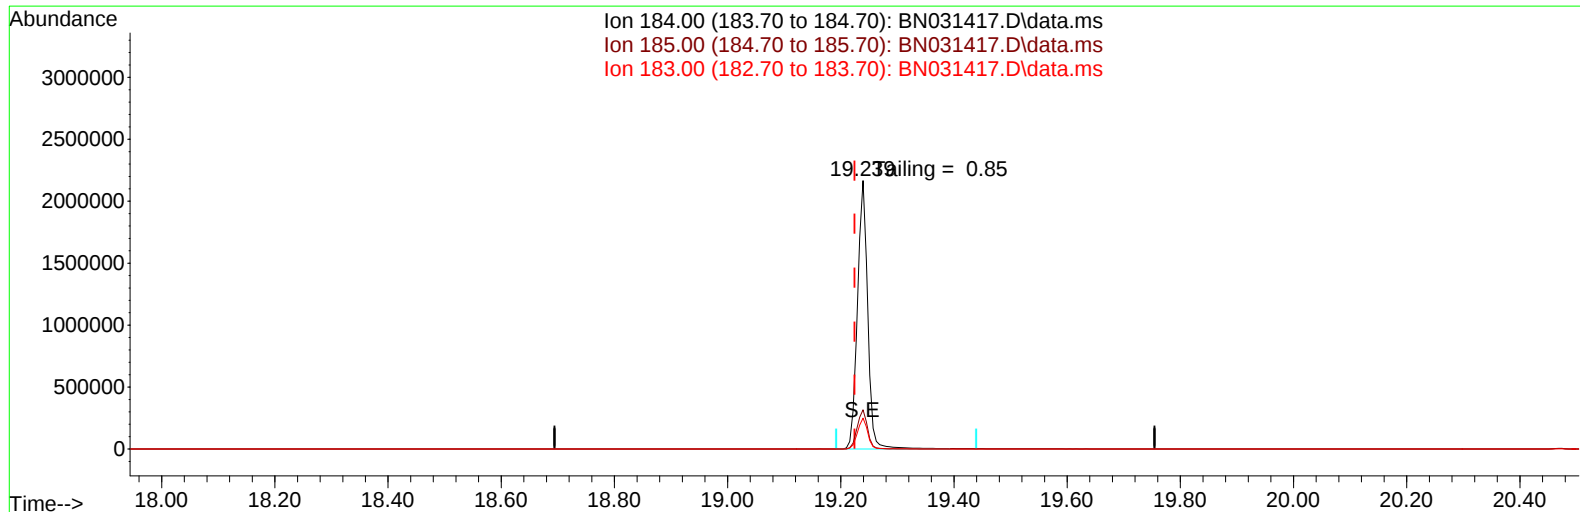

TIC: BN031417.D\data.ms

(77) Benzidine

19.239min (+ 0.015) 0.00 ng

response 2733936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/7/2024	BNA_N	<u>BN031417.D</u>
Compound Name	Response	Retention Time
DDT	1277363	20.469
DDD	11170	20.08
DDE	116	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11286	1288649	0.88

Instrument :
BNA_N
ClientSampleId :
DFTPP