
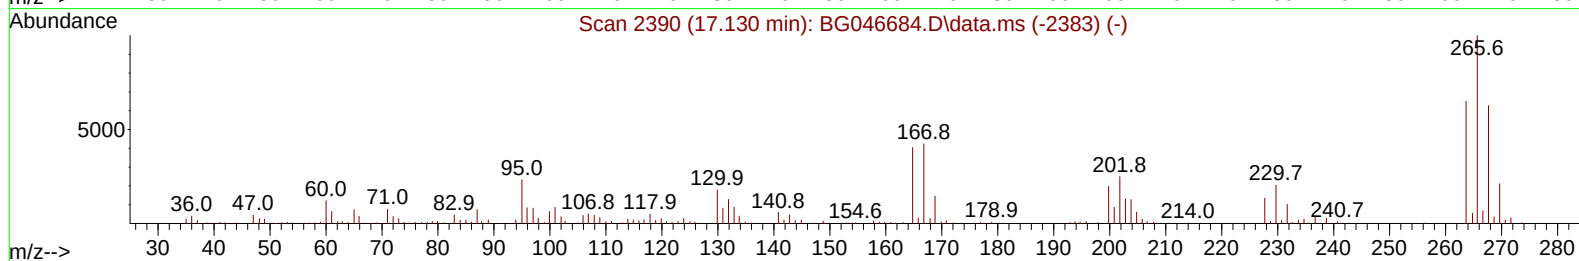
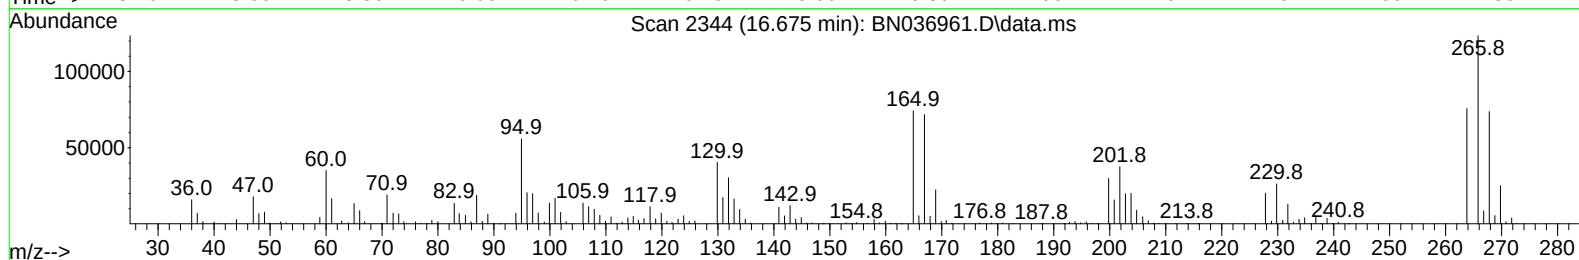


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050725\
Data File : BN036961.D
Acq On : 07 May 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 16:12:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

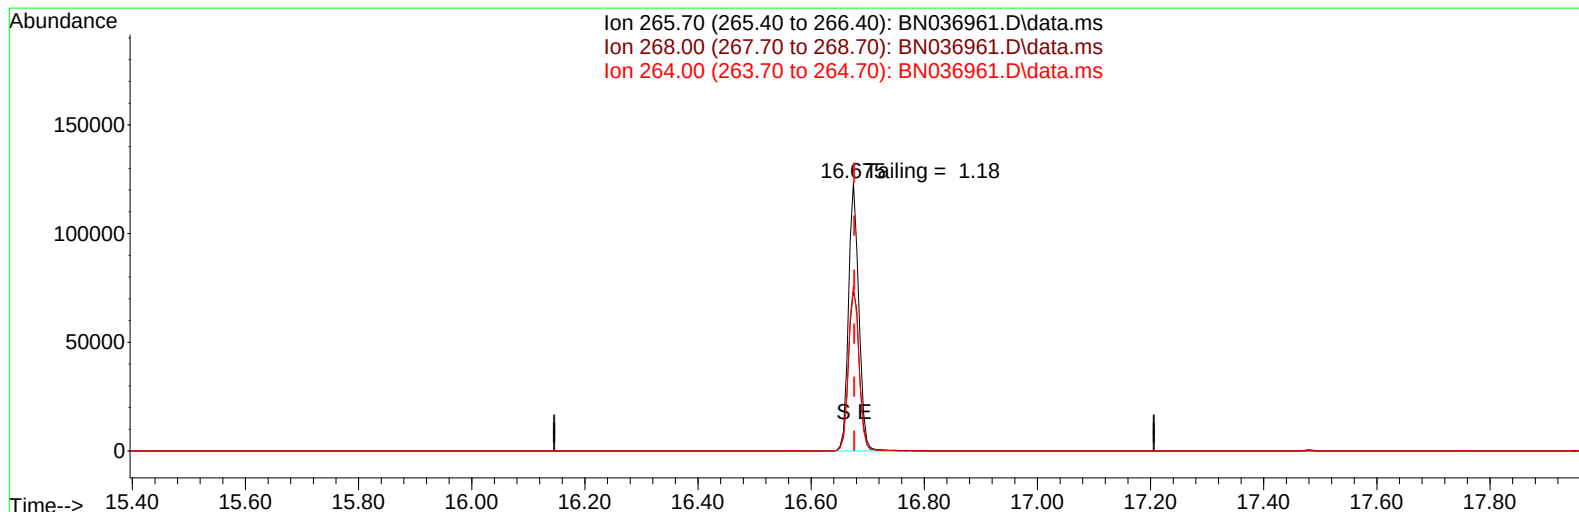

TIC: BN036961.D\data.ms

(70) Pentachlorophenol (C)




16.675min (-0.001) 16880.98 ng

response 157251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.69
264.00	61.60	61.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050725\
Data File : BN036961.D
Acq On : 07 May 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 16:10:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

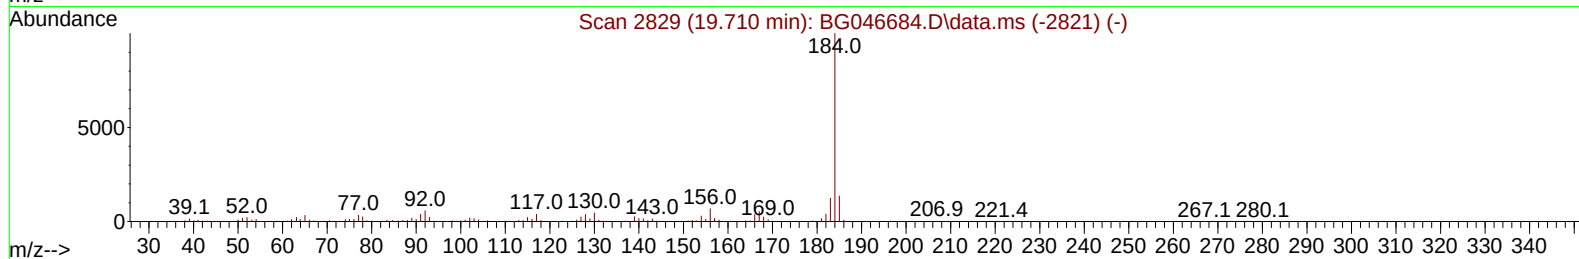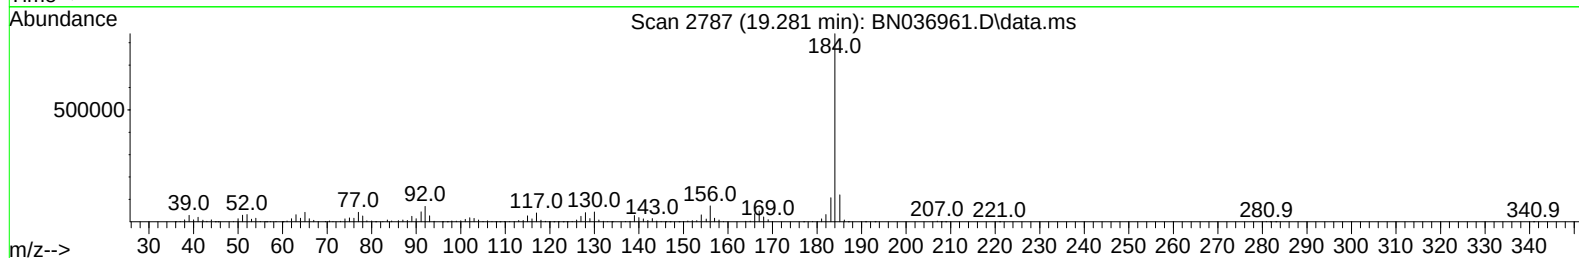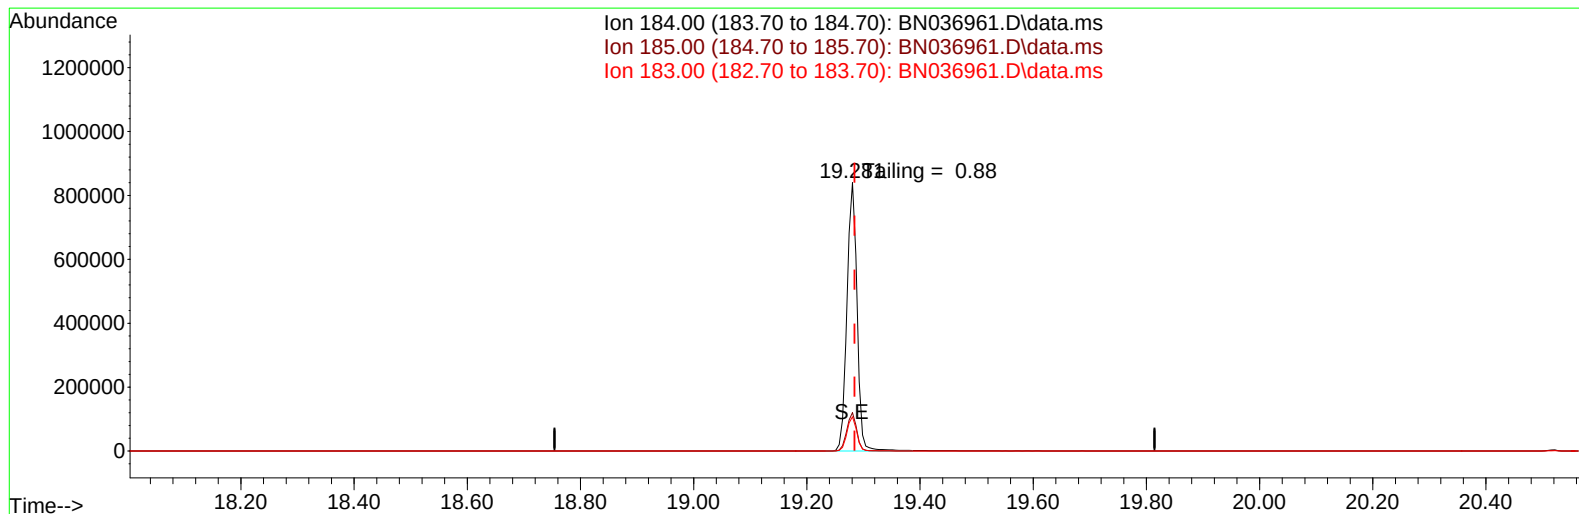

TIC: BN036961.D\data.ms

(77) Benzidine

19.281min (-0.003) 0.00 ng

response 1045231

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.75
0.00	0.00	0.00