

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
 Data File : BN025358.D
 Acq On : 09 May 2023 07:30
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: May 09 08:00:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 06:15:50 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	6839	0.400	ng	0.00
7) Naphthalene-d8	10.707	136	22375	0.400	ng	0.00
13) Acenaphthene-d10	14.544	164	13191	0.400	ng	0.00
19) Phenanthrene-d10	17.298	188	29173	0.400	ng	0.00
29) Chrysene-d12	21.491	240	26845	0.400	ng	# 0.00
35) Perylene-d12	23.927	264	23982	0.400	ng	0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.455	112	7263	0.436	ng	0.00
5) Phenol-d6	7.073	99	9659	0.462	ng	0.00
8) Nitrobenzene-d5	9.074	82	7696	0.418	ng	0.00
11) 2-Methylnaphthalene-d10	12.302	152	13719	0.449	ng	0.00
14) 2,4,6-Tribromophenol	16.045	330	2883	0.428	ng	0.00
15) 2-Fluorobiphenyl	13.165	172	21542	0.476	ng	-0.01
27) Fluoranthene-d10	19.330	212	31207	0.433	ng	0.00
31) Terphenyl-d14	19.924	244	26430	0.488	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.310	88	3173	0.442	ng	96
3) n-Nitrosodimethylamine	3.650	42	5246	0.478	ng	94
6) bis(2-Chloroethyl)ether	7.326	93	7448	0.404	ng	97
9) Naphthalene	10.760	128	26100	0.455	ng	99
10) Hexachlorobutadiene	11.038	225	5021	0.462	ng	# 98
12) 2-Methylnaphthalene	12.377	142	17839	0.440	ng	98
16) Acenaphthylene	14.266	152	26324	0.446	ng	99
17) Acenaphthene	14.608	154	16704	0.455	ng	98
18) Fluorene	15.592	166	21902	0.435	ng	99
20) 4,6-Dinitro-2-methylph...	15.722	198	393	0.342	ng	88
21) 4-Bromophenyl-phenylether	16.479	248	6877	0.423	ng	95
22) Hexachlorobenzene	16.603	284	7907	0.450	ng	100
23) Atrazine	16.752	200	5033	0.354	ng	98
24) Pentachlorophenol	16.963	266	3219	0.740	ng	92
25) Phenanthrene	17.336	178	36166	0.448	ng	100
26) Anthracene	17.435	178	32489	0.430	ng	100
28) Fluoranthene	19.359	202	43167	0.428	ng	99
30) Pyrene	19.722	202	45535	0.496	ng	100
32) Benzo(a)anthracene	21.482	228	40790	0.450	ng	99
33) Chrysene	21.527	228	42290	0.468	ng	99
34) Bis(2-ethylhexyl)phtha...	21.392	149	24407	0.343	ng	98
36) Indeno(1,2,3-cd)pyrene	26.465	276	36656	0.381	ng	99
37) Benzo(b)fluoranthene	23.182	252	36608	0.482	ng	96
38) Benzo(k)fluoranthene	23.232	252	37859	0.476	ng	98
39) Benzo(a)pyrene	23.825	252	35271	0.453	ng	98
40) Dibenzo(a,h)anthracene	26.483	278	29713	0.391	ng	99
41) Benzo(g,h,i)perylene	27.249	276	30939	0.371	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
 Data File : BN025358.D
 Acq On : 09 May 2023 07:30
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Quant Time: May 09 08:00:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 06:15:50 2023
 Response via : Initial Calibration

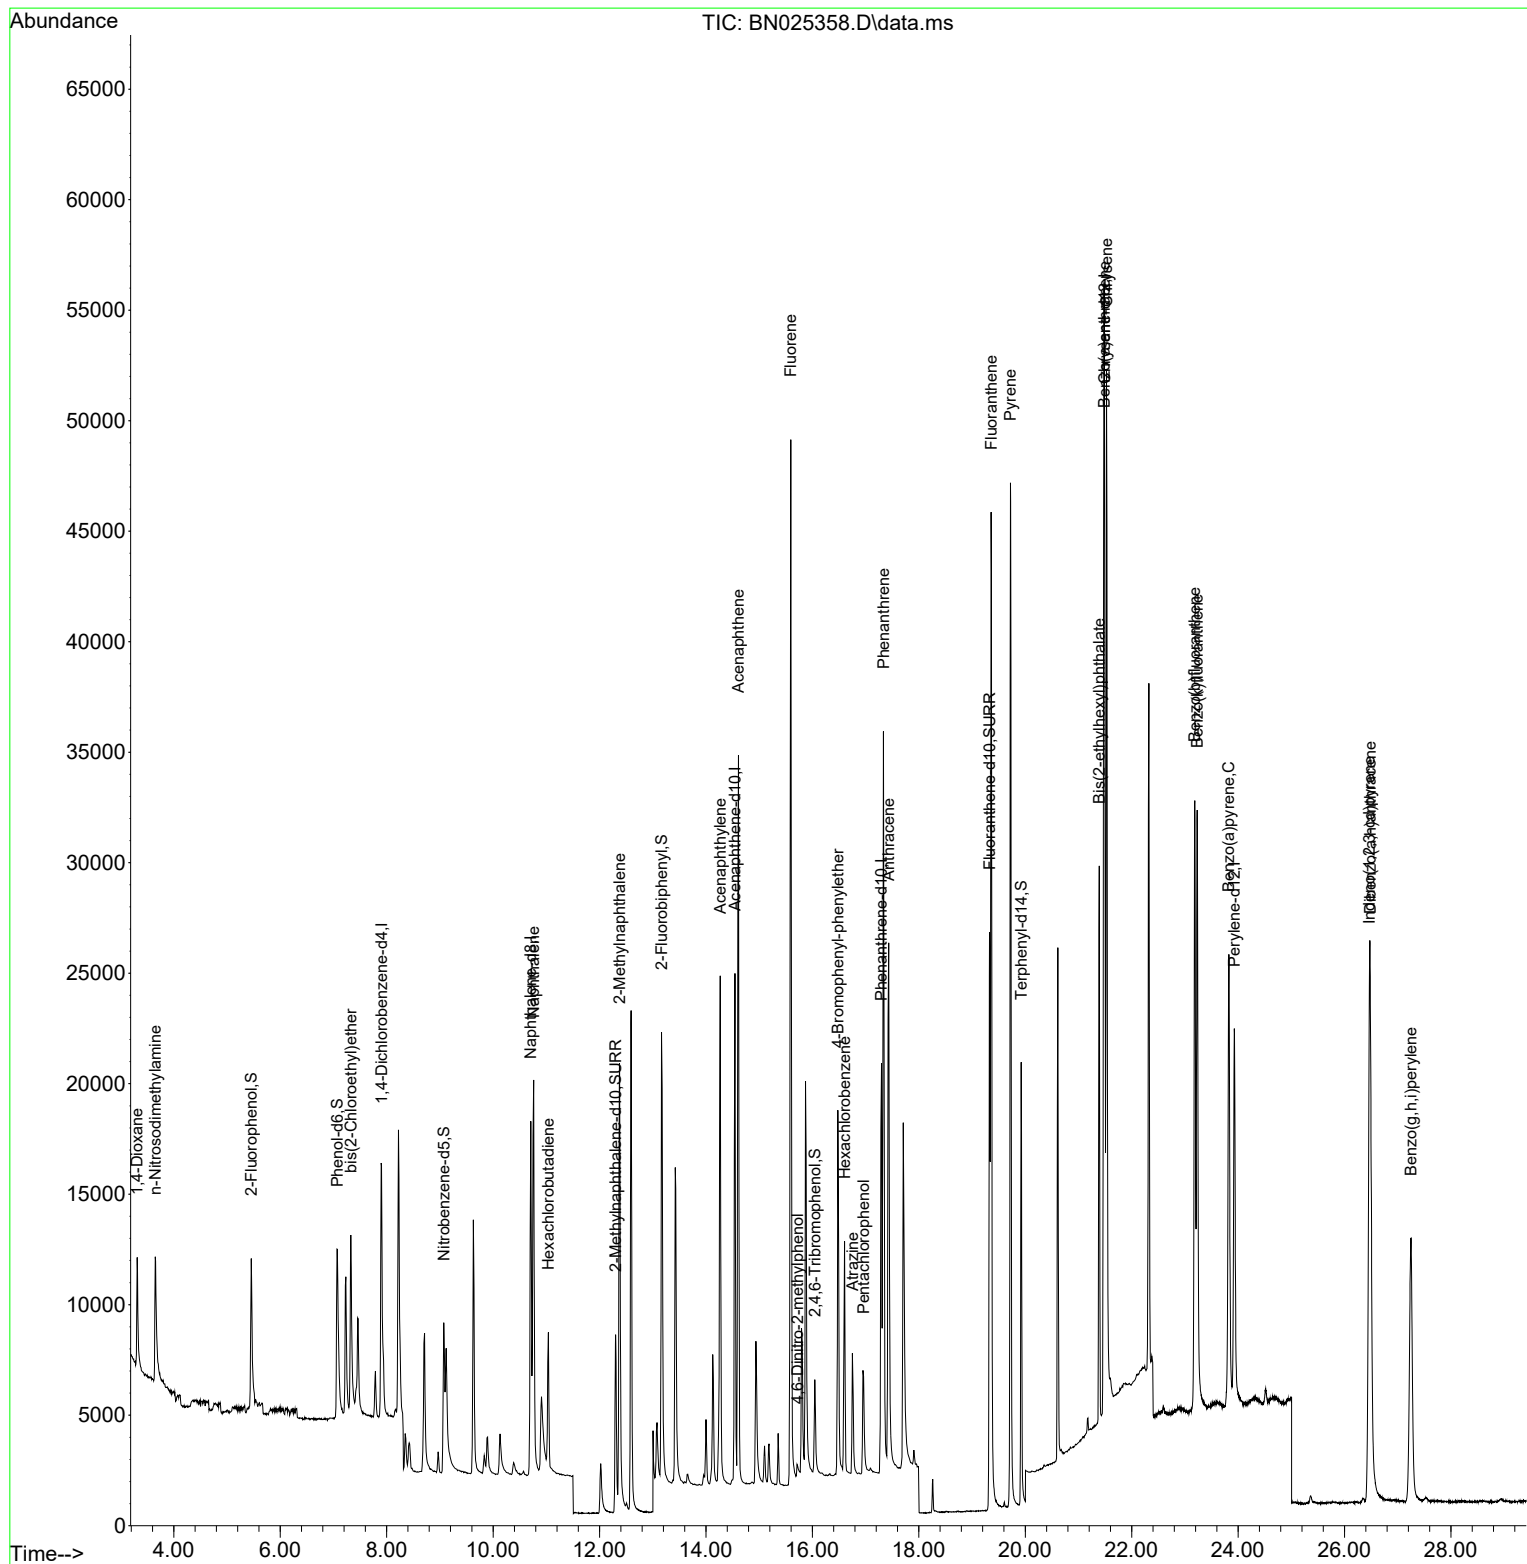






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.904 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC



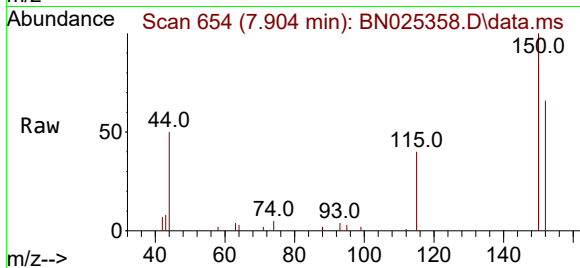



Tgt Ion:152 Resp: 6839
 Ion Ratio Lower Upper
 152 100
 150 152.2 123.8 185.8
 115 61.5 52.9 79.3

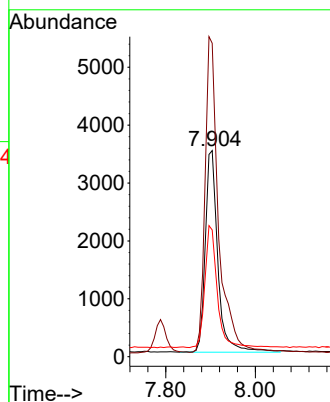

#2
 1,4-Dioxane
 Concen: 0.442 ng
 RT: 3.310 min Scan# 18
 Delta R.T. -0.007 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30

Tgt Ion: 88 Resp: 3173
 Ion Ratio Lower Upper
 88 100
 43 41.9 37.2 55.8
 58 91.4 71.5 107.3


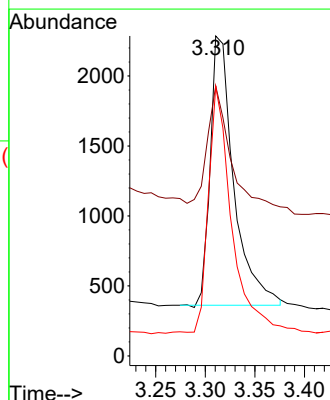
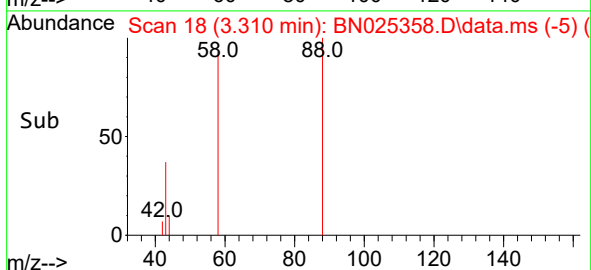
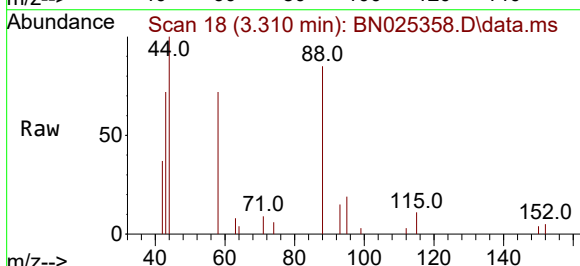




#3
n-Nitrosodimethylamine
Concen: 0.478 ng
RT: 3.650 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 5246
Ion Ratio Lower Upper
42 100
74 93.7 79.9 119.9
44 8.5 7.0 10.6

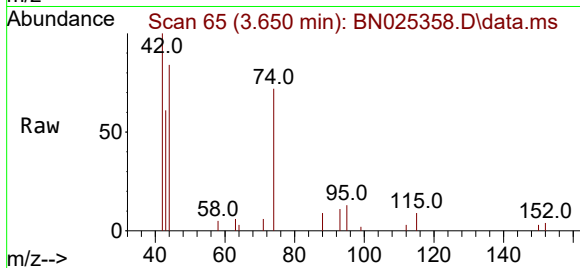

#4
2-Fluorophenol
Concen: 0.436 ng
RT: 5.455 min Scan# 315
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion: 112 Resp: 7263
Ion Ratio Lower Upper
112 100
64 64.2 51.5 77.3
63 34.4 27.8 41.6




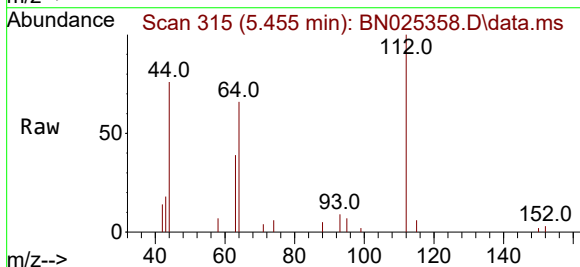




#5
Phenol-d6
Concen: 0.462 ng
RT: 7.073 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 9659
Ion Ratio Lower Upper
99 100
42 27.2 22.0 33.0
71 36.2 28.7 43.1

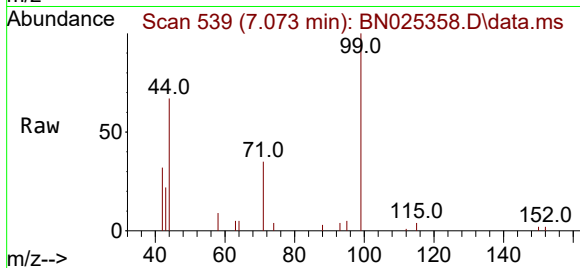

#6
bis(2-Chloroethyl)ether
Concen: 0.404 ng
RT: 7.326 min Scan# 574
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion: 93 Resp: 7448
Ion Ratio Lower Upper
93 100
63 87.1 67.8 101.6
95 34.8 26.7 40.1




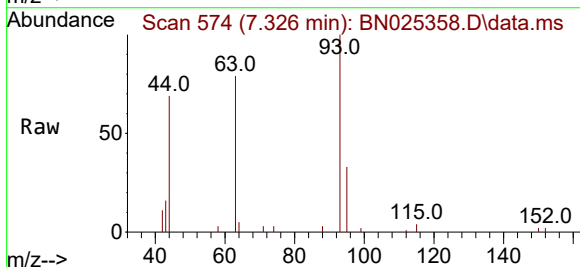




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:136 Resp: 22375
Ion Ratio Lower Upper
136 100
137 11.4 9.4 14.2
54 11.9 8.5 12.7
68 7.6 5.8 8.8

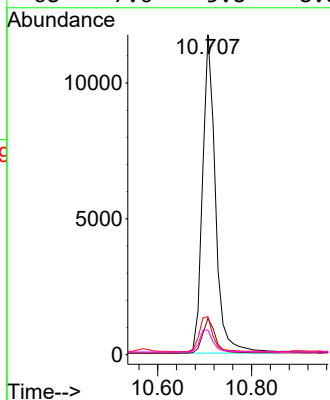

#8
Nitrobenzene-d5
Concen: 0.418 ng
RT: 9.074 min Scan# 782
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion: 82 Resp: 7696
Ion Ratio Lower Upper
82 100
128 40.1 35.3 52.9
54 67.7 48.7 73.1



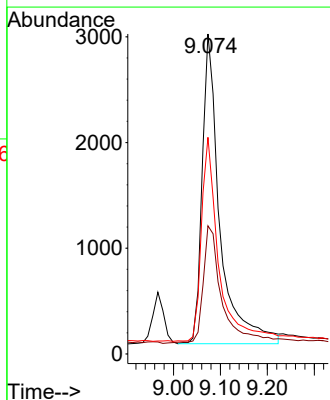





#9
Naphthalene
Concen: 0.455 ng
RT: 10.760 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128 Resp: 26100
Ion Ratio Lower Upper
128 100
129 11.3 9.4 14.2
127 13.5 11.0 16.6



#10
Hexachlorobutadiene
Concen: 0.462 ng
RT: 11.038 min Scan# 966
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:225 Resp: 5021
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 49.8 74.8


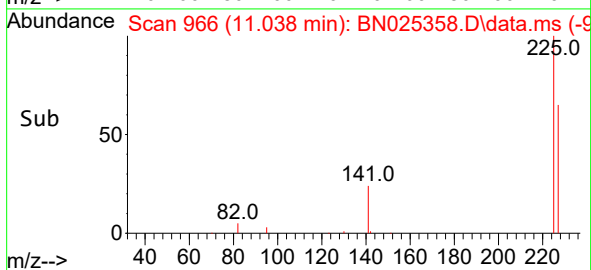






#11
2-Methylnaphthalene-d10
Concen: 0.449 ng
RT: 12.302 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 13719
Ion Ratio Lower Upper
152 100
151 20.4 16.4 24.6

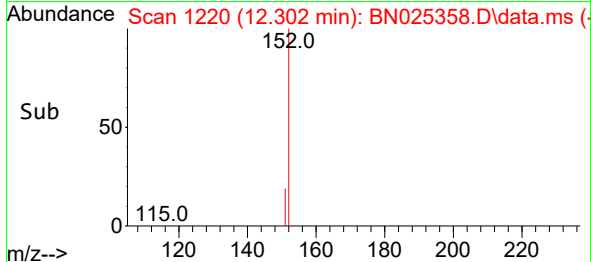

#12
2-Methylnaphthalene
Concen: 0.440 ng
RT: 12.377 min Scan# 1240
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:142 Resp: 17839
Ion Ratio Lower Upper
142 100
141 87.3 70.5 105.7
115 37.5 31.6 47.4


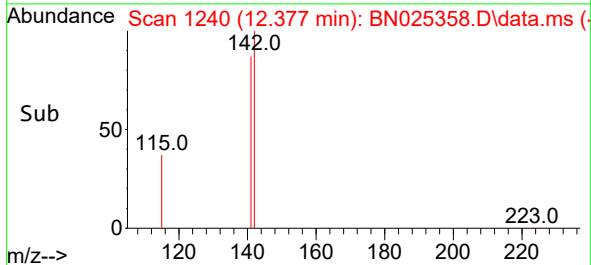




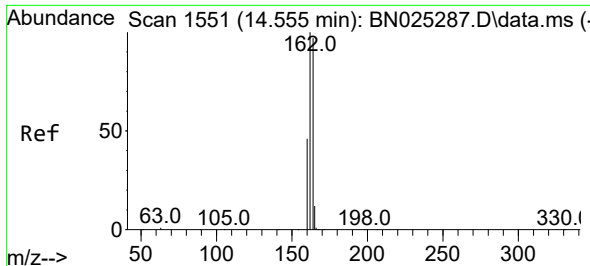

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.544 min Scan# 1550
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 13191
Ion Ratio Lower Upper
164 100
162 102.6 82.1 123.1
160 48.7 38.3 57.5

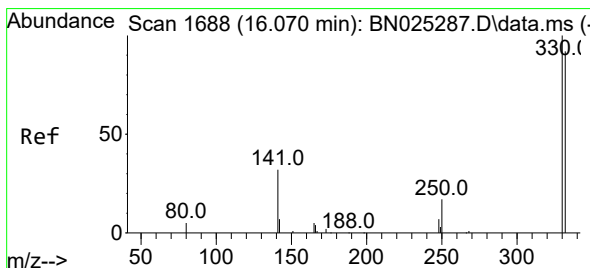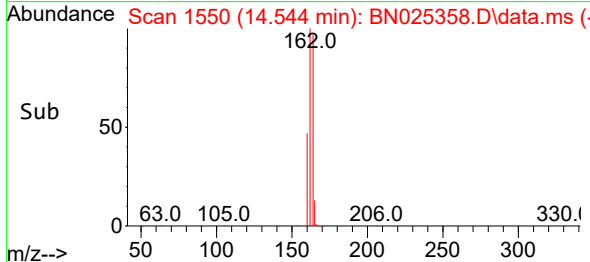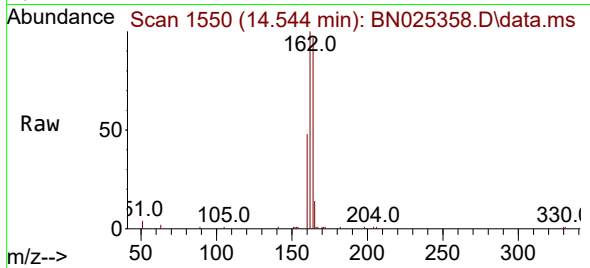

#14
2,4,6-Tribromophenol
Concen: 0.428 ng
RT: 16.045 min Scan# 1686
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:330 Resp: 2883
Ion Ratio Lower Upper
330 100
332 96.1 77.4 116.0
141 38.7 28.9 43.3


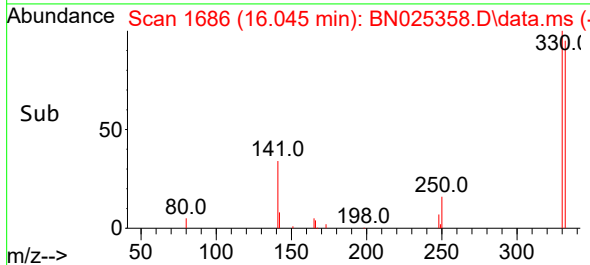

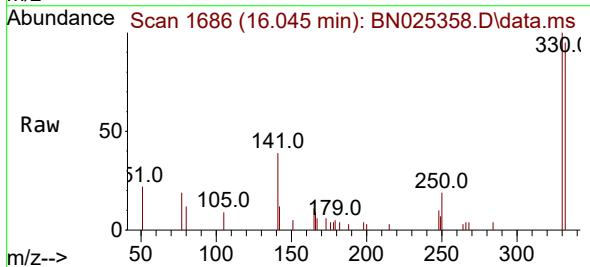




#15
2-Fluorobiphenyl
Concen: 0.476 ng
RT: 13.165 min Scan# 1423
Delta R.T. -0.011 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 21542
Ion Ratio Lower Upper
172 100
171 35.4 27.9 41.9
170 24.5 19.0 28.4

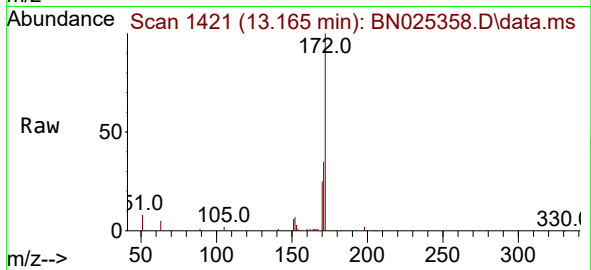

#16
Acenaphthylene
Concen: 0.446 ng
RT: 14.266 min Scan# 1524
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:152 Resp: 26324
Ion Ratio Lower Upper
152 100
151 19.7 16.1 24.1
153 13.0 10.3 15.5


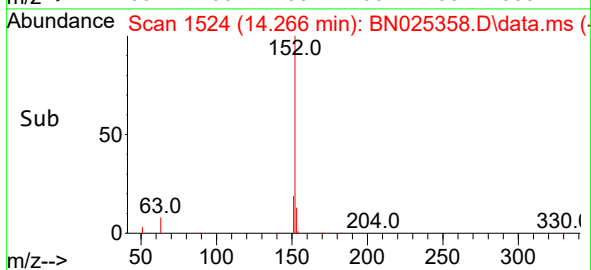






#17
Acenaphthene
Concen: 0.455 ng
RT: 14.608 min Scan# 1556
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 16704
Ion Ratio Lower Upper
154 100
153 115.8 91.3 136.9
152 57.9 44.7 67.1



#18
Fluorene
Concen: 0.435 ng
RT: 15.592 min Scan# 1648
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:166 Resp: 21902
Ion Ratio Lower Upper
166 100
165 98.0 79.0 118.4
167 13.1 10.3 15.5

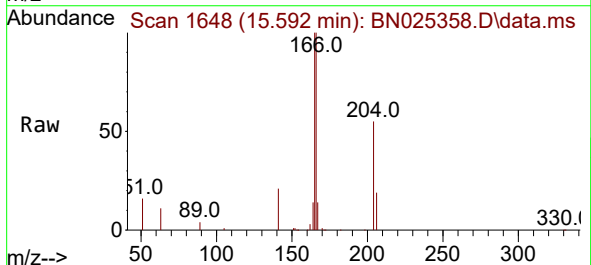



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.298 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:188 Resp: 29173

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.7 8.0 12.0

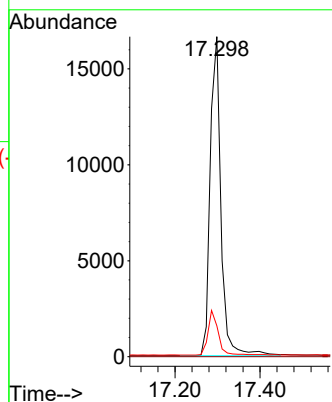

#20

4,6-Dinitro-2-methylphenol

Concen: 0.342 ng

RT: 15.722 min Scan# 1660

Delta R.T. 0.000 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30




Tgt Ion:198 Resp: 393


Ion Ratio Lower Upper

198 100

51 224.3 162.1 243.1

105 95.6 83.1 124.7


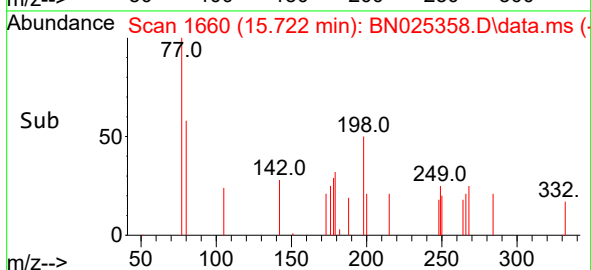




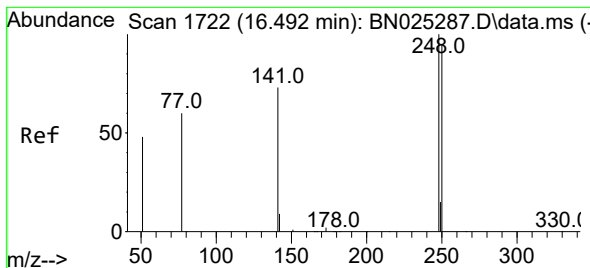

#21
4-Bromophenyl-phenylether
Concen: 0.423 ng
RT: 16.479 min Scan# 1721
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 6877
Ion Ratio Lower Upper
248 100
250 91.2 76.0 114.0
141 80.6 59.9 89.9

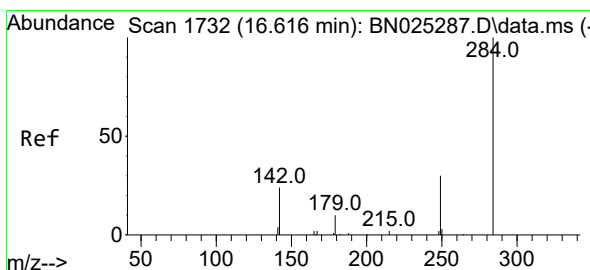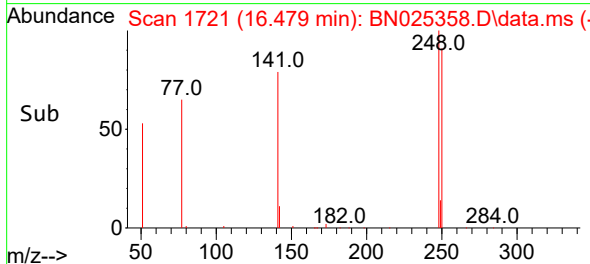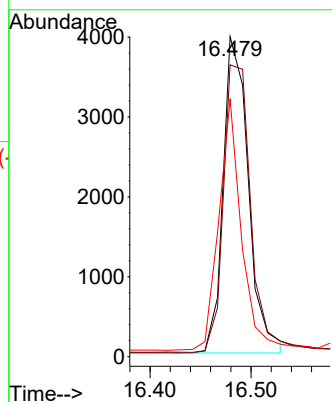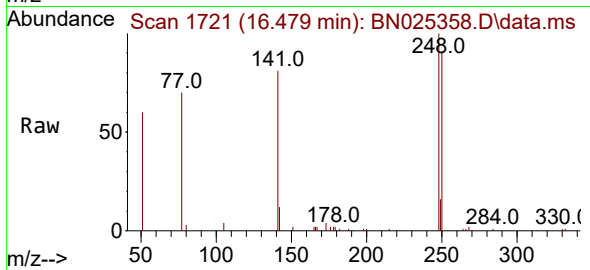

#22
Hexachlorobenzene
Concen: 0.450 ng
RT: 16.603 min Scan# 1731
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:284 Resp: 7907
Ion Ratio Lower Upper
284 100
142 37.6 30.0 45.0
249 31.6 25.0 37.6

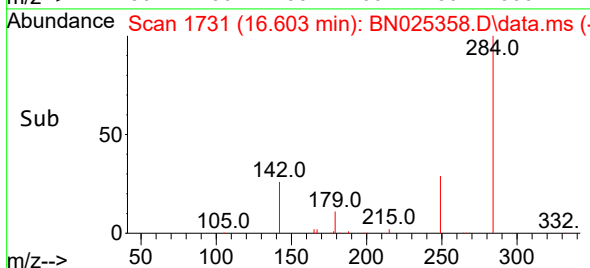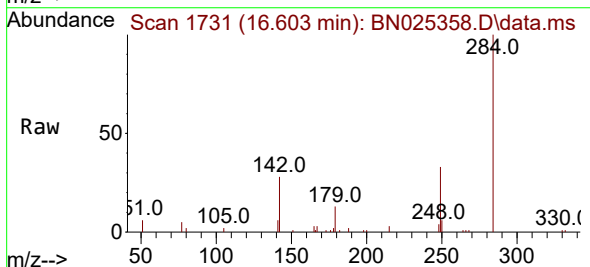



#23

Atrazine

Concen: 0.354 ng

RT: 16.752 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:200 Resp: 5033

Ion Ratio Lower Upper

200 100

173 30.0 26.3 39.5

215 46.7 37.2 55.8

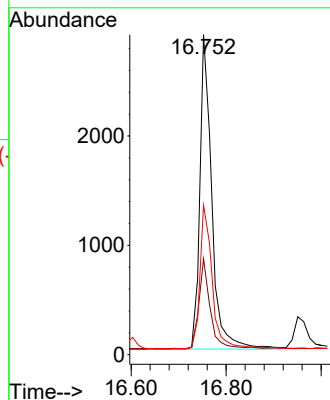

#24

Pentachlorophenol

Concen: 0.740 ng

RT: 16.963 min Scan# 1760

Delta R.T. 0.000 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30




Tgt Ion:266 Resp: 3219


Ion Ratio Lower Upper

266 100

264 62.1 43.0 64.4

268 63.2 47.4 71.2


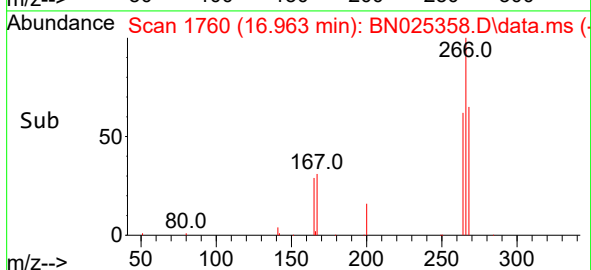
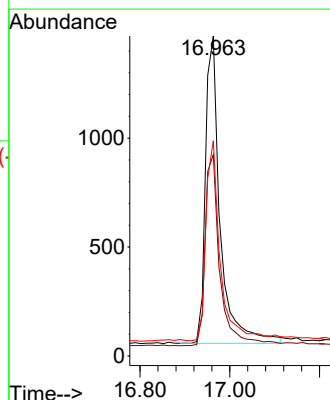





#25
Phenanthrene
Concen: 0.448 ng
RT: 17.336 min Scan# 1790
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 36166
Ion Ratio Lower Upper
178 100
176 19.2 15.5 23.3
179 15.5 12.4 18.6



#26
Anthracene
Concen: 0.430 ng
RT: 17.435 min Scan# 1798
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:178 Resp: 32489
Ion Ratio Lower Upper
178 100
176 18.6 14.9 22.3
179 15.0 12.0 18.0


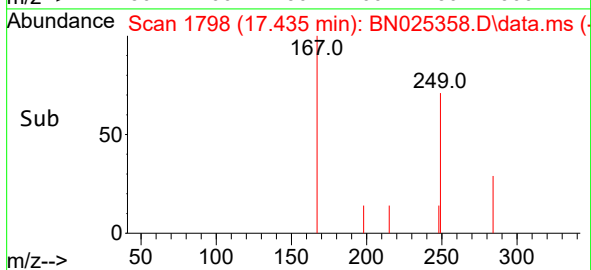






#27
Fluoranthene-d10
Concen: 0.433 ng
RT: 19.330 min Scan# 2158
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 31207
Ion Ratio Lower Upper
212 100
106 15.5 12.6 19.0
104 8.6 7.0 10.6

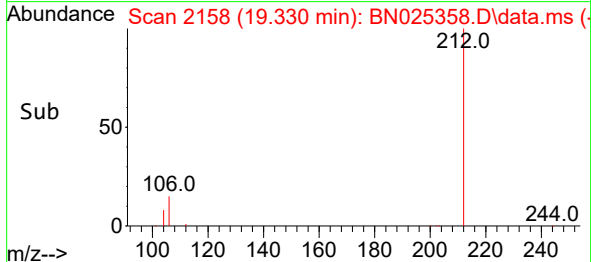

#28
Fluoranthene
Concen: 0.428 ng
RT: 19.359 min Scan# 2165
Delta R.T. 0.000 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Tgt Ion:202 Resp: 43167
Ion Ratio Lower Upper
202 100
101 11.8 9.8 14.8
203 17.0 13.5 20.3

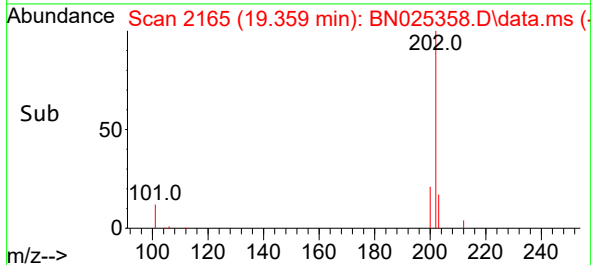

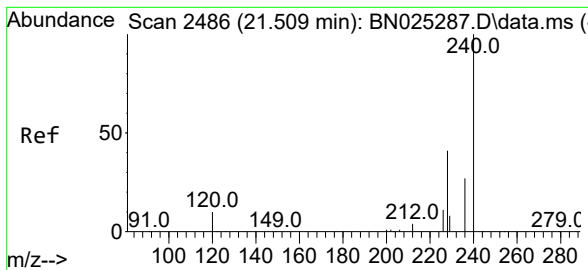

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.491 min Scan# 2484

Delta R.T. 0.005 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:240 Resp: 26845

Ion Ratio Lower Upper

240 100

120 16.4 10.3 15.5#

236 28.1 22.3 33.5

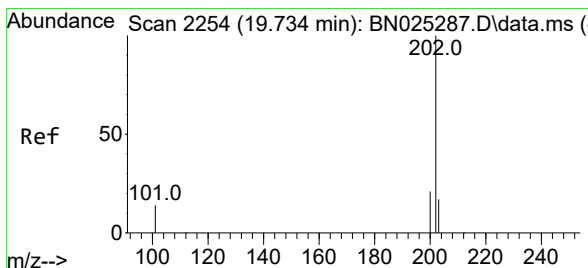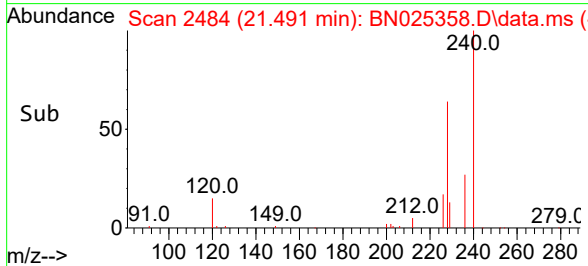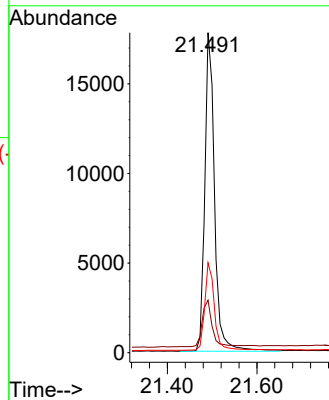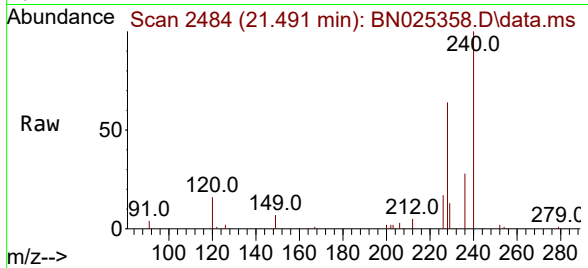

#30

Pyrene

Concen: 0.496 ng

RT: 19.722 min Scan# 2251

Delta R.T. -0.004 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30




Tgt Ion:202 Resp: 45535


Ion Ratio Lower Upper

202 100

200 21.0 16.8 25.2

203 17.9 14.4 21.6


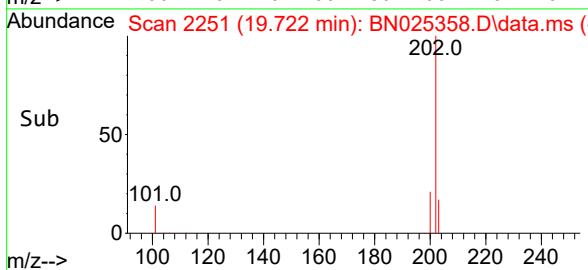
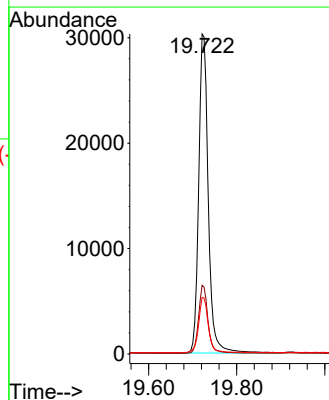
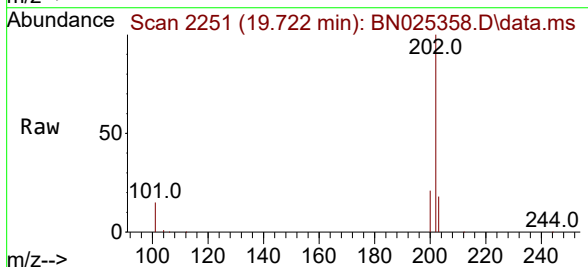




#31
 Terphenyl-d14
 Concen: 0.488 ng
 RT: 19.924 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:244 Resp: 26430
 Ion Ratio Lower Upper
 244 100
 212 8.8 7.1 10.7
 122 0.0 0.0 0.0

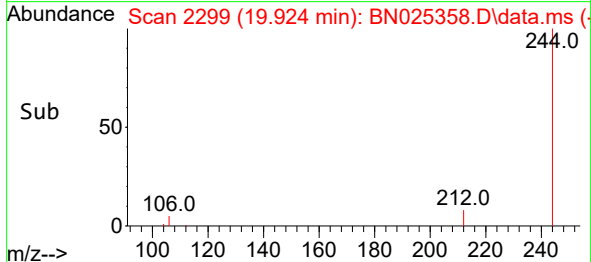

#32
 Benzo(a)anthracene
 Concen: 0.450 ng
 RT: 21.482 min Scan# 2483
 Delta R.T. 0.014 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30

Tgt Ion:228 Resp: 40790
 Ion Ratio Lower Upper
 228 100
 226 27.1 22.5 33.7
 229 20.1 16.2 24.2

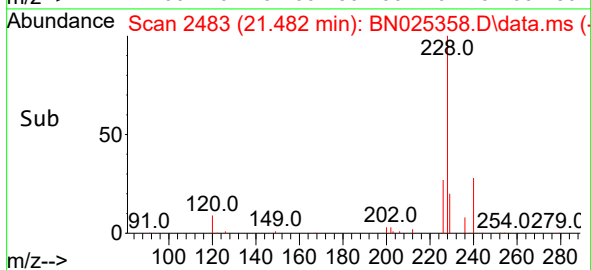



#33

Chrysene

Concen: 0.468 ng

RT: 21.527 min Scan# 2488

Delta R.T. 0.005 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:228 Resp: 42290

Ion Ratio Lower Upper

228 100

226 31.1 24.6 36.8

229 19.5 16.2 24.4



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.343 ng

RT: 21.392 min Scan# 2473

Delta R.T. 0.014 min

Lab File: BN025358.D

Acq: 09 May 2023 07:30




Tgt Ion:149 Resp: 24407


Ion Ratio Lower Upper

149 100

167 26.7 22.2 33.4

279 3.3 2.6 4.0


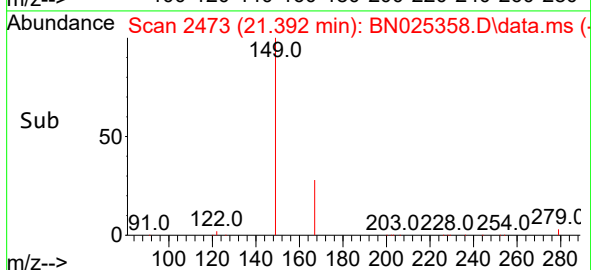
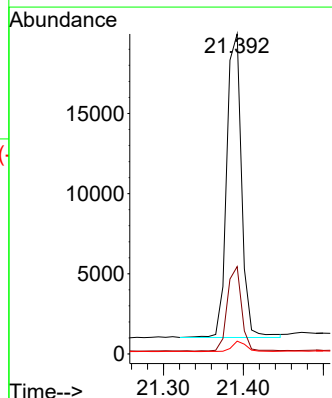





#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.927 min Scan# 3107
 Delta R.T. 0.016 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	264	Resp:	23982
Ion Ratio	Lower	Upper	
264	100		
260	25.6	21.5	32.3
265	49.4	46.2	69.4

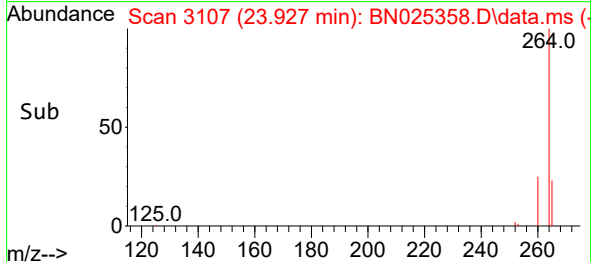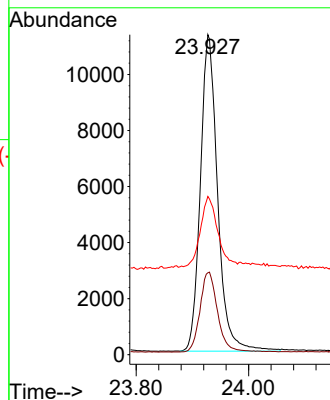

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.381 ng
 RT: 26.465 min Scan# 3975
 Delta R.T. 0.008 min
 Lab File: BN025358.D
 Acq: 09 May 2023 07:30

Tgt Ion:	276	Resp:	36656
Ion Ratio	Lower	Upper	
276	100		
138	27.6	22.5	33.7
277	24.7	19.8	29.6


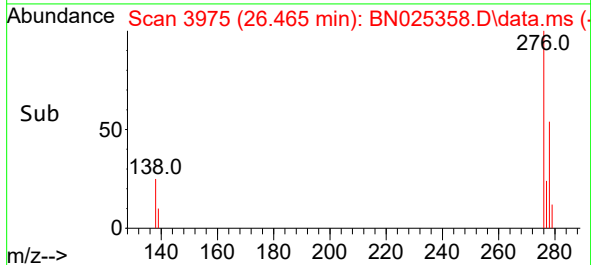
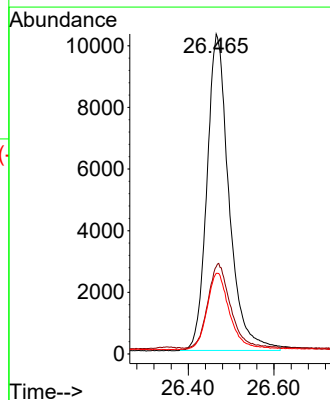





#37
Benzo(b)fluoranthene
Concen: 0.482 ng
RT: 23.182 min Scan# 2852
Delta R.T. 0.010 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 36608
Ion Ratio Lower Upper
252 100
253 24.4 20.8 31.2
125 14.6 13.4 20.2

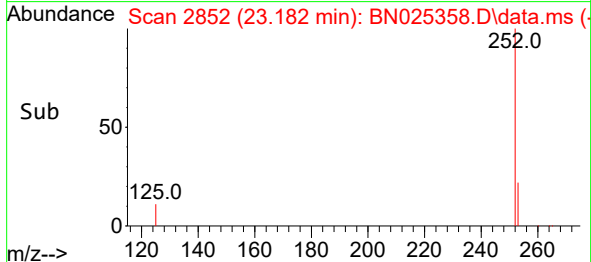

#38
Benzo(k)fluoranthene
Concen: 0.476 ng
RT: 23.232 min Scan# 2869
Delta R.T. 0.013 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30


Tgt Ion:252 Resp: 37859
Ion Ratio Lower Upper
252 100
253 24.9 20.6 30.8
125 14.9 13.1 19.7

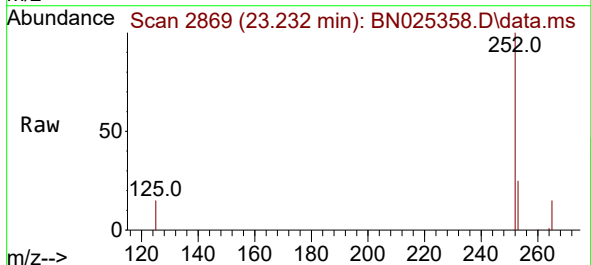






#39
Benzo(a)pyrene
Concen: 0.453 ng
RT: 23.825 min Scan# 3073
Delta R.T. 0.013 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 35271
Ion Ratio Lower Upper
252 100
253 25.9 21.4 32.0
125 17.6 15.4 23.2

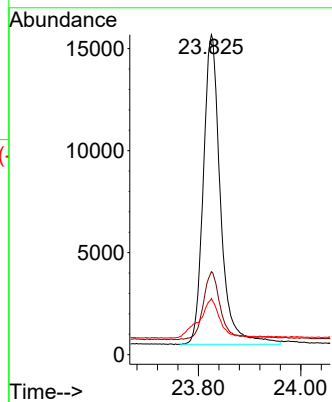

#40
Dibenzo(a,h)anthracene
Concen: 0.391 ng
RT: 26.483 min Scan# 3981
Delta R.T. 0.010 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30


Tgt Ion:278 Resp: 29713
Ion Ratio Lower Upper
278 100
139 21.4 17.6 26.4
279 26.7 21.6 32.4

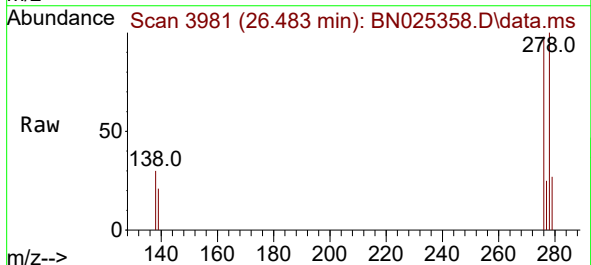

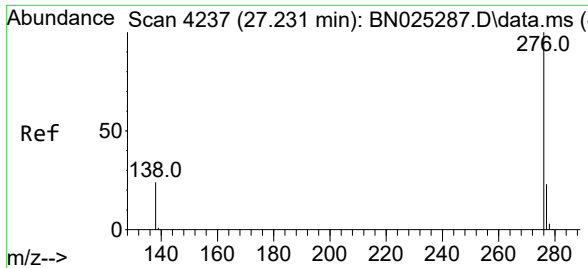

#41
Benzo(g,h,i)perylene
Concen: 0.371 ng
RT: 27.249 min Scan# 41
Delta R.T. 0.013 min
Lab File: BN025358.D
Acq: 09 May 2023 07:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

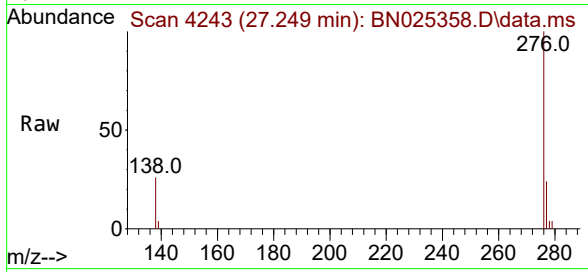

Tgt Ion:276 Resp: 30939
Ion Ratio Lower Upper
276 100
277 24.4 20.1 30.1
138 25.8 21.0 31.6

