
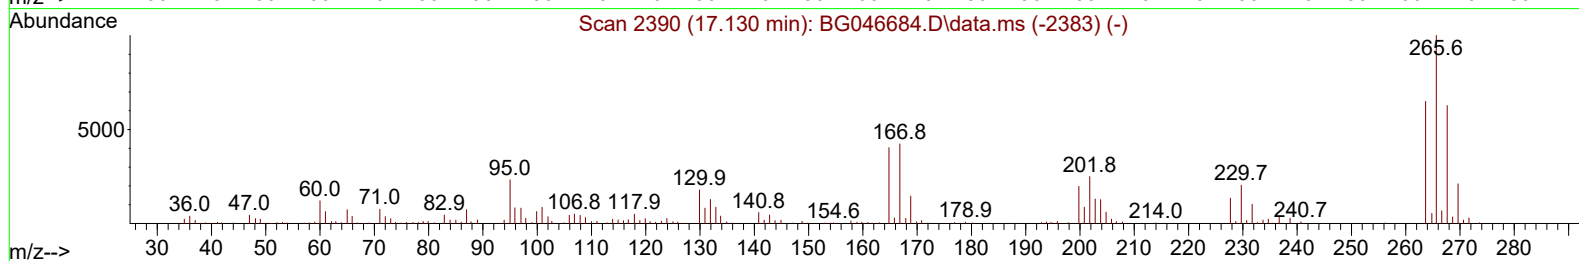
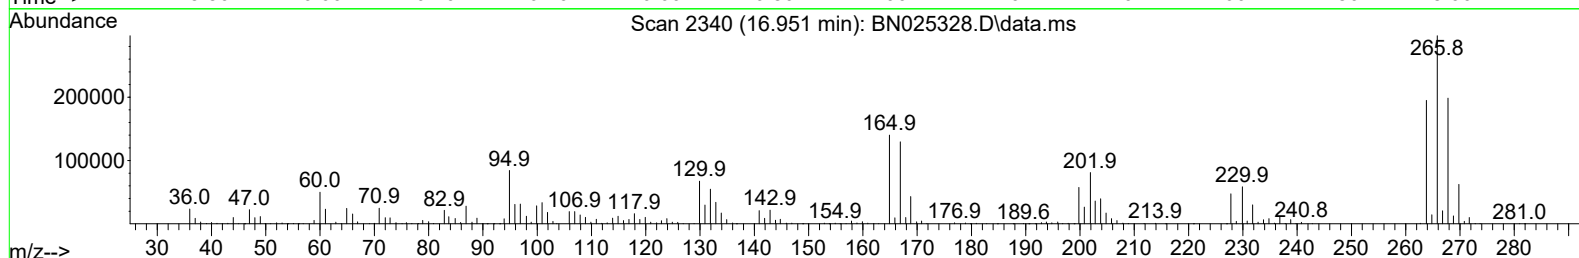


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN050823\  
 Data File : BN025328.D  
 Acq On : 08 May 2023 12:12  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 08:17:07 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue May 09 08:17:02 2023  
 Response via : Initial Calibration

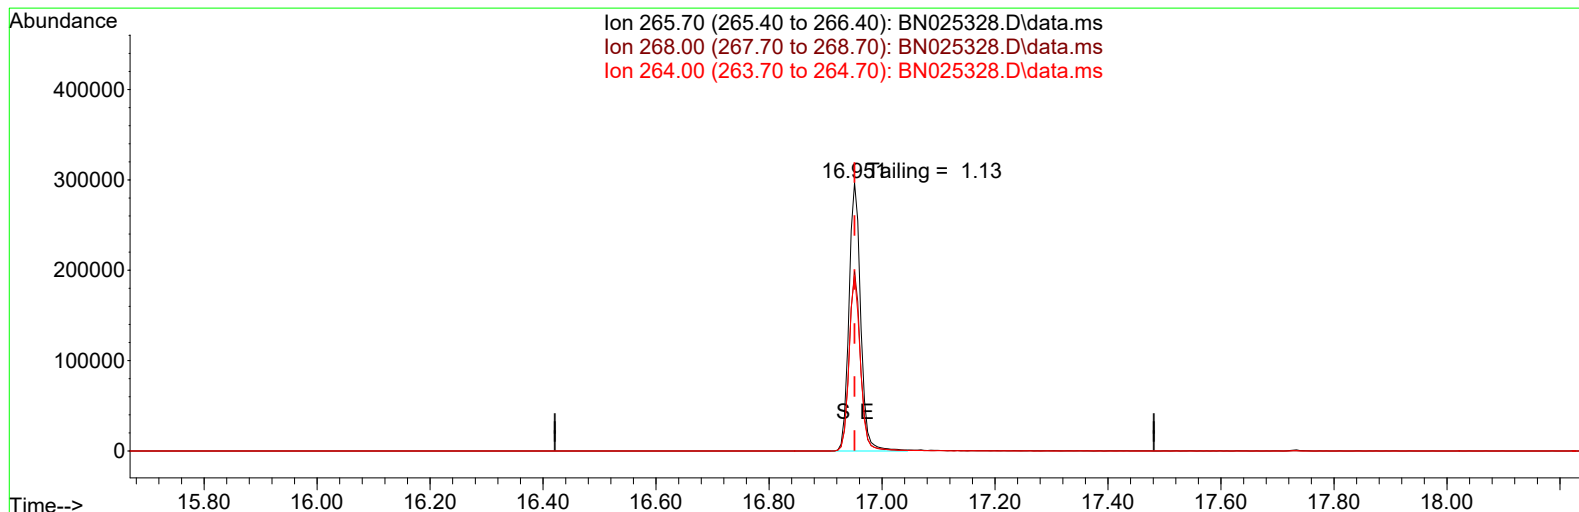

TIC: BN025328.D\data.ms

**(70) Pentachlorophenol (C)**




16.951min ( 0.000) 23474.17 ng

response 429968

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.79  |
| 264.00 | 61.60  | 65.60  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN050823\  
Data File : BN025328.D  
Acq On : 08 May 2023 12:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 08:17:07 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 09 08:17:02 2023  
Response via : Initial Calibration

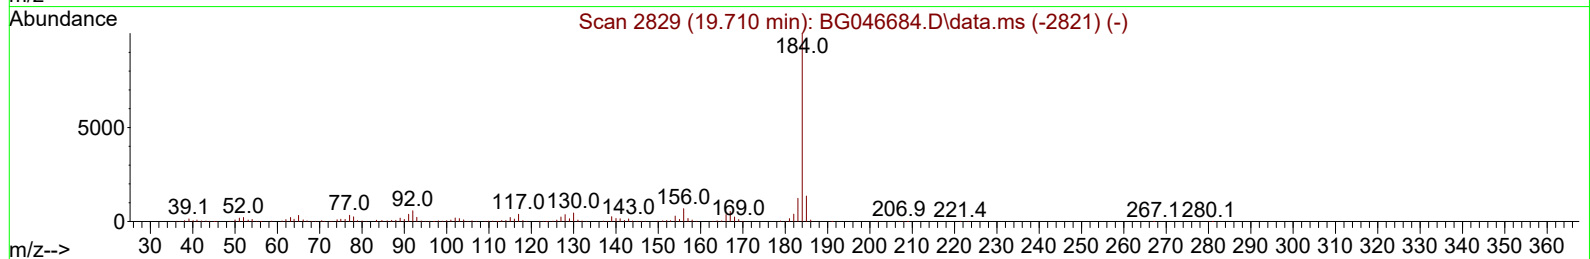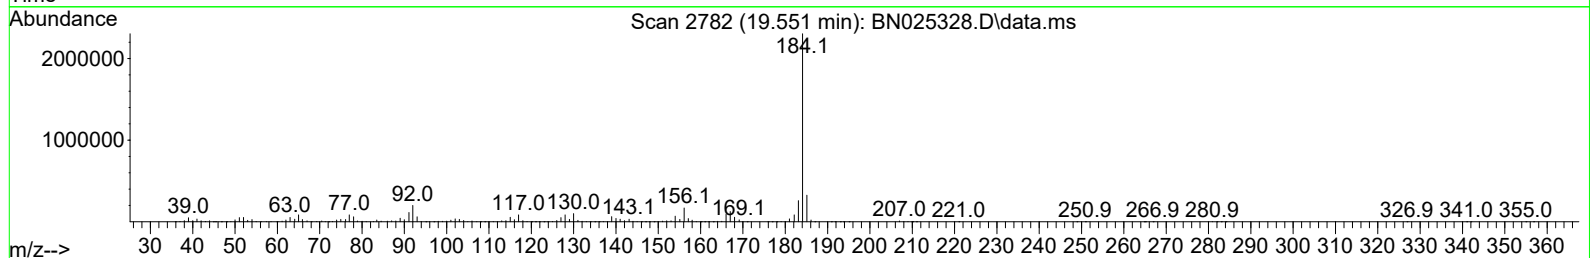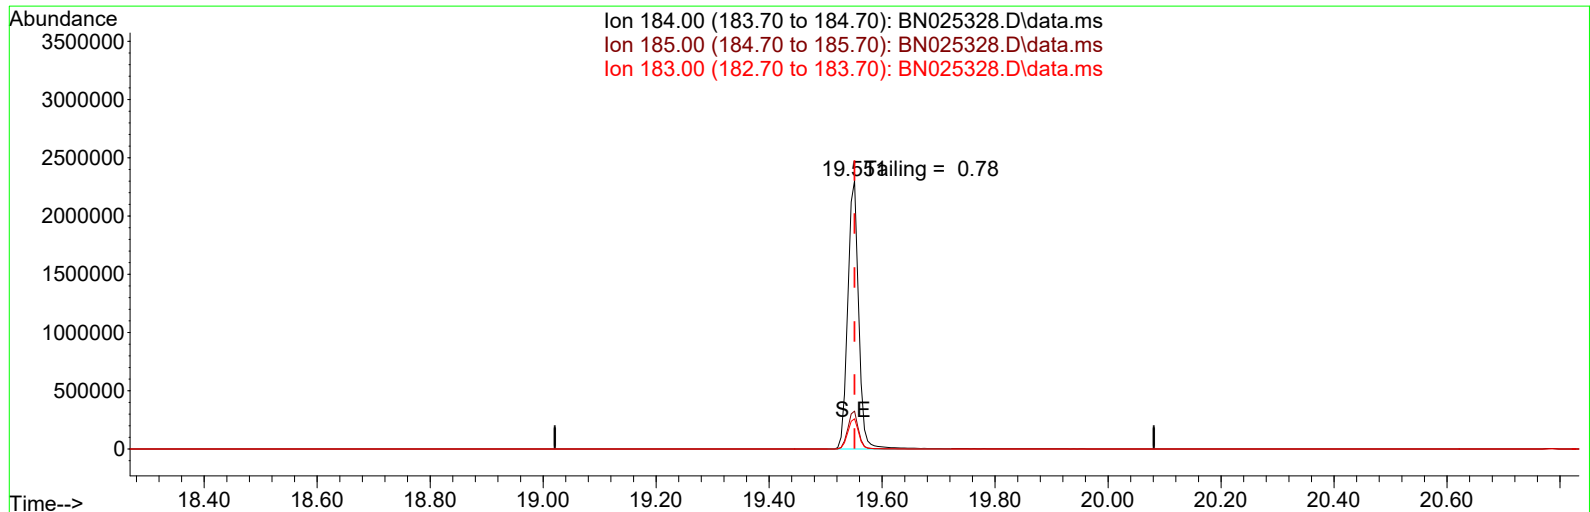

TIC: BN025328.D\data.ms

**(77) Benzidine****19.551min ( 0.000) 1684591.20 ng****response 3115689**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.13  |
| 183.00 | 13.20  | 11.28  |
| 0.00   | 0.00   | 0.00   |