
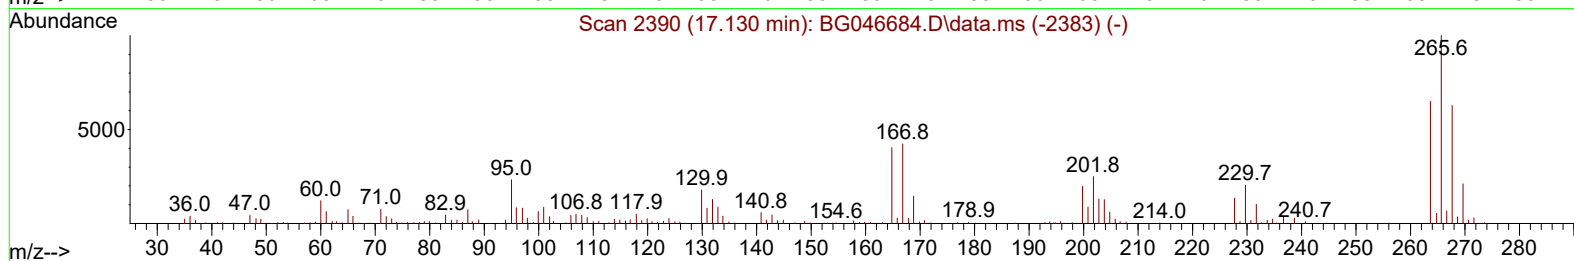
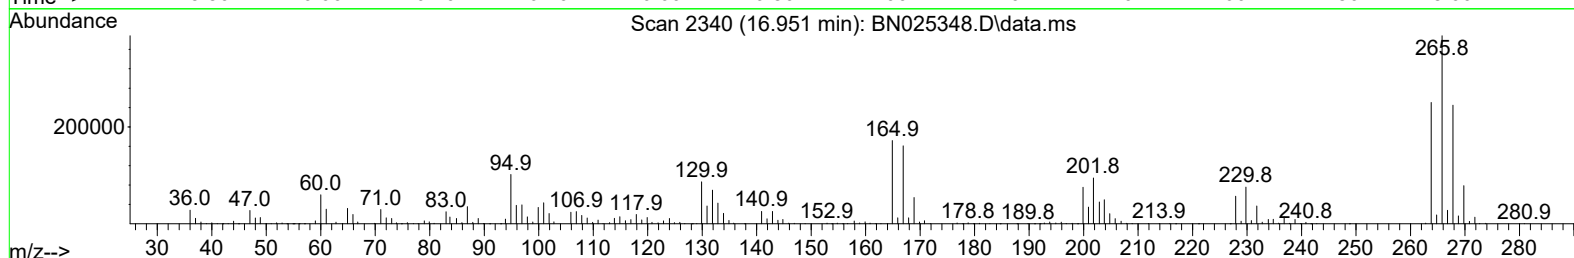


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025348.D
Acq On : 09 May 2023 00:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 08:18:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 08:17:02 2023
Response via : Initial Calibration

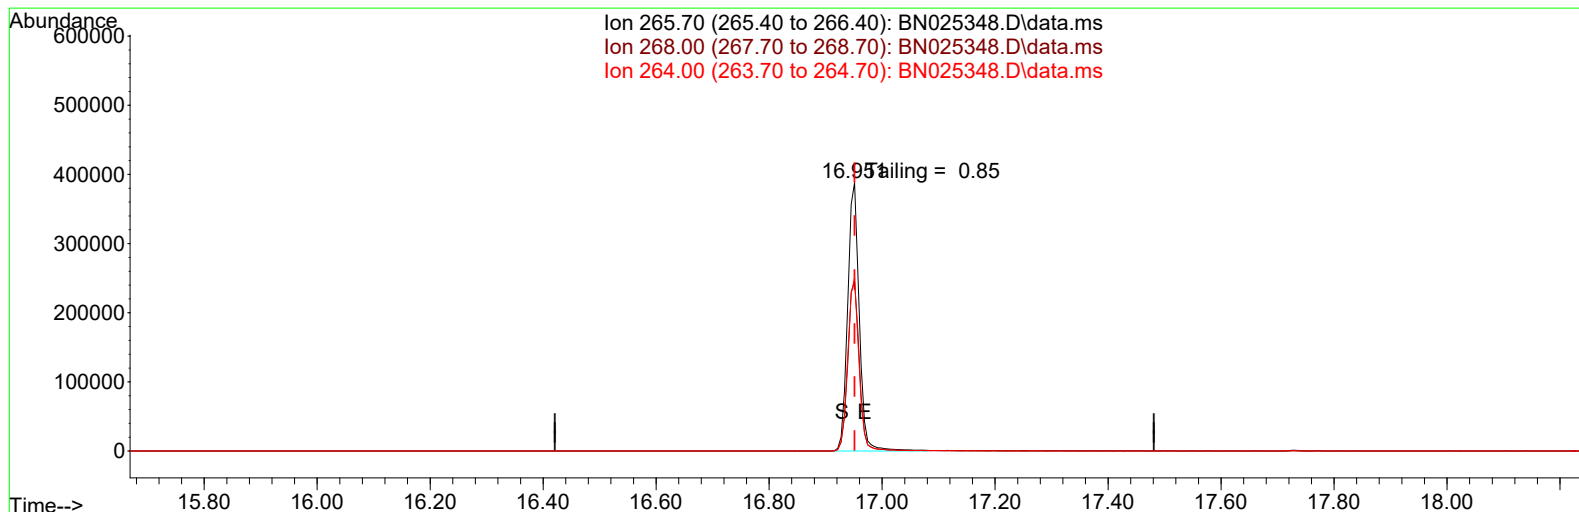

TIC: BN025348.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.000) 27755.93 ng

response 554138

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025348.D
Acq On : 09 May 2023 00:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 09 08:18:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 08:17:02 2023
Response via : Initial Calibration

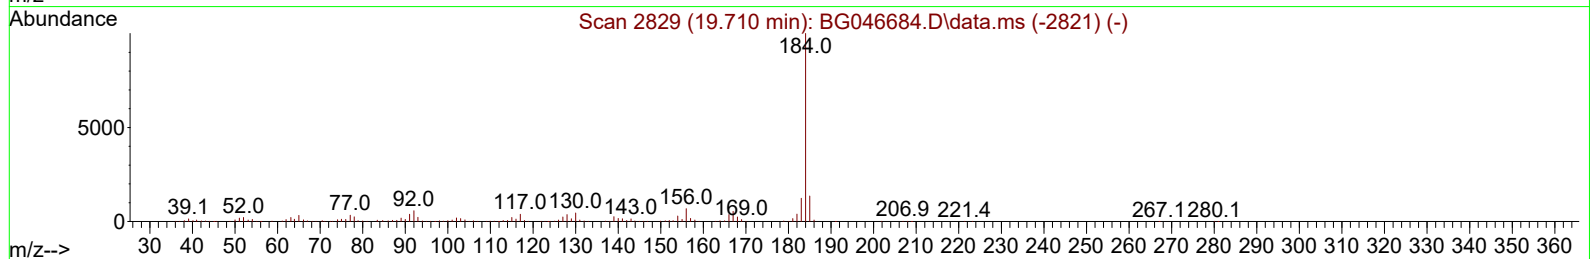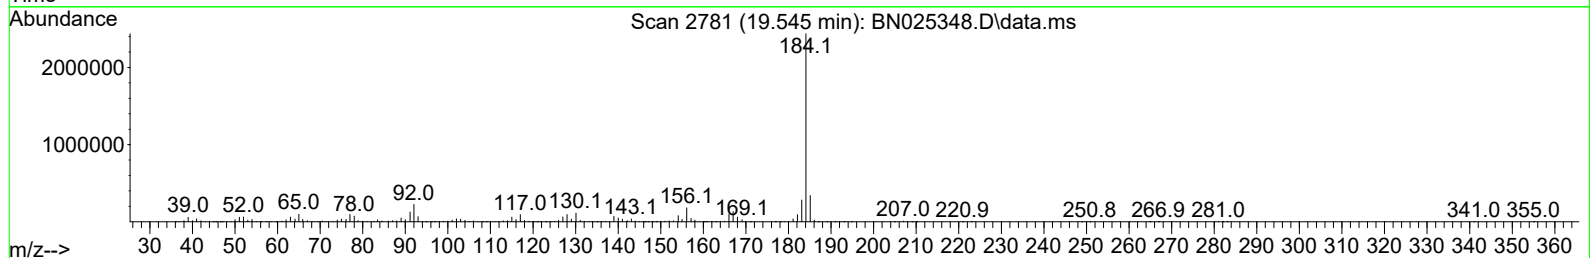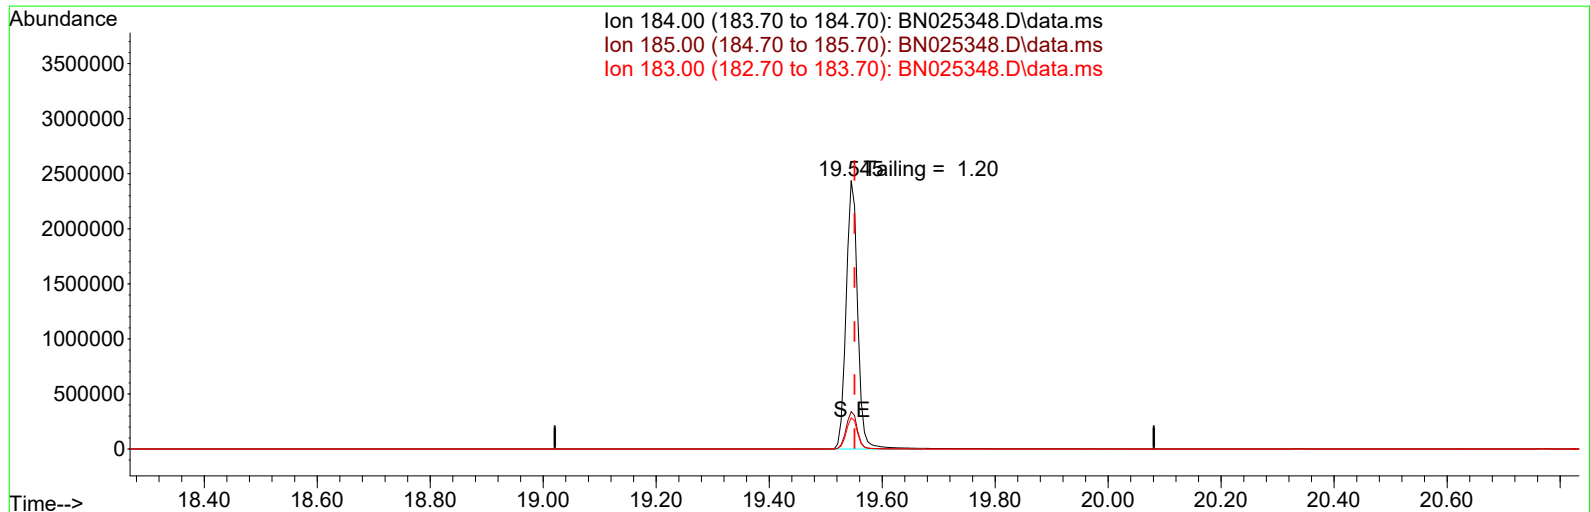

TIC: BN025348.D\data.ms

(77) Benzidine**19.545min (-0.006) 978542.03 ng****response 3468851**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.63
0.00	0.00	0.00