
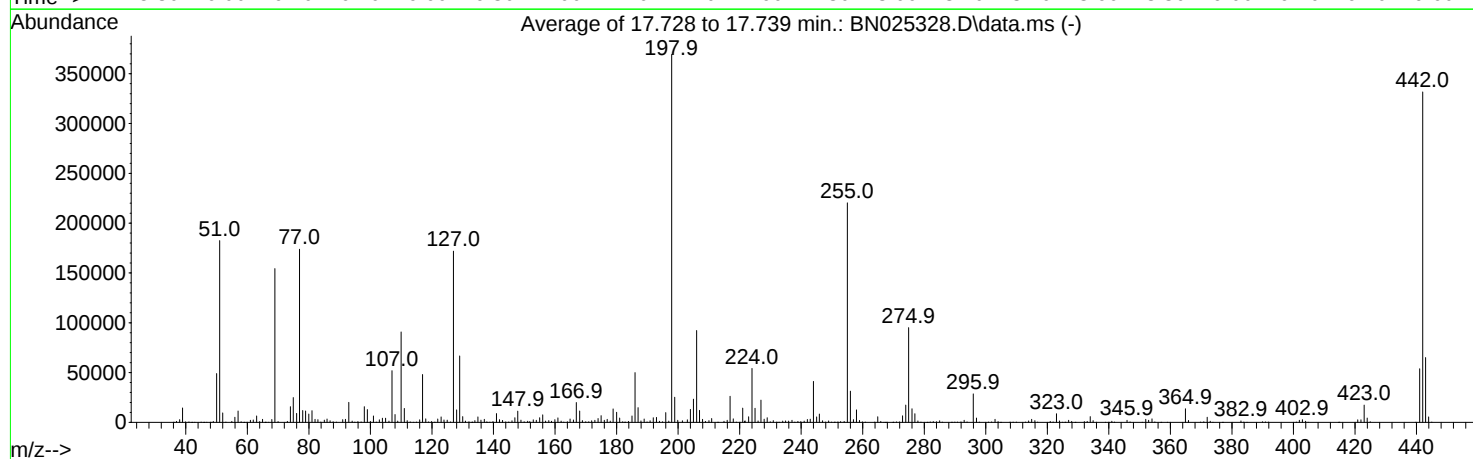


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
 Data File : BN025328.D
 Acq On : 08 May 2023 12:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 09 10:18:02 2023

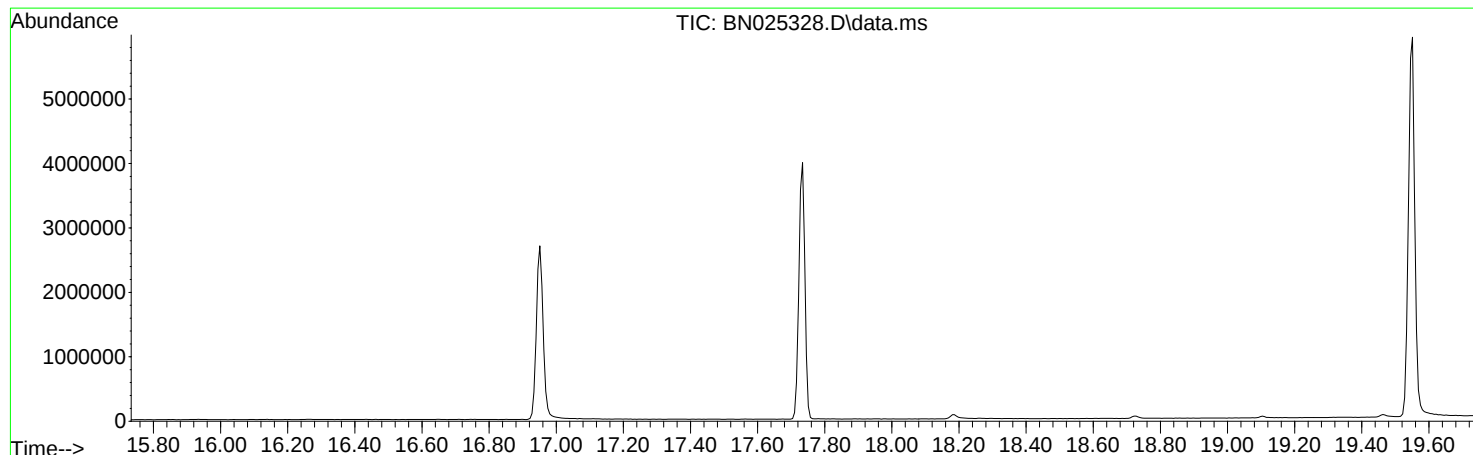

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	182557	PASS
68	69	0.00	2	1.8	2838	PASS
69	198	0.00	100	41.8	154388	PASS
70	69	0.00	2	0.6	880	PASS
127	198	10	80	46.5	171899	PASS
197	198	0.00	2	0.3	1249	PASS
198	198	100	100	100.0	369323	PASS
199	198	5	9	6.8	25187	PASS
275	198	10	60	25.8	95115	PASS
365	198	1	100	3.7	13629	PASS
441	198	0.01	100	14.6	53816	PASS
442	442	50	100	100.0	331755	PASS
443	442	15	24	19.6	65125	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2023	BNA_N	<u>BN025328.D</u>
Compound Name	Response	Retention Time
DDT	1314517	20.786
DDD	13913	20.392
DDE	566	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14479	1328996	1.09

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
 Data File : BN025328.D
 Acq On : 08 May 2023 12:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 09 08:17:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 08:17:02 2023
 Response via : Initial Calibration

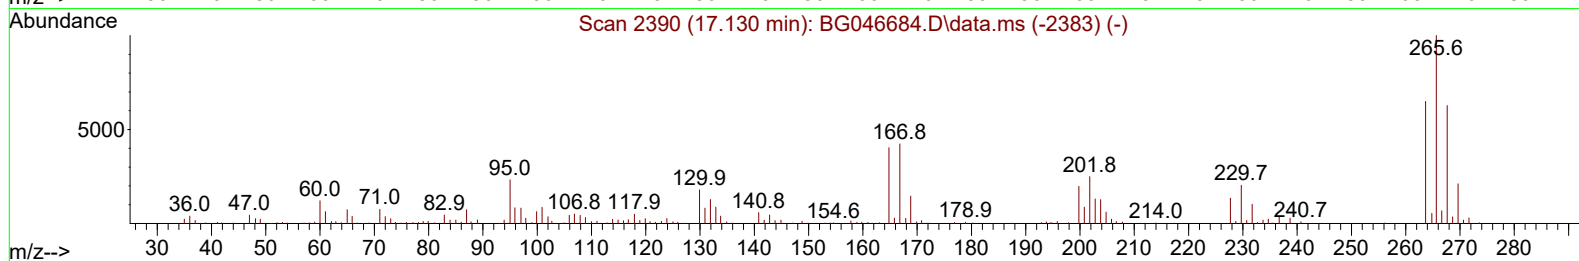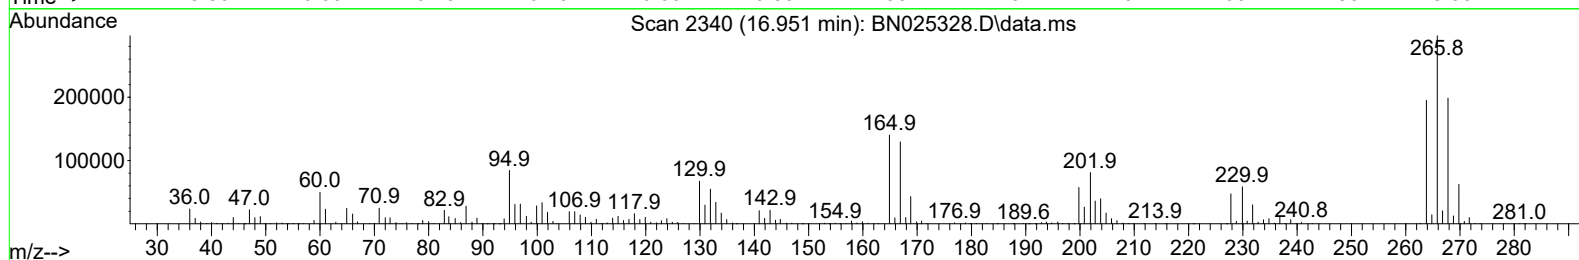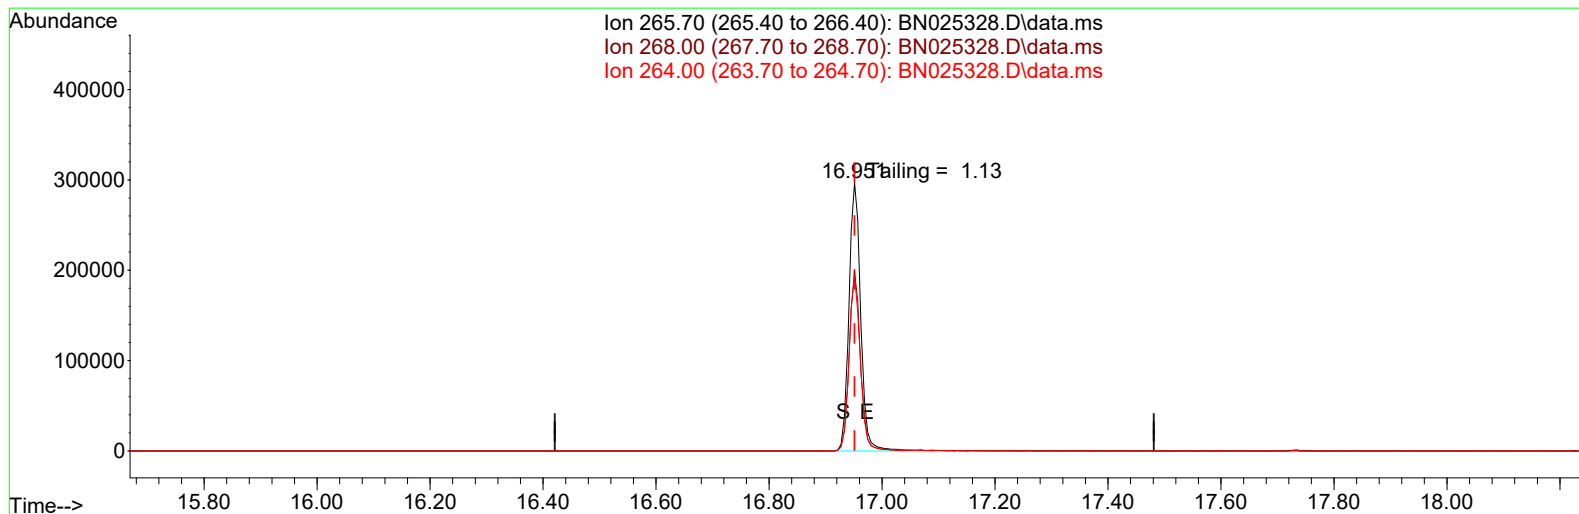

TIC: BN025328.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 23474.17 ng




response 429968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.79
264.00	61.60	65.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025328.D
Acq On : 08 May 2023 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 09 08:17:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 08:17:02 2023
Response via : Initial Calibration

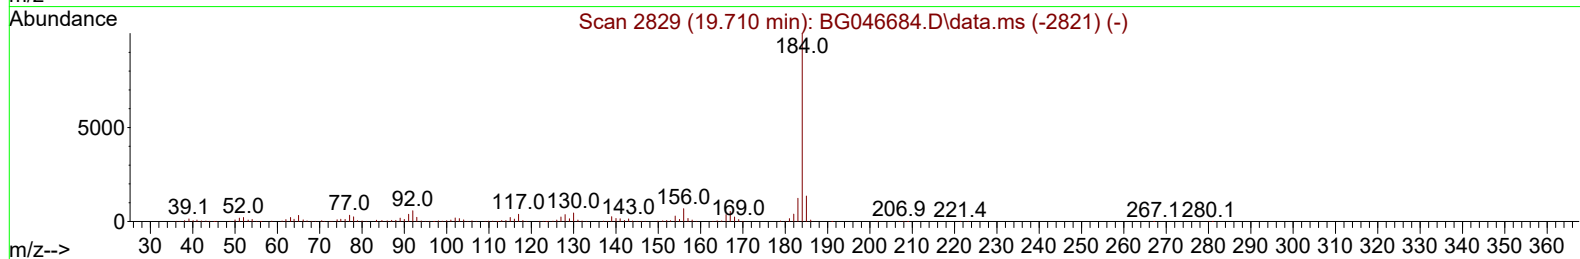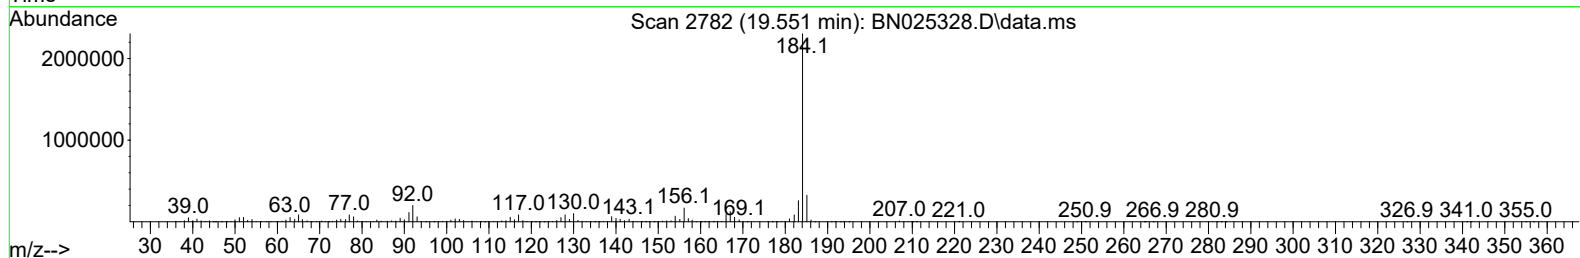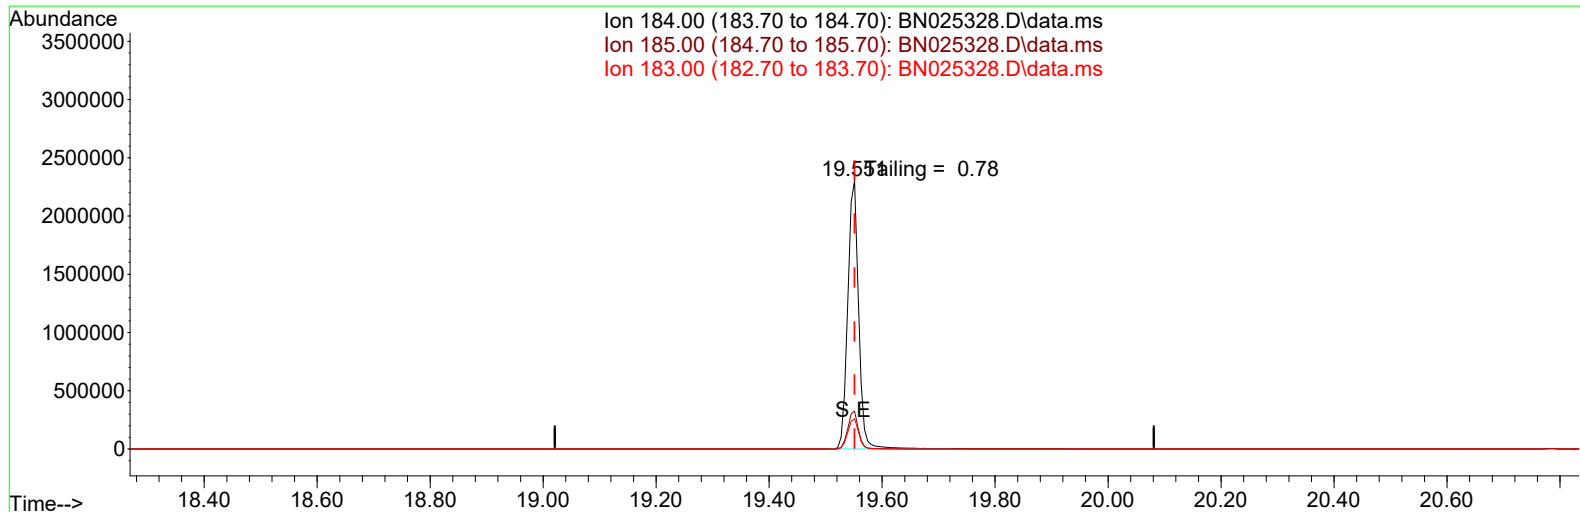

TIC: BN025328.D\data.ms

(77) Benzidine

19.551min (0.000) 1684591.20 ng

response 3115689

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	13.20	11.28
0.00	0.00	0.00