
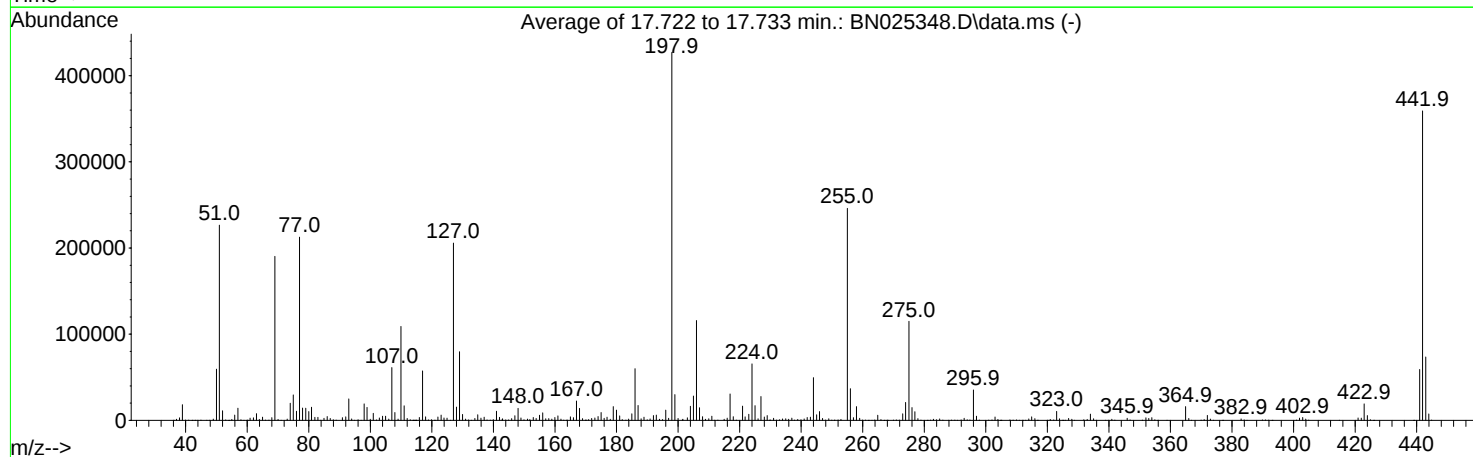


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025348.D
Acq On : 09 May 2023 00:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 09 10:18:02 2023

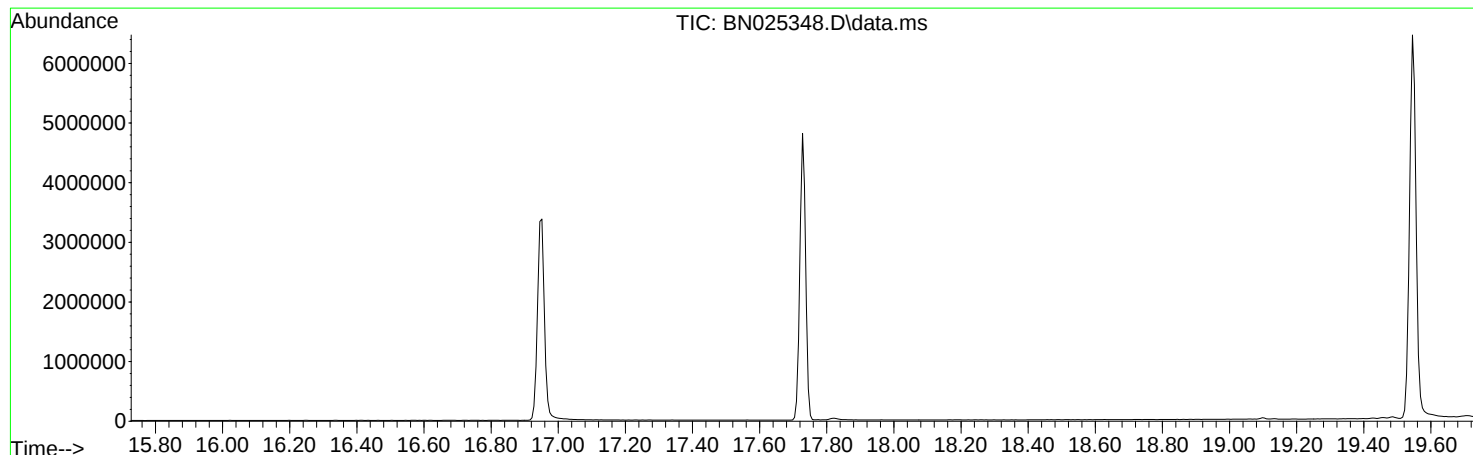

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	226625	PASS
68	69	0.00	2	1.7	3217	PASS
69	198	0.00	100	44.6	190293	PASS
70	69	0.00	2	0.6	1069	PASS
127	198	10	80	48.2	205760	PASS
197	198	0.00	2	0.6	2495	PASS
198	198	100	100	100.0	426901	PASS
199	198	5	9	7.0	29883	PASS
275	198	10	60	26.9	114885	PASS
365	198	1	100	3.8	16024	PASS
441	198	0.01	100	13.8	59011	PASS
442	442	50	100	100.0	359040	PASS
443	442	15	24	20.5	73523	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2023	BNA_N	<u>BN025348.D</u>
Compound Name	Response	Retention Time
DDT	578643	20.774
DDD	765013	20.333
DDE	1040	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
766053	1344696	56.97

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025348.D
Acq On : 09 May 2023 00:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 09 08:18:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 08:17:02 2023
Response via : Initial Calibration

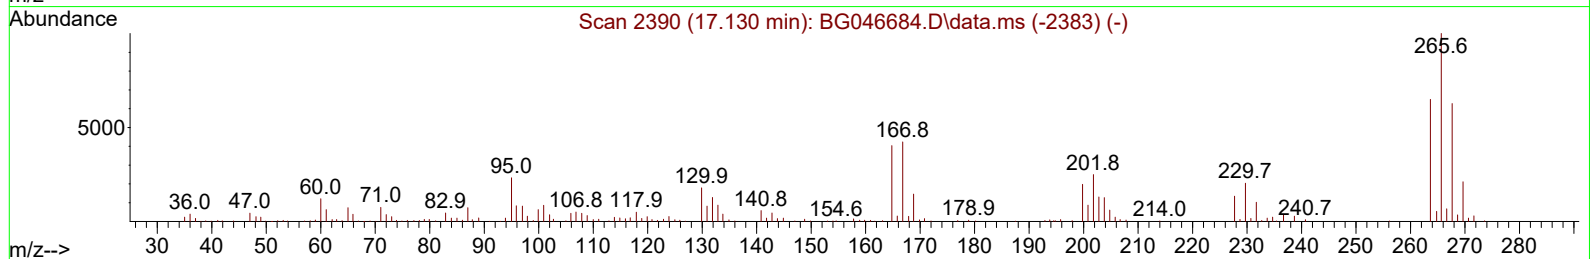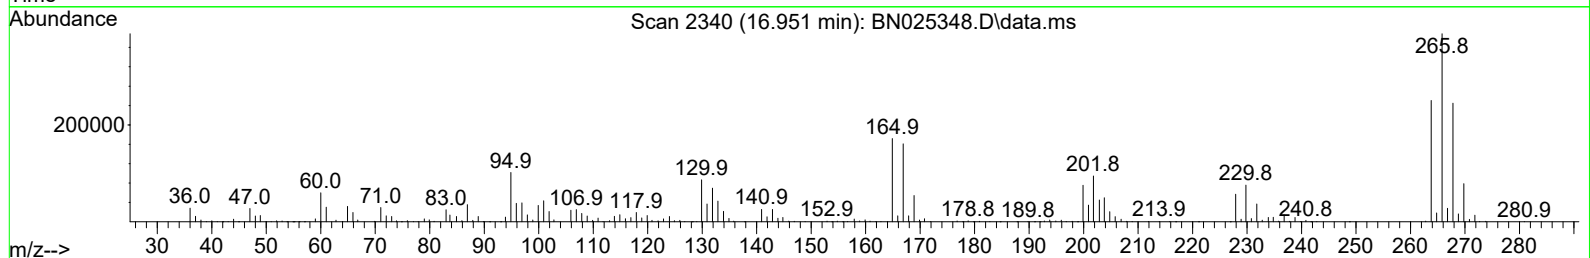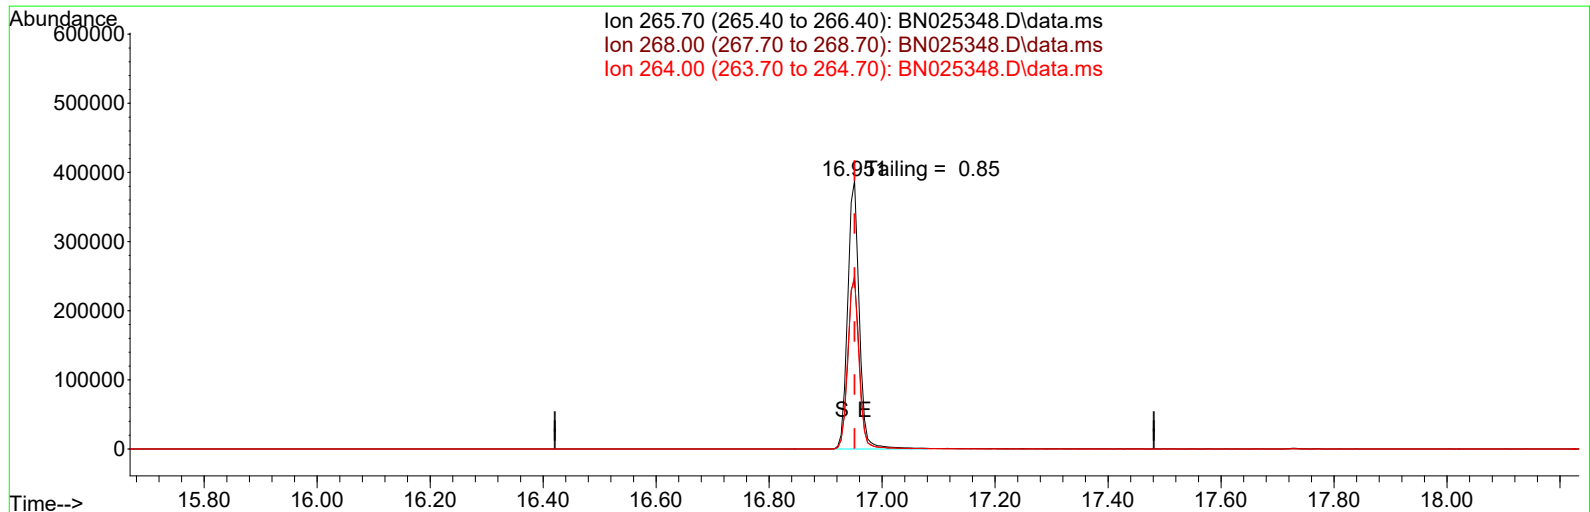

TIC: BN025348.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 27755.93 ng




response 554138

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	64.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050823\
Data File : BN025348.D
Acq On : 09 May 2023 00:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 09 08:18:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 08:17:02 2023
Response via : Initial Calibration

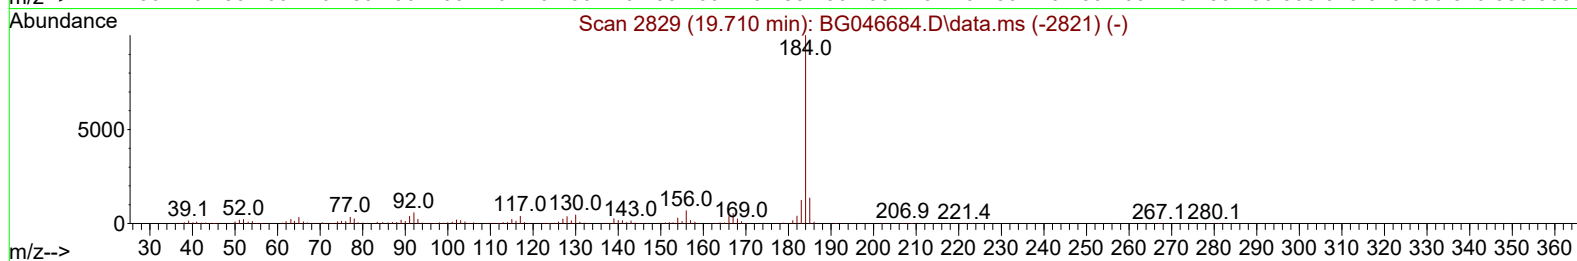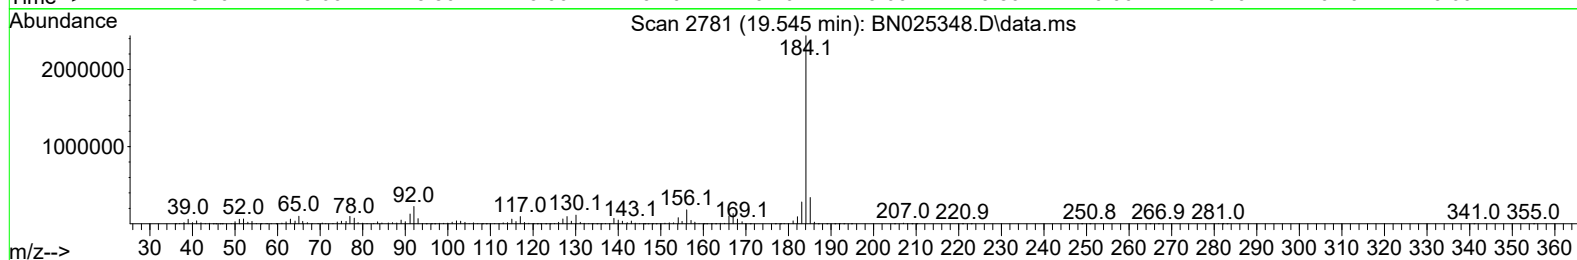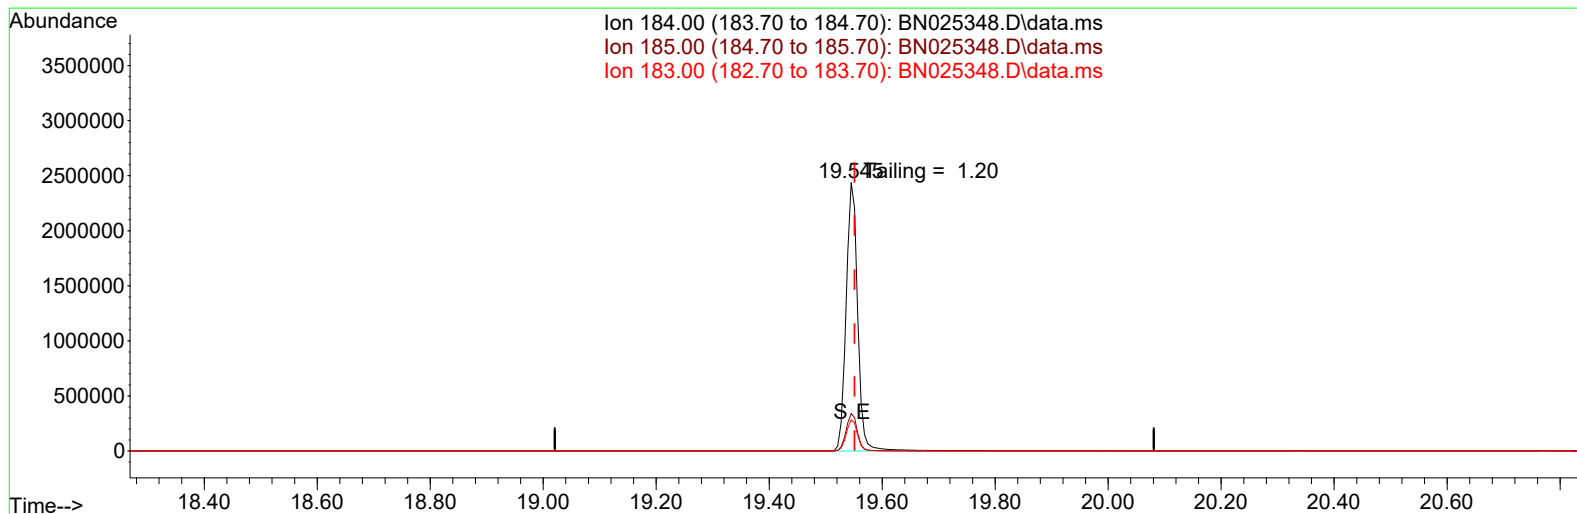

TIC: BN025348.D\data.ms

(77) Benzidine

19.545min (-0.006) 978542.03 ng

response 3468851

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.63
0.00	0.00	0.00