
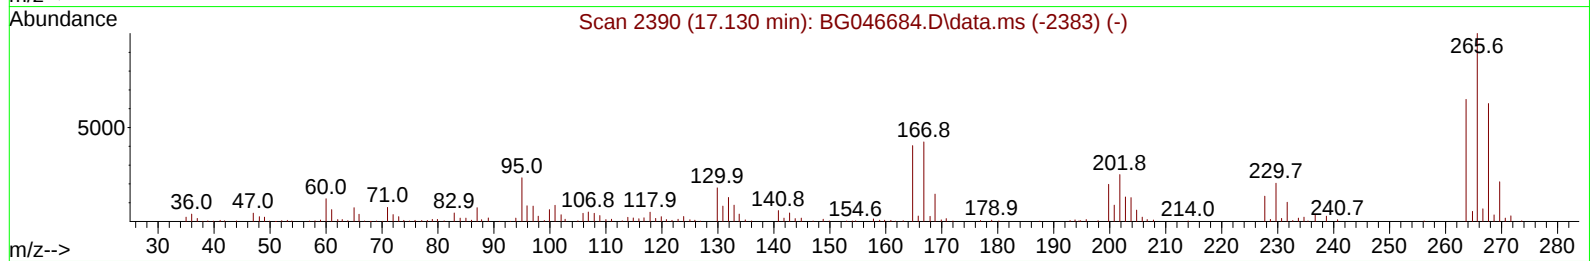
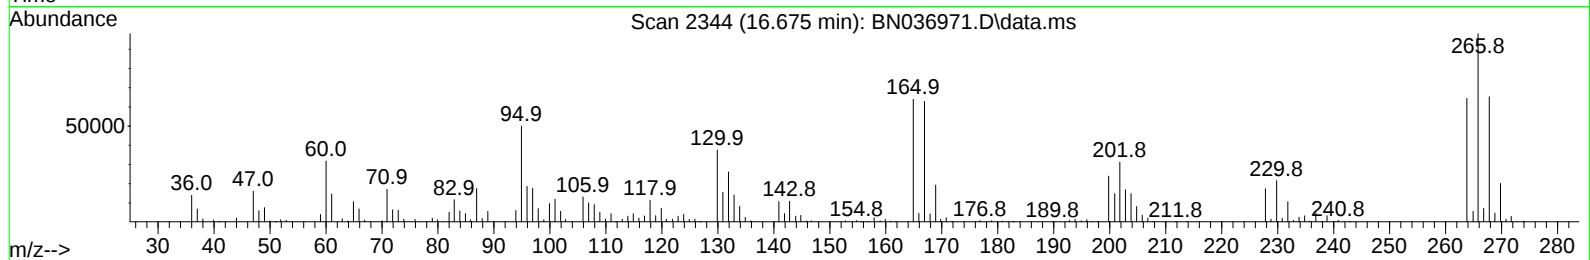


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050825\
Data File : BN036971.D
Acq On : 08 May 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

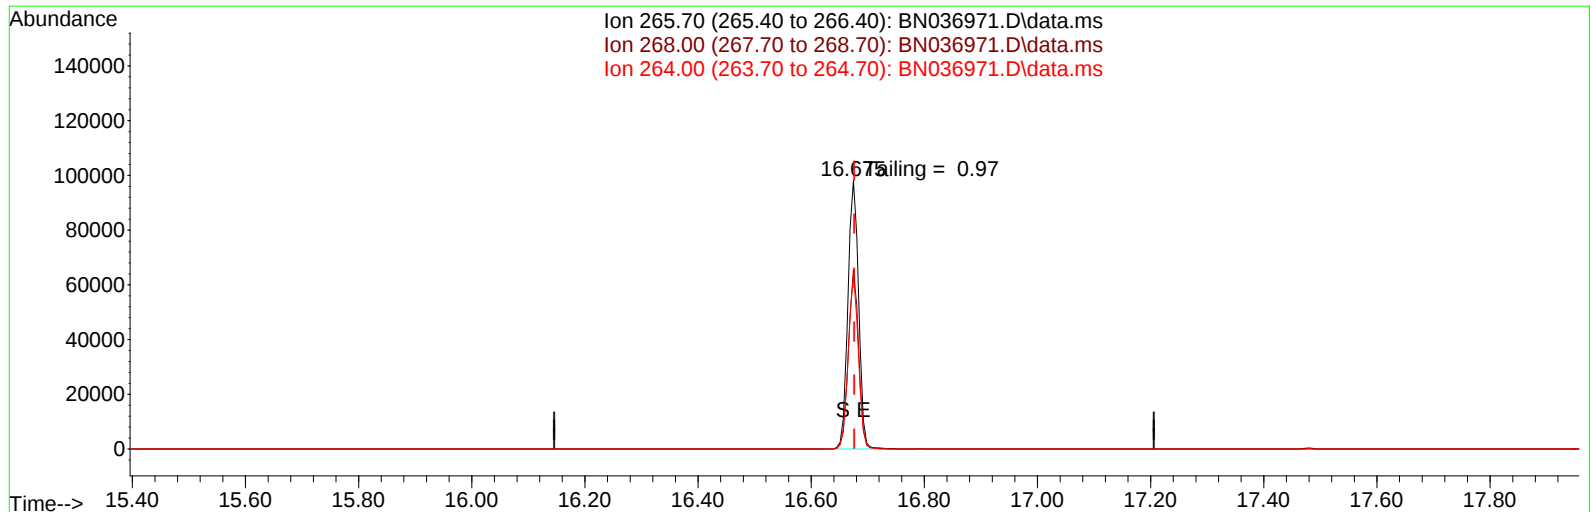

TIC: BN036971.D\data.ms

(70) Pentachlorophenol (C)




16.675min (-0.001) 17886.24 ng

response 128997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.51
264.00	61.60	65.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050825\
Data File : BN036971.D
Acq On : 08 May 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

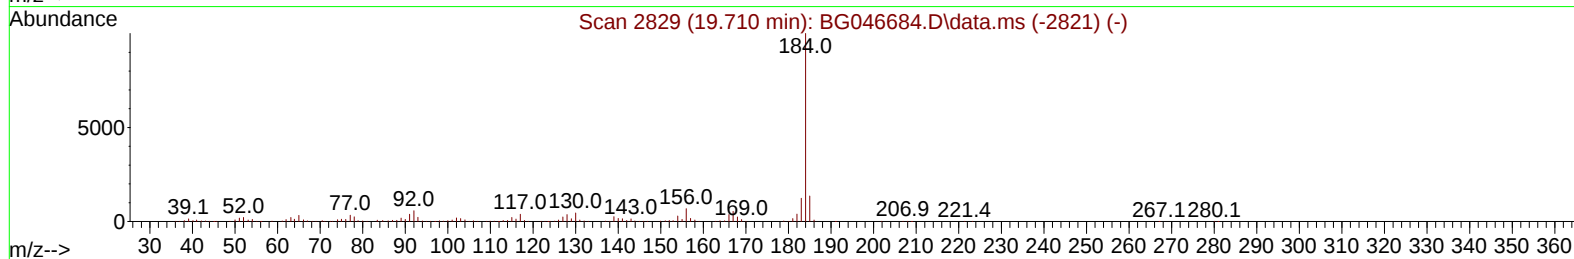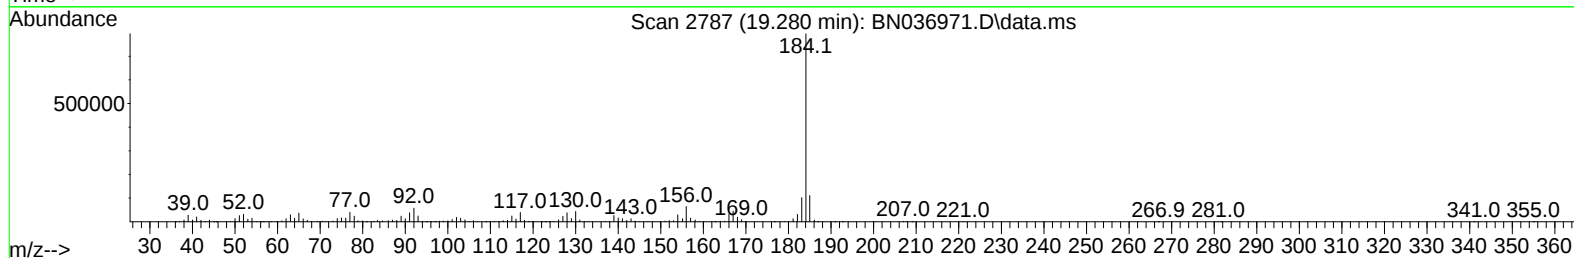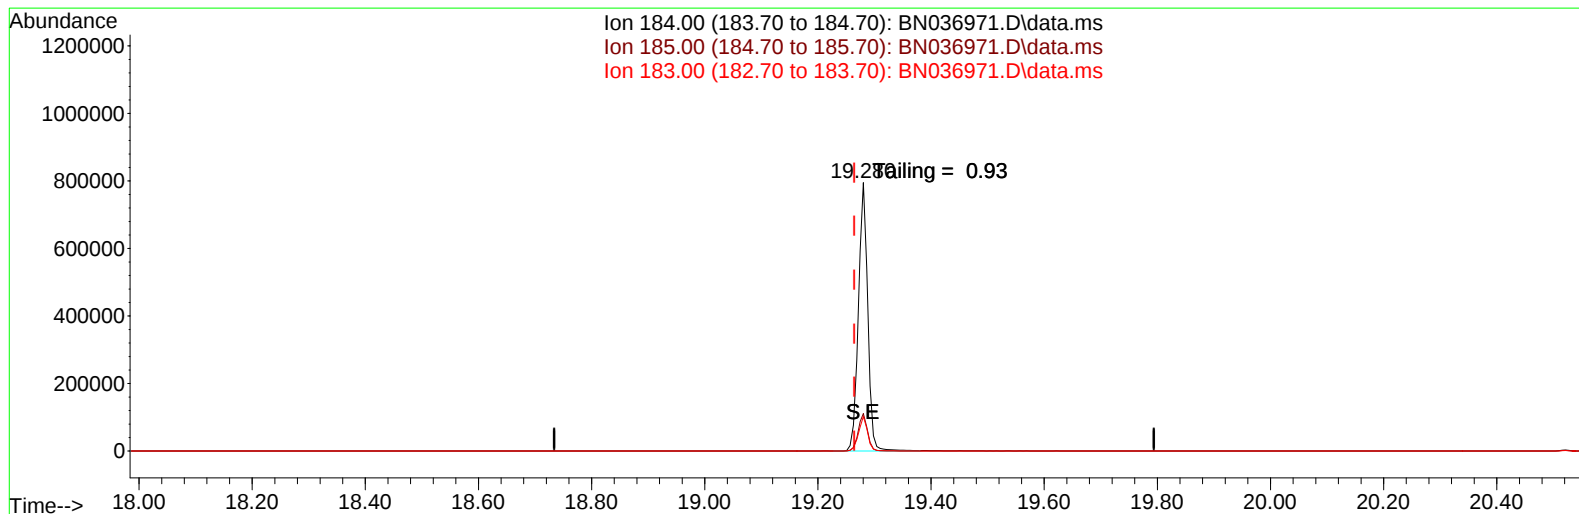

TIC: BN036971.D\data.ms

(77) Benzidine**19.280min (+ 0.016) 0.00 ng****response 917971**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	12.91
0.00	0.00	0.00