
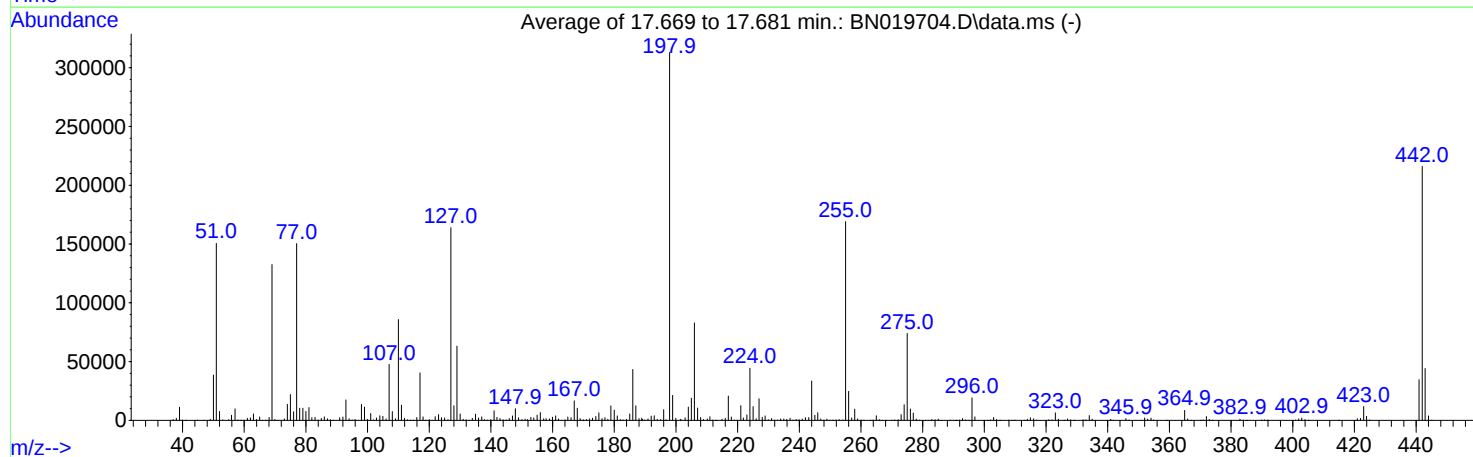


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050922\
 Data File : BN019704.D
 Acq On : 09 May 2022 15:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 10 01:35:26 2022

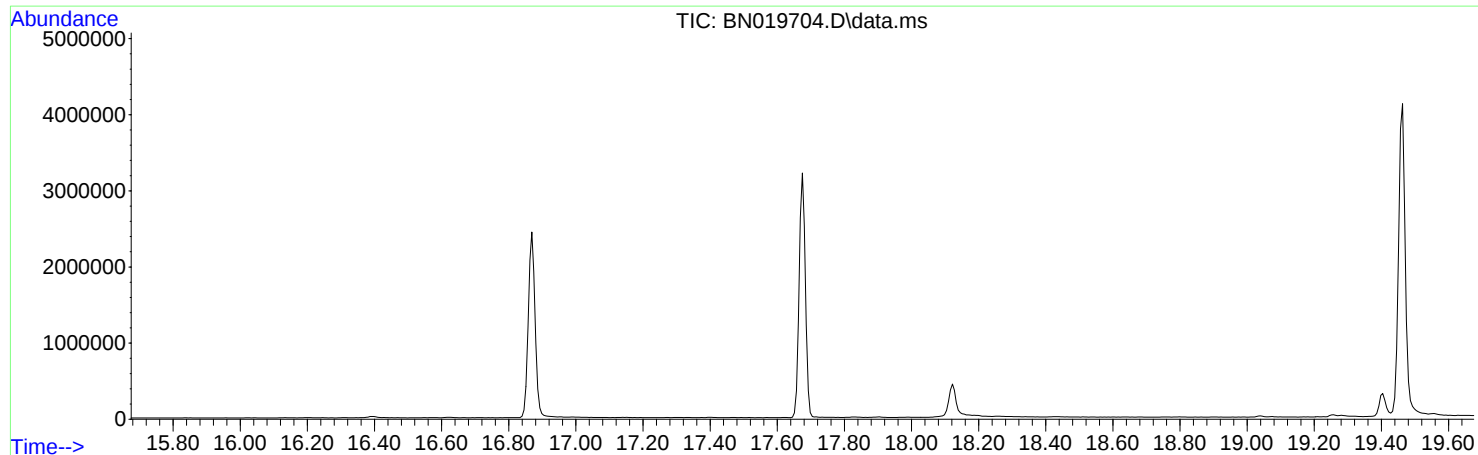




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	150575	PASS
68	69	0.00	2	1.8	2416	PASS
69	198	0.00	100	42.4	132573	PASS
70	69	0.00	2	0.6	813	PASS
127	198	10	80	52.4	163861	PASS
197	198	0.00	2	0.2	595	PASS
198	198	100	100	100.0	312917	PASS
199	198	5	9	6.8	21232	PASS
275	198	10	60	23.6	73960	PASS
365	198	1	100	2.7	8508	PASS
441	198	0.01	100	11.1	34640	PASS
442	442	50	100	100.0	215957	PASS
443	442	15	24	20.4	44112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050922\
Data File : BN019704.D
Acq On : 09 May 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 04:03:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

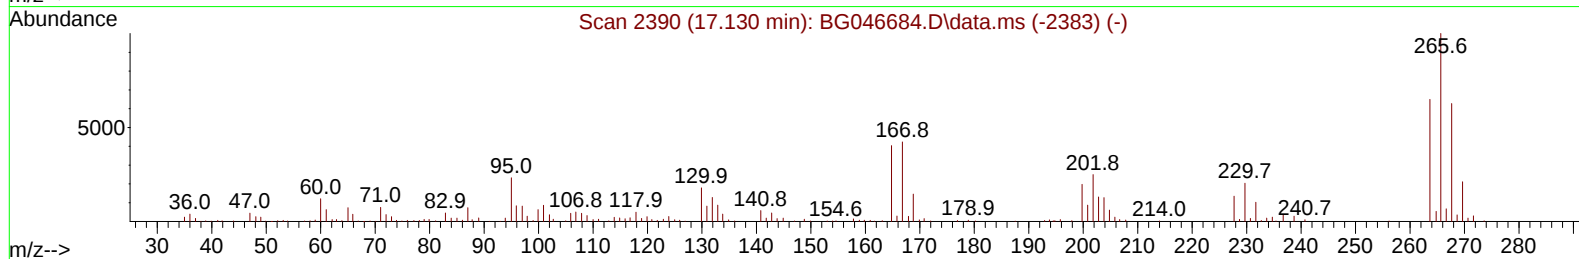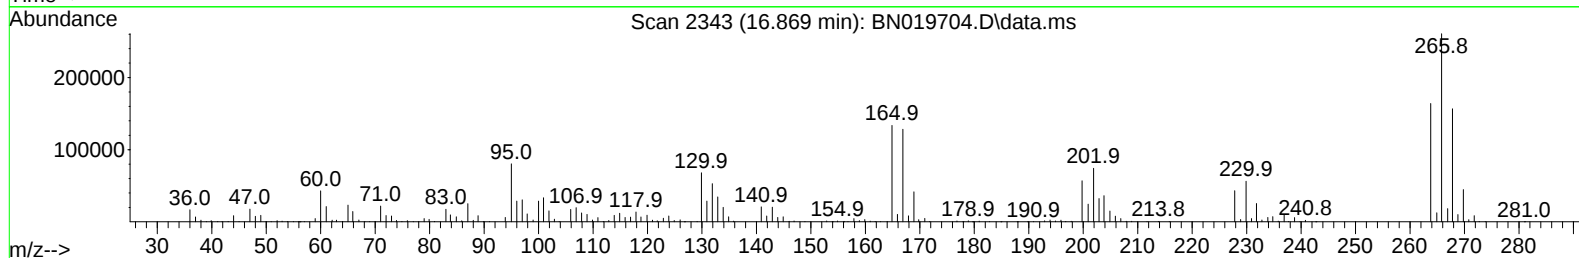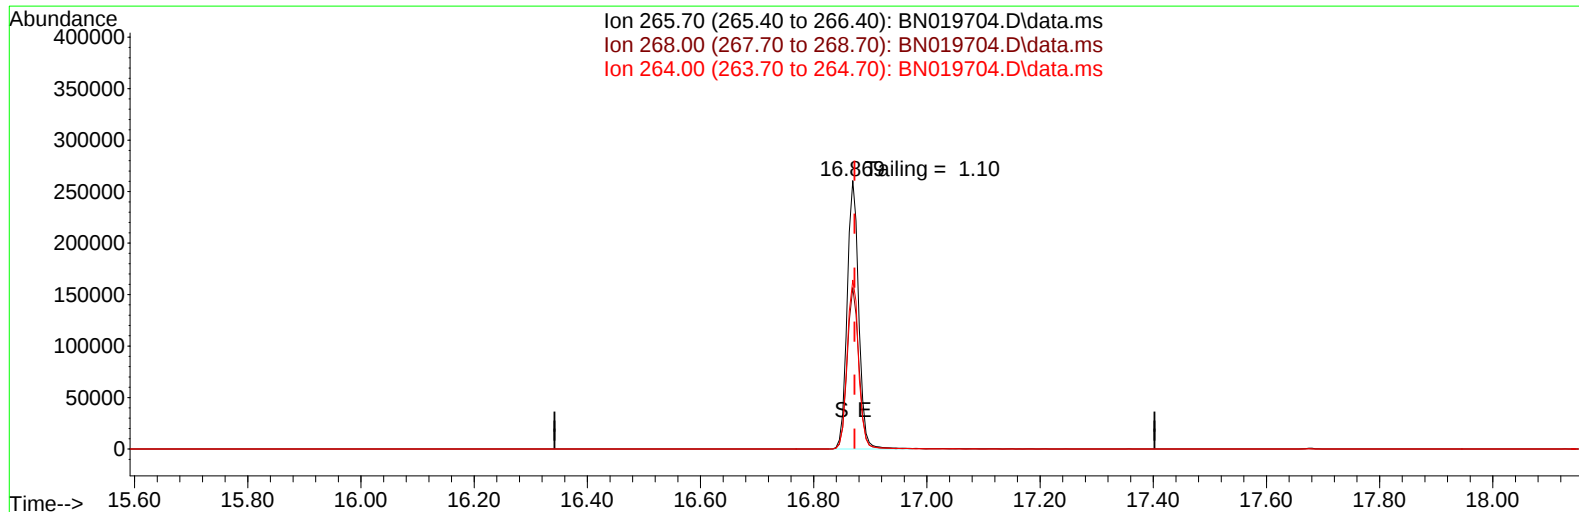

TIC: BN019704.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 20903.86 ng




response 370749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.13
264.00	61.60	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050922\
Data File : BN019704.D
Acq On : 09 May 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 04:03:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

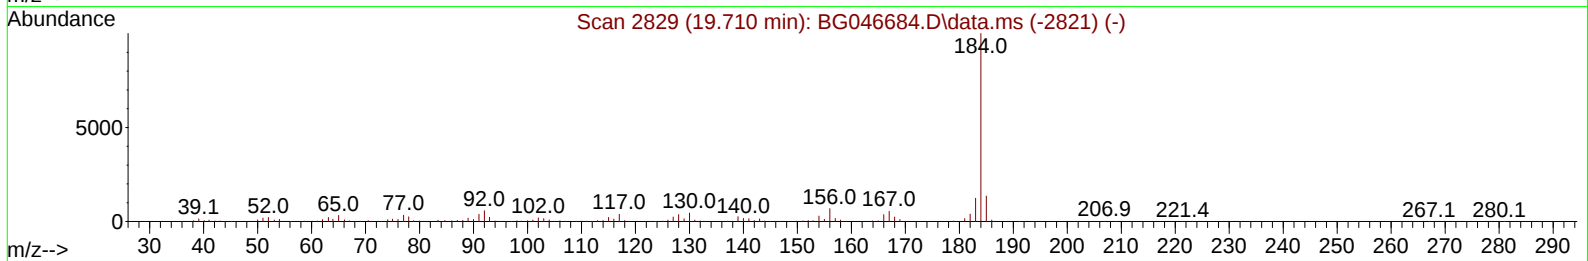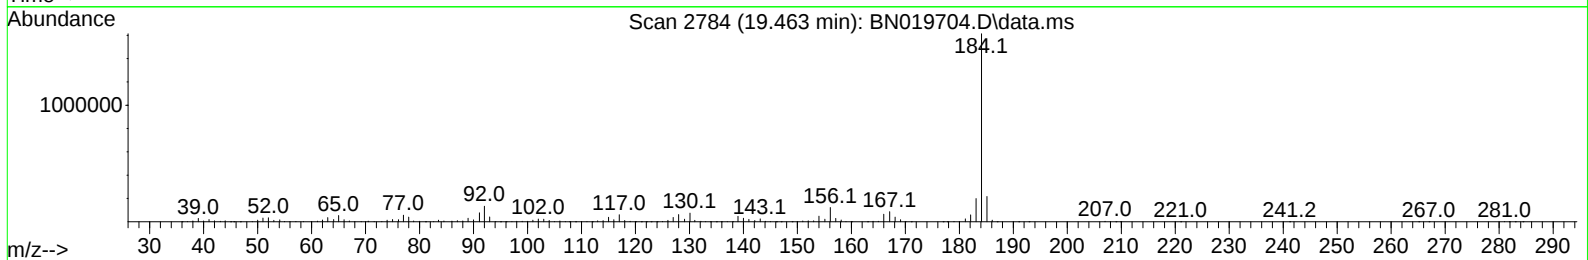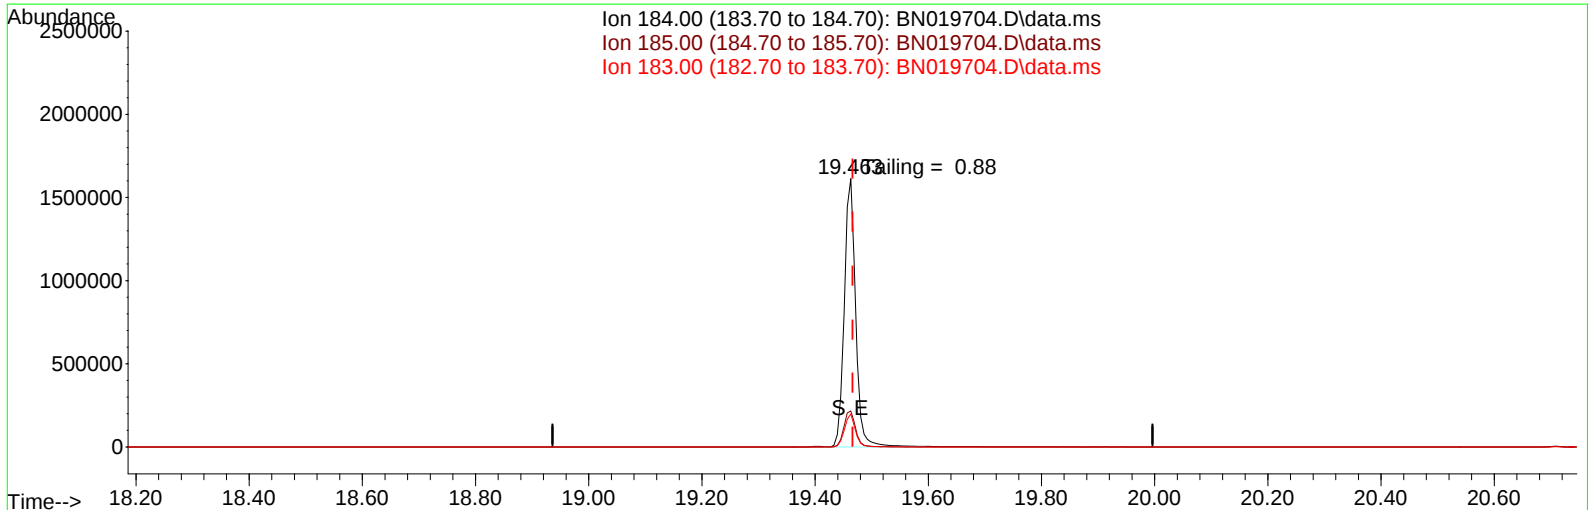

TIC: BN019704.D\data.ms

(77) Benzidine

19.463min (-0.003) 0.00 ng

response 2271110

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	12.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/9/2022	BNA_N	<u>BN019704.D</u>
Compound Name	Response	Retention Time
DDT	1060995	20.71
DDD	7873	20.263
DDE	0	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7873	1068868	0.74

Instrument :
BNA_N
ClientSampleId :
DFTPP