
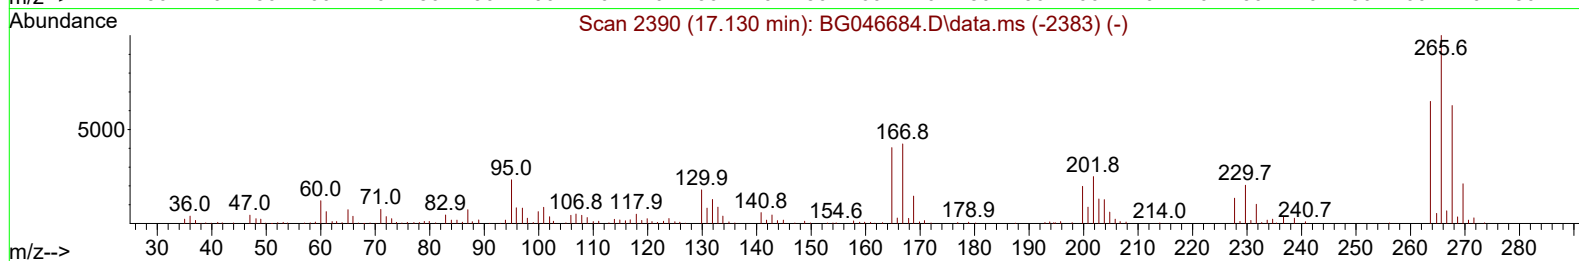
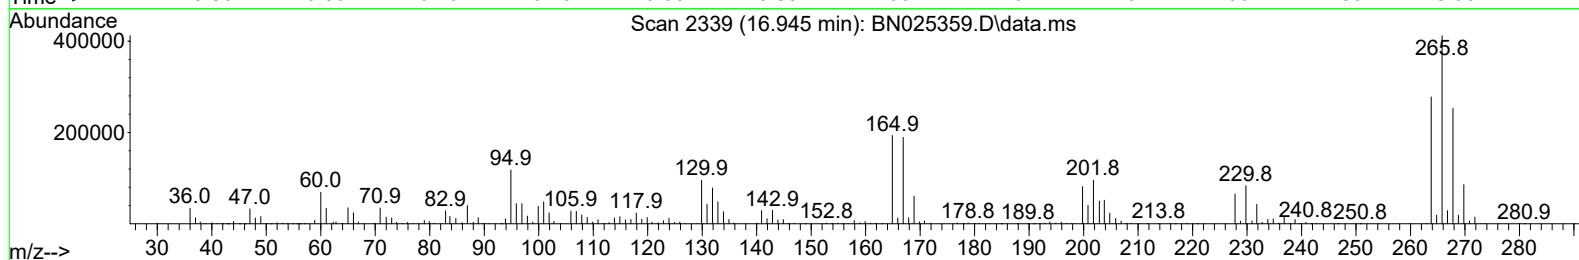


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050923\
Data File : BN025359.D
Acq On : 09 May 2023 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 06:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 06:00:45 2023
Response via : Initial Calibration

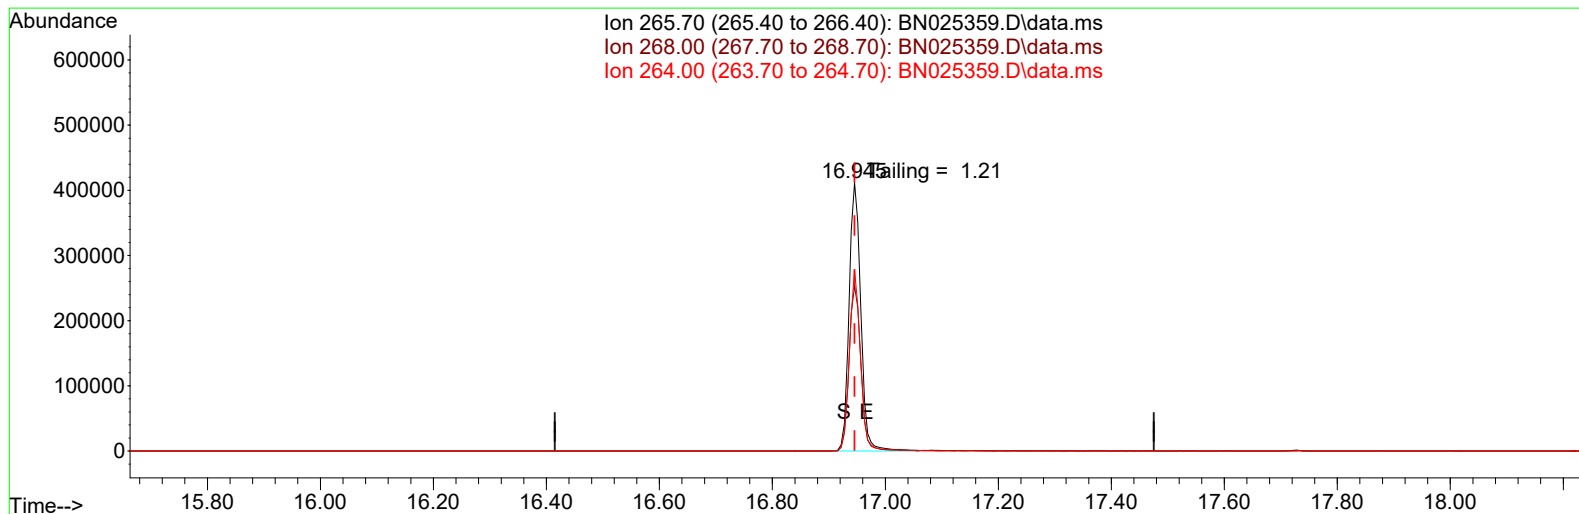

TIC: BN025359.D\data.ms

(70) Pentachlorophenol (C)




16.945min (0.000) 24835.90 ng

response 594268

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.41
264.00	61.60	67.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050923\
Data File : BN025359.D
Acq On : 09 May 2023 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 06:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 06:00:45 2023
Response via : Initial Calibration

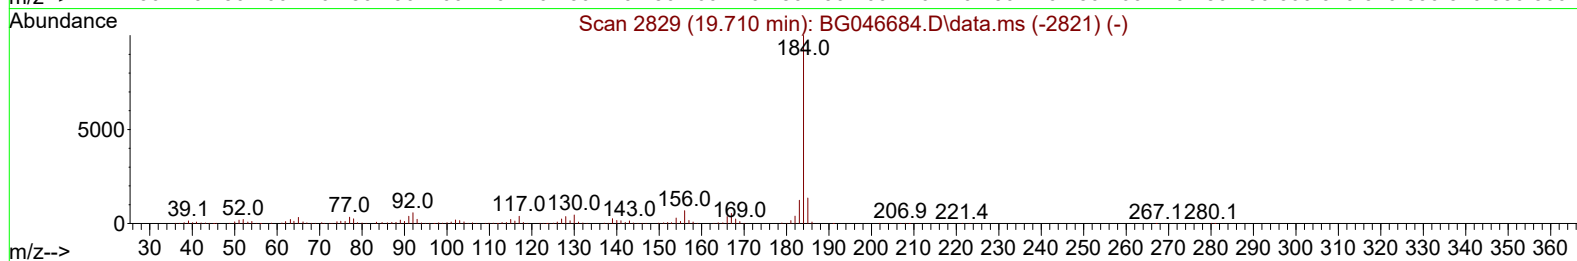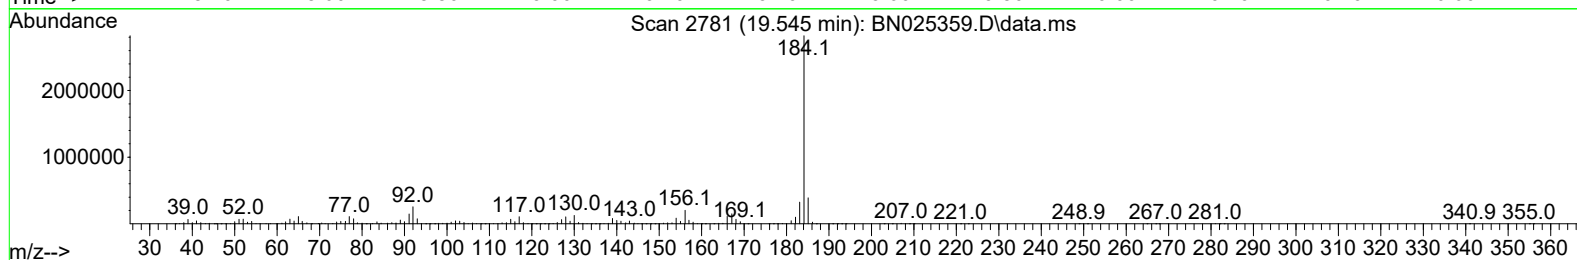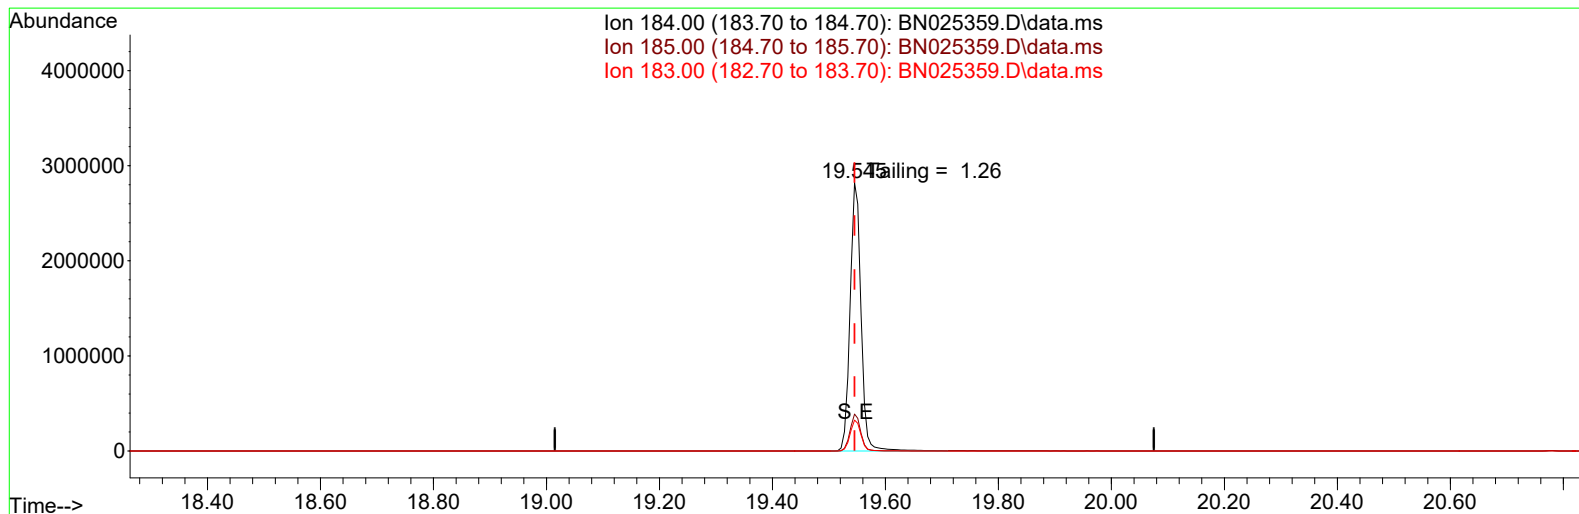

TIC: BN025359.D\data.ms

(77) Benzidine**19.545min (0.000) 1992618.10 ng****response 3808238**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.53
0.00	0.00	0.00