
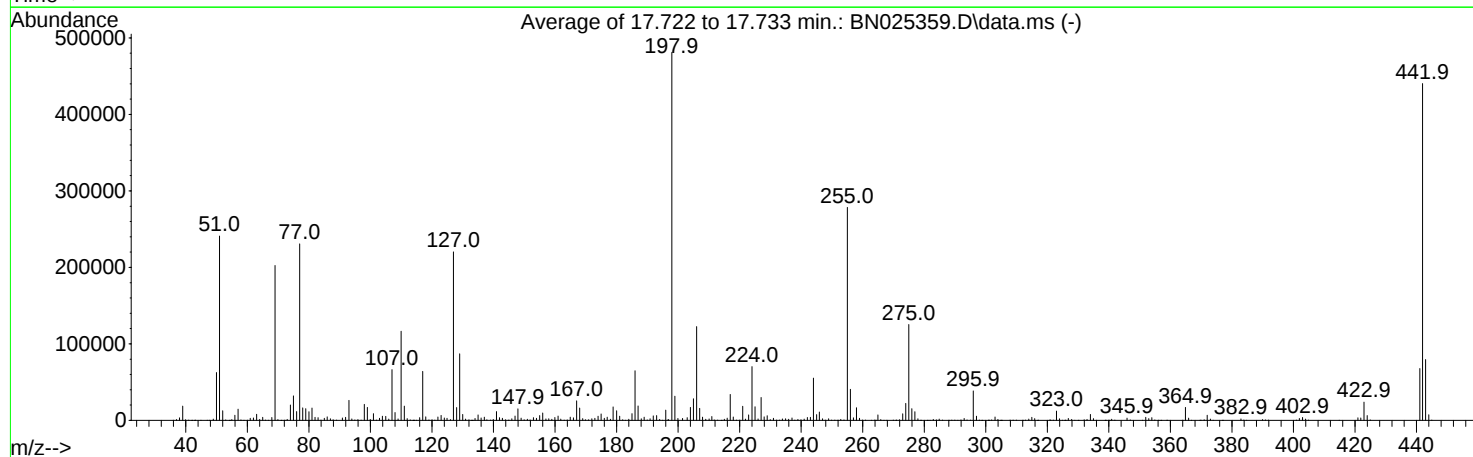


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050923\
Data File : BN025359.D
Acq On : 09 May 2023 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 09 10:18:02 2023

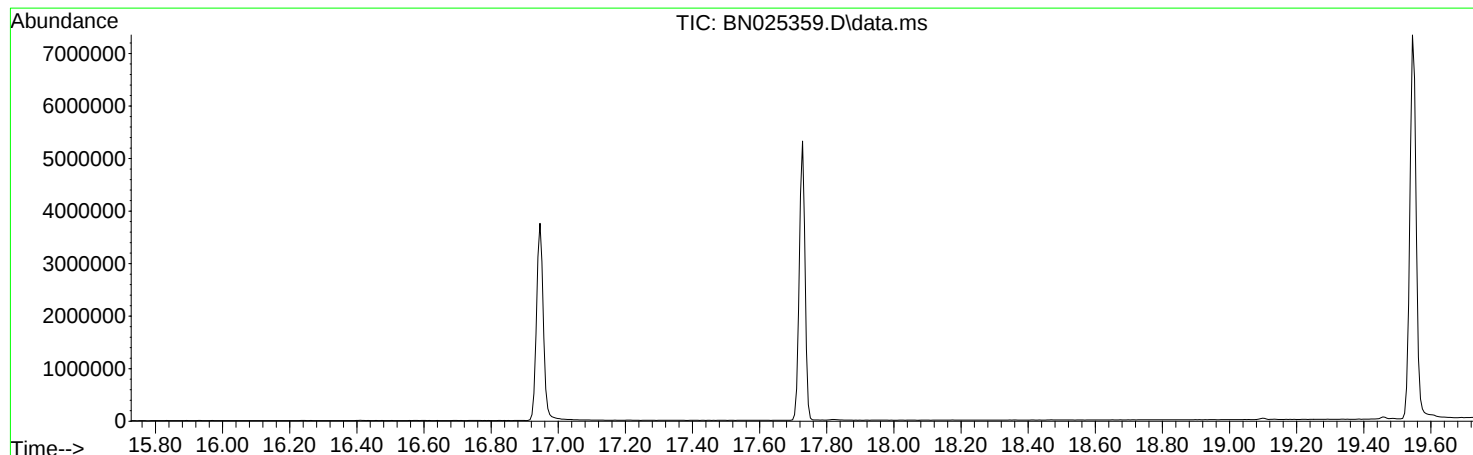

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	240906	PASS
68	69	0.00	2	1.8	3734	PASS
69	198	0.00	100	42.1	202581	PASS
70	69	0.00	2	0.5	974	PASS
127	198	10	80	45.8	220181	PASS
197	198	0.00	2	0.2	1063	PASS
198	198	100	100	100.0	480939	PASS
199	198	5	9	6.6	31645	PASS
275	198	10	60	26.1	125355	PASS
365	198	1	100	3.5	16958	PASS
441	198	0.01	100	14.1	67773	PASS
442	442	50	100	100.0	440341	PASS
443	442	15	24	18.1	79597	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/9/2023	BNA_N	<u>BN025359.D</u>
Compound Name	Response	Retention Time
DDT	1042786	20.78
DDD	522551	20.339
DDE	1684	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
524235	1567021	33.45

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050923\
Data File : BN025359.D
Acq On : 09 May 2023 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 06:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 06:00:45 2023
Response via : Initial Calibration

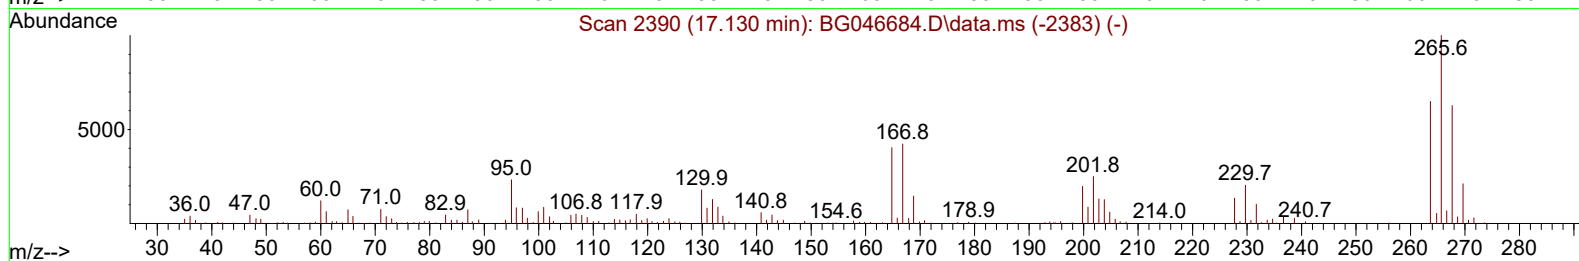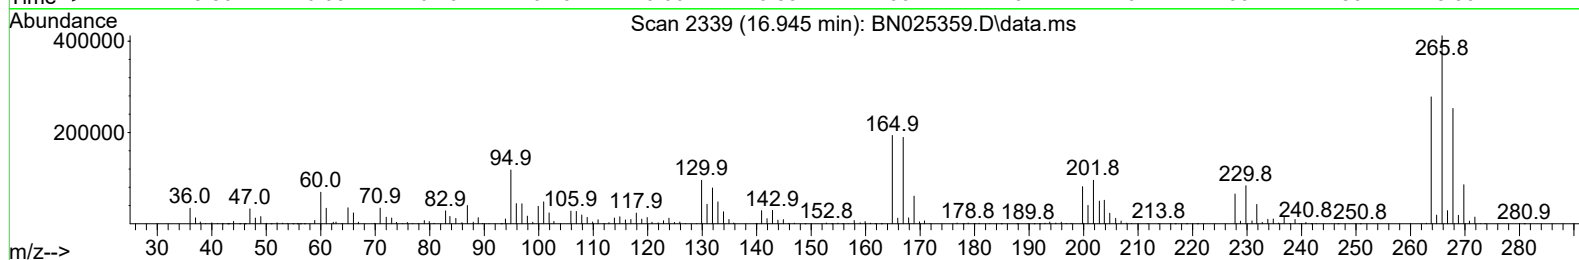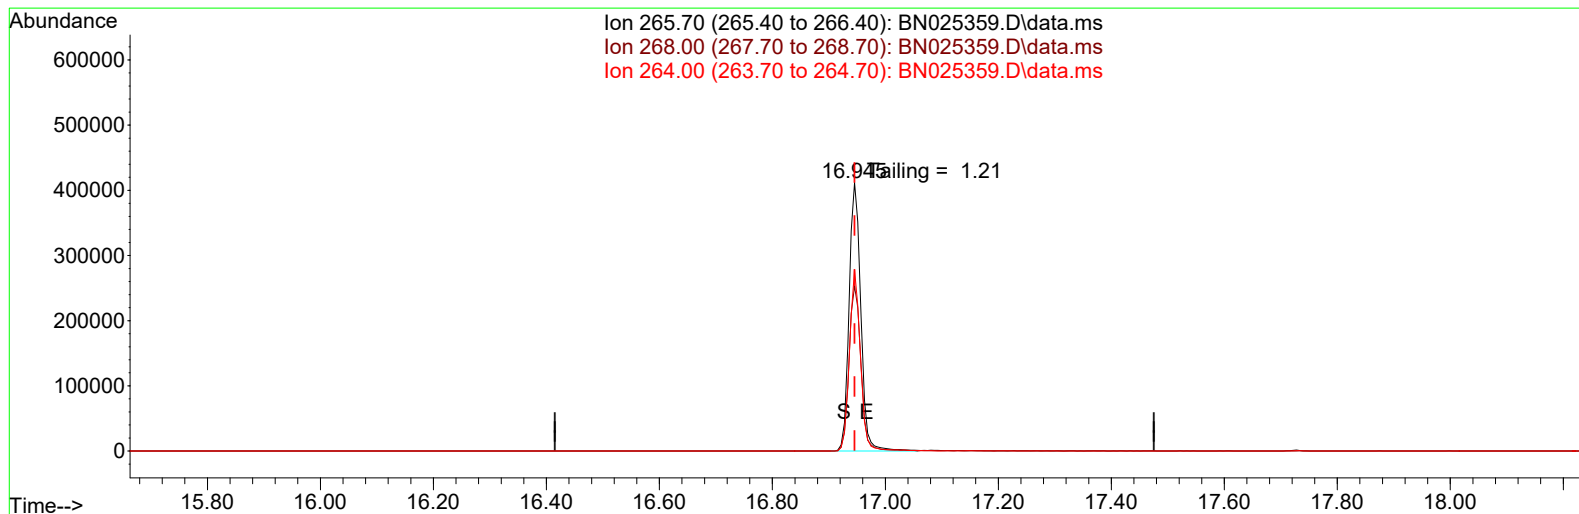

TIC: BN025359.D\data.ms

(70) Pentachlorophenol (C)

16.945min (0.000) 24835.90 ng




response 594268

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.41
264.00	61.60	67.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050923\
Data File : BN025359.D
Acq On : 09 May 2023 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 10 06:00:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 06:00:45 2023
Response via : Initial Calibration

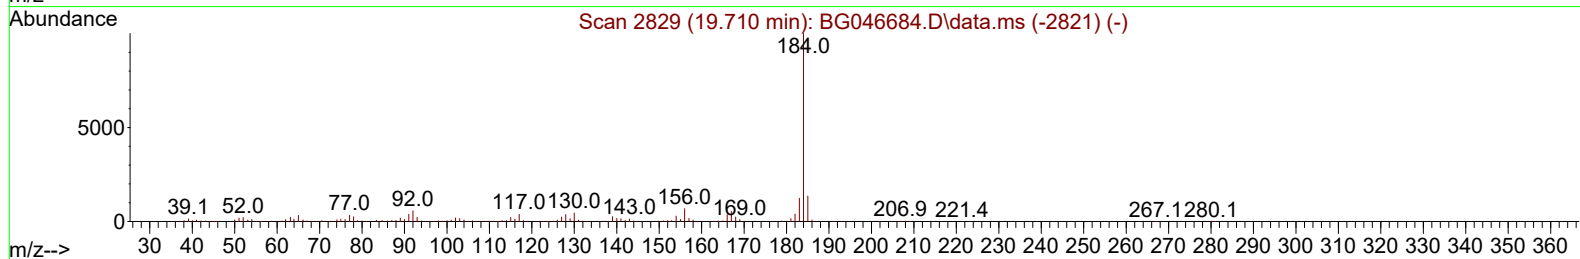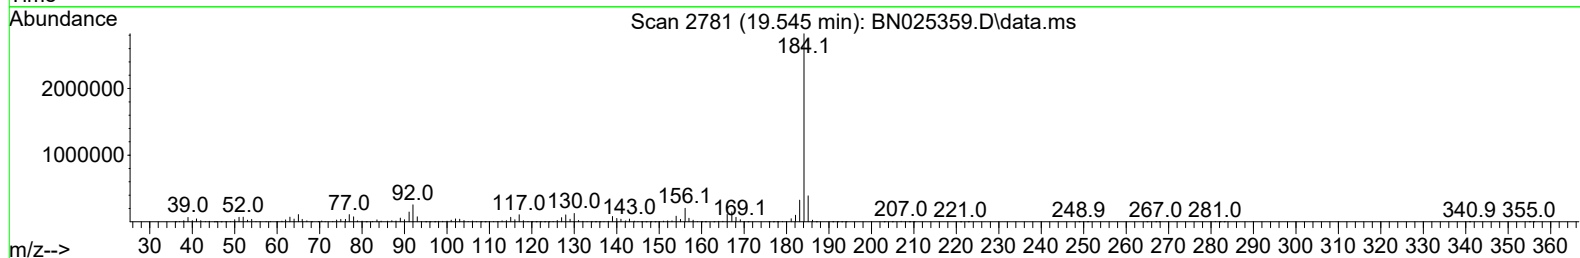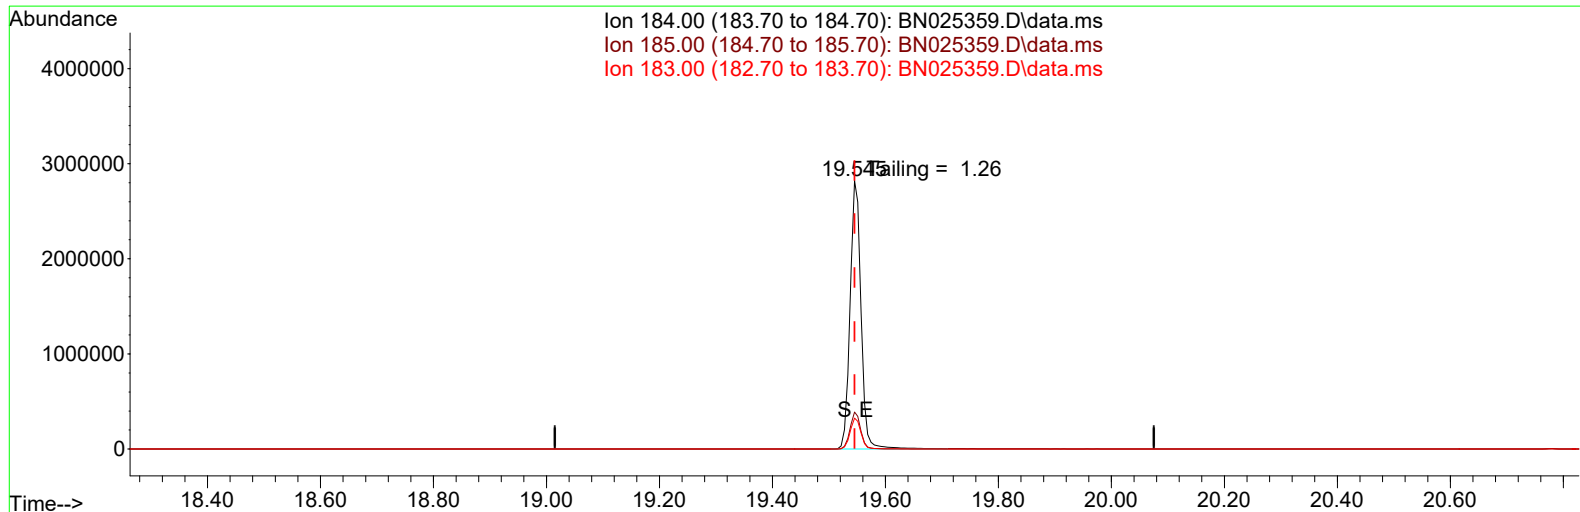

TIC: BN025359.D\data.ms

(77) Benzidine

19.545min (0.000) 1992618.10 ng

response 3808238

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.53
0.00	0.00	0.00