
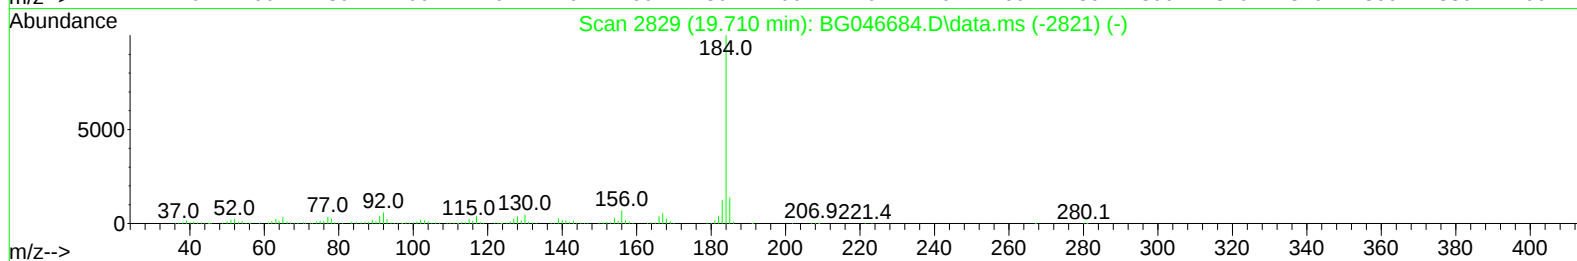
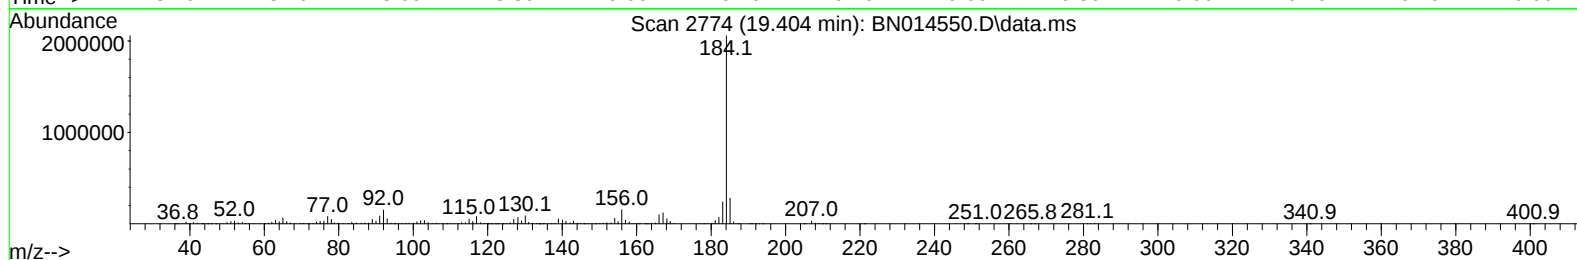


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051021\
Data File : BN014550.D
Acq On : 10 May 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 12:31:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 08 04:11:21 2021
Response via : Initial Calibration

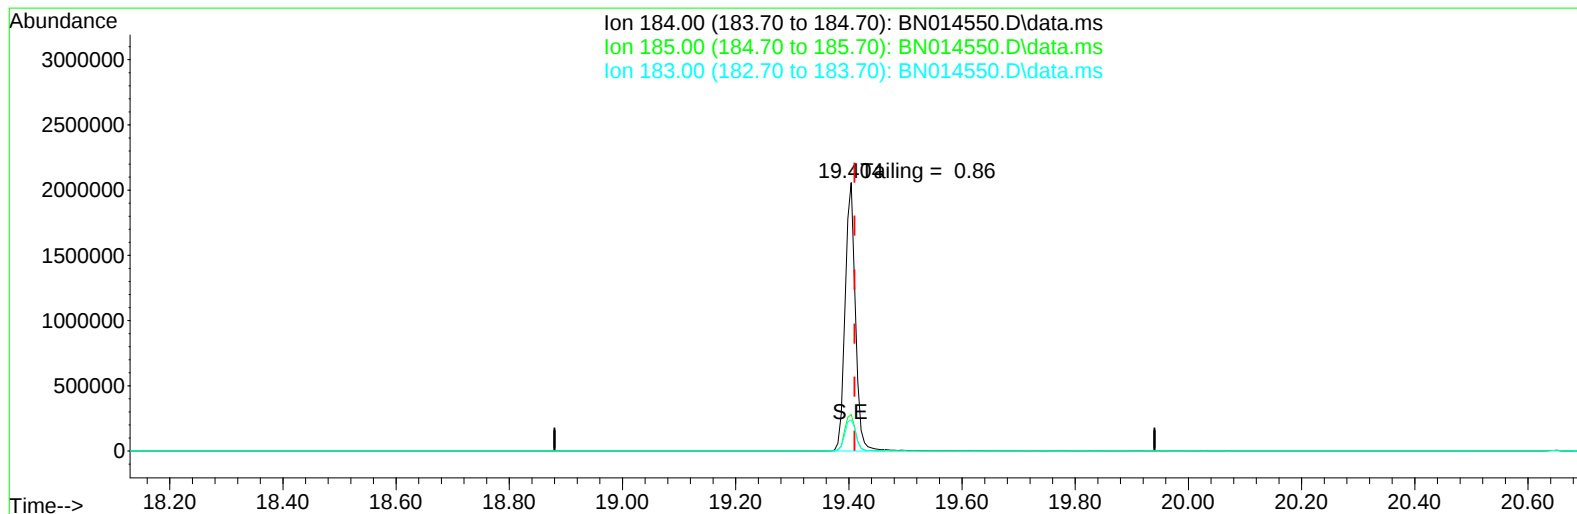




TIC: BN014550.D\data.ms

(77) Benzidine**19.404min (-0.006) 731933.20 ng****response 2594643**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.62
183.00	13.20	11.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051021\
Data File : BN014550.D
Acq On : 10 May 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 12:31:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 08 04:11:21 2021
Response via : Initial Calibration

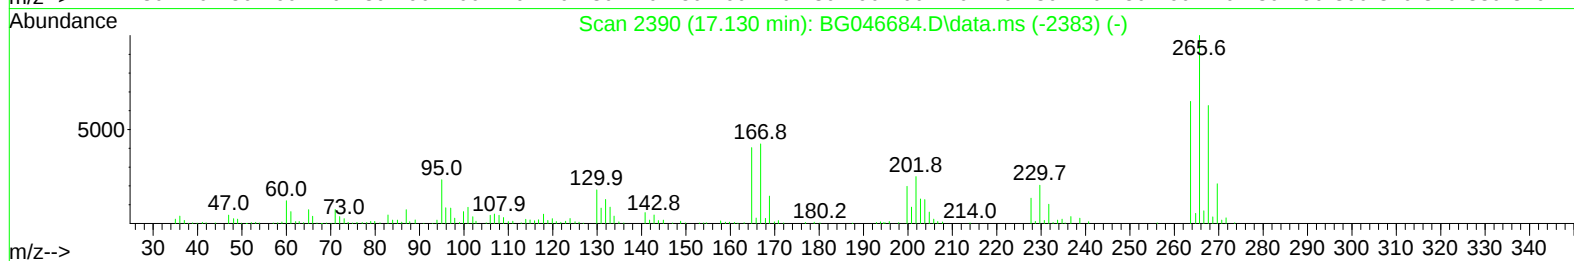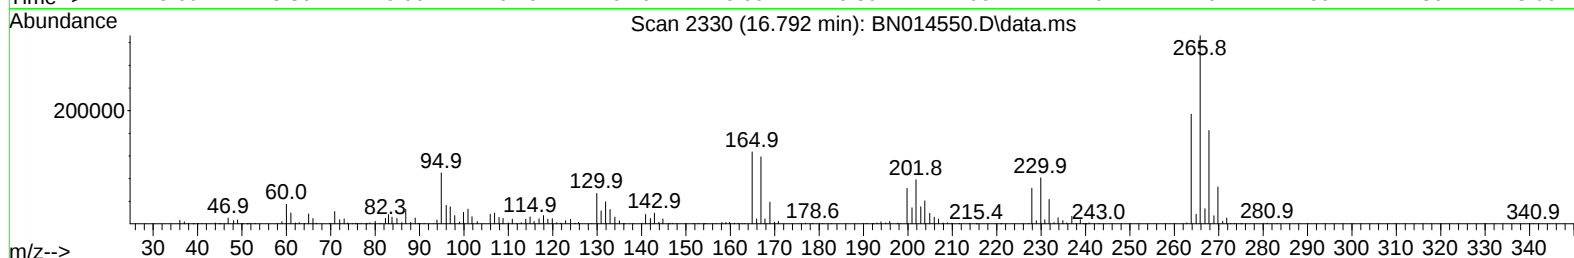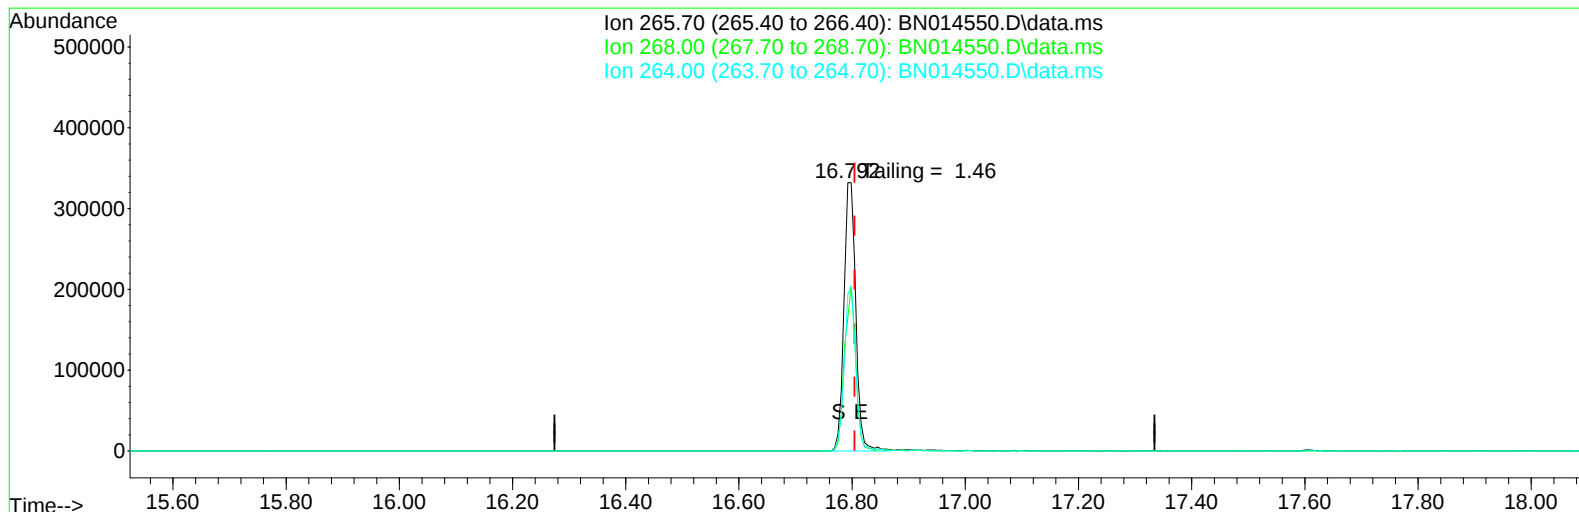

TIC: BN014550.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.012) 16569.30 ng

response **484368**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	49.70#
264.00	61.60	58.37
0.00	0.00	0.00