


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051021\
 Data File : BN014550.D
 Acq On : 10 May 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 07 17:32:10 2021

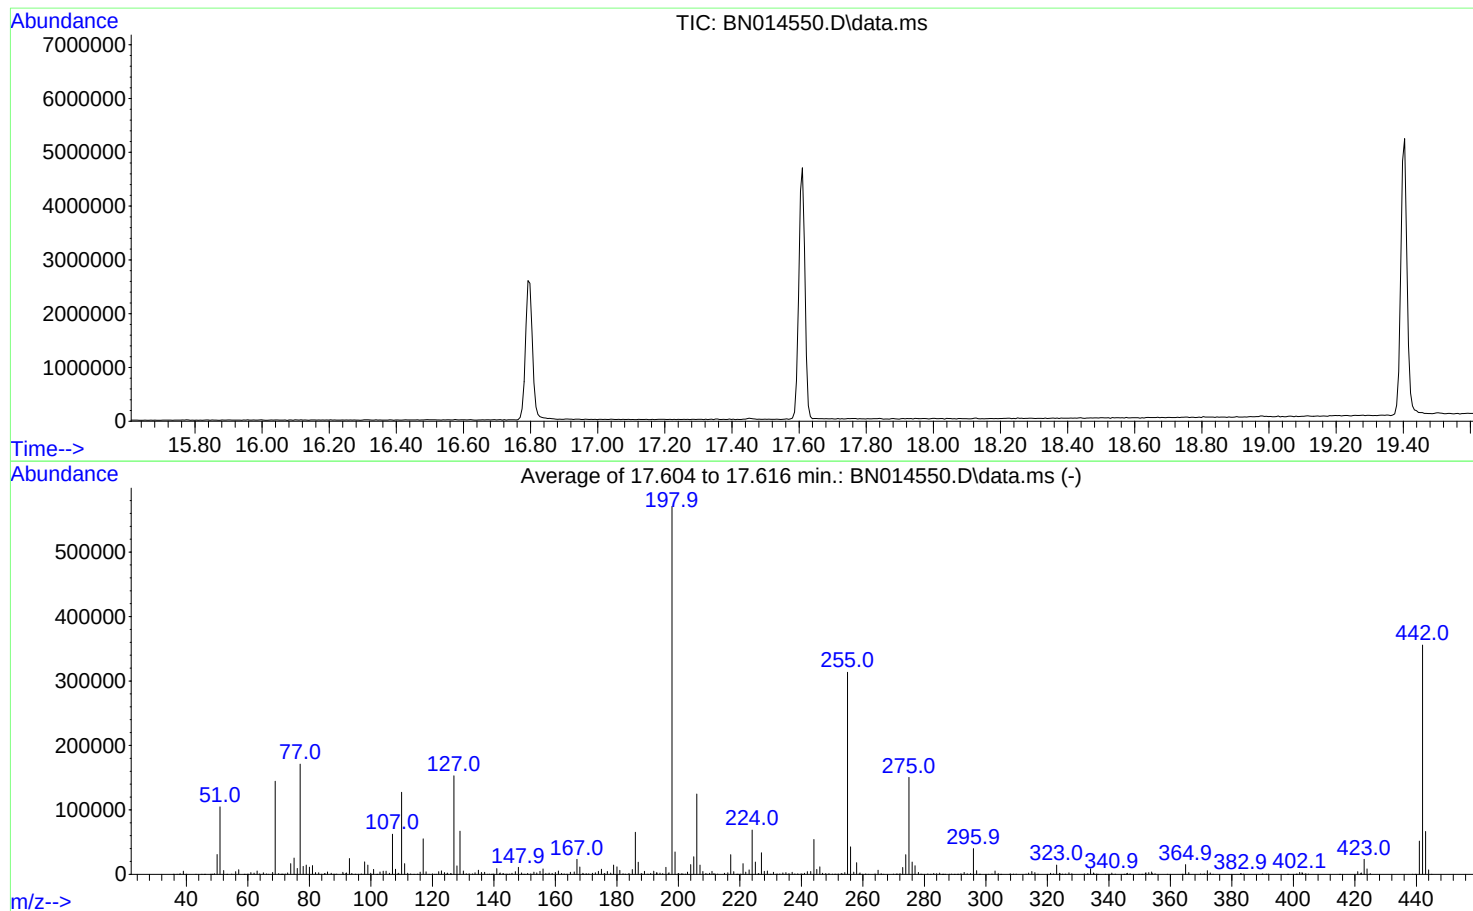




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.4	104878	PASS
68	69	0.00	2	2.0	2880	PASS
69	198	0.00	100	25.3	144568	PASS
70	69	0.00	2	0.9	1313	PASS
127	198	10	80	26.8	152869	PASS
197	198	0.00	2	0.5	2621	PASS
198	198	100	100	100.0	570752	PASS
199	198	5	9	6.1	34709	PASS
275	198	10	60	26.3	150349	PASS
365	198	1	100	2.6	15062	PASS
441	198	0.01	100	9.1	51768	PASS
442	442	50	100	100.0	355648	PASS
443	442	15	24	18.7	66432	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051021\
 Data File : BN014550.D
 Acq On : 10 May 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 10 12:31:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

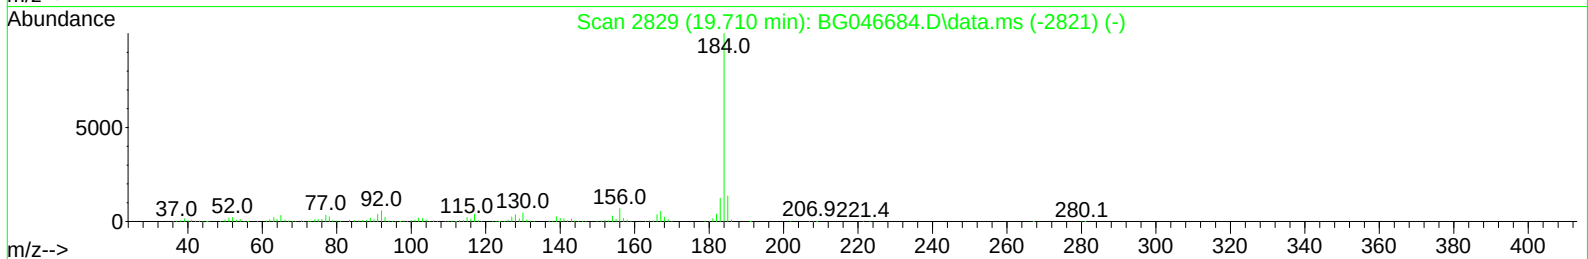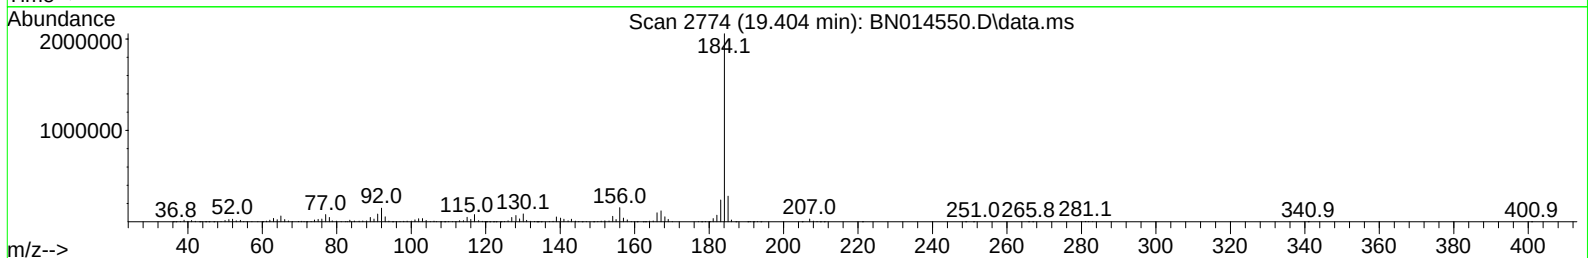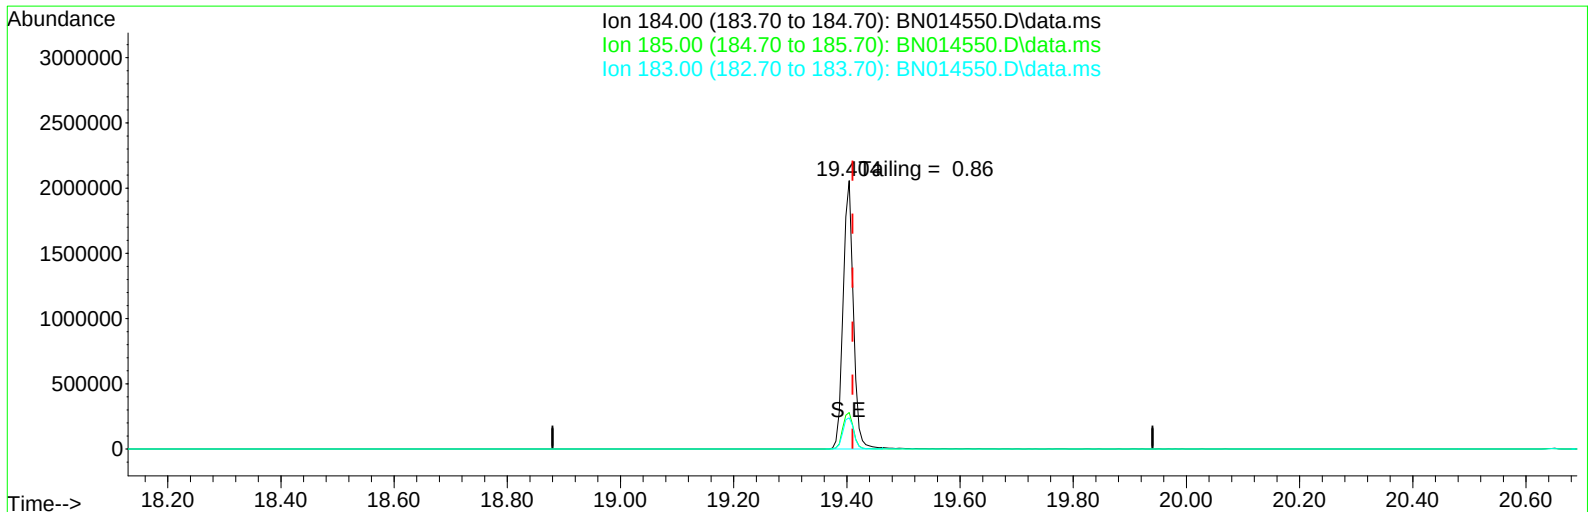

TIC: BN014550.D\data.ms

(77) Benzidine

19.404min (-0.006) 731933.20 ng




response 2594643

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.62
183.00	13.20	11.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051021\
 Data File : BN014550.D
 Acq On : 10 May 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 10 12:31:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

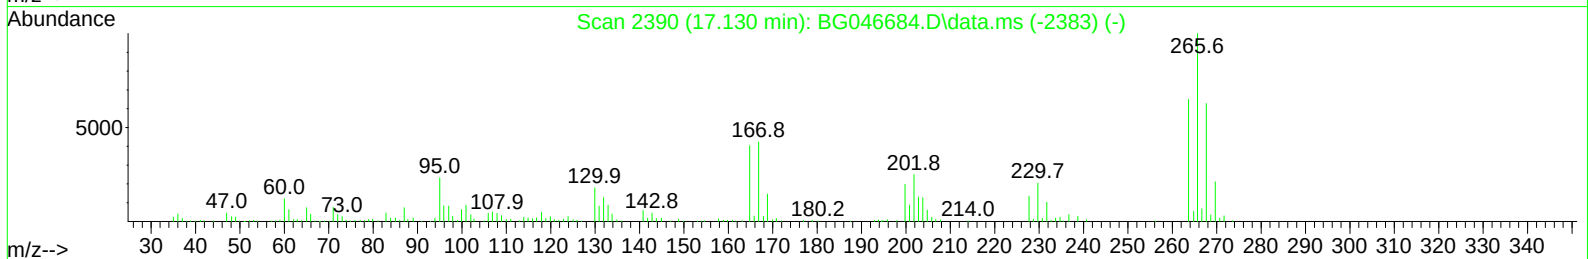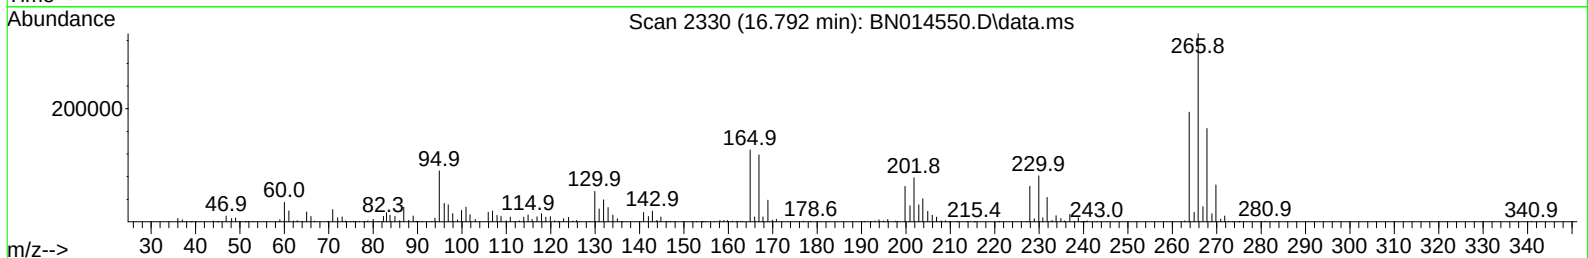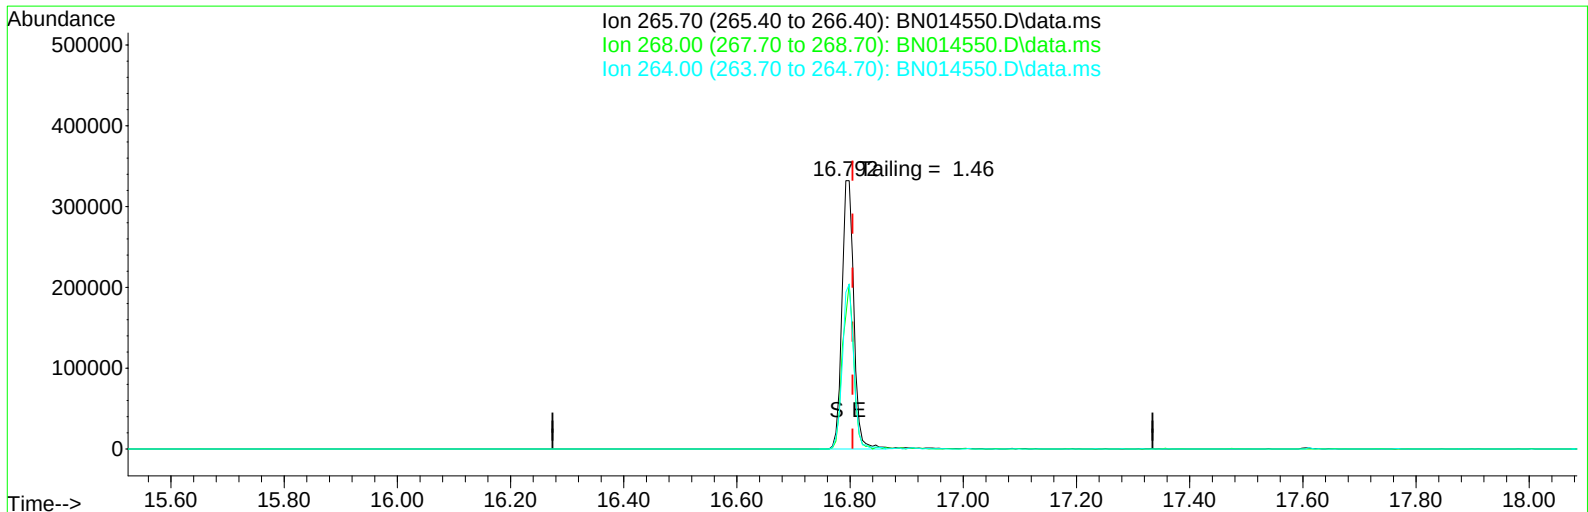

TIC: BN014550.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.012) 16569.30 ng

response 484368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	49.70#
264.00	61.60	58.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2021	BNA_N	<u>BN014550.D</u>
Compound Name	Response	Retention Time
DDT	1548537	20.65
DDD	8003	20.2
DDE	3039	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11042	1559579	0.71

Instrument :
BNA_N
ClientSampleId :
DFTPP