

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
 Data File : BN025376.D
 Acq On : 10 May 2023 12:09
 Operator : CG/JU
 Sample : 02479-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW949DL

Quant Time: May 11 01:10:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 10 12:11:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	7001	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	24499	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164	15130	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	31210	0.400	ng/ul	0.00
17) Chrysene-d12	21.494	240	27164	0.400	ng/ul	# 0.00
23) Perylene-d12	23.911	264	28563	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	2292	0.316	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.299	152	817	0.026	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	2460	0.034	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.759	128	27506	0.438	ng/ul	99
7) 2-Methylnaphthalene	12.370	142	29524	0.768	ng/ul	100
8) 1-Methylnaphthalene	12.590	142	23724	0.579	ng/ul	100
10) Acenaphthylene	14.265	152	22353	0.397	ng/ul#	93
11) Acenaphthene	14.607	153	82451	1.735	ng/ul	98
12) Fluorene	15.593	166	94888	1.787	ng/ul	99
14) Pentachlorophenol	16.958	266	168	0.027	ng/ul#	89
15) Phenanthrene	17.338	178	1932129	21.932	ng/ul	99
16) Anthracene	17.427	178	478677	6.642	ng/ul	99
19) Fluoranthene	19.354	202	3595023	36.598	ng/ul	97
20) Pyrene	19.721	202	3129523	31.008	ng/ul	99
21) Benzo(a)anthracene	21.476	228	1543520	18.857	ng/ul	98
22) Chrysene	21.529	228	1452512	16.267	ng/ul	97
24) Benzo(b)fluoranthene	23.174	252	2229667	19.241	ng/ul	95
26) Benzo(a)pyrene	23.803	252	1175418	12.259	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	26.420	276	725274	6.565	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.427	278	178392	2.067	ng/ul	96
29) Benzo(g,h,i)perylene	27.205	276	646732	6.885	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
Data File : BN025376.D
Acq On : 10 May 2023 12:09
Operator : CG/JU
Sample : 02479-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW949DL

Quant Time: May 11 01:10:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 12:11:16 2023
Response via : Initial Calibration




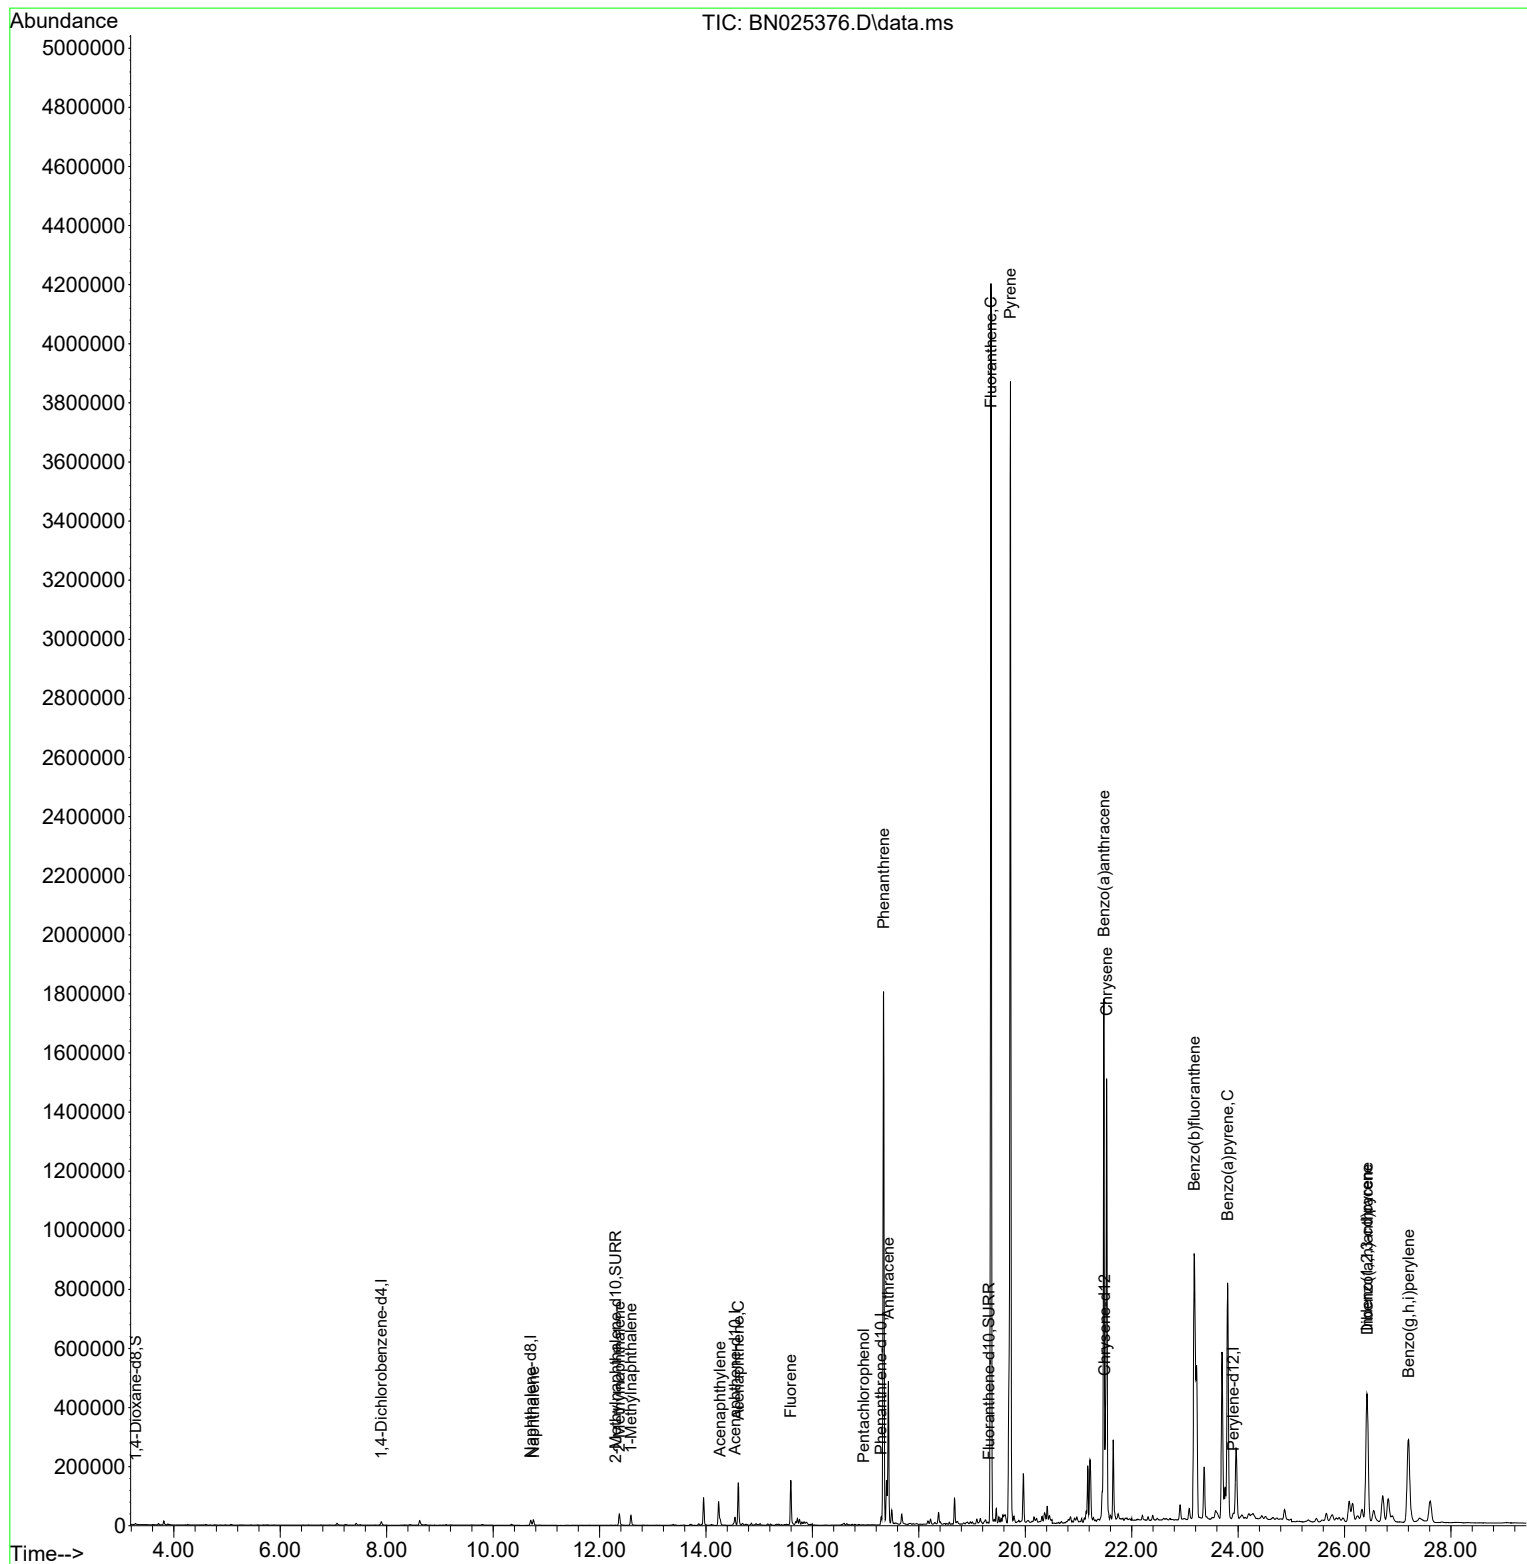


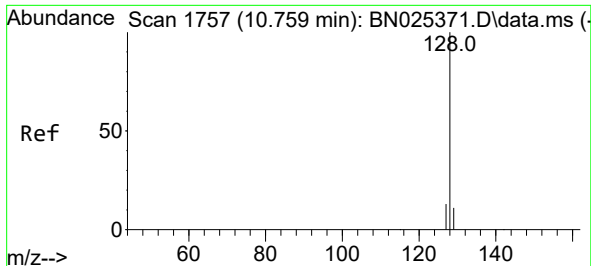

#5
Naphthalene
Concen: 0.438 ng/ul
RT: 10.759 min Scan# 1757
Delta R.T. 0.000 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09




Instrument :
BNA_N
ClientSampleId :
EW949DL


Tgt Ion:128 Resp: 27506
Ion Ratio Lower Upper
128 100
129 11.9 9.0 13.6
127 13.4 10.7 16.1

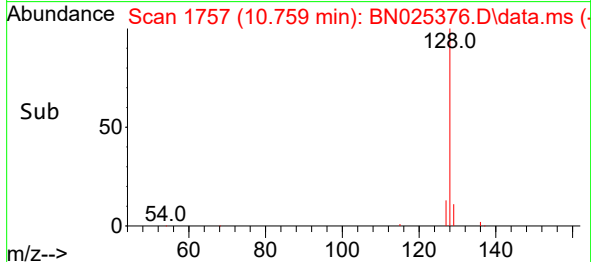

#7
2-Methylnaphthalene
Concen: 0.768 ng/ul
RT: 12.370 min Scan# 2050
Delta R.T. -0.005 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09

Tgt Ion:142 Resp: 29524
Ion Ratio Lower Upper
142 100
141 88.9 71.4 107.0


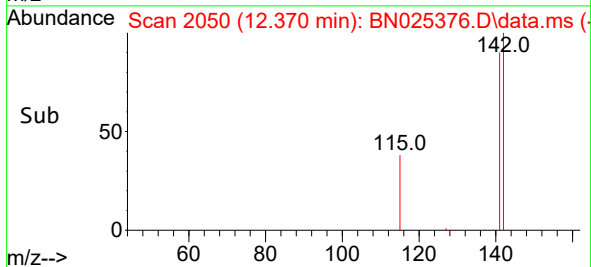

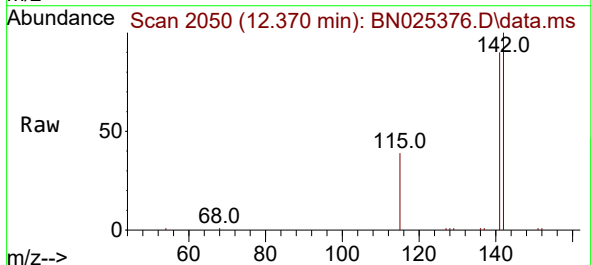


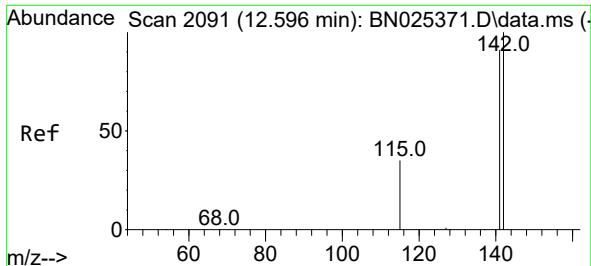

#8
1-Methylnaphthalene
Concen: 0.579 ng/ul
RT: 12.590 min Scan# 2091
Delta R.T. -0.005 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09




Instrument :
BNA_N
ClientSampleId :
EW949DL


Tgt Ion:142 Resp: 23724
Ion Ratio Lower Upper
142 100
141 92.1 73.8 110.6

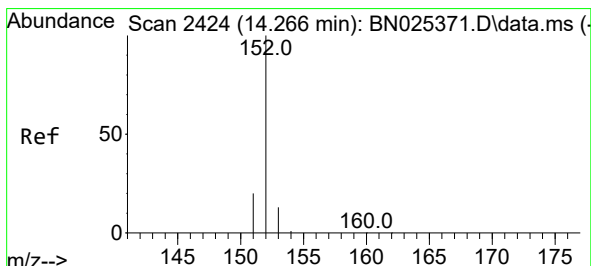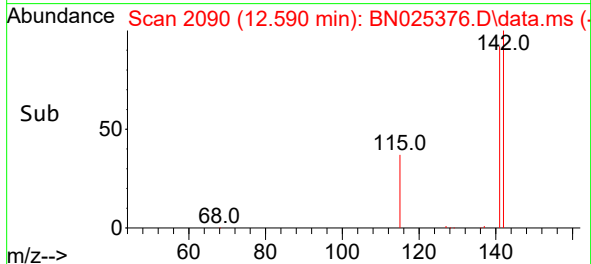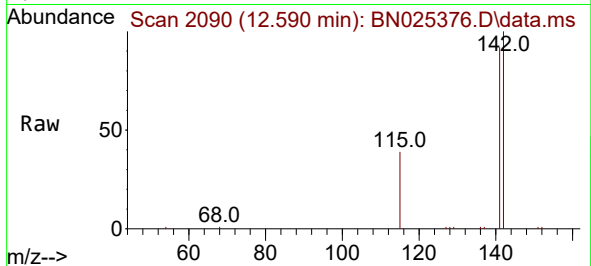

#10
Acenaphthylene
Concen: 0.397 ng/ul
RT: 14.265 min Scan# 2424
Delta R.T. -0.001 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09

Tgt Ion:152 Resp: 22353
Ion Ratio Lower Upper
152 100
151 21.9 16.0 24.0
153 18.0 10.8 16.2#

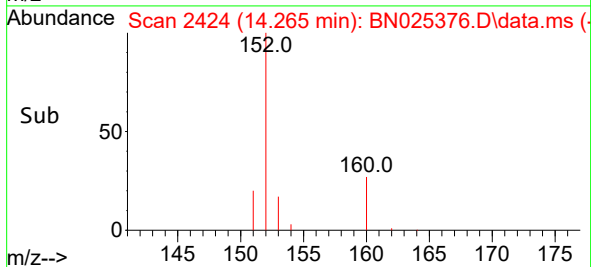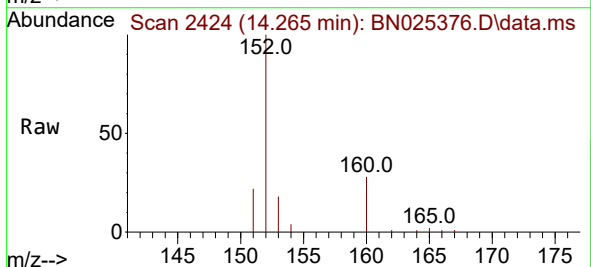



#11

Acenaphthene

Concen: 1.735 ng/ul

RT: 14.607 min Scan# 2498

Delta R.T. -0.001 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09

Instrument :

BNA_N

ClientSampleId :

EW949DL





Tgt Ion:153 Resp: 82451

Ion Ratio Lower Upper

153 100

152 48.2 40.2 60.4

154 87.7 69.4 104.2

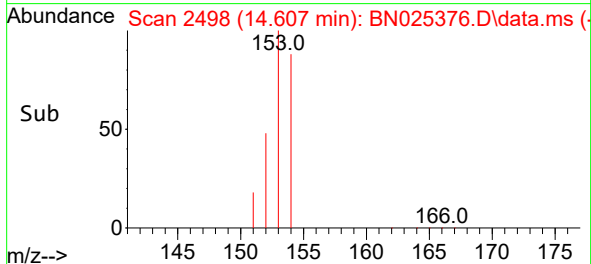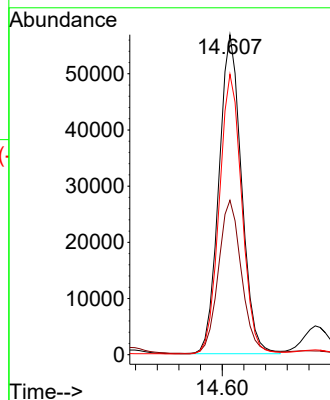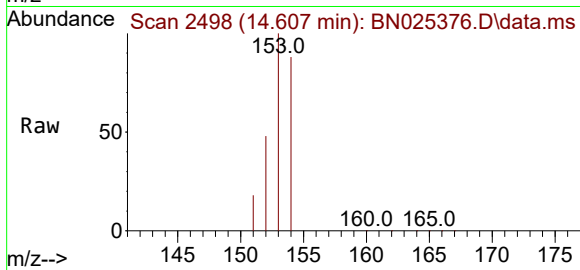

#12

Fluorene

Concen: 1.787 ng/ul

RT: 15.593 min Scan# 2711

Delta R.T. -0.010 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09




Tgt Ion:166 Resp: 94888


Ion Ratio Lower Upper

166 100

165 98.7 78.1 117.1

167 15.0 11.0 16.6



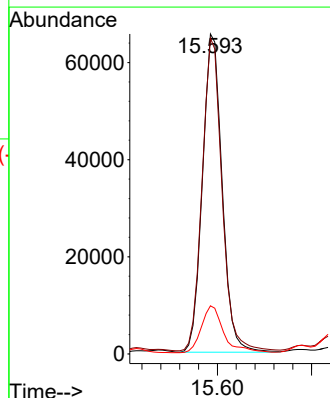
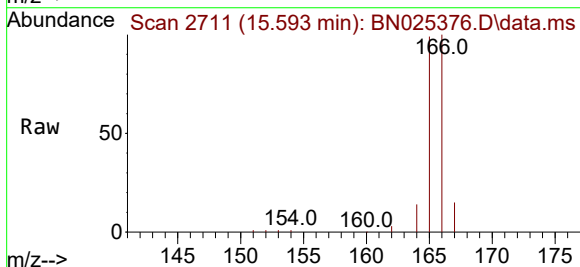


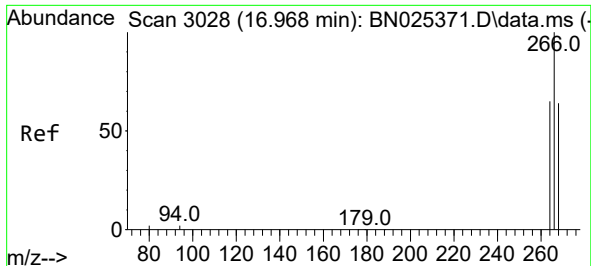

#14
 Pentachlorophenol
 Concen: 0.027 ng/ul
 RT: 16.958 min Scan# 3028
 Delta R.T. -0.009 min
 Lab File: BN025376.D
 Acq: 10 May 2023 12:09




Instrument :
 BNA_N
 ClientSampleId :
 EW949DL


Tgt Ion:266 Resp: 168
 Ion Ratio Lower Upper
 266 100
 264 58.3 49.6 74.4
 268 50.6 51.3 76.9#

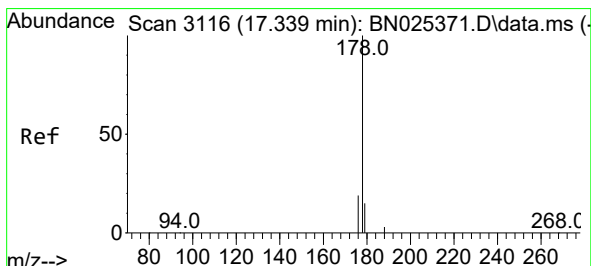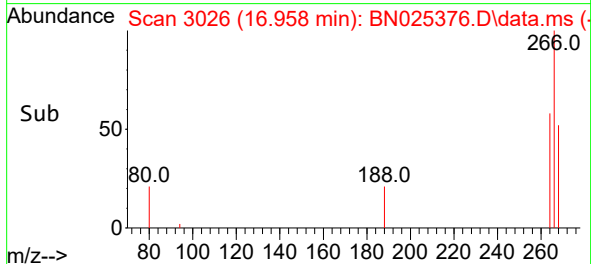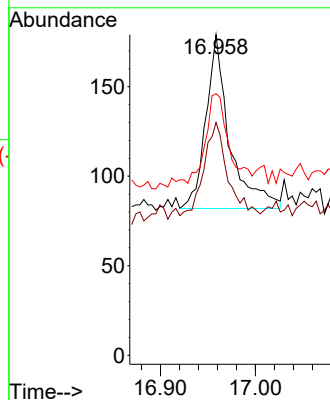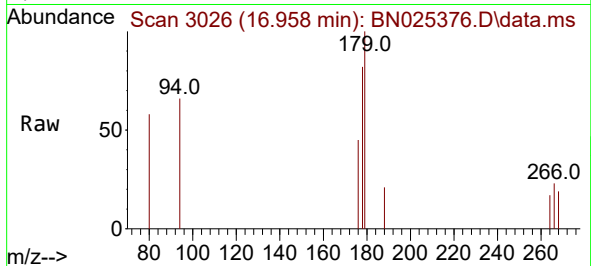

#15
 Phenanthrene
 Concen: 21.932 ng/ul
 RT: 17.338 min Scan# 3116
 Delta R.T. -0.001 min
 Lab File: BN025376.D
 Acq: 10 May 2023 12:09

Tgt Ion:178 Resp: 1932129
 Ion Ratio Lower Upper
 178 100
 179 15.4 12.5 18.7
 176 19.1 15.6 23.4


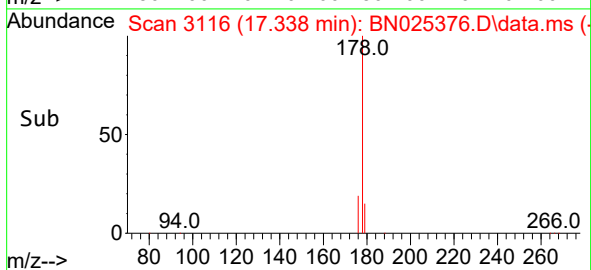
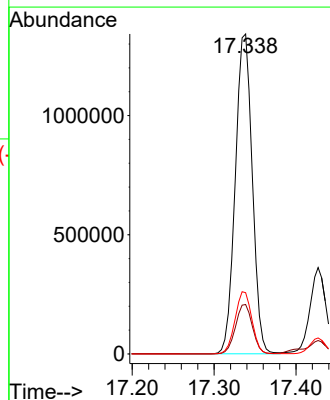
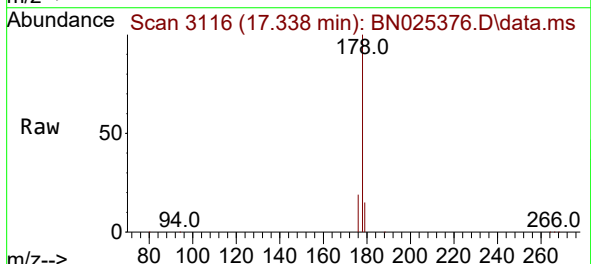


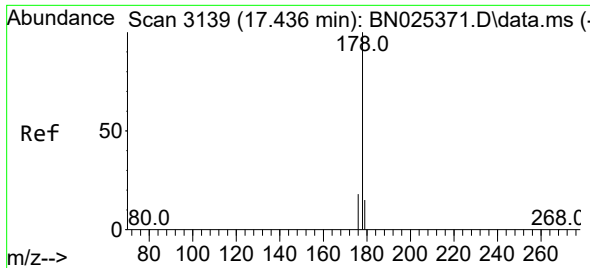

#16
 Anthracene
 Concen: 6.642 ng/ul
 RT: 17.427 min Scan# 3139
 Delta R.T. -0.009 min
 Lab File: BN025376.D
 Acq: 10 May 2023 12:09




Instrument :
 BNA_N
 ClientSampleId :
 EW949DL


Tgt Ion:178 Resp: 478677
 Ion Ratio Lower Upper
 178 100
 179 15.6 12.7 19.1
 176 18.6 15.3 22.9

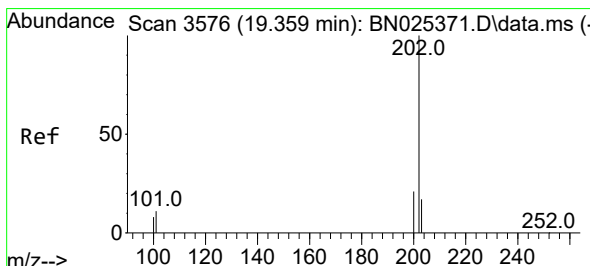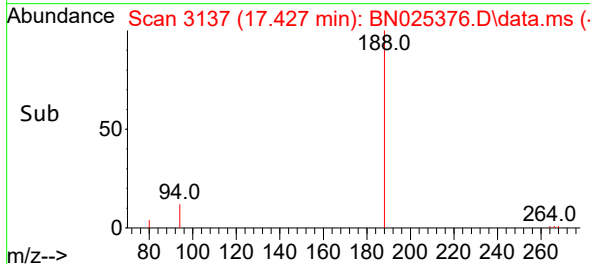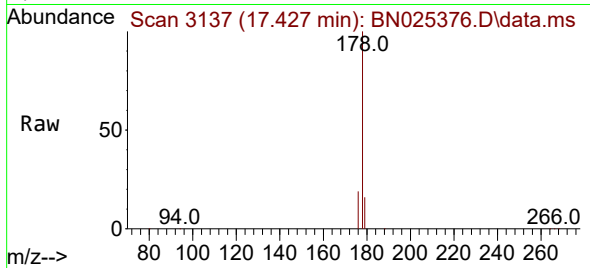

#19
 Fluoranthene
 Concen: 36.598 ng/ul
 RT: 19.354 min Scan# 3575
 Delta R.T. -0.005 min
 Lab File: BN025376.D
 Acq: 10 May 2023 12:09

Tgt Ion:202 Resp: 3595023
 Ion Ratio Lower Upper
 202 100
 101 13.4 9.7 14.5
 100 10.1 7.3 10.9

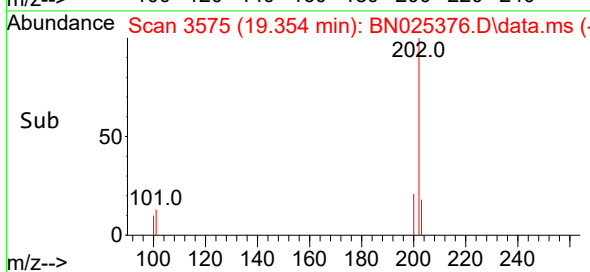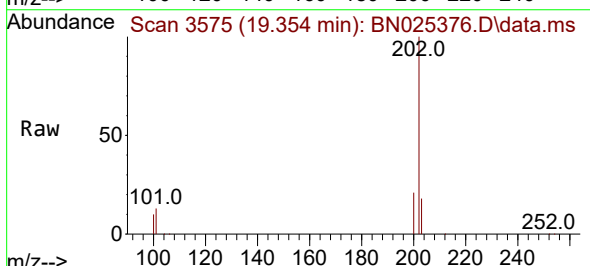

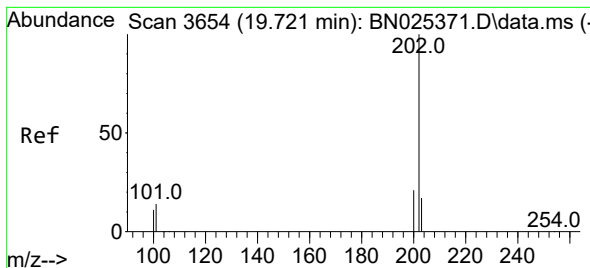

#20

Pyrene

Concen: 31.008 ng/ul

RT: 19.721 min Scan# 3654

Delta R.T. -0.000 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09

Instrument :

BNA_N

ClientSampleId :

EW949DL





Tgt Ion:202 Resp: 3129523

Ion Ratio Lower Upper

202 100

101 14.6 11.3 16.9

100 11.6 9.2 13.8

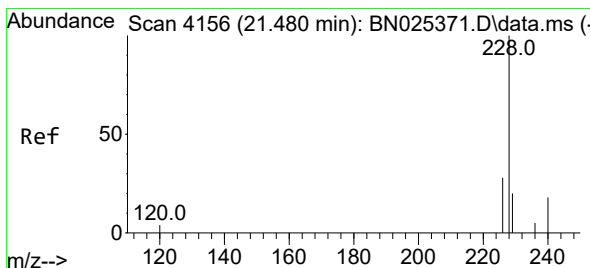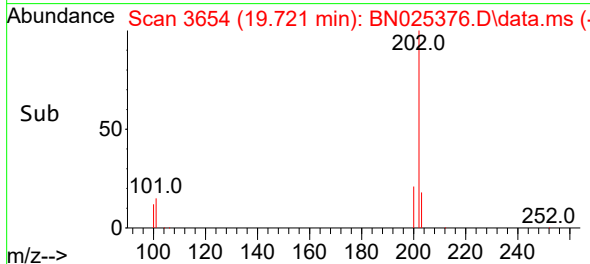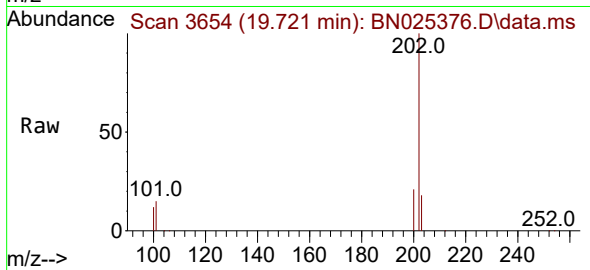

#21

Benzo(a)anthracene

Concen: 18.857 ng/ul

RT: 21.476 min Scan# 4155

Delta R.T. -0.003 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09




Tgt Ion:228 Resp: 1543520


Ion Ratio Lower Upper

228 100

229 20.9 15.6 23.4

226 28.2 22.1 33.1

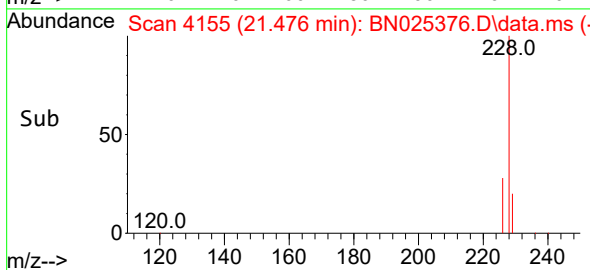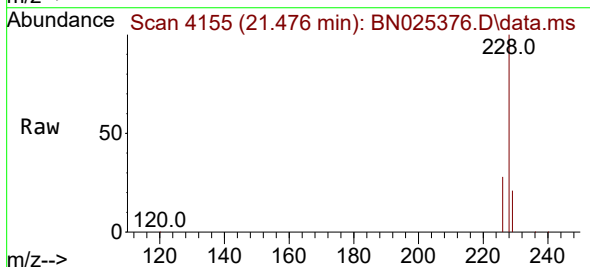

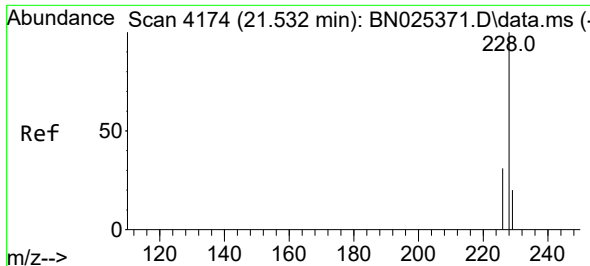

#22

Chrysene

Concen: 16.267 ng/ul

RT: 21.529 min Scan# 4173

Delta R.T. -0.003 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09

Instrument :

BNA_N

ClientSampleId :

EW949DL





Tgt Ion:228 Resp: 1452512

Ion Ratio Lower Upper

228 100

226 30.8 24.5 36.7

229 22.3 15.8 23.6

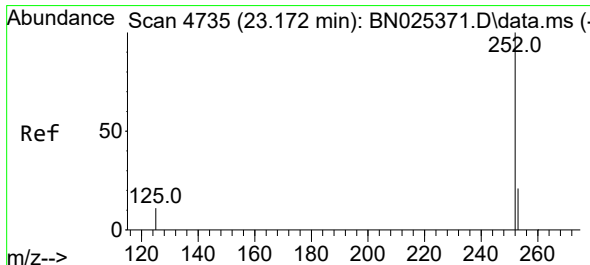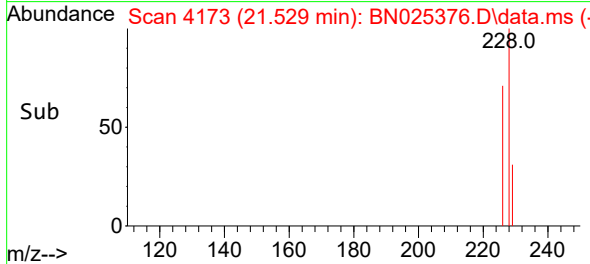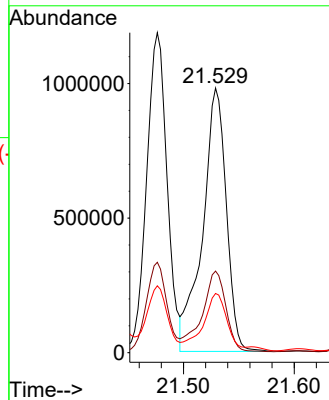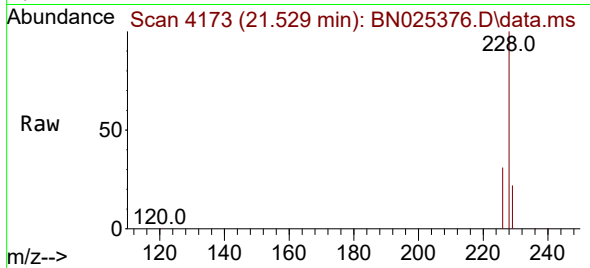

#24

Benzo(b)fluoranthene

Concen: 19.241 ng/ul

RT: 23.174 min Scan# 4736

Delta R.T. 0.003 min

Lab File: BN025376.D

Acq: 10 May 2023 12:09




Tgt Ion:252 Resp: 2229667


Ion Ratio Lower Upper

252 100

253 22.8 0.0 50.2

125 12.7 0.0 30.4


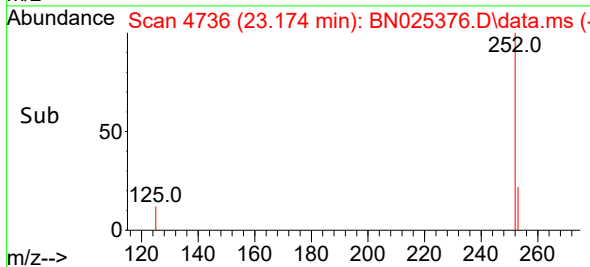
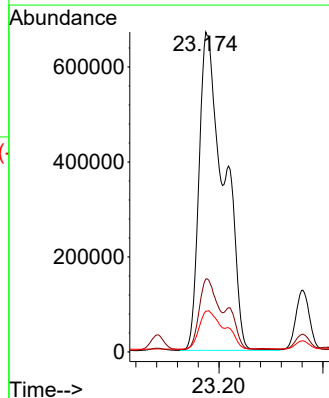
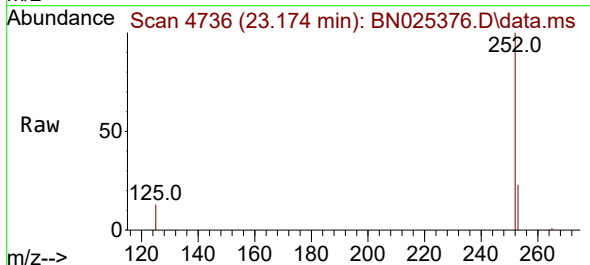




#26
Benzo(a)pyrene
Concen: 12.259 ng/ul
RT: 23.803 min Scan# 4951
Delta R.T. -0.003 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09




Instrument :
BNA_N
ClientSampleId :
EW949DL


Tgt Ion:252 Resp: 1175418
Ion Ratio Lower Upper
252 100
253 22.9 21.4 32.2
125 13.3 14.6 22.0#

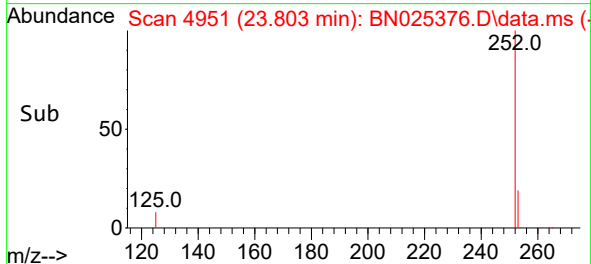

#27
Indeno(1,2,3-cd)pyrene
Concen: 6.565 ng/ul
RT: 26.420 min Scan# 5784
Delta R.T. -0.007 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09

Tgt Ion:276 Resp: 725274
Ion Ratio Lower Upper
276 100
138 24.6 21.9 32.9
227 0.2 0.1 0.1#


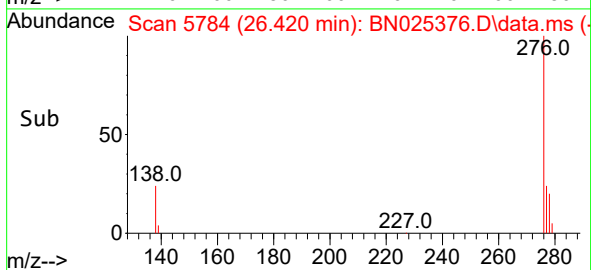

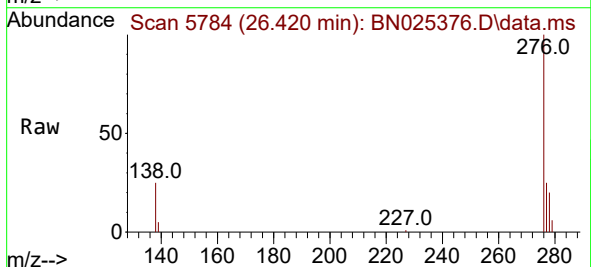


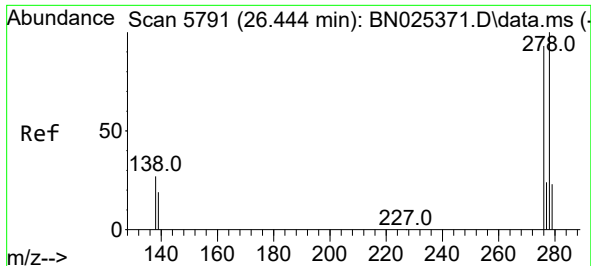

#28
Dibenzo(a,h)anthracene
Concen: 2.067 ng/ul
RT: 26.427 min Scan# 51
Delta R.T. -0.017 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09

Instrument :
BNA_N
ClientSampleId :
EW949DL

Tgt Ion:278 Resp: 178392
Ion Ratio Lower Upper
278 100
139 24.2 17.0 25.6
279 28.5 21.8 32.8

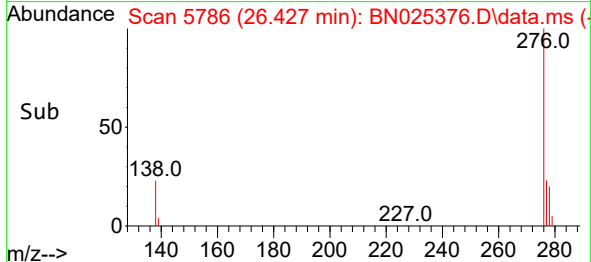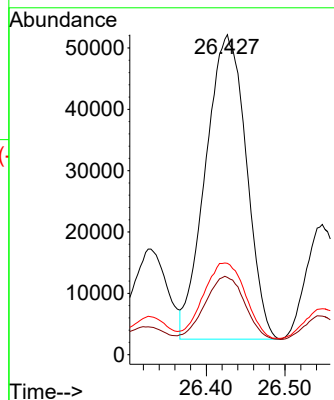

#29
Benzo(g,h,i)perylene
Concen: 6.885 ng/ul
RT: 27.205 min Scan# 6018
Delta R.T. 0.006 min
Lab File: BN025376.D
Acq: 10 May 2023 12:09

Tgt Ion:276 Resp: 646732
Ion Ratio Lower Upper
276 100
138 24.9 20.3 30.5
277 24.5 19.8 29.6

