

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
 Data File : BN025379.D
 Acq On : 10 May 2023 13:57
 Operator : CG/JU
 Sample : PB152658BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK658

Quant Time: May 11 01:11:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 10 12:11:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	6860	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	24699	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.547	164	15214	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	30215	0.400	ng/ul	0.00
17) Chrysene-d12	21.491	240	28124	0.400	ng/ul	0.00
23) Perylene-d12	23.914	264	26239	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	42696	6.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	10408	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.326	212	26570	0.358	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.689	202	3812	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.750	252	7311	0.083	ng/ul#	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
Data File : BN025379.D
Acq On : 10 May 2023 13:57
Operator : CG/JU
Sample : PB152658BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK658

Quant Time: May 11 01:11:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 10 12:11:16 2023
Response via : Initial Calibration




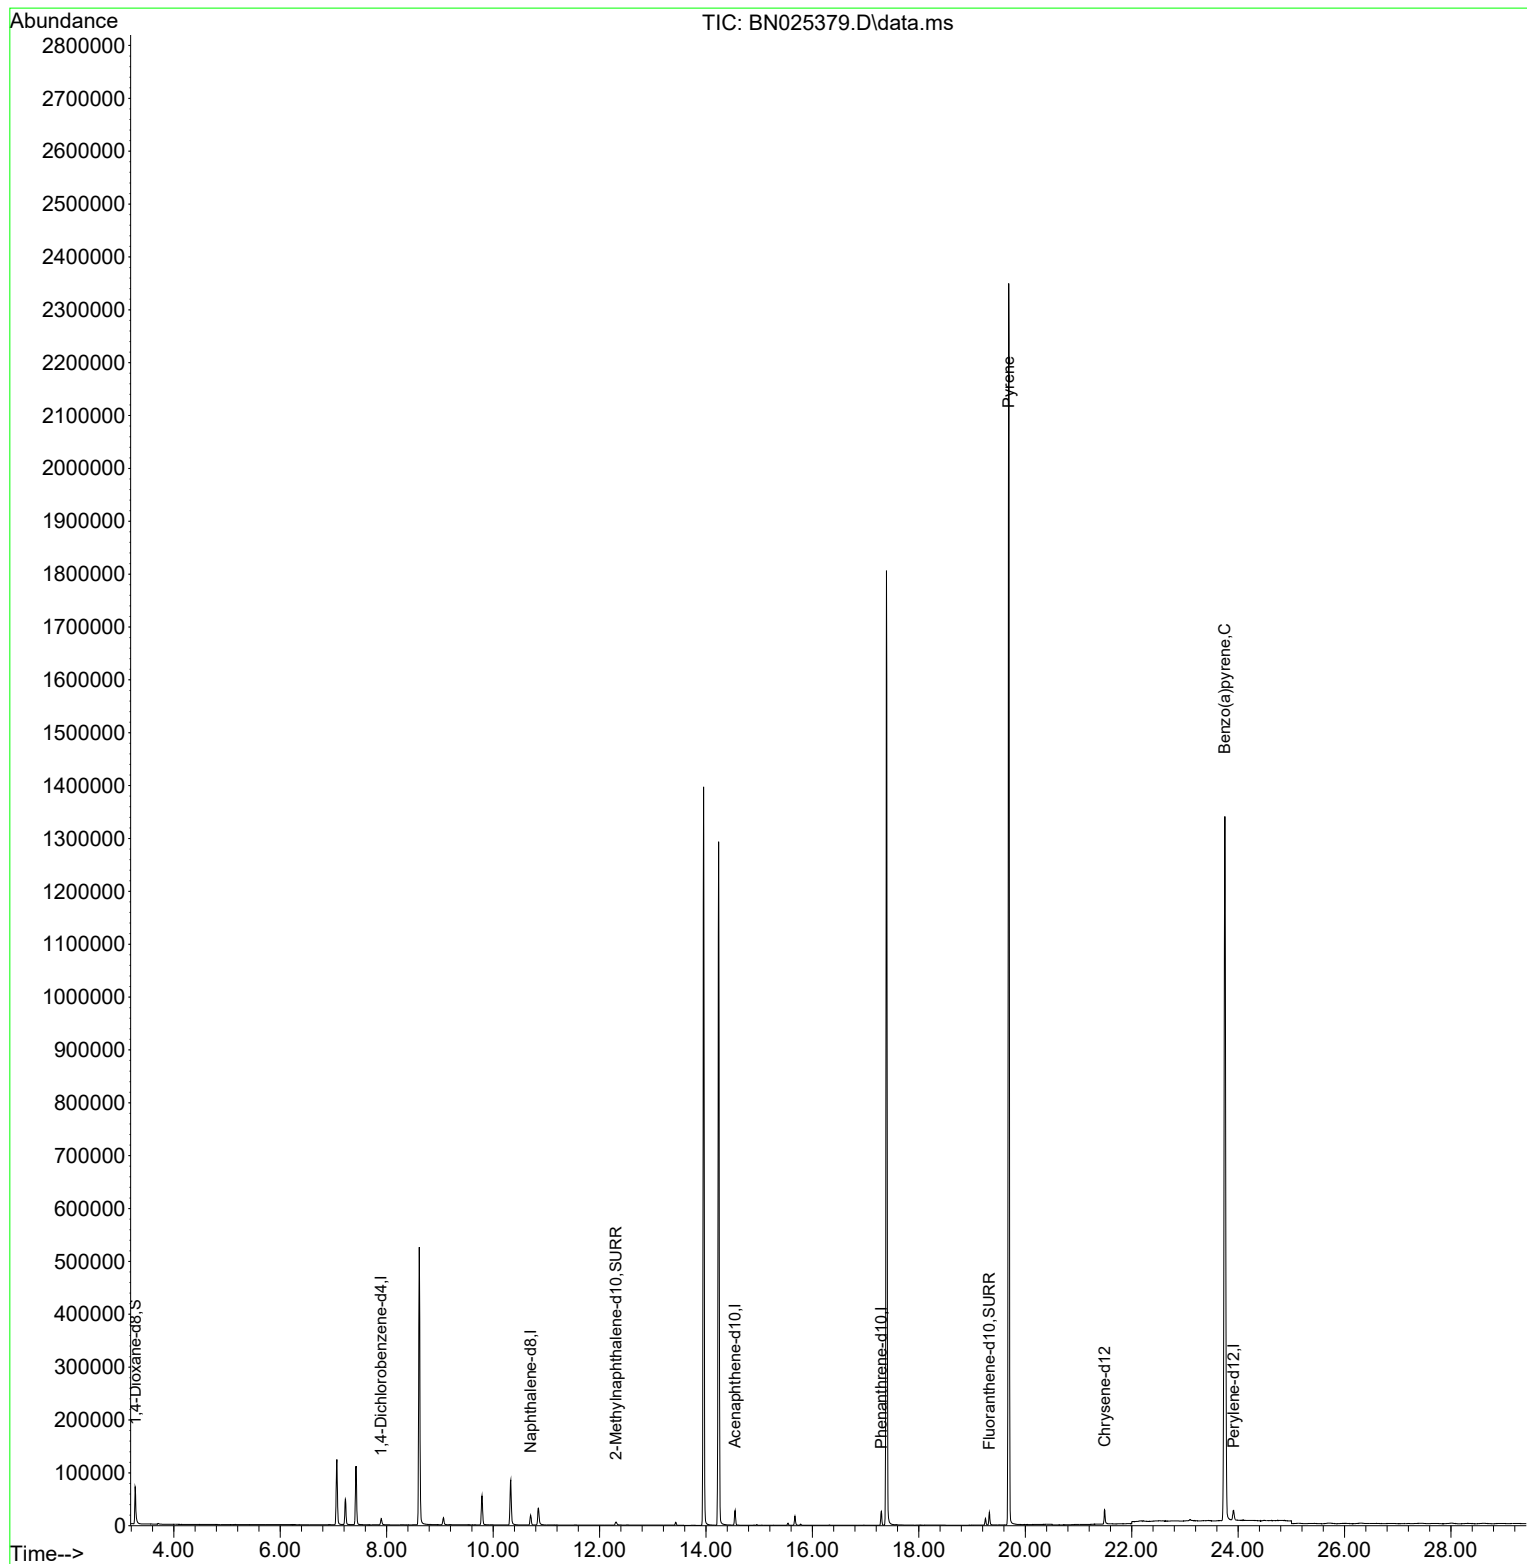


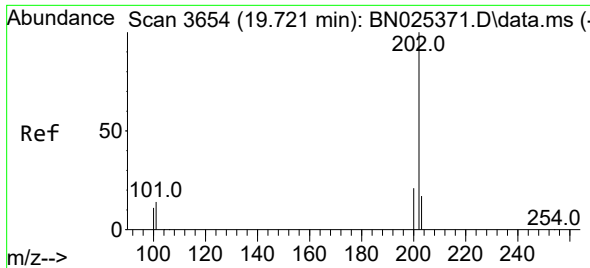

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.689 min Scan# 30
Delta R.T. -0.033 min
Lab File: BN025379.D
Acq: 10 May 2023 13:57

Instrument :
BNA_N
ClientSampleId :
SBLK658

Tgt Ion:202 Resp: 3812
Ion Ratio Lower Upper
202 100
101 167.5 11.3 16.9#
100 1233.5 9.2 13.8#

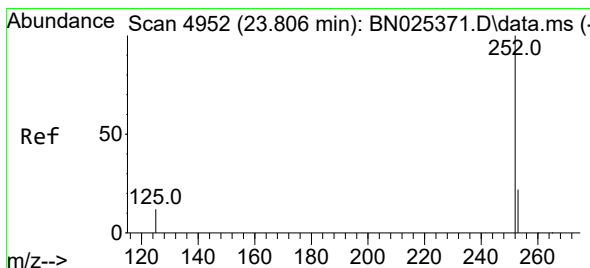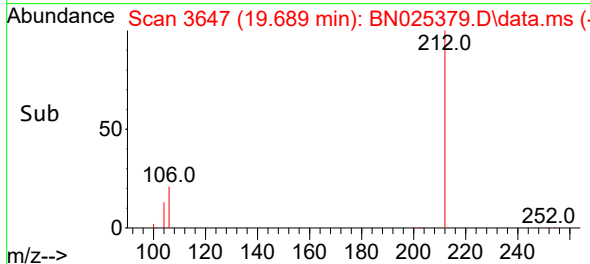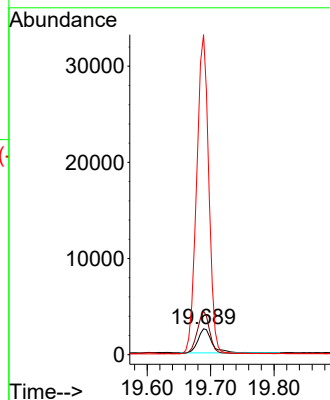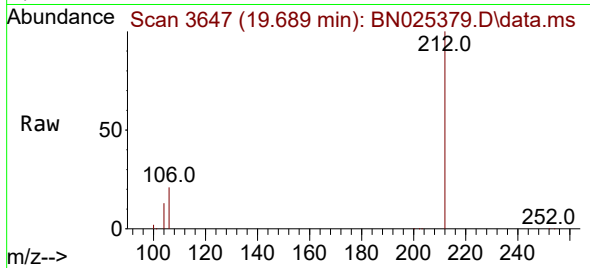

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.750 min Scan# 4933
Delta R.T. -0.056 min
Lab File: BN025379.D
Acq: 10 May 2023 13:57

Tgt Ion:252 Resp: 7311
Ion Ratio Lower Upper
252 100
253 55.4 21.4 32.2#
125 77.8 14.6 22.0#

