

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
 Data File : BN025383.D
 Acq On : 10 May 2023 16:43
 Operator : CG/JU
 Sample : PB152658BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK658

Quant Time: May 11 02:08:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 02:07:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	7876	0.400	ng/ul	0.00
4) Naphthalene-d8	10.704	136	26194	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.548	164	15637	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.293	188	32553	0.400	ng/ul	0.00
17) Chrysene-d12	21.495	240	26757	0.400	ng/ul	# 0.00
23) Perylene-d12	23.912	264	26544	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.272	96	43984	5.393	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	10975	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.327	212	26820	0.380	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.694	202	4041	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.754	252	6851	0.077	ng/ul#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051023\
Data File : BN025383.D
Acq On : 10 May 2023 16:43
Operator : CG/JU
Sample : PB152658BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK658

Quant Time: May 11 02:08:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 02:07:13 2023
Response via : Initial Calibration




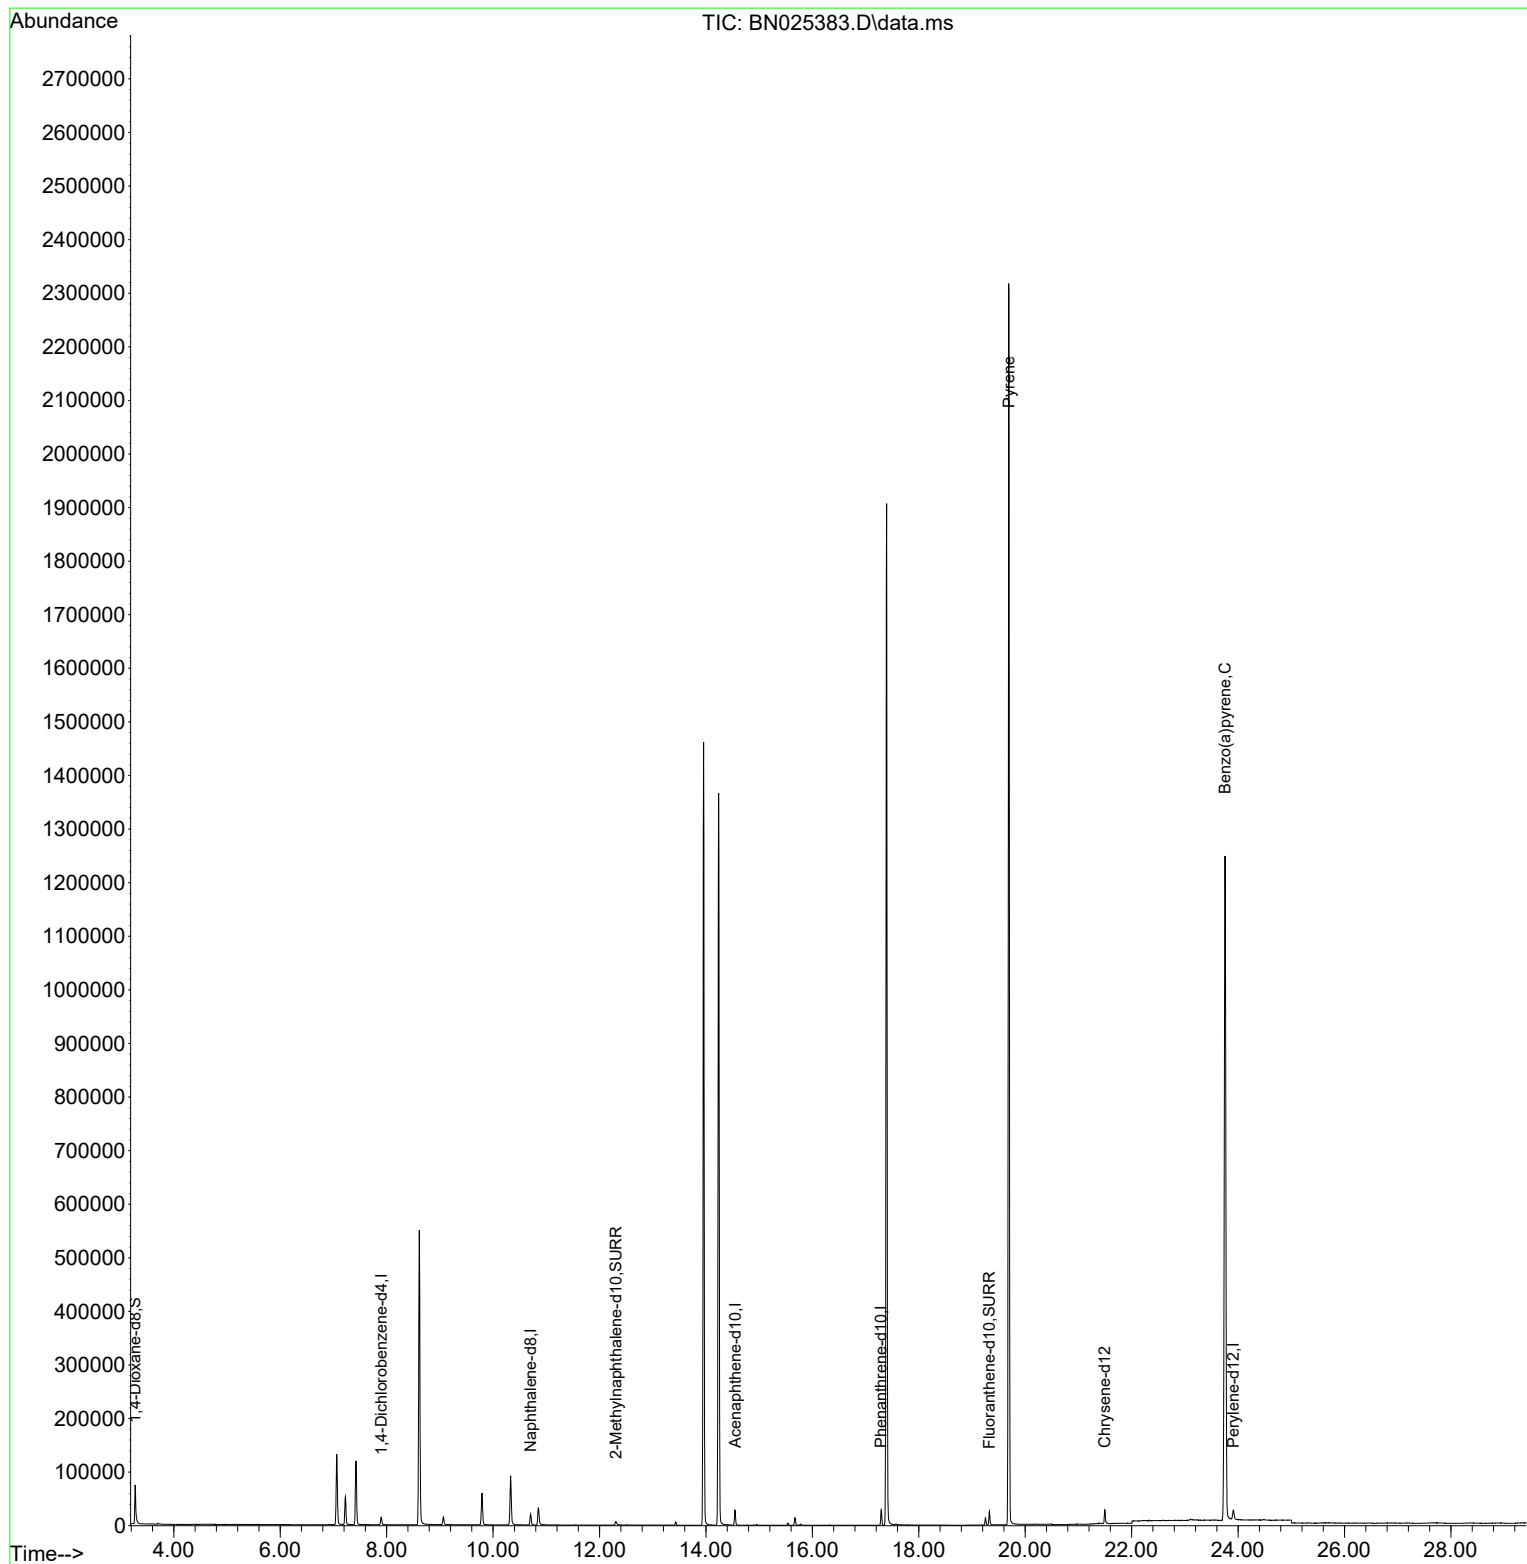


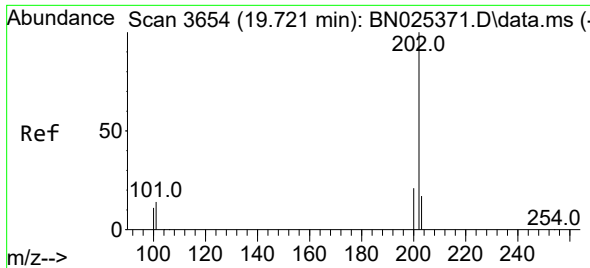

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.694 min Scan# 30
Delta R.T. -0.028 min
Lab File: BN025383.D
Acq: 10 May 2023 16:43

Instrument :
BNA_N
ClientSampleId :
SBLK658

Tgt Ion:202 Resp: 4041
Ion Ratio Lower Upper
202 100
101 153.0 11.3 16.9#
100 1078.7 9.2 13.8#

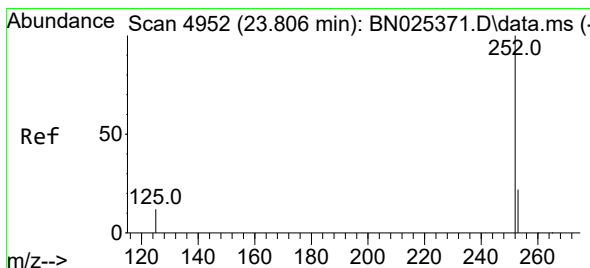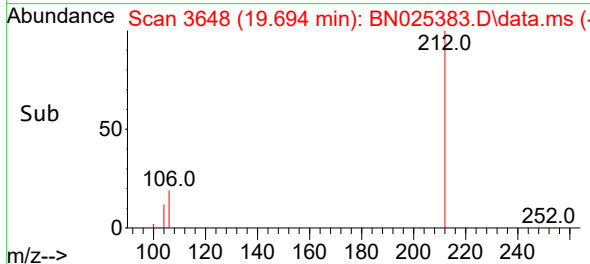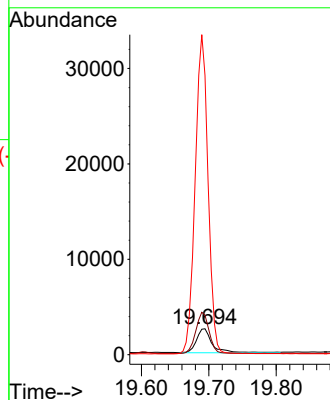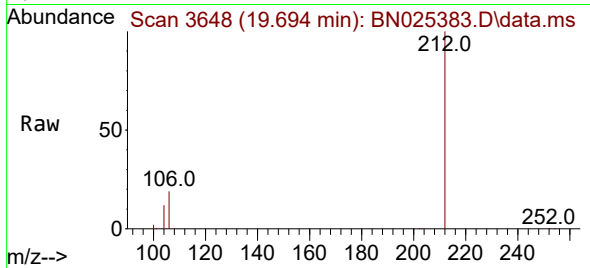

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.754 min Scan# 4934
Delta R.T. -0.064 min
Lab File: BN025383.D
Acq: 10 May 2023 16:43

Tgt Ion:252 Resp: 6851
Ion Ratio Lower Upper
252 100
253 57.2 21.4 32.2#
125 82.7 14.6 22.0#

