
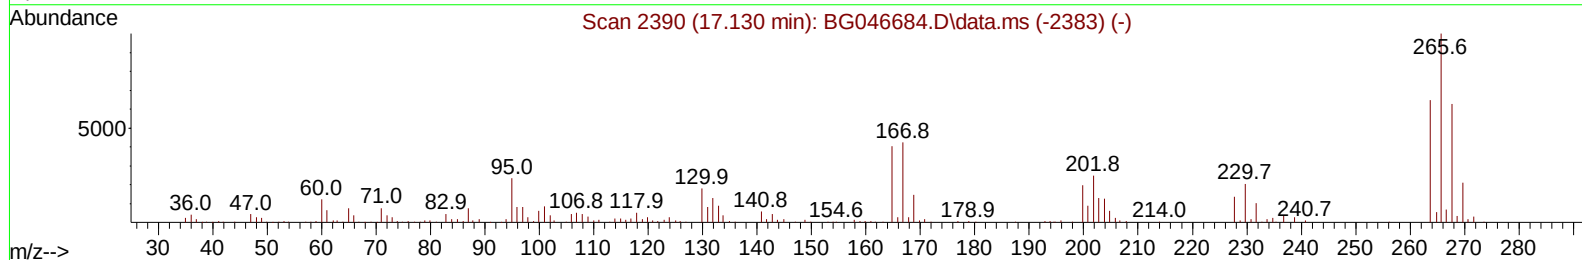
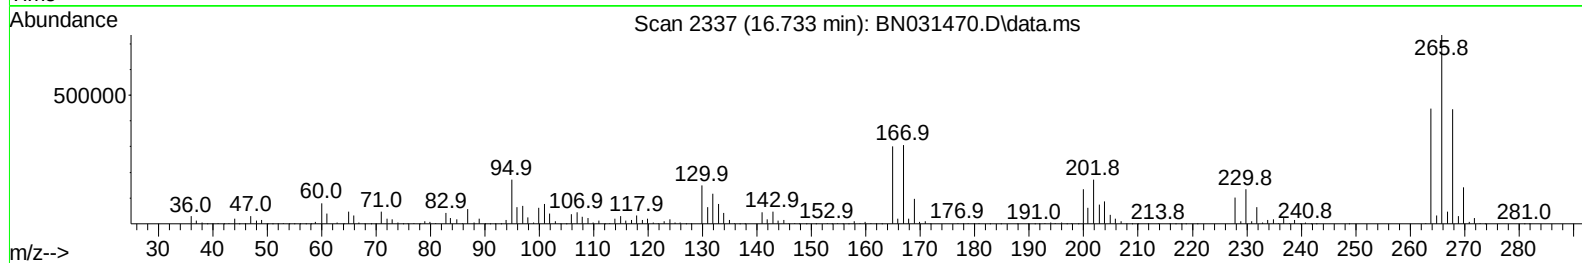


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031470.D
Acq On : 10 May 2024 20:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 04:10:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

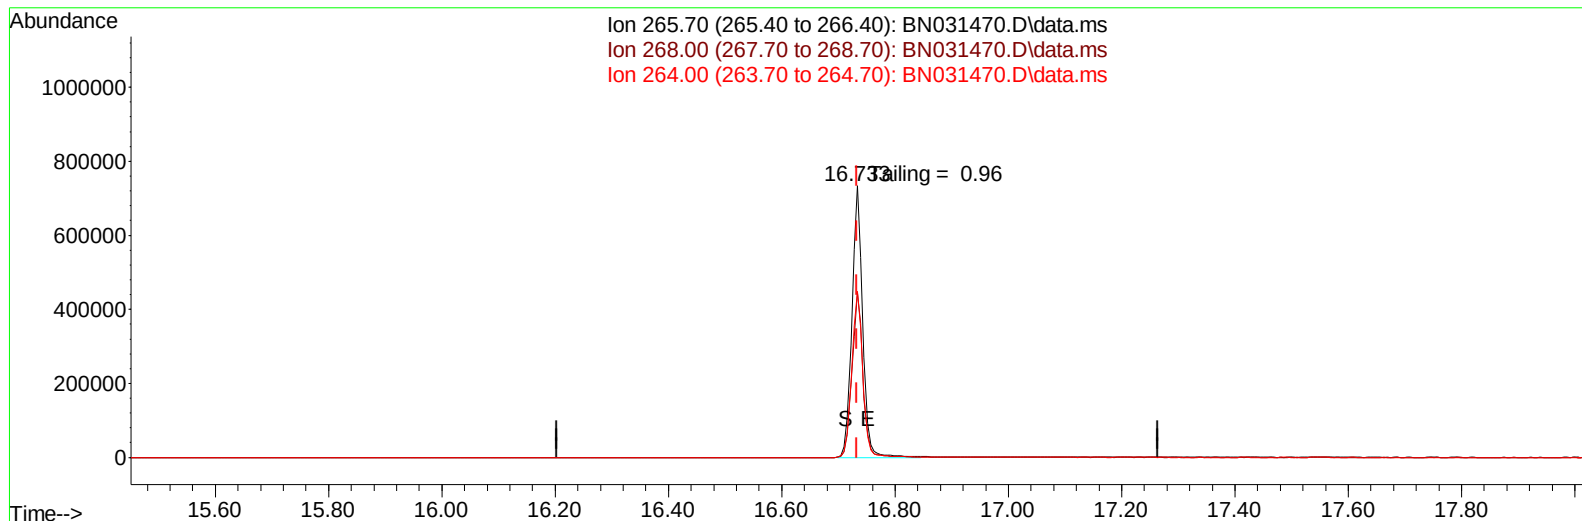




TIC: BN031470.D\data.ms

(70) Pentachlorophenol (C)**16.733min (+ 0.000) 25399.82 ng****response 979315**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.67
264.00	61.60	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031470.D
Acq On : 10 May 2024 20:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 04:10:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

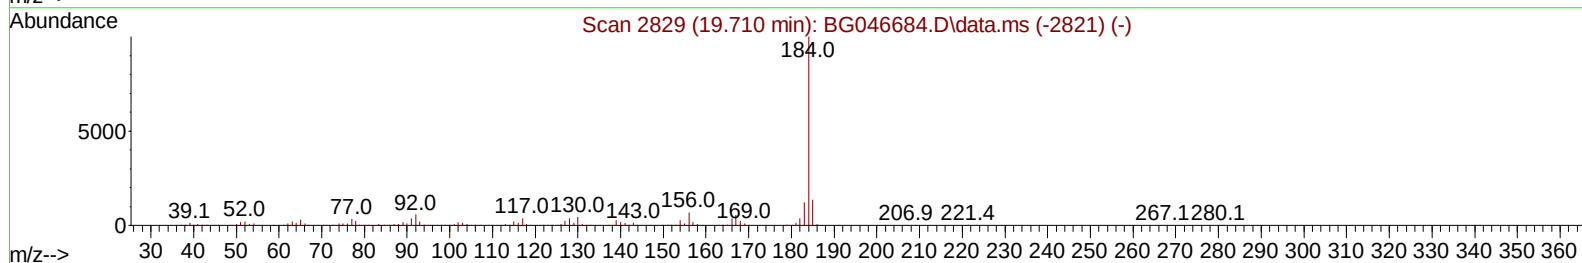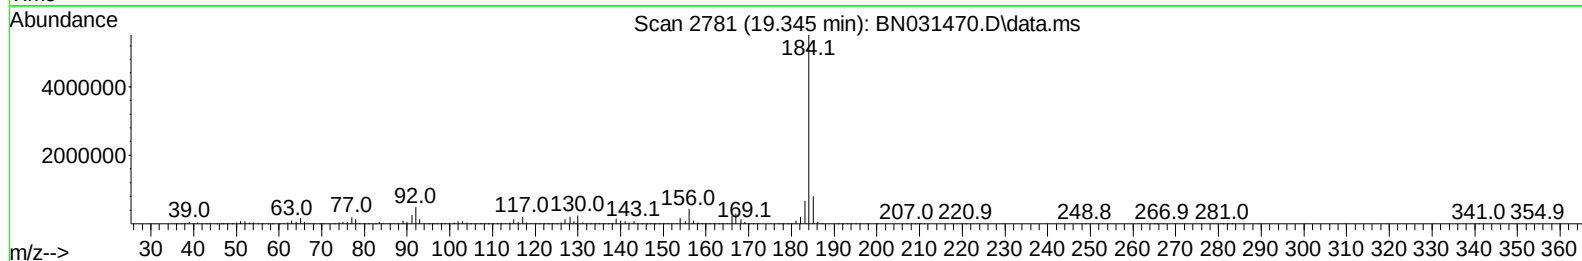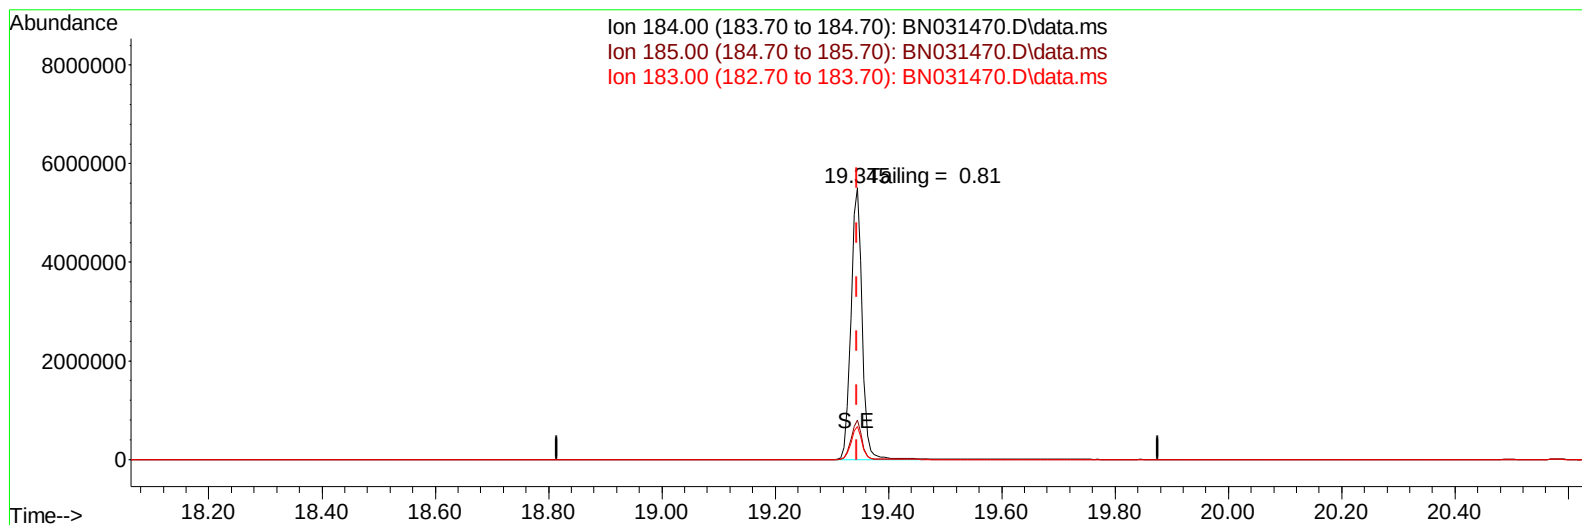

TIC: BN031470.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 0.00 ng

response 7617104

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	12.20
0.00	0.00	0.00