
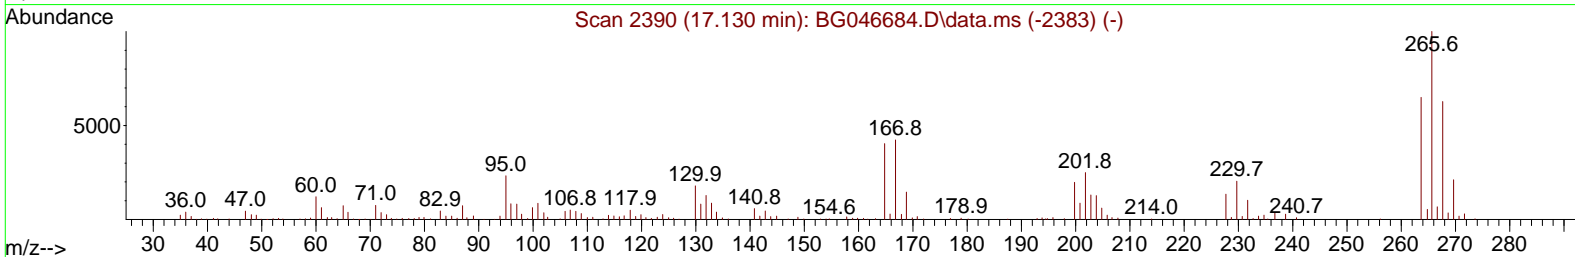
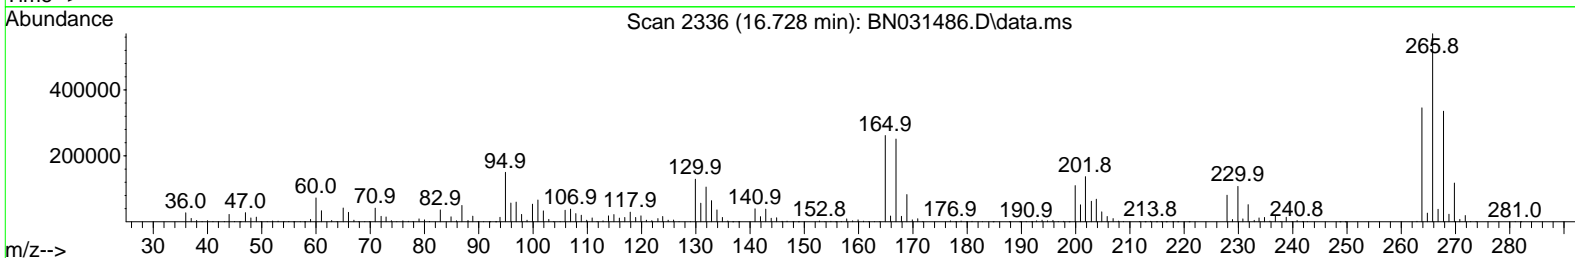


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051024\  
 Data File : BN031486.D  
 Acq On : 11 May 2024 06:56  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 13 01:37:44 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat May 11 04:09:05 2024  
 Response via : Initial Calibration

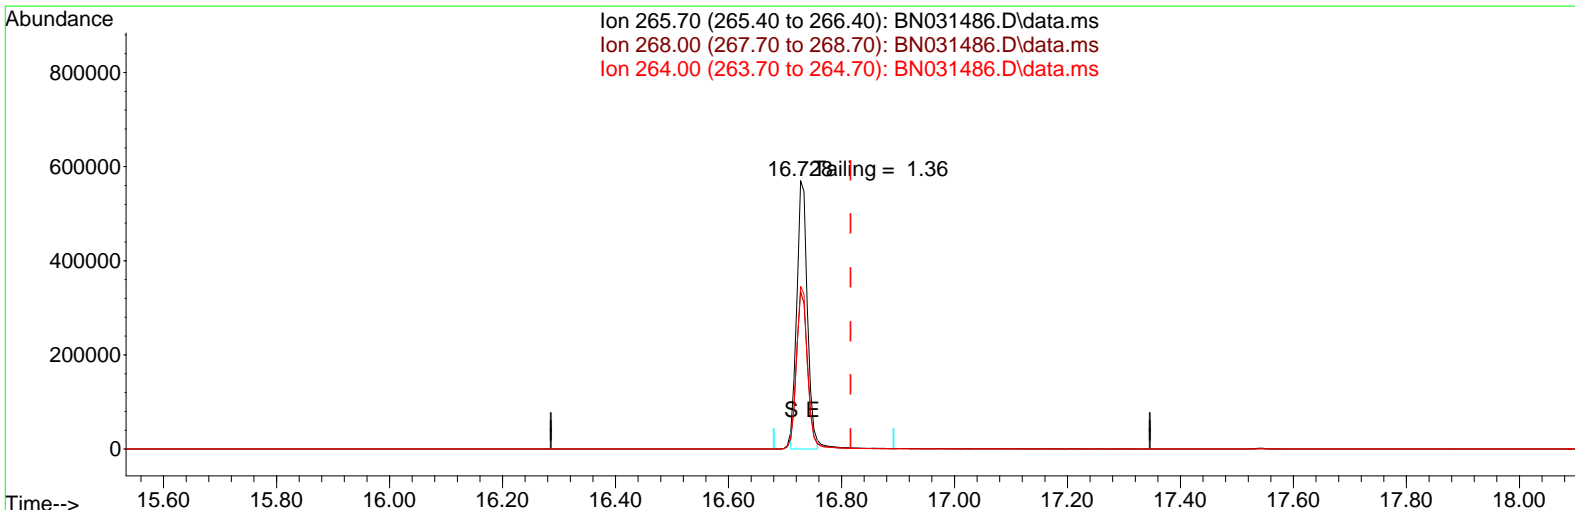

TIC: BN031486.D\data.ms

(70) Pentachlorophenol (C)




16.728min (-0.088) 22220.06 ng

response 778072

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.81
264.00	61.60	60.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051024\  
 Data File : BN031486.D  
 Acq On : 11 May 2024 06:56  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 13 01:37:44 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat May 11 04:09:05 2024  
 Response via : Initial Calibration

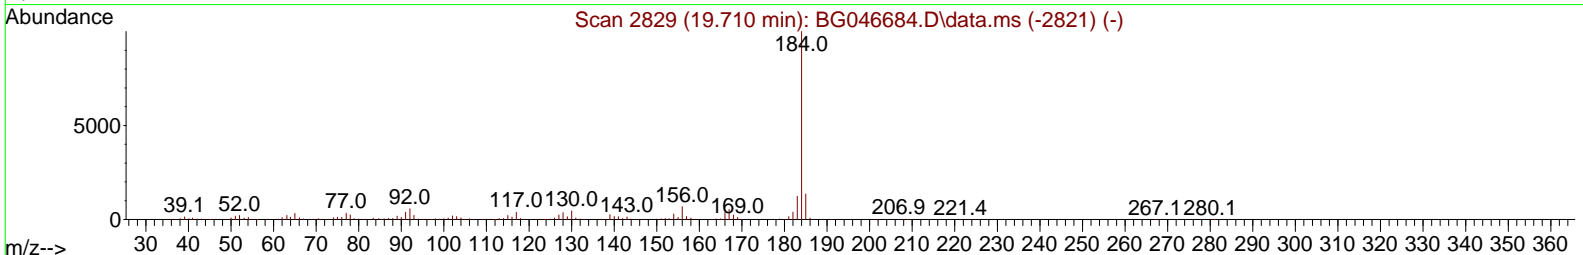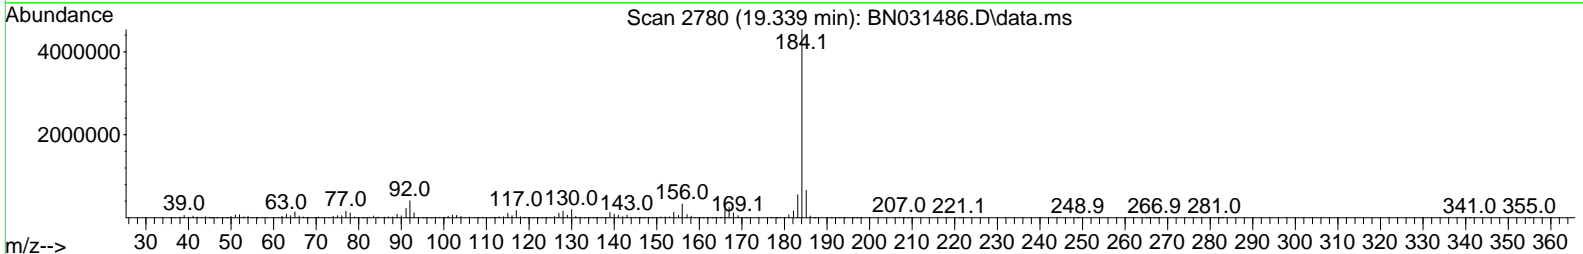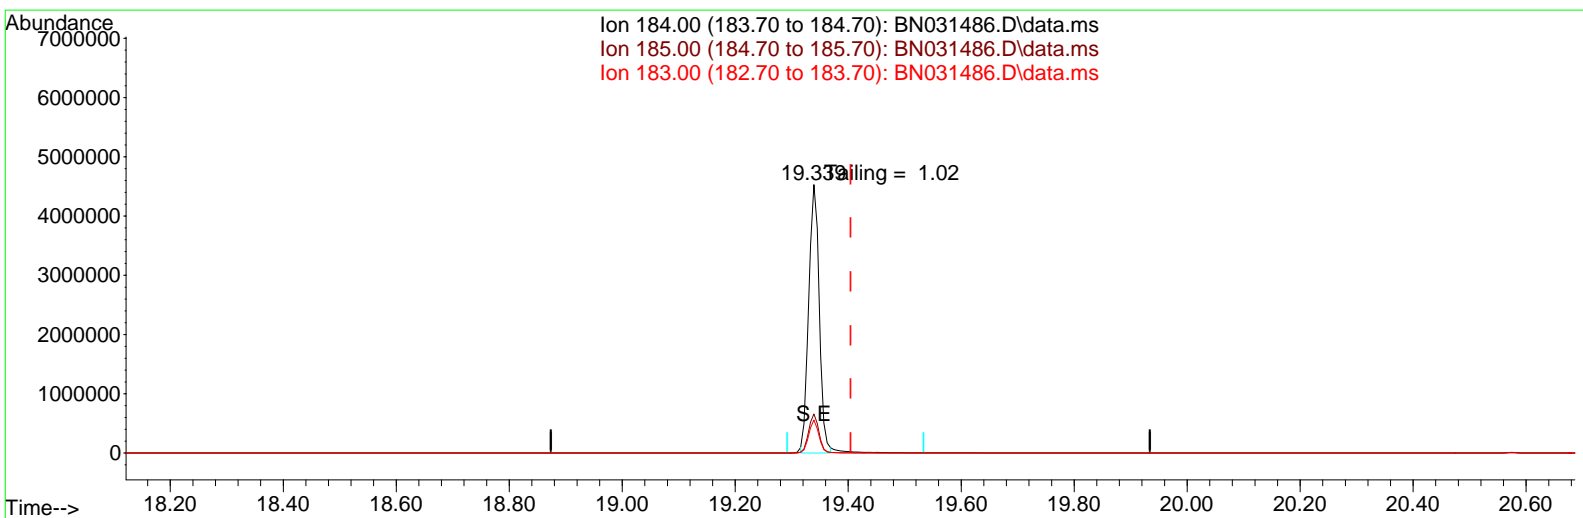

TIC: BN031486.D\data.ms

(77) Benzidine

19.339min (-0.065)	0.00 ng
response	6029877
Ion	Exp% Act%
184.00	100.00 100.00
185.00	15.50 14.57
183.00	13.20 12.29
0.00	0.00 0.00