
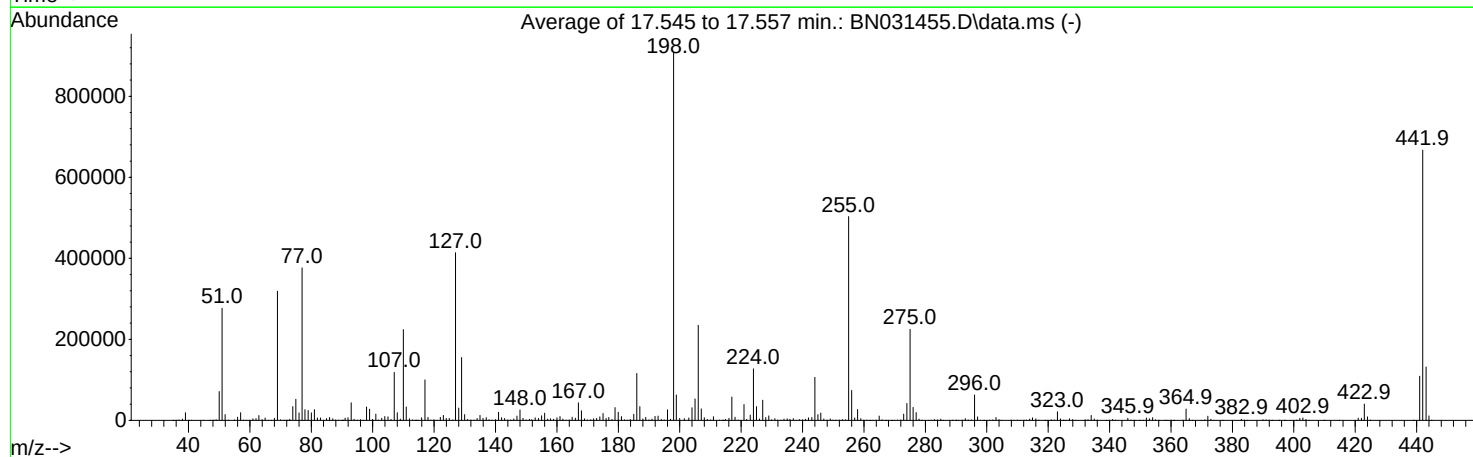


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051024\  
Data File : BN031455.D  
Acq On : 10 May 2024 07:57  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN050924.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri May 10 02:12:24 2024

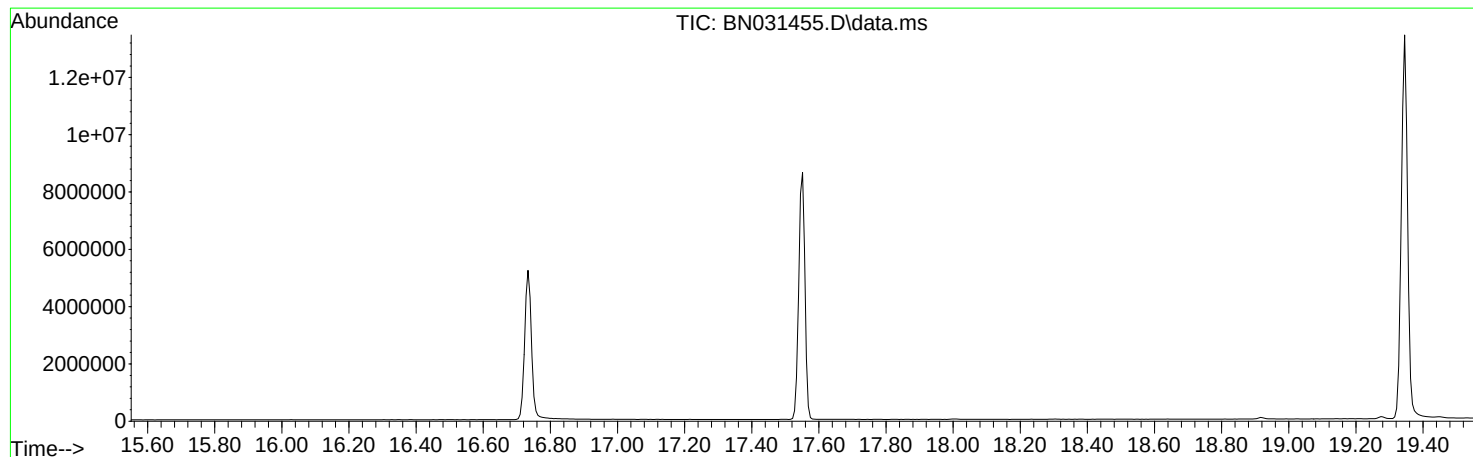

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2467

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 51     | 198     | 10     | 80     | 30.5  | 277045 | PASS      |
| 68     | 69      | 0.00   | 2      | 1.6   | 5177   | PASS      |
| 69     | 198     | 0.00   | 100    | 35.1  | 318650 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 1461   | PASS      |
| 127    | 198     | 10     | 80     | 45.6  | 414059 | PASS      |
| 197    | 198     | 0.00   | 2      | 0.3   | 2786   | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 908053 | PASS      |
| 199    | 198     | 5      | 9      | 6.9   | 62747  | PASS      |
| 275    | 198     | 10     | 60     | 24.8  | 224832 | PASS      |
| 365    | 198     | 1      | 100    | 3.1   | 28019  | PASS      |
| 441    | 198     | 0.01   | 100    | 12.0  | 109040 | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 667285 | PASS      |
| 443    | 442     | 15     | 24     | 19.8  | 131856 | PASS      |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/10/2024     | BNA_N            | <u>BN031455.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2954116          | 20.586             |
| DDD           | 40488            | 20.192             |
| DDE           | 1069             | 19.633             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 41557         | 2995673          | 1.39               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051024\  
Data File : BN031455.D  
Acq On : 10 May 2024 07:57  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: May 11 04:09:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 11 04:09:05 2024  
Response via : Initial Calibration

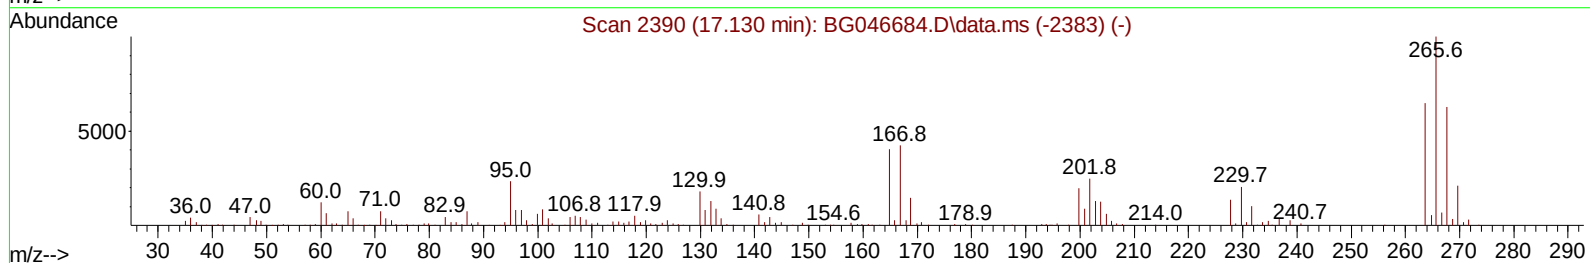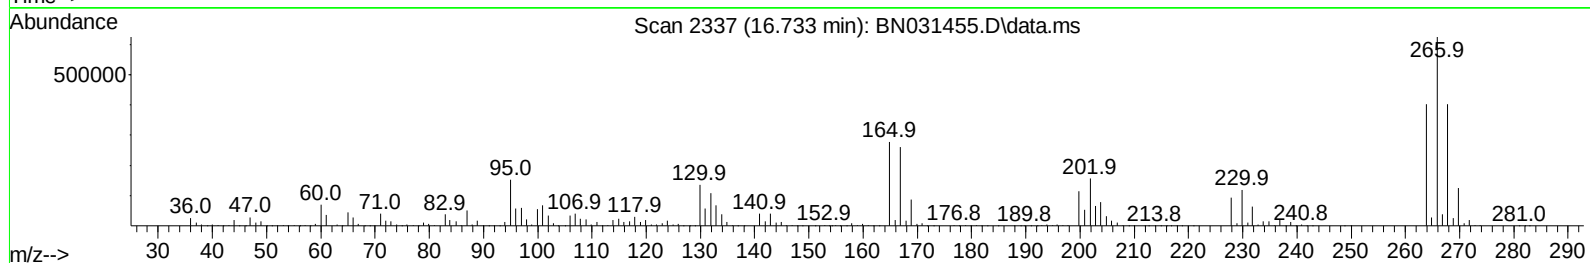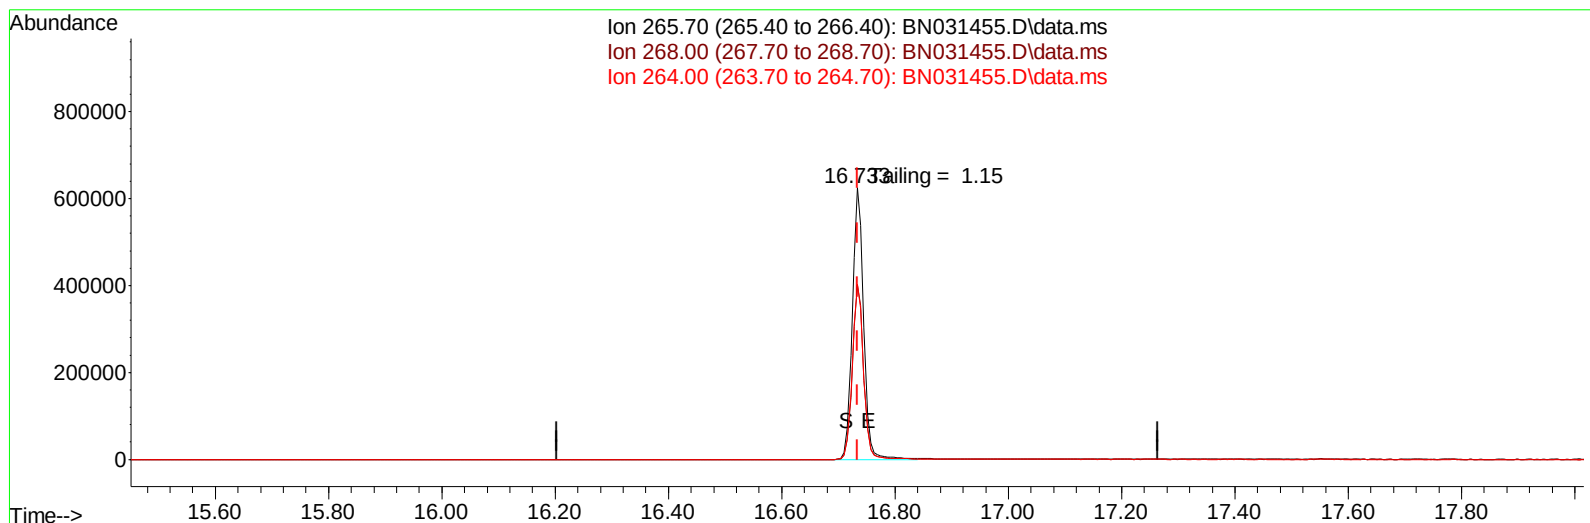

TIC: BN031455.D\data.ms

**(70) Pentachlorophenol (C)**

**16.733min ( 0.000) 21242.53 ng**




**response 882875**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.26  |
| 264.00 | 61.60  | 64.45  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051024\  
Data File : BN031455.D  
Acq On : 10 May 2024 07:57  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: May 11 04:09:10 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 11 04:09:05 2024  
Response via : Initial Calibration

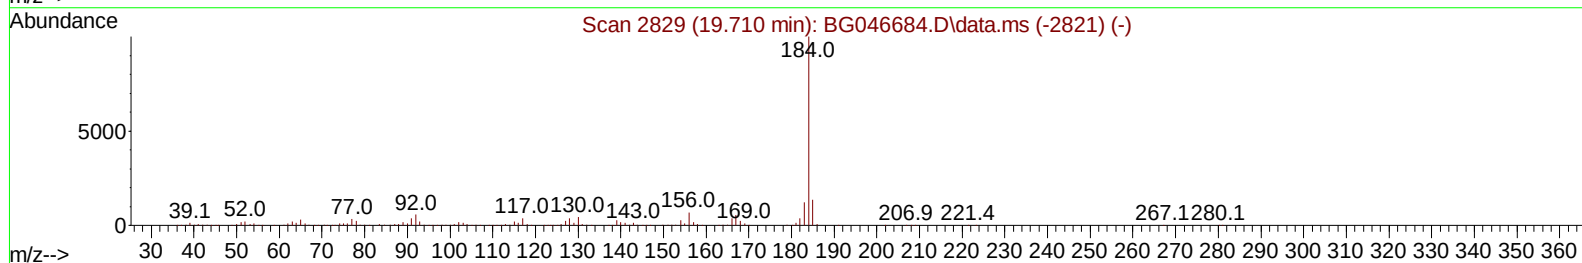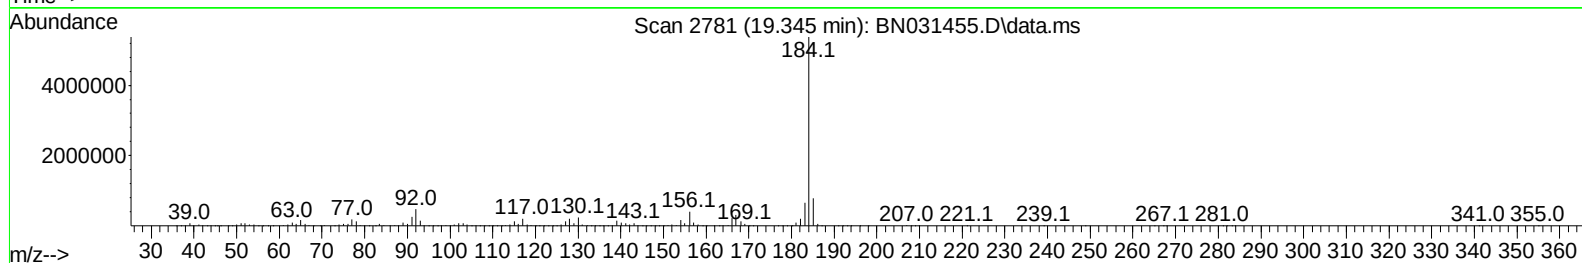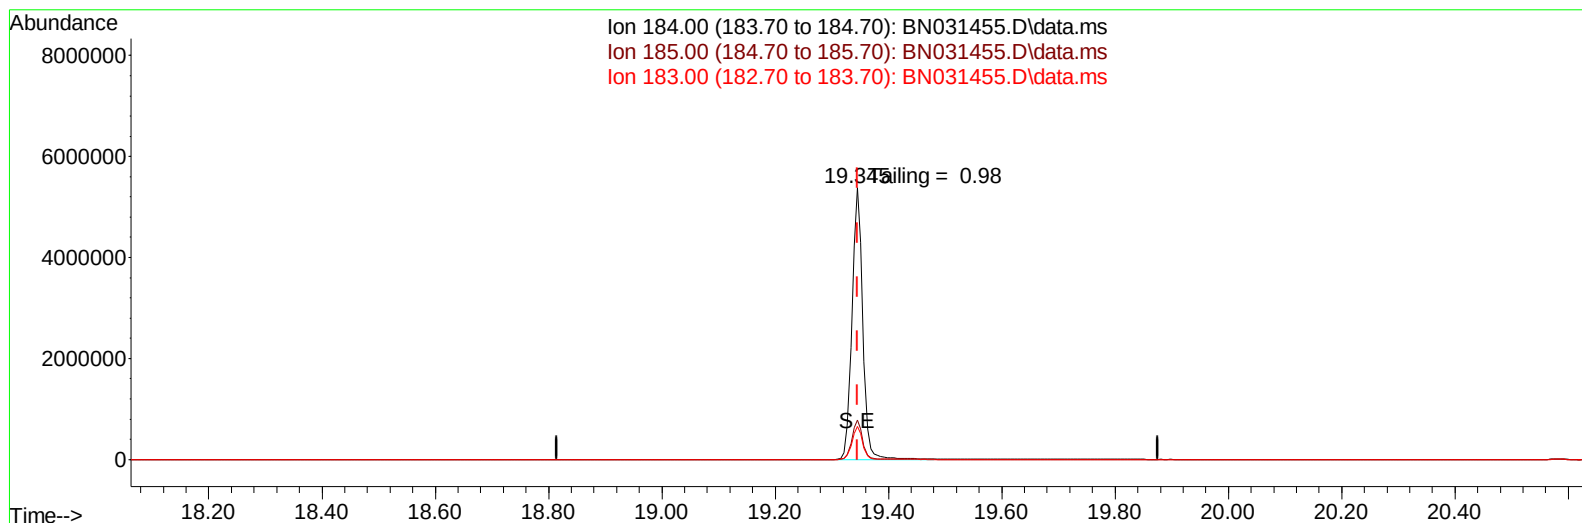

TIC: BN031455.D\data.ms

(77) Benzidine

19.345min ( 0.000) 0.00 ng

response 7193540

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.44  |
| 183.00 | 13.20  | 12.23  |
| 0.00   | 0.00   | 0.00   |