
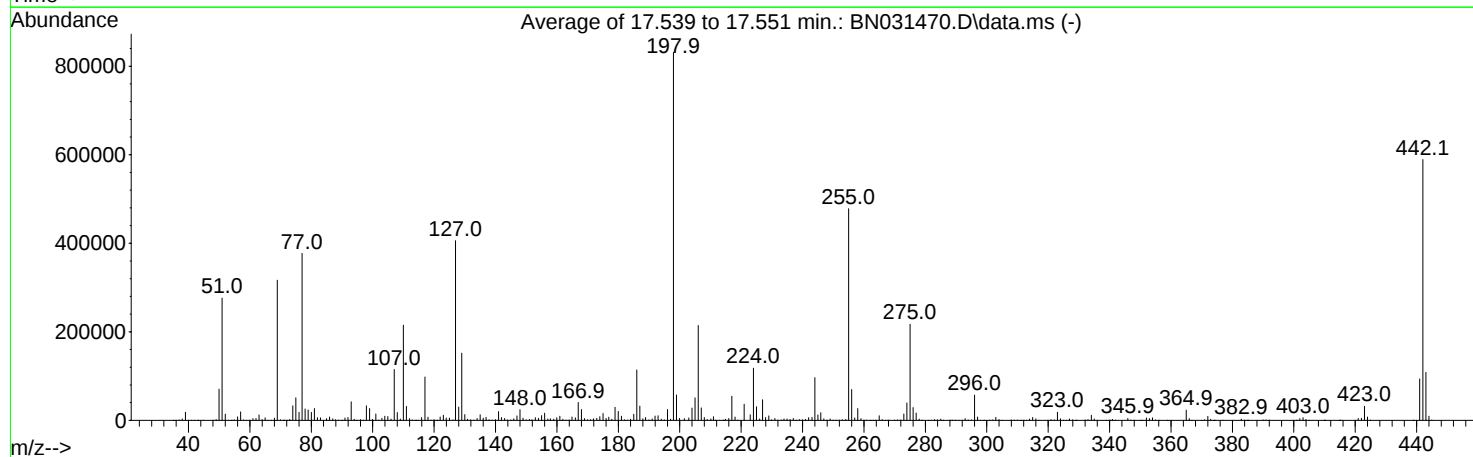


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031470.D
Acq On : 10 May 2024 20:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

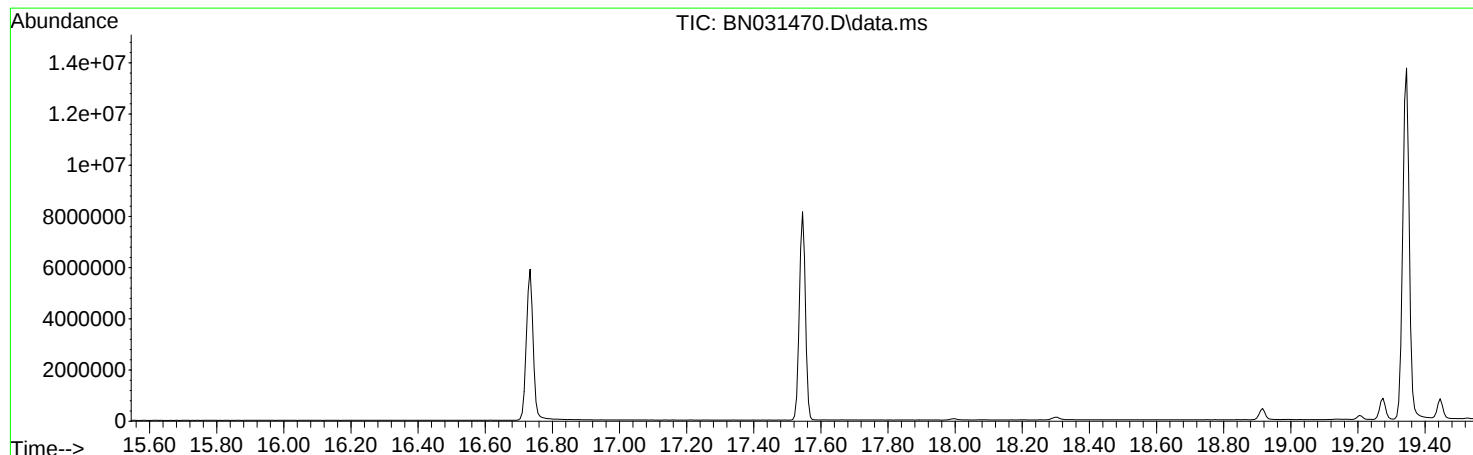

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.2	276192	PASS
68	69	0.00	2	1.6	5118	PASS
69	198	0.00	100	38.1	316730	PASS
70	69	0.00	2	0.5	1510	PASS
127	198	10	80	48.8	405824	PASS
197	198	0.00	2	0.3	2394	PASS
198	198	100	100	100.0	830976	PASS
199	198	5	9	6.9	57531	PASS
275	198	10	60	26.1	217067	PASS
365	198	1	100	2.8	23080	PASS
441	198	0.01	100	11.3	93811	PASS
442	442	50	100	100.0	589248	PASS
443	442	15	24	18.4	108515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/10/2024	BNA_N	<u>BN031470.D</u>
Compound Name	Response	Retention Time
DDT	3267380	20.58
DDD	71241	20.139
DDE	860	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
72101	3339481	2.16

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031470.D
Acq On : 10 May 2024 20:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 11 04:10:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

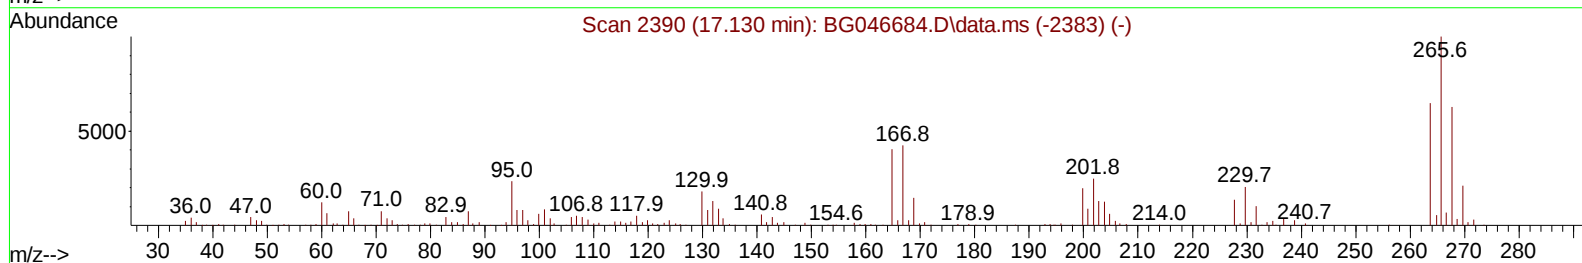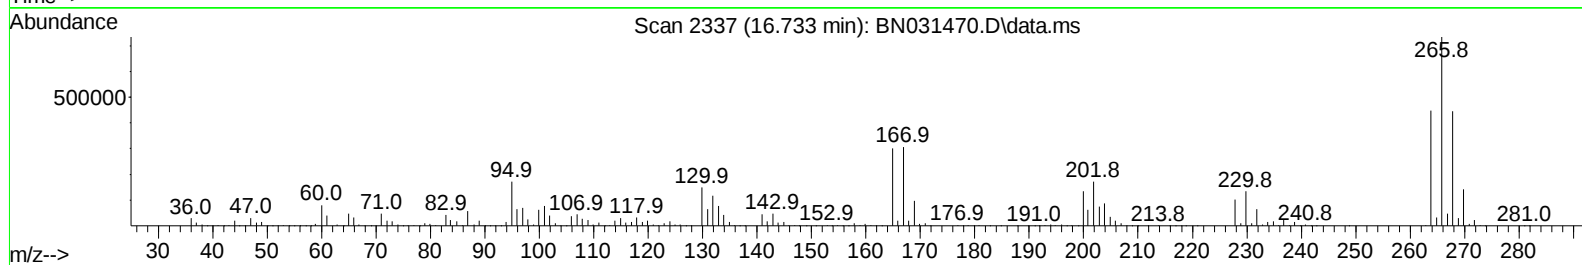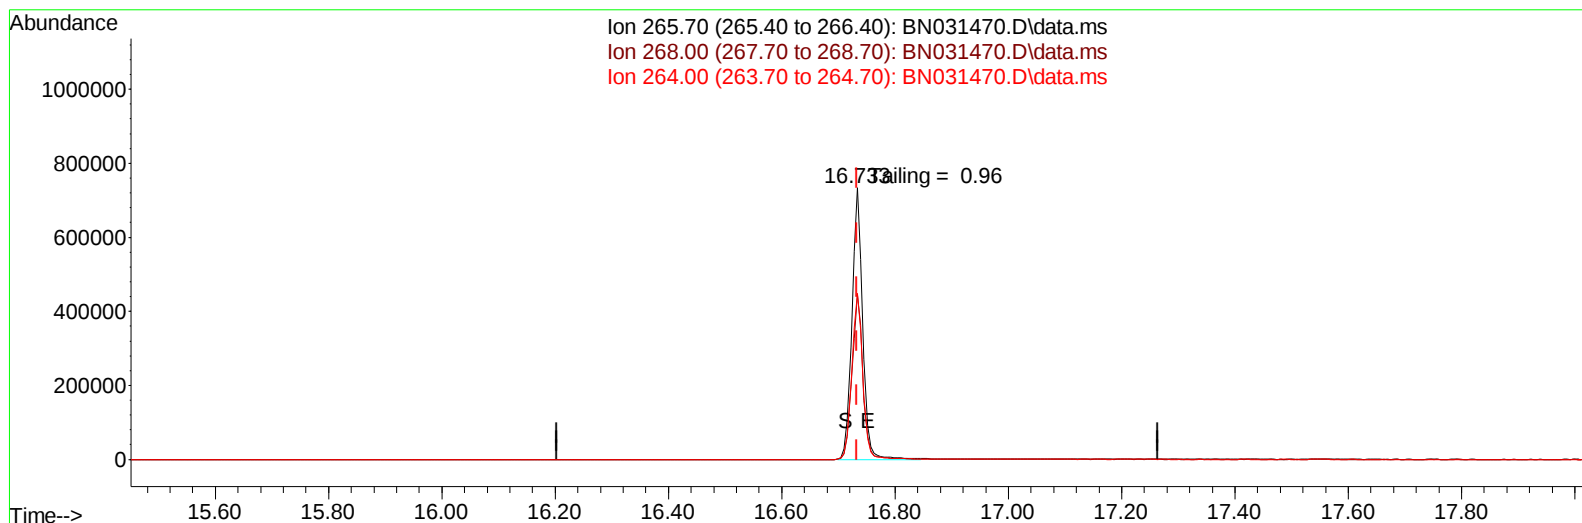

TIC: BN031470.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.000) 25399.82 ng




response 979315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.67
264.00	61.60	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031470.D
Acq On : 10 May 2024 20:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 11 04:10:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

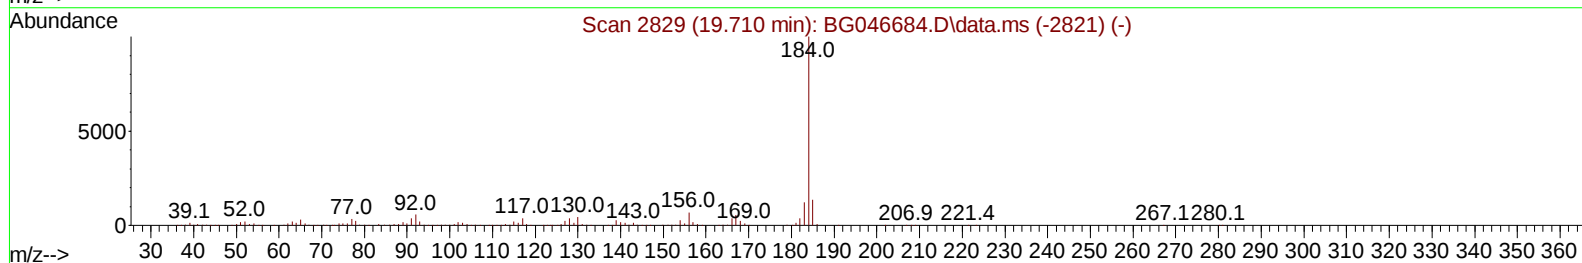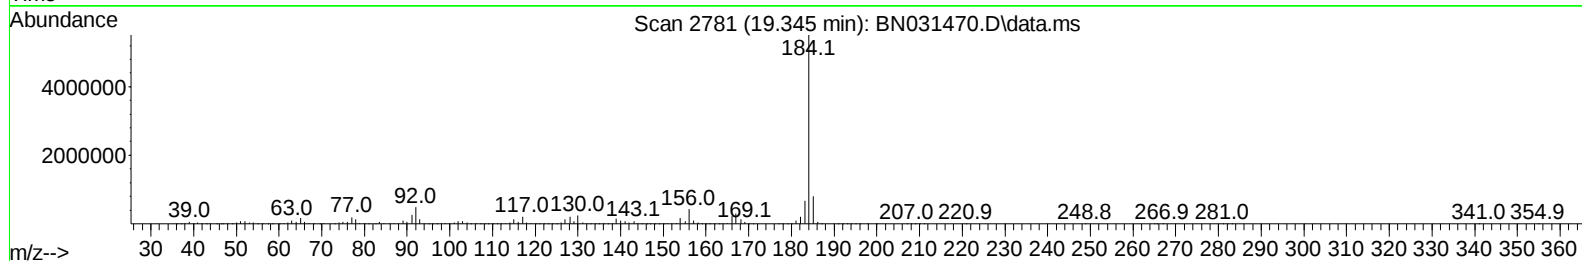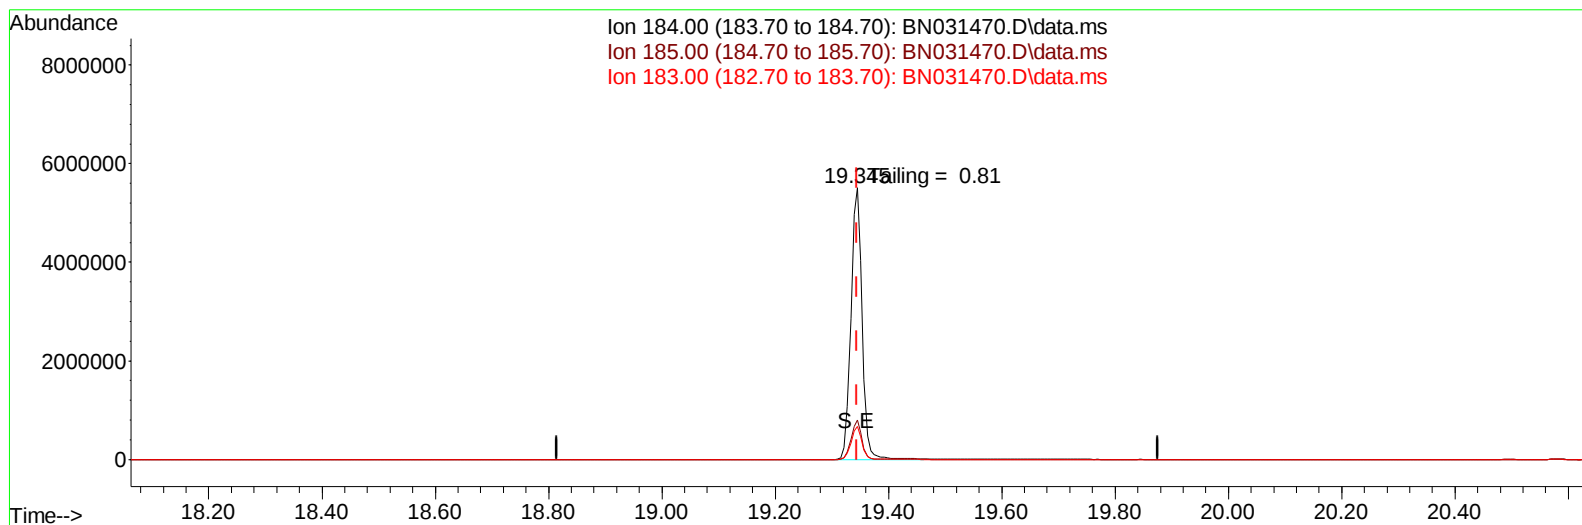

TIC: BN031470.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 0.00 ng

response 7617104

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	12.20
0.00	0.00	0.00