
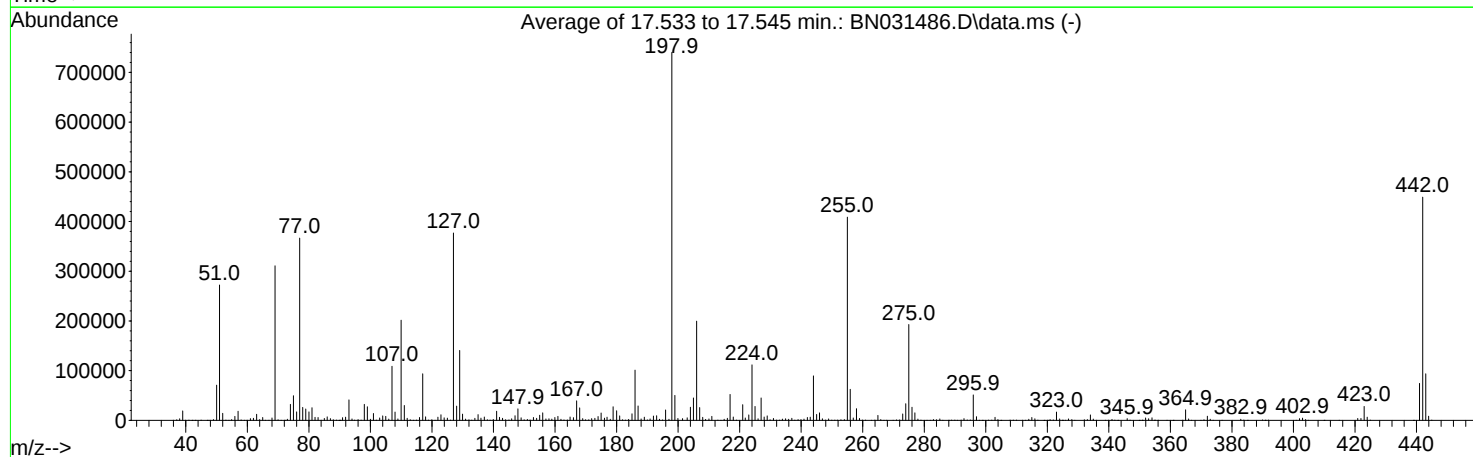


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031486.D
Acq On : 11 May 2024 06:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

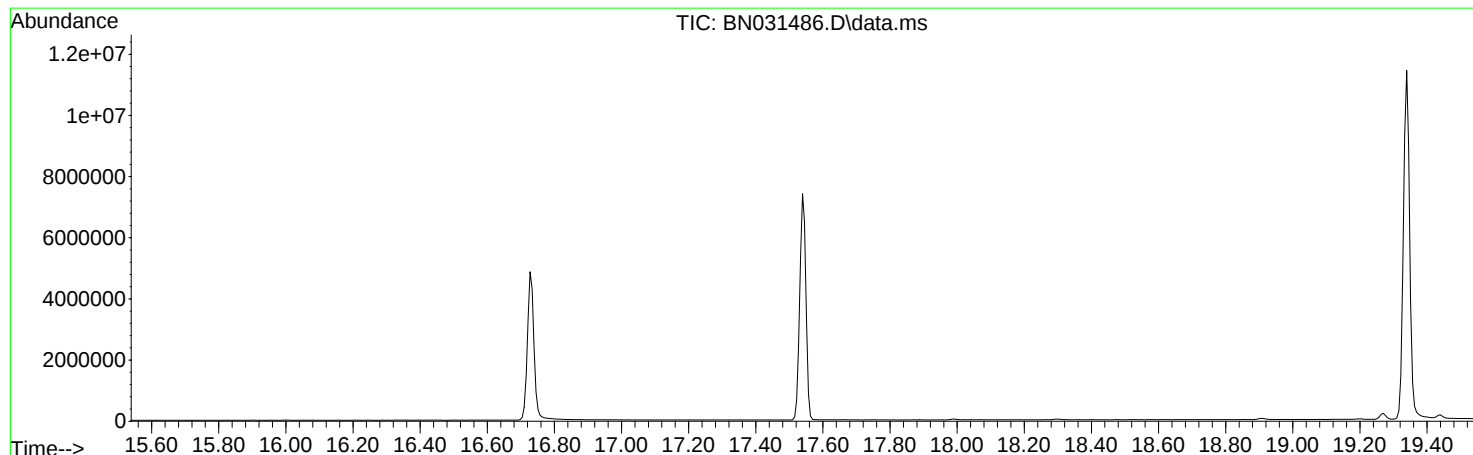

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	36.8	272347	PASS
68	69	0.00	2	1.6	4985	PASS
69	198	0.00	100	42.0	310884	PASS
70	69	0.00	2	0.5	1425	PASS
127	198	10	80	50.9	376917	PASS
197	198	0.00	2	0.3	2359	PASS
198	198	100	100	100.0	739968	PASS
199	198	5	9	6.8	50307	PASS
275	198	10	60	26.1	192981	PASS
365	198	1	100	2.9	21366	PASS
441	198	0.01	100	10.1	74467	PASS
442	442	50	100	100.0	448960	PASS
443	442	15	24	20.8	93576	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/10/2024	BNA_N	<u>BN031486.D</u>
Compound Name	Response	Retention Time
DDT	2684650	20.574
DDD	35983	20.133
DDE	715	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36698	2721348	1.35

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031486.D
Acq On : 11 May 2024 06:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 01:37:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

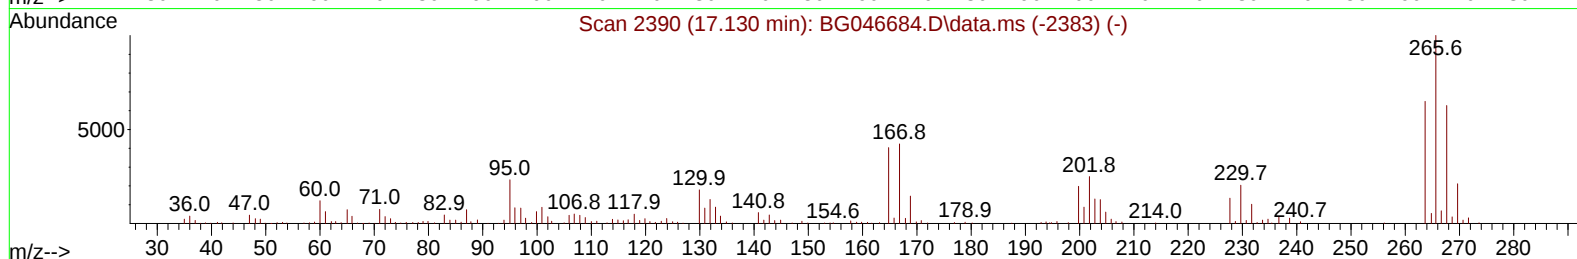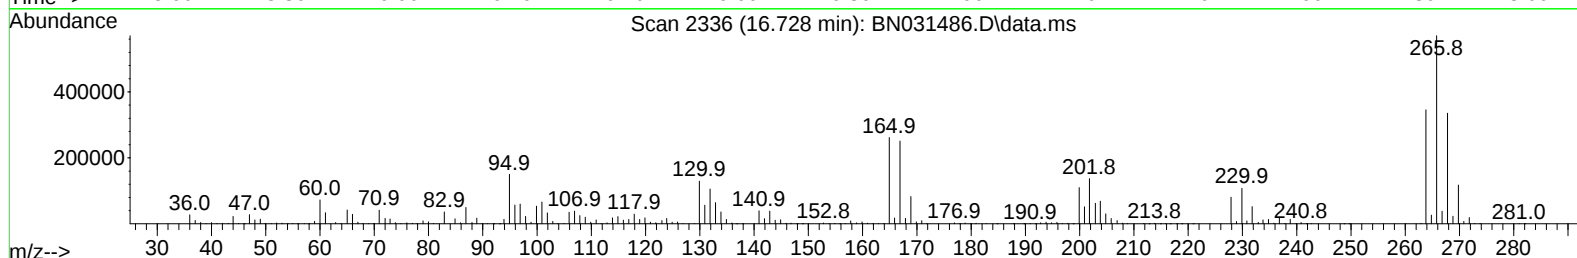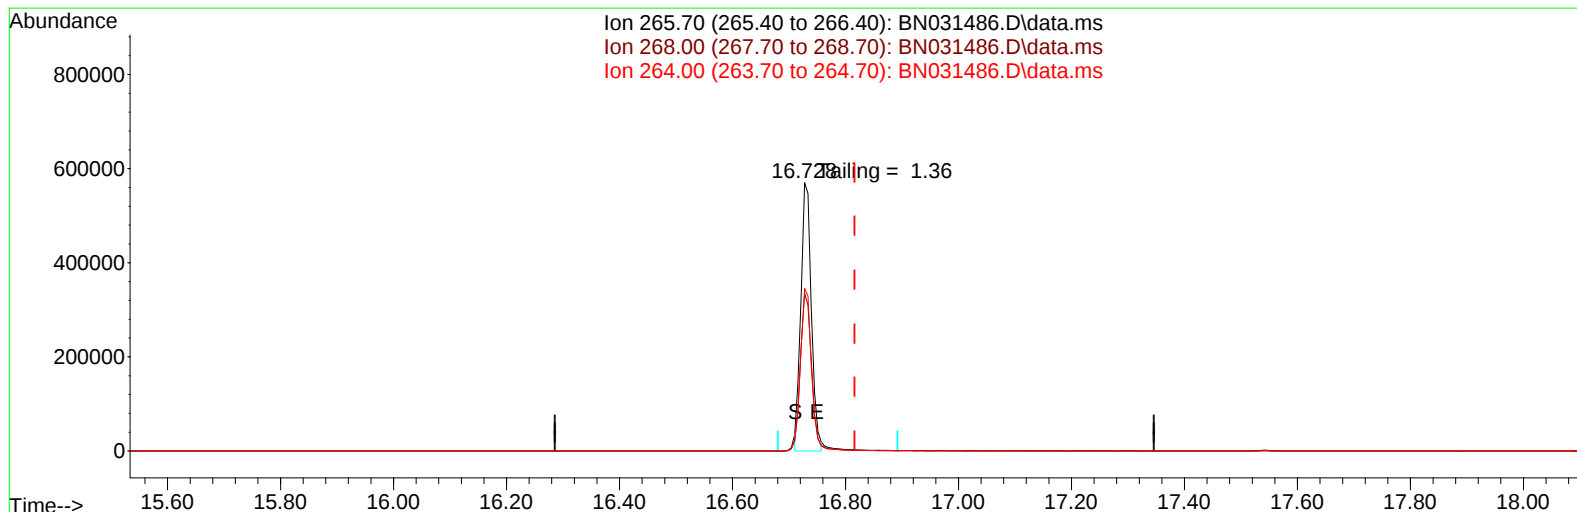

TIC: BN031486.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.088) 22220.06 ng




response 778072

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.81
264.00	61.60	60.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051024\
Data File : BN031486.D
Acq On : 11 May 2024 06:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 01:37:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

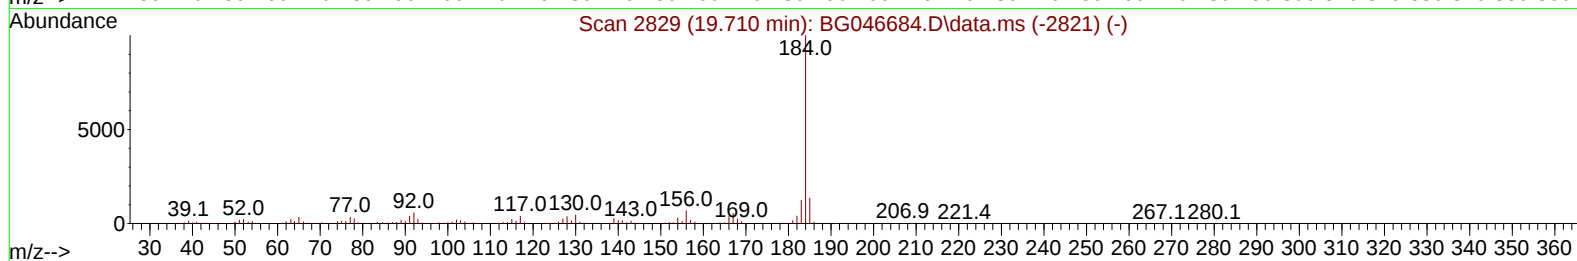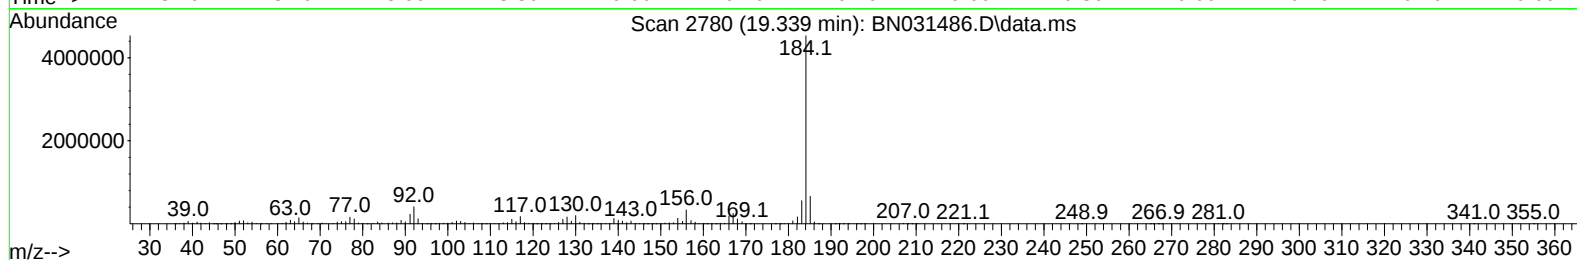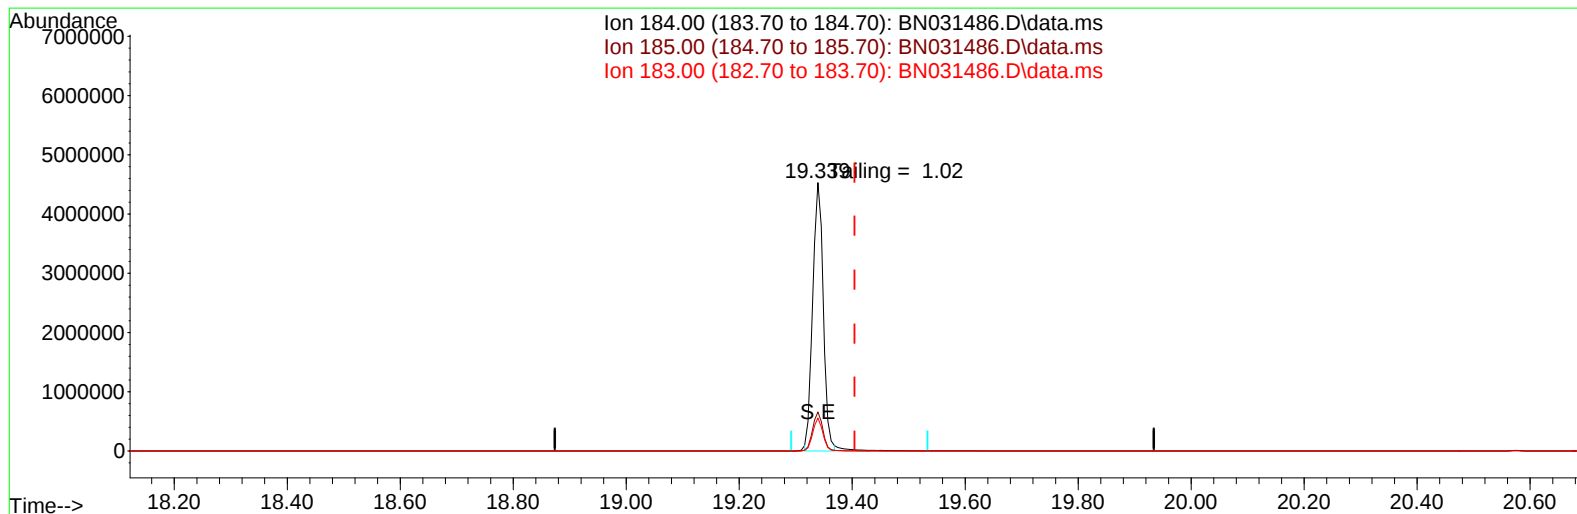

TIC: BN031486.D\data.ms

(77) Benzidine

19.339min (-0.065) 0.00 ng

response 6029877

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.57
183.00	13.20	12.29
0.00	0.00	0.00