
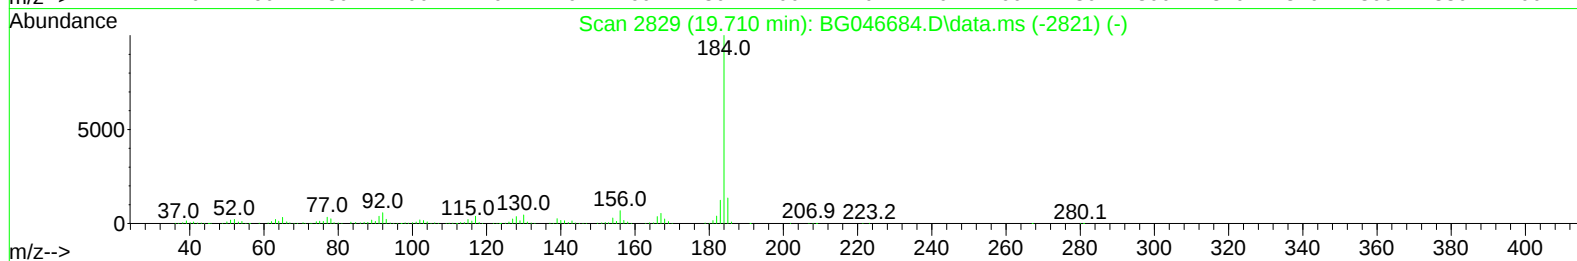
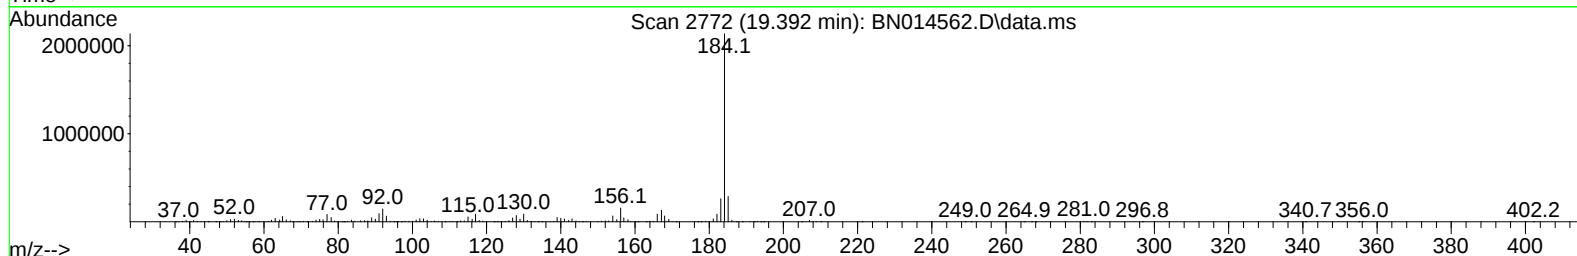


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BP051121\
 Data File : BN014562.D
 Acq On : 11 May 2021 15:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 16:17:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

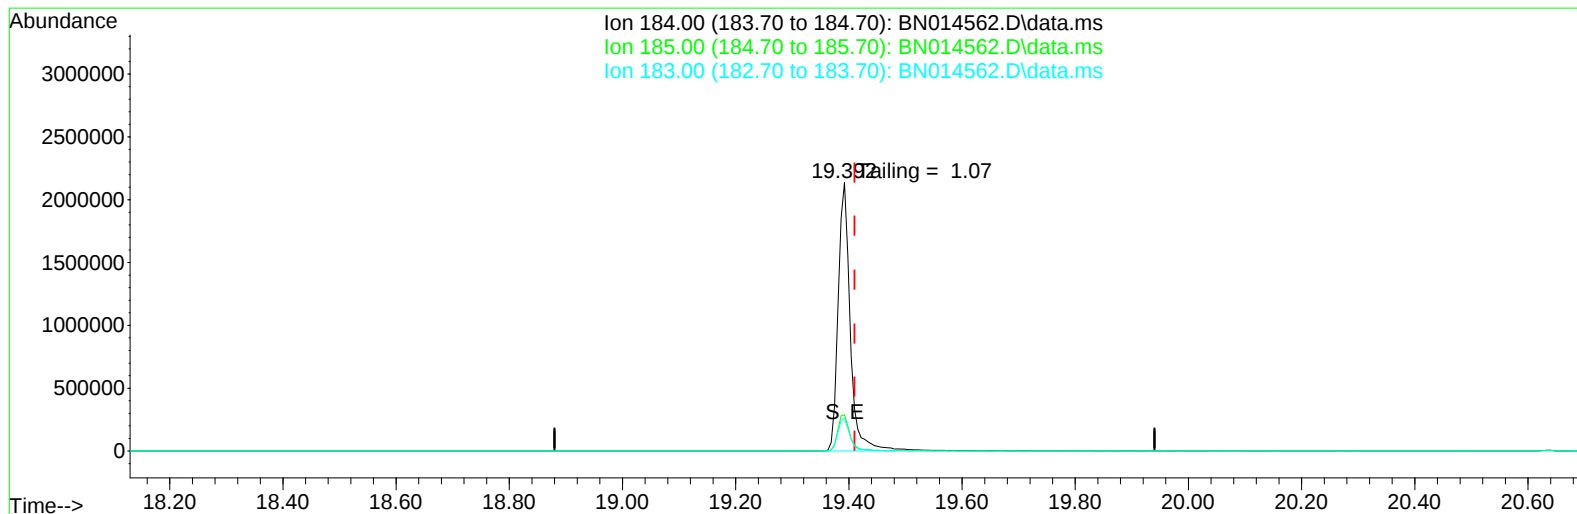




TIC: BN014562.D\data.ms

(77) Benzidine**19.392min (-0.018) 929499.03 ng****response 3180389**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	12.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BP051121\
Data File : BN014562.D
Acq On : 11 May 2021 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 16:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 08 04:11:21 2021
Response via : Initial Calibration

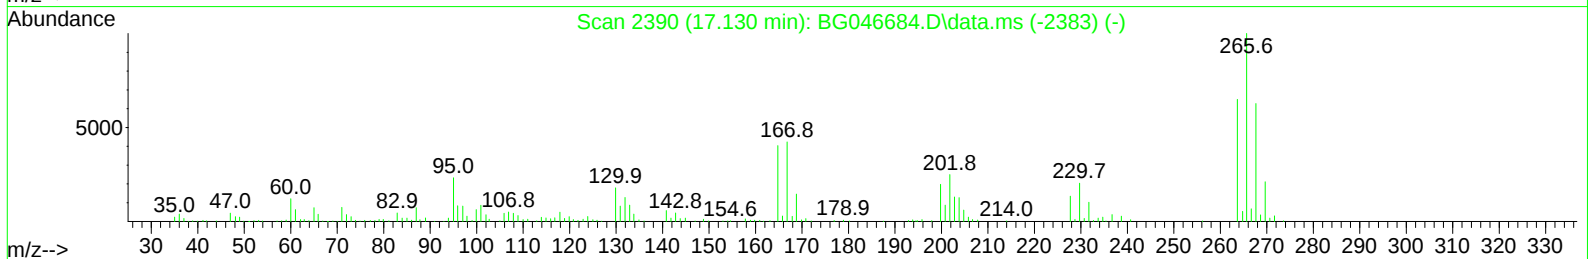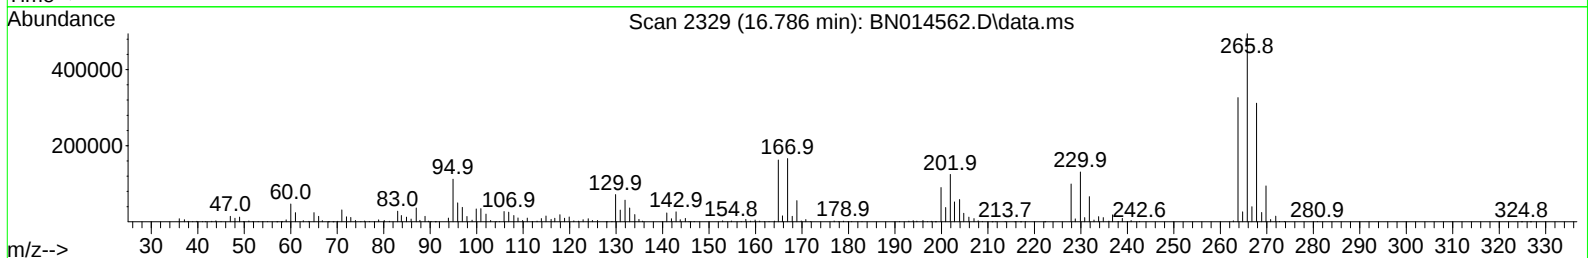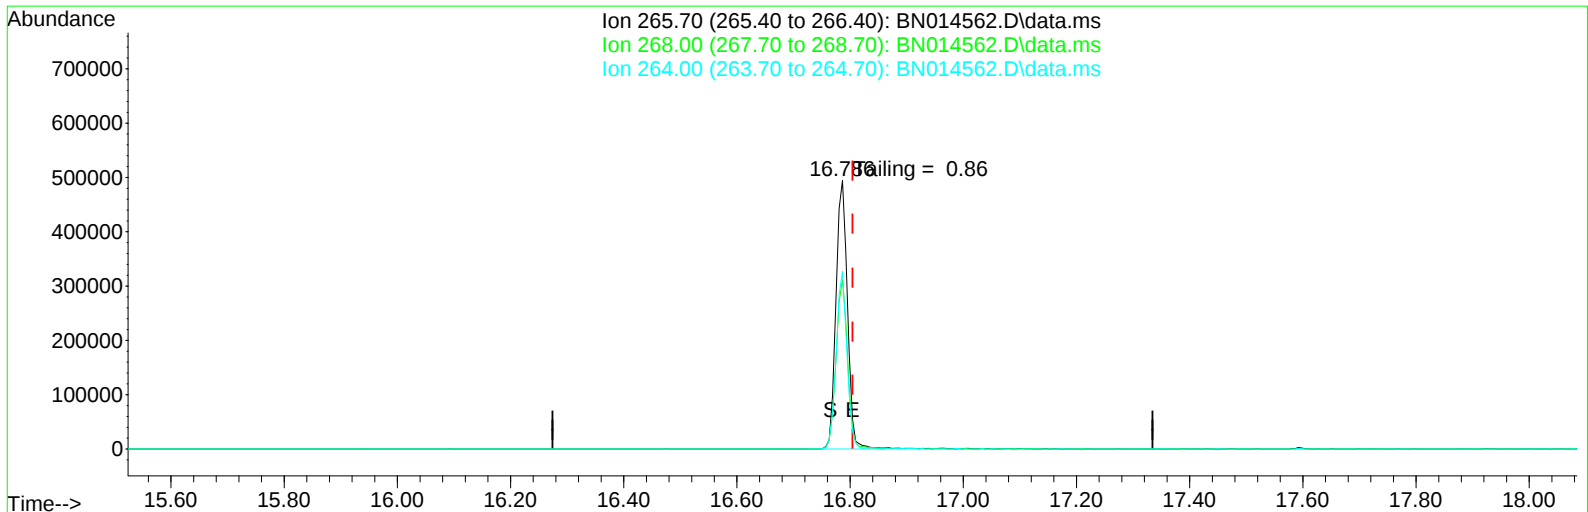

TIC: BN014562.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.018) 22269.12 ng

response 696603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.07
264.00	61.60	66.10
0.00	0.00	0.00