

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051121\
 Data File : BN014569.D
 Acq On : 11 May 2021 19:20
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Manual Integrations
 APPROVED

mohammad
 5/12/2021 2:05:33 PM

Quant Time: May 12 09:39:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 12 09:38:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.741	152	842	0.40	ng	# 0.00
7) Naphthalene-d8	10.530	136	2756	0.40	ng	# 0.00
13) Acenaphthene-d10	14.384	164	2058	0.40	ng	0.00
19) Phenanthrene-d10	17.140	188	4754	0.40	ng	0.01
29) Chrysene-d12	21.332	240	6608	0.40	ng	0.00
35) Perylene-d12	23.603	264	5951	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.333	112	9685	4.35	ng	0.00
5) Phenol-d6	6.903	99	13735	4.62	ng	0.00
8) Nitrobenzene-d5	8.883	82	12236	5.14	ng	0.00
11) 2-Methylnaphthalene-d10	12.120	152	33394	4.98	ng	0.00
14) 2,4,6-Tribromophenol	15.882	330	5230	5.47	ng	0.00
15) 2-Fluorobiphenyl	13.001	172	35669	4.73	ng	0.00
27) Fluoranthene-d10	19.171	212	107653	5.08	ng	0.00
31) Terphenyl-d14	19.776	244	74489	4.78	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.295	88	4554	3.55	ng	96
3) n-Nitrosodimethylamine	3.609	42	1929m	4.56	ng	
6) bis(2-Chloroethyl)ether	7.169	93	11459	4.66	ng	91
9) Naphthalene	10.568	128	35718	4.91	ng	98
10) Hexachlorobutadiene	10.873	225	8556	4.88	ng	# 100
12) 2-Methylnaphthalene	12.195	142	26469	5.00	ng	# 92
16) Acenaphthylene	14.105	152	40993	5.41	ng	99
17) Acenaphthene	14.448	154	28277	5.05	ng	95
18) Fluorene	15.437	166	36885	4.89	ng	100
21) 4-Bromophenyl-phenylether	16.337	248	14842	5.10	ng	# 91
22) Hexachlorobenzene	16.446	284	15244	4.94	ng	92
23) Atrazine	16.605	200	10575	5.71	ng	92
24) Pentachlorophenol	16.787	266	5909	5.76	ng	# 42
25) Phenanthrene	17.177	178	63666	4.88	ng	99
26) Anthracene	17.262	178	58870	5.37	ng	100
28) Fluoranthene	19.201	202	86967	5.03	ng	98
30) Pyrene	19.563	202	87420	4.82	ng	99
32) Benzo(a)anthracene	21.311	228	96563	5.03	ng	99
33) Chrysene	21.364	228	97673	4.86	ng	100
34) Bis(2-ethylhexyl)phtha...	21.258	149	28910	5.42	ng	# 79
36) Indeno(1,2,3-cd)pyrene	25.903	276	122503	5.12	ng	# 90
37) Benzo(b)fluoranthene	22.922	252	103739	5.11	ng	# 91
38) Benzo(k)fluoranthene	22.963	252	104803	4.98	ng	# 92
39) Benzo(a)pyrene	23.504	252	90564	5.28	ng	# 83
40) Dibenzo(a,h)anthracene	25.920	278	104783	5.12	ng	# 90
41) Benzo(g,h,i)perylene	26.598	276	99977	5.13	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051121\
Data File : BN014569.D
Acq On : 11 May 2021 19:20
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:33 PM


Quant Time: May 12 09:39:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 12 09:38:59 2021
Response via : Initial Calibration

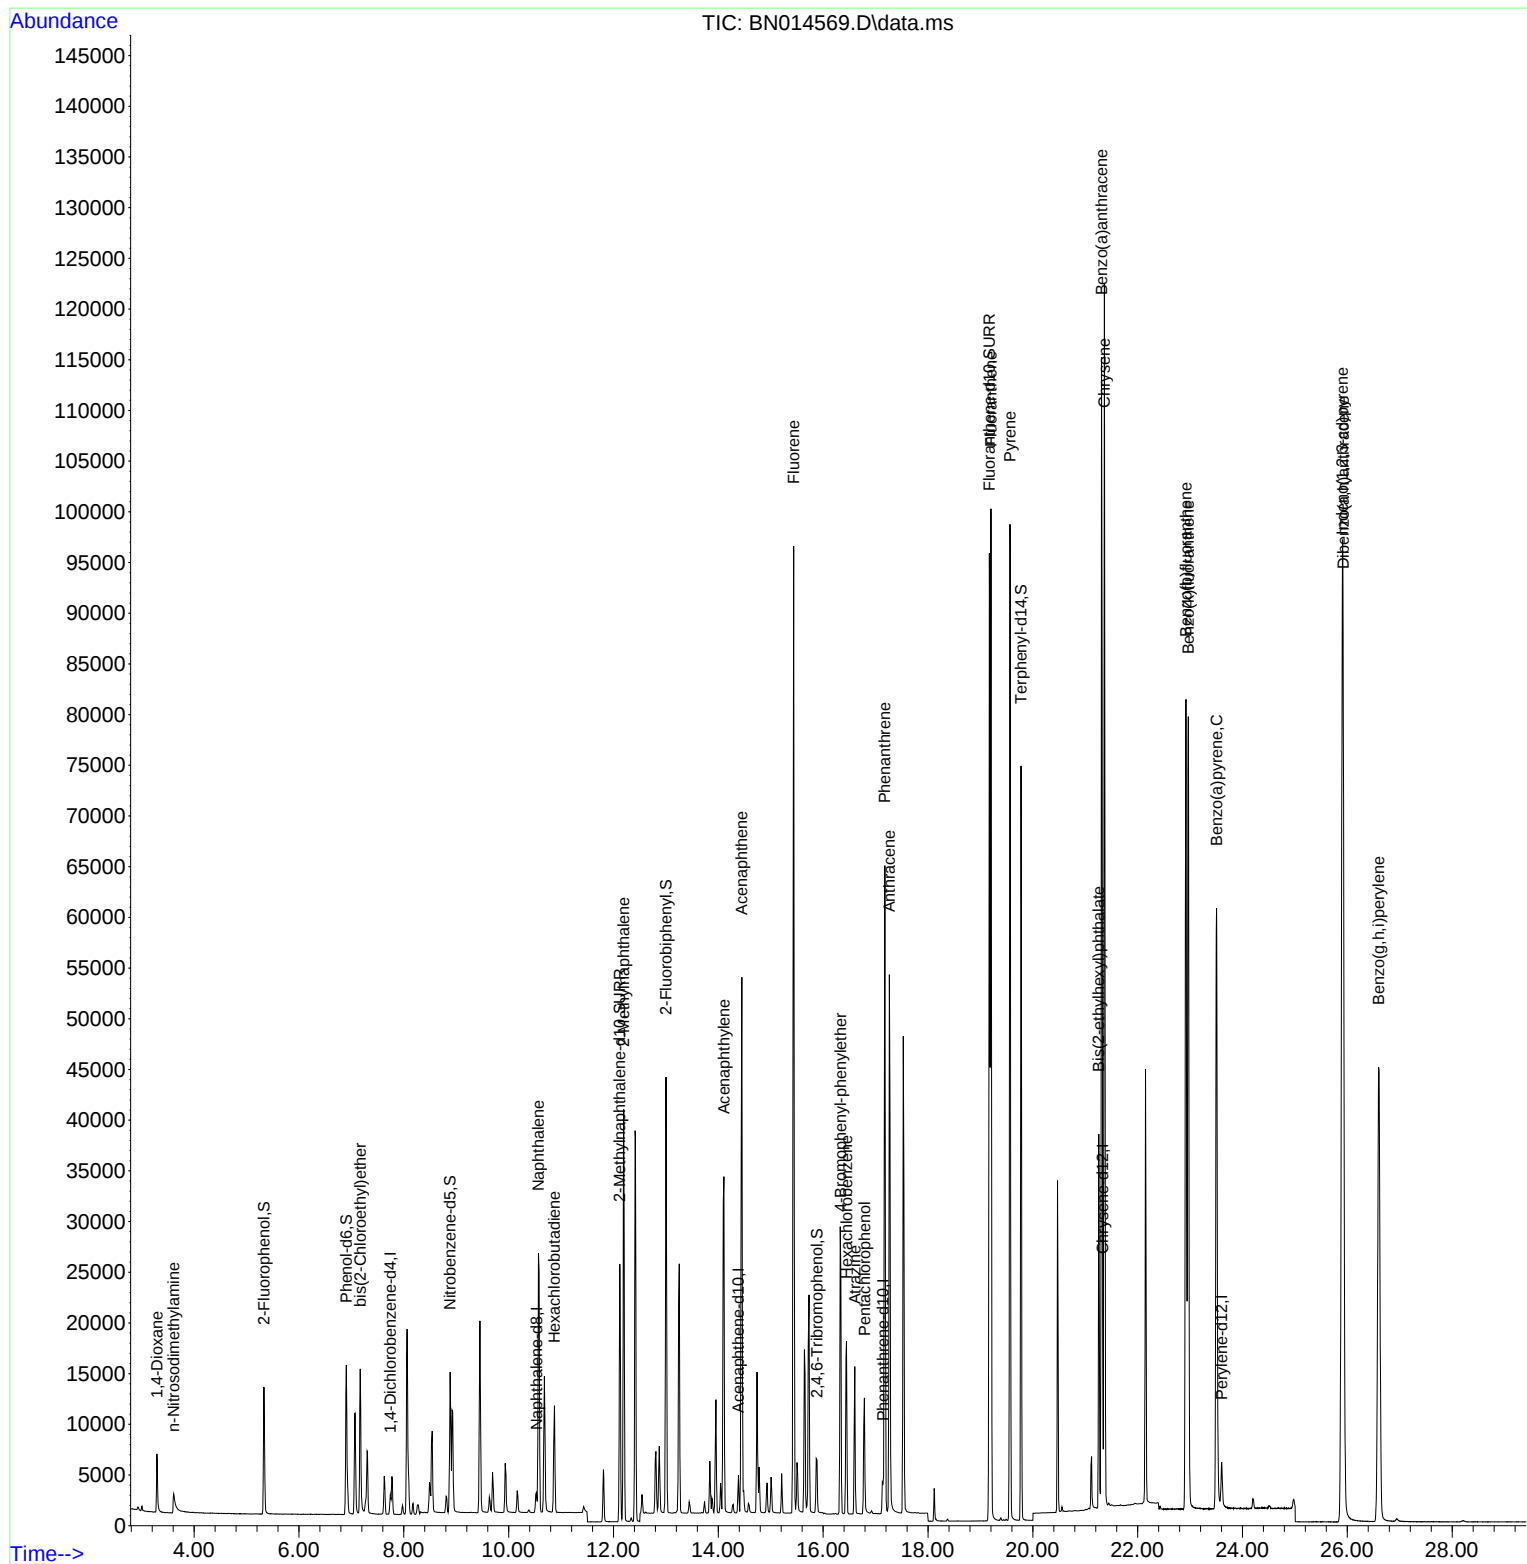



#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.741 min Scan# 616
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20




Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Tgt Ion:152 Resp: 842
Ion Ratio Lower Upper
152 100
150 154.2 123.8 185.8
115 83.1 47.0 70.4#

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:33 PM

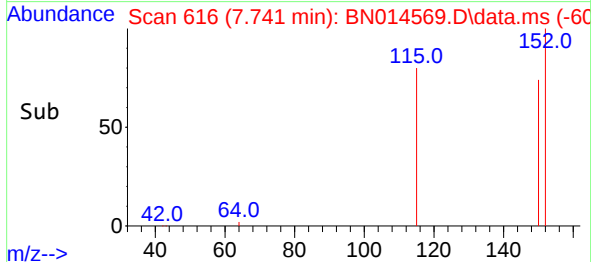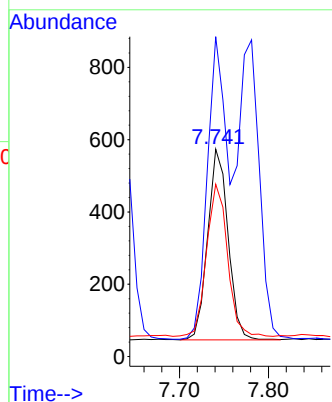


#2
1,4-Dioxane
Concen: 3.55 ng
RT: 3.295 min Scan# 64
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

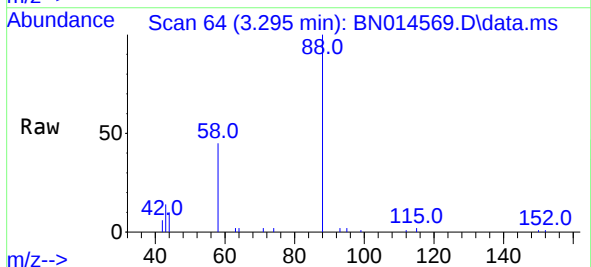

Tgt Ion: 88 Resp: 4554
Ion Ratio Lower Upper
88 100
58 57.6 44.4 66.6
43 16.6 15.9 23.9

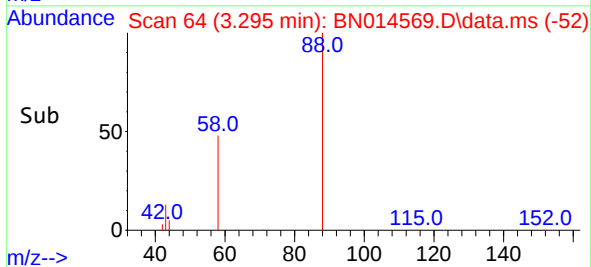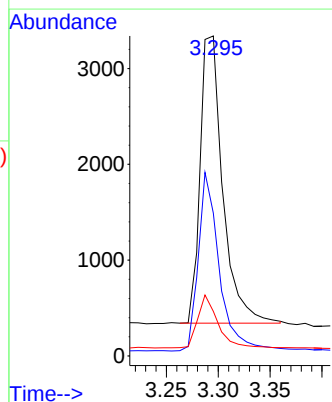







#3
n-Nitrosodimethylamine
Concen: 4.56 ng m
RT: 3.609 min Scan# 103
Delta R.T. -0.161 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 42 Resp: 1929
Ion Ratio Lower Upper
42 100
74 0.0 175.1 262.7#
44 0.0 7.5 11.3#

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM



#4
2-Fluorophenol
Concen: 4.35 ng
RT: 5.333 min Scan# 317
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 112 Resp: 9685
Ion Ratio Lower Upper
112 100
64 57.0 41.8 62.6
63 29.8 22.0 33.0

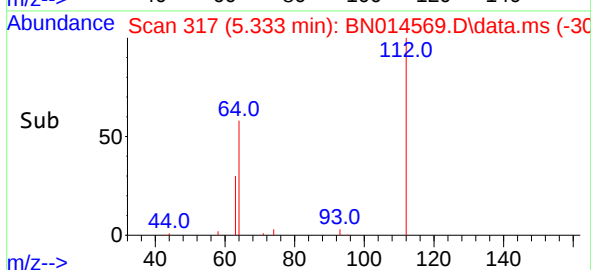







#5
Phenol-d6
Concen: 4.62 ng
RT: 6.903 min Scan# 512
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 99 Resp: 13735
Ion Ratio Lower Upper
99 100
42 11.4 13.2 19.8#
71 41.6 26.2 39.2#

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

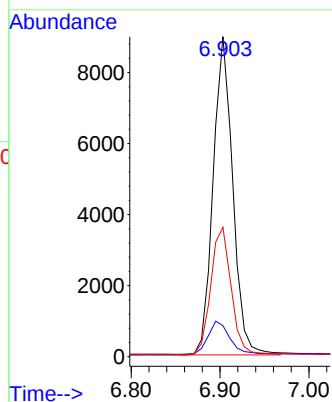

#6
bis(2-Chloroethyl)ether
Concen: 4.66 ng
RT: 7.169 min Scan# 545
Delta R.T. -0.008 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 93 Resp: 11459
Ion Ratio Lower Upper
93 100
63 62.2 58.0 87.0
95 33.0 27.0 40.6

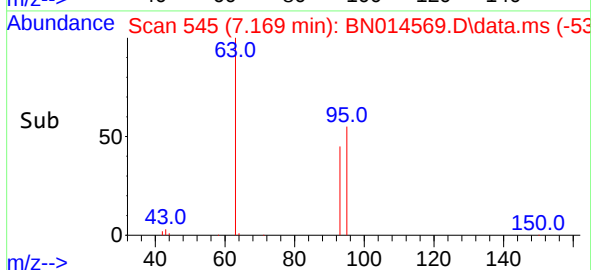

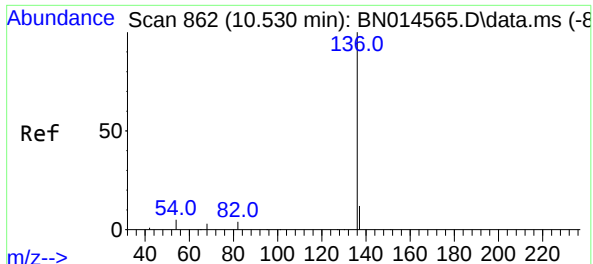





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.530 min Scan# 862
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	136	Resp:	2756
Ion	Ratio	Lower	Upper
136	100		
137	13.3	8.9	13.3#
54	7.3	3.8	5.8#
68	7.4	3.8	5.6#




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

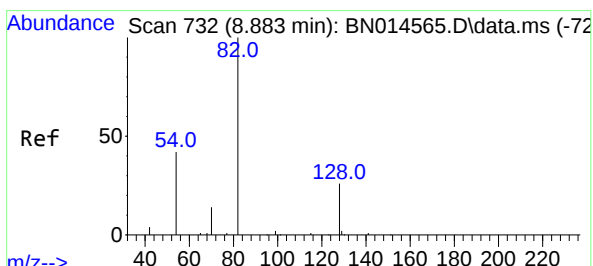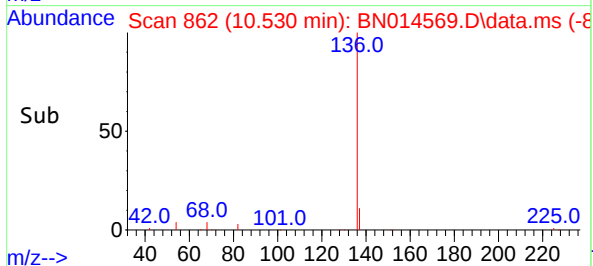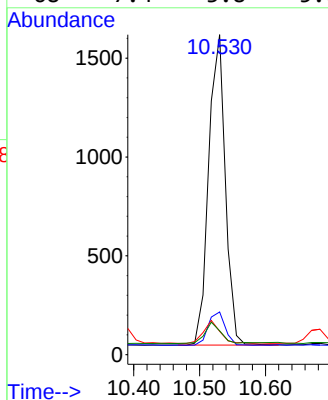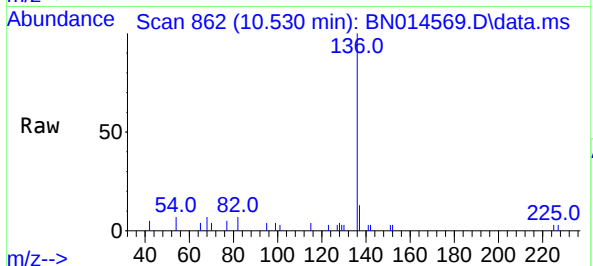

#8
Nitrobenzene-d5
Concen: 5.14 ng
RT: 8.883 min Scan# 732
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	82	Resp:	12236
Ion	Ratio	Lower	Upper
82	100		
128	28.6	29.5	44.3#
54	39.3	36.9	55.3

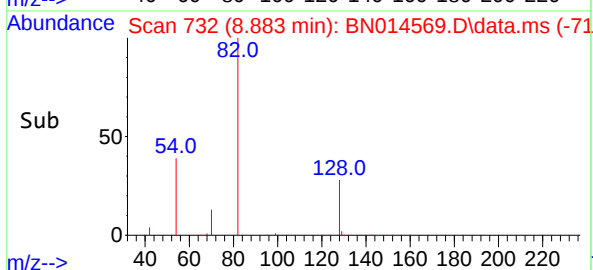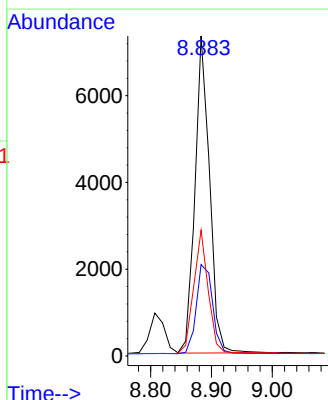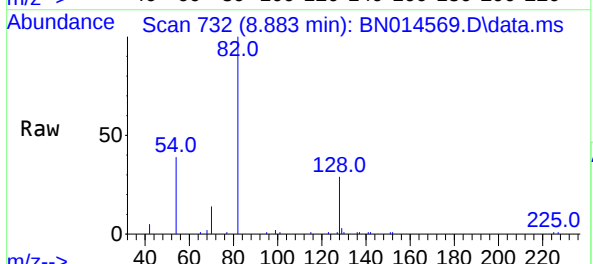

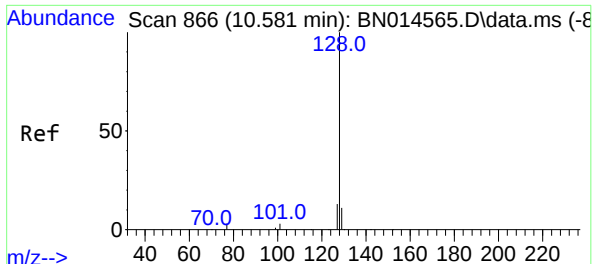





#9
Naphthalene
Concen: 4.91 ng
RT: 10.568 min Scan# 865
Delta R.T. -0.013 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	128	Resp:	35718
Ion Ratio	Lower	Upper	
128	100		
129	11.0	9.0	13.4
127	14.3	10.4	15.6

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

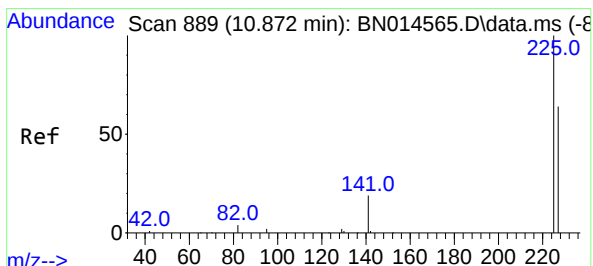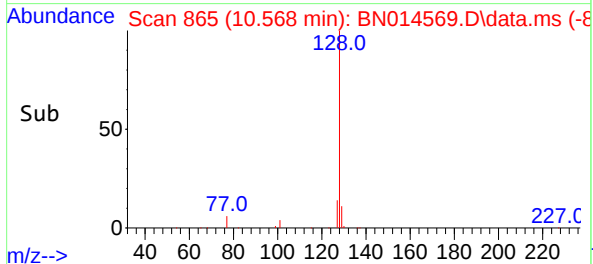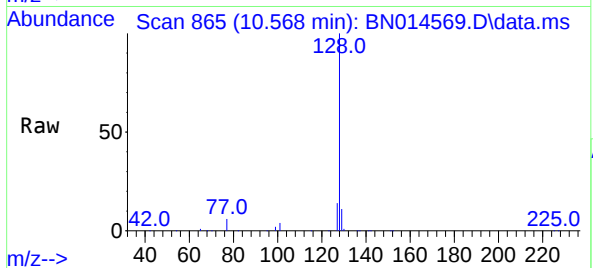

#10
Hexachlorobutadiene
Concen: 4.88 ng
RT: 10.873 min Scan# 889
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	225	Resp:	8556
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.9	50.9	76.3

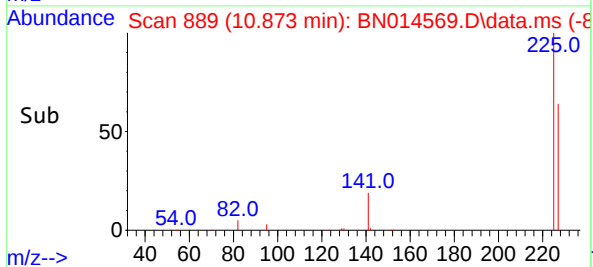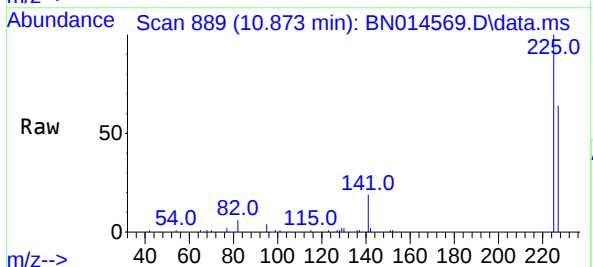







#11
2-Methylnaphthalene-d10
Concen: 4.98 ng
RT: 12.120 min Scan# 1077
Delta R.T. -0.004 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:152 Resp: 33394
Ion Ratio Lower Upper
152 100
151 20.6 16.2 24.2

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM




#12
2-Methylnaphthalene
Concen: 5.00 ng
RT: 12.195 min Scan# 1094
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:142 Resp: 26469
Ion Ratio Lower Upper
142 100
141 89.5 70.2 105.4
115 46.7 26.7 40.1#

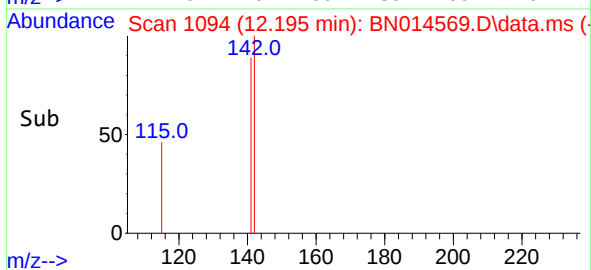







#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.384 min Scan# 1312
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20





Tgt Ion:164 Resp: 2058
Ion Ratio Lower Upper
164 100
162 101.4 78.6 118.0
160 46.0 35.8 53.8

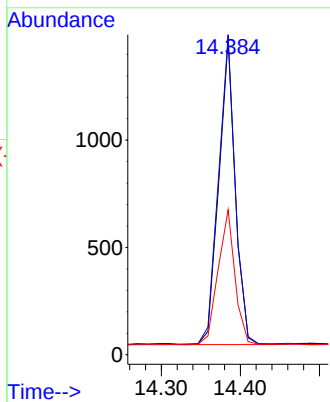

#14
2,4,6-Tribromophenol
Concen: 5.47 ng
RT: 15.882 min Scan# 1430
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

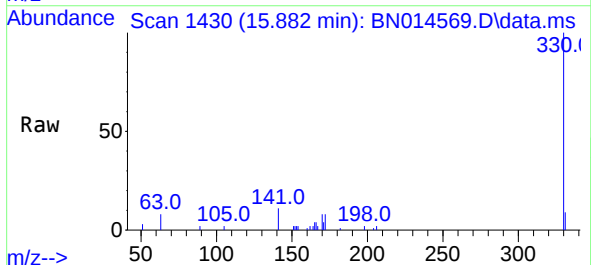


Tgt Ion:330 Resp: 5230
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 27.9 27.0 40.4

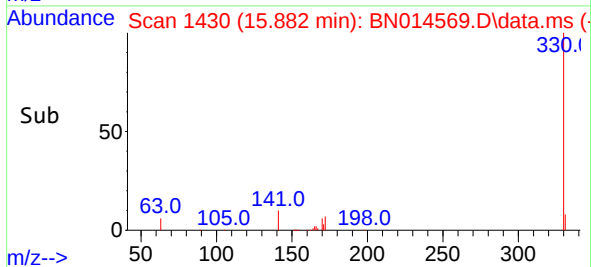

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:33 PM

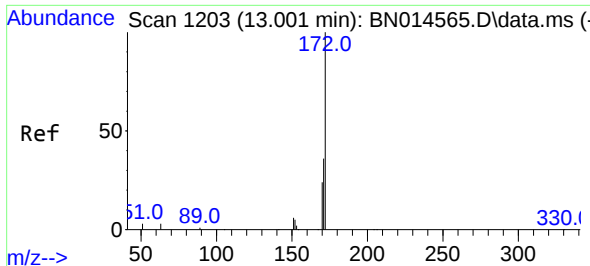





#15
2-Fluorobiphenyl
Concen: 4.73 ng
RT: 13.001 min Scan# 1203
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:172 Resp: 35669
Ion Ratio Lower Upper
172 100
171 36.6 27.1 40.7
170 24.3 18.3 27.5

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

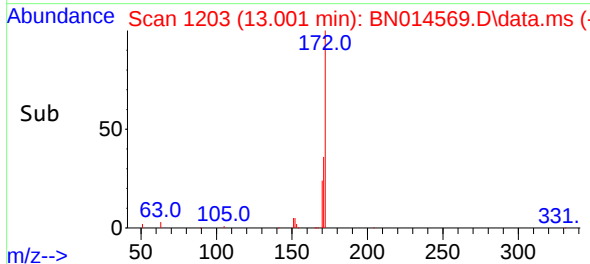


#16
Acenaphthylene
Concen: 5.41 ng
RT: 14.105 min Scan# 1290
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:152 Resp: 40993
Ion Ratio Lower Upper
152 100
151 20.4 15.6 23.4
153 13.1 10.5 15.7

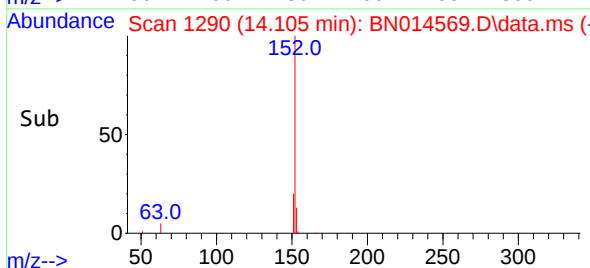
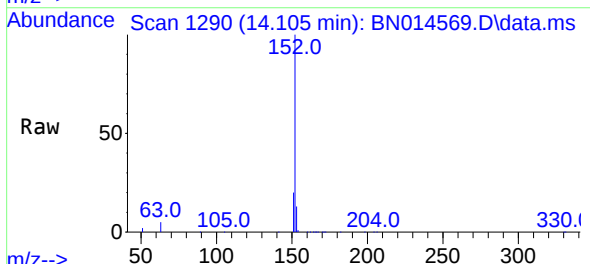


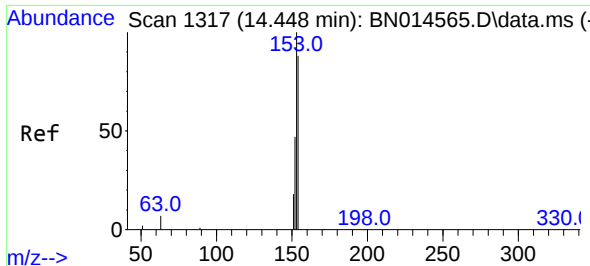

#17
Acenaphthene
Concen: 5.05 ng
RT: 14.448 min Scan# 1317
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20




Tgt Ion:154 Resp: 28277
Ion Ratio Lower Upper
154 100
153 107.9 90.2 135.4
152 52.3 46.2 69.2

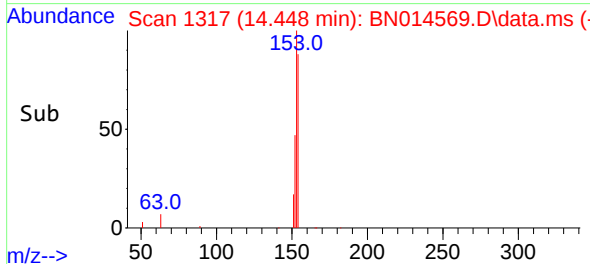


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:33 PM




#18
Fluorene
Concen: 4.89 ng
RT: 15.437 min Scan# 1395
Delta R.T. 0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

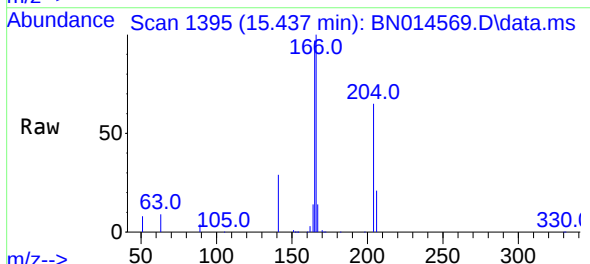


Tgt Ion:166 Resp: 36885
Ion Ratio Lower Upper
166 100
165 98.0 78.4 117.6
167 13.5 10.7 16.1



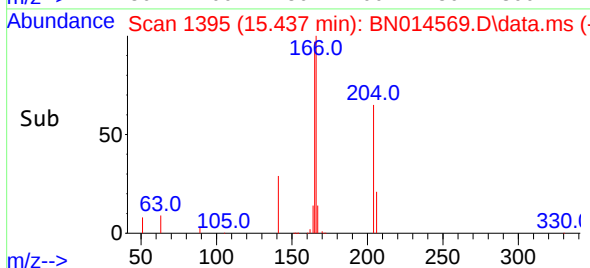





#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.140 min Scan# 1533
Delta R.T. 0.012 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20





Tgt Ion:188 Resp: 4754
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.5 5.2 7.8

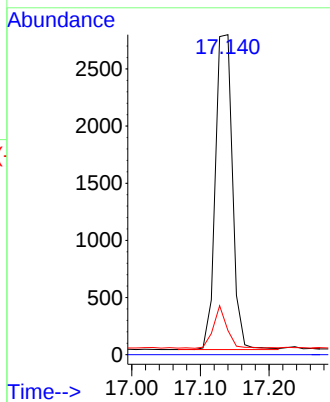

#21
4-Bromophenyl-phenylether
Concen: 5.10 ng
RT: 16.337 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

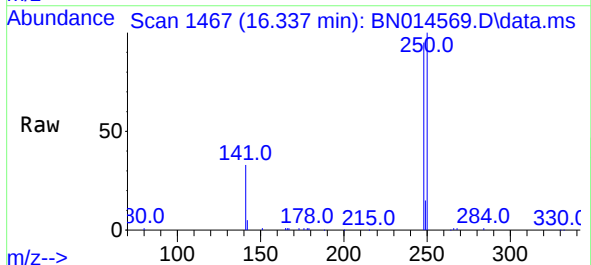


Tgt Ion:248 Resp: 14842
Ion Ratio Lower Upper
248 100
250 105.6 80.5 120.7
141 34.4 37.2 55.8#

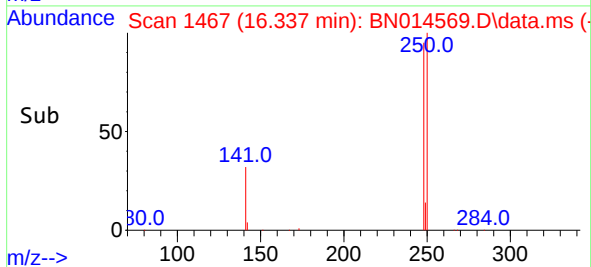


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:33 PM



#22
Hexachlorobenzene
Concen: 4.94 ng
RT: 16.446 min Scan# 1476
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

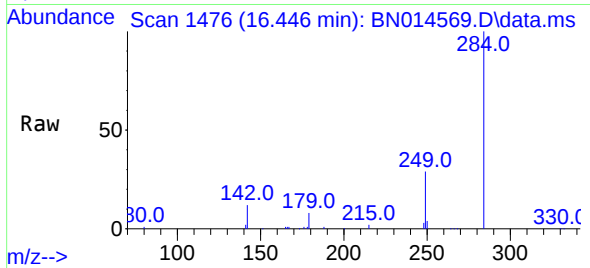


Tgt Ion:284 Resp: 15244
Ion Ratio Lower Upper
284 100
142 27.9 26.6 39.8
249 32.9 23.6 35.4

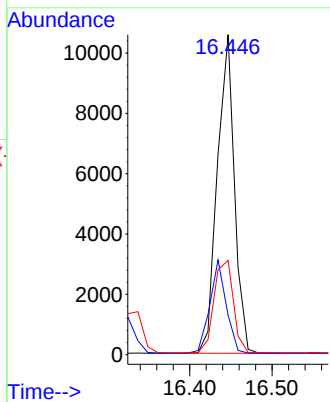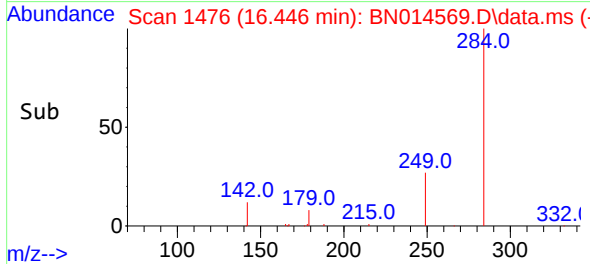


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:33 PM

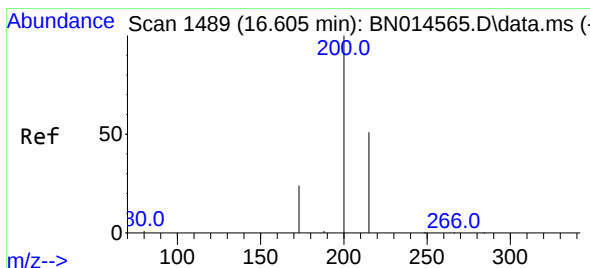


#23
Atrazine
Concen: 5.71 ng
RT: 16.605 min Scan# 1489
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

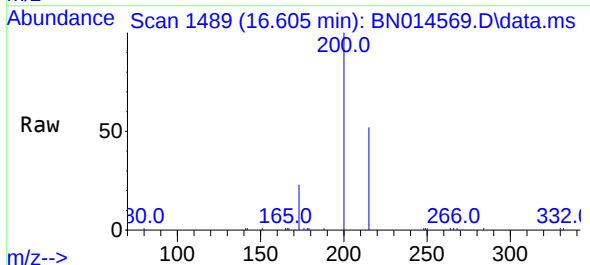

Tgt Ion:200 Resp: 10575
Ion Ratio Lower Upper
200 100
173 23.5 23.0 34.6
215 52.3 38.6 57.8

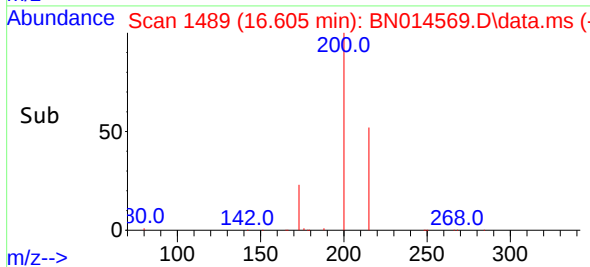







#24
Pentachlorophenol
Concen: 5.76 ng
RT: 16.787 min Scan# 1504
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	266	Resp:	5909
Ion Ratio	Lower	Upper	
266	100		
264	61.9	24.2	36.4#
268	63.1	25.2	37.8#

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

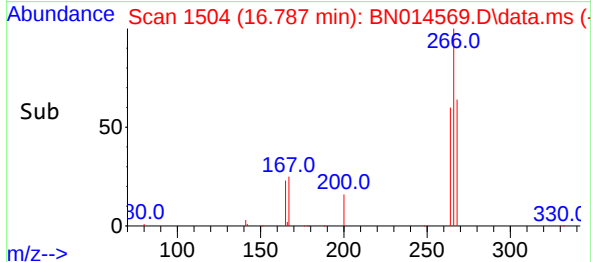

#25
Phenanthrene
Concen: 4.88 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	178	Resp:	63666
Ion Ratio	Lower	Upper	
178	100		
176	19.3	15.2	22.8
179	15.3	12.4	18.6

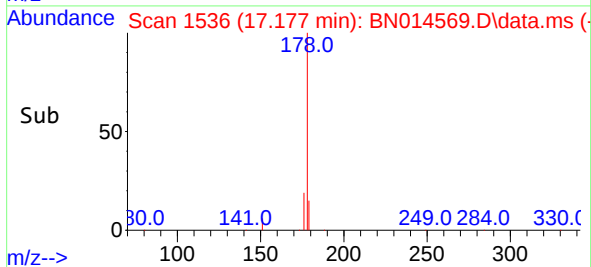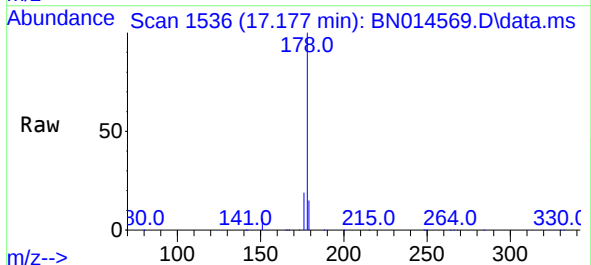

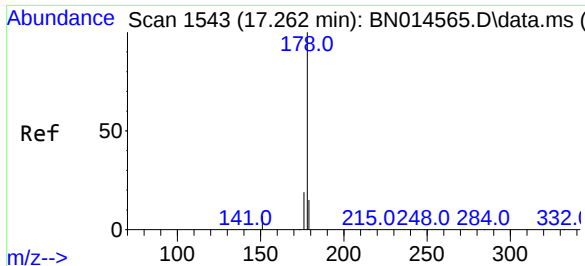





#26
 Anthracene
 Concen: 5.37 ng
 RT: 17.262 min Scan# 1543
 Delta R.T. -0.000 min
 Lab File: BN014569.D
 Acq: 11 May 2021 19:20

Tgt Ion:	178	Resp:	58870
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.8	22.2
179	15.5	12.2	18.2

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0




Manual Integrations
 APPROVED


mohammad
 5/12/2021 2:05:33 PM

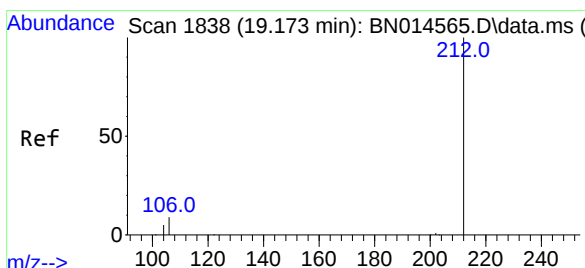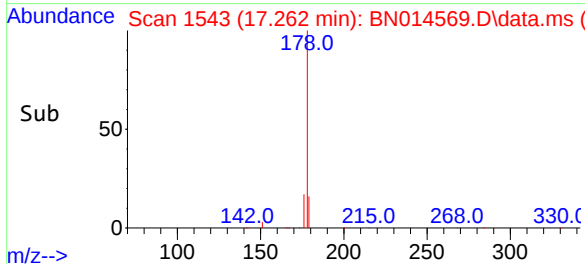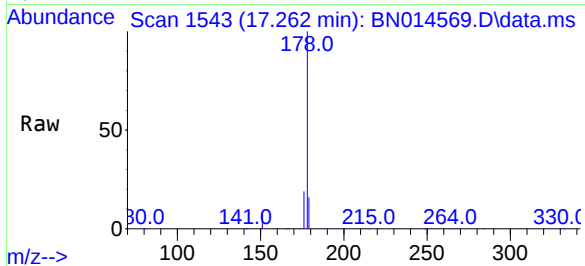

#27
 Fluoranthene-d10
 Concen: 5.08 ng
 RT: 19.171 min Scan# 1839
 Delta R.T. -0.003 min
 Lab File: BN014569.D
 Acq: 11 May 2021 19:20

Tgt Ion:	212	Resp:	107653
Ion	Ratio	Lower	Upper
212	100		
106	10.1	10.1	15.1
104	5.8	5.4	8.2

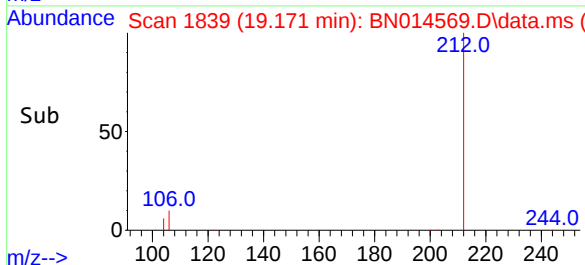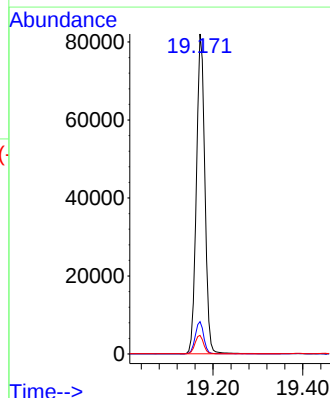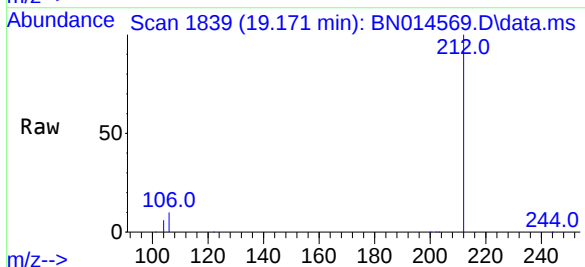







#28
Fluoranthene
Concen: 5.03 ng
RT: 19.201 min Scan# 1845
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	202	Resp:	86967
Ion Ratio	Lower	Upper	
202	100		
101	9.6	8.4	12.6
203	17.6	13.5	20.3

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM



#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.332 min Scan# 2132
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	240	Resp:	6608
Ion Ratio	Lower	Upper	
240	100		
120	6.7	5.8	8.8
236	27.1	20.6	30.8

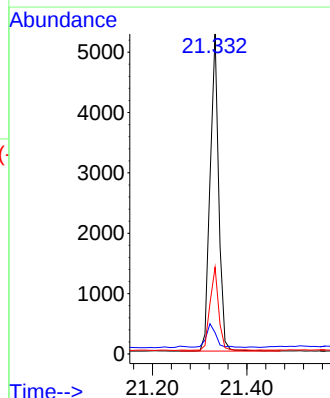







#30
Pyrene
Concen: 4.82 ng
RT: 19.563 min Scan# 1918
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:202 Resp: 87420
Ion Ratio Lower Upper
202 100
200 21.0 16.3 24.5
203 17.5 14.0 21.0

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM



#31
Terphenyl-d14
Concen: 4.78 ng
RT: 19.776 min Scan# 1961
Delta R.T. 0.002 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:244 Resp: 74489
Ion Ratio Lower Upper
244 100
212 7.0 6.0 9.0
122 7.7 9.3 13.9#

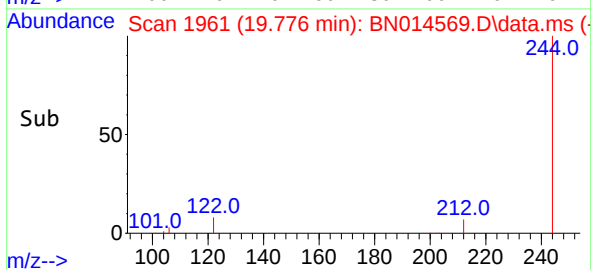







#32
Benzo(a)anthracene
Concen: 5.03 ng
RT: 21.311 min Scan# 2130
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	228	Resp:	96563
Ion Ratio	Lower	Upper	
228	100		
226	28.0	21.7	32.5
229	19.2	15.7	23.5

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

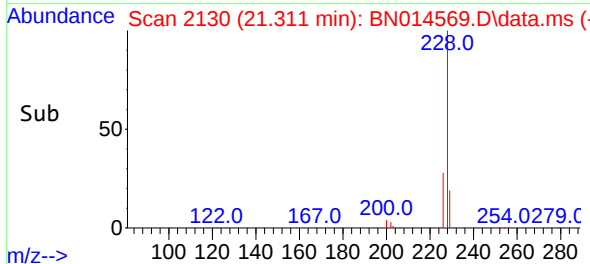

#33
Chrysene
Concen: 4.86 ng
RT: 21.364 min Scan# 2135
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:	228	Resp:	97673
Ion Ratio	Lower	Upper	
228	100		
226	29.9	23.8	35.6
229	19.3	15.6	23.4

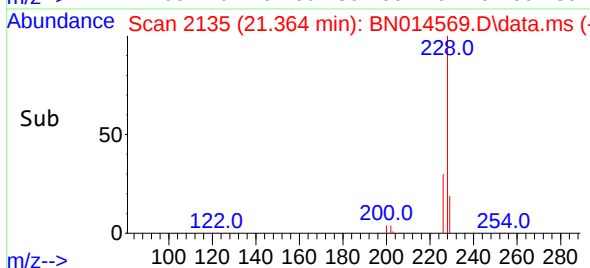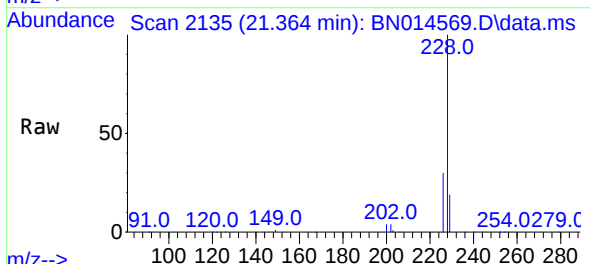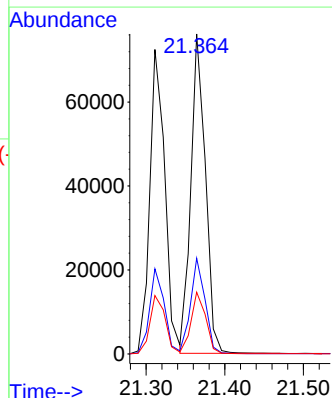

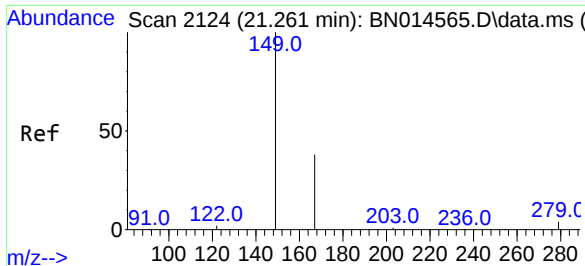





#34
Bis(2-ethylhexyl)phthalate
Concen: 5.42 ng
RT: 21.258 min Scan# 2125
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:149 Resp: 28910
Ion Ratio Lower Upper
149 100
167 37.3 20.5 30.7#
279 6.7 2.9 4.3#

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

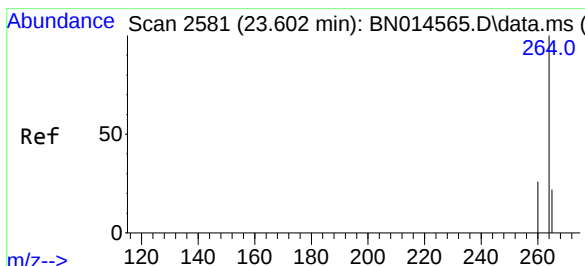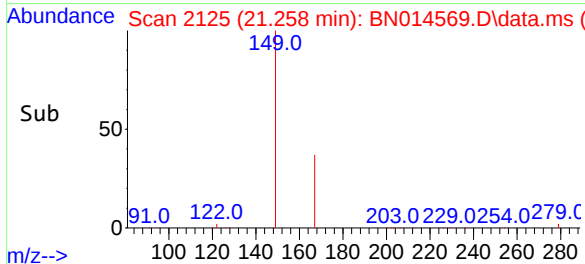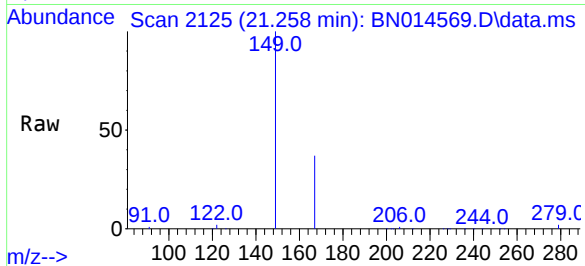

#35
Perylene-d12
Concen: 0.40 ng
RT: 23.603 min Scan# 2583
Delta R.T. 0.001 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:264 Resp: 5951
Ion Ratio Lower Upper
264 100
260 26.6 19.5 29.3
265 55.9 35.4 53.0#

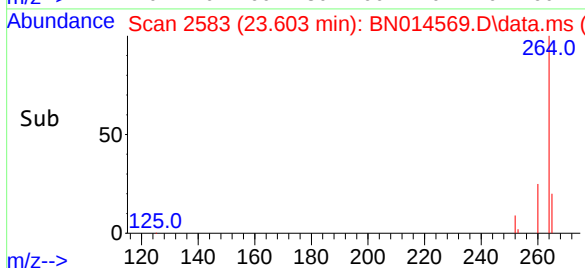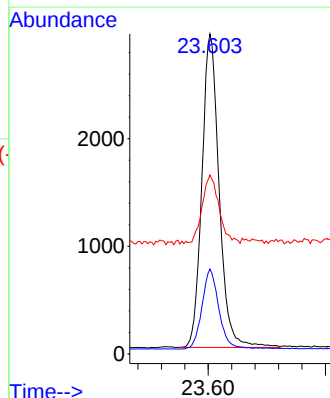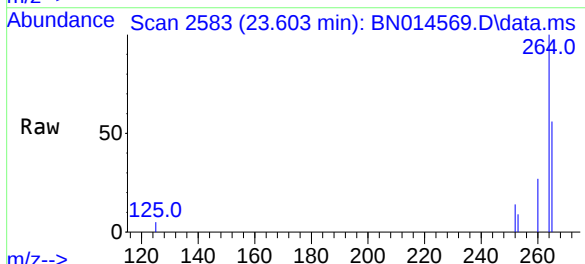







#36
Indeno(1,2,3-cd)pyrene
Concen: 5.12 ng
RT: 25.903 min Scan# 3255
Delta R.T. 0.001 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 276 Resp: 122503
Ion Ratio Lower Upper
276 100
138 13.8 18.8 28.2#
277 25.5 19.8 29.8

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM



#37
Benzo(b)fluoranthene
Concen: 5.11 ng
RT: 22.922 min Scan# 2384
Delta R.T. 0.004 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion: 252 Resp: 103739
Ion Ratio Lower Upper
252 100
253 21.9 19.6 29.4
125 6.2 10.3 15.5#

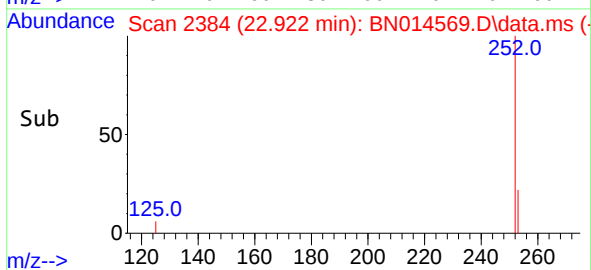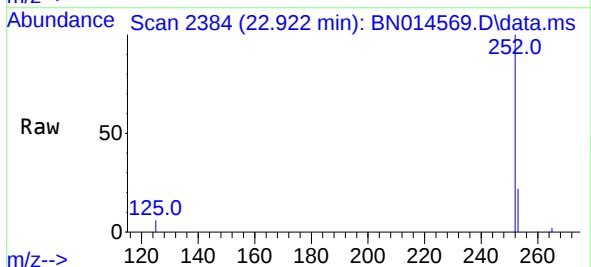







#38
Benzo(k)fluoranthene
Concen: 4.98 ng
RT: 22.963 min Scan# 2396
Delta R.T. 0.001 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:252 Resp: 104803
Ion Ratio Lower Upper
252 100
253 22.1 19.7 29.5
125 6.4 9.7 14.5#

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:33 PM

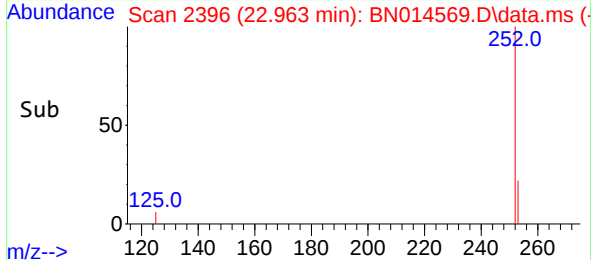

#39
Benzo(a)pyrene
Concen: 5.28 ng
RT: 23.504 min Scan# 2554
Delta R.T. 0.001 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:252 Resp: 90564
Ion Ratio Lower Upper
252 100
253 21.9 21.8 32.6
125 7.0 14.9 22.3#

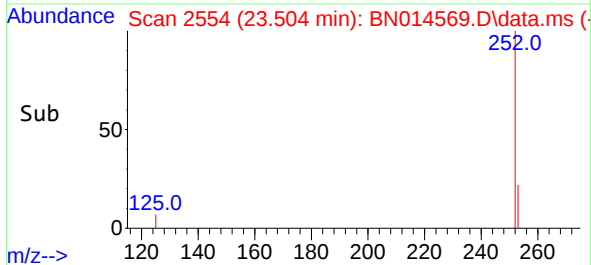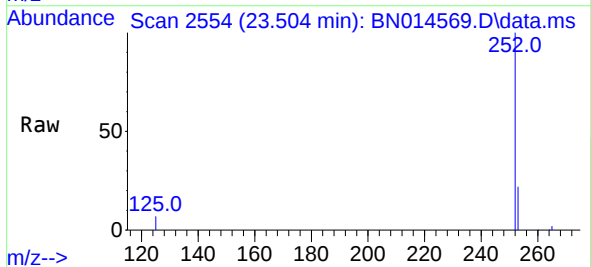







#40
Dibenzo(a,h)anthracene
Concen: 5.12 ng
RT: 25.920 min Scan# 3260
Delta R.T. 0.004 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:278 Resp: 104783
Ion Ratio Lower Upper
278 100
139 8.8 13.9 20.9#
279 23.7 20.7 31.1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:33 PM



#41
Benzo(g,h,i)perylene
Concen: 5.13 ng
RT: 26.598 min Scan# 3458
Delta R.T. -0.003 min
Lab File: BN014569.D
Acq: 11 May 2021 19:20

Tgt Ion:276 Resp: 99977
Ion Ratio Lower Upper
276 100
277 24.0 19.6 29.4
138 12.1 17.5 26.3#

