

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051121\
 Data File : BN014570.D
 Acq On : 11 May 2021 19:55
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN051121

Manual Integrations
 APPROVED

mohammad
 5/12/2021 2:05:36 PM

Quant Time: May 12 09:54:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 12 09:51:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.741	152	768	0.40	ng	# 0.00
7) Naphthalene-d8	10.530	136	2978	0.40	ng	# 0.00
13) Acenaphthene-d10	14.384	164	2157	0.40	ng	0.00
19) Phenanthrene-d10	17.128	188	5273	0.40	ng	# 0.00
29) Chrysene-d12	21.324	240	6853	0.40	ng	#-0.01
35) Perylene-d12	23.602	264	6731	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.333	112	748	0.37	ng	0.00
5) Phenol-d6	6.903	99	1041	0.38	ng	0.00
8) Nitrobenzene-d5	8.883	82	893	0.35	ng	0.00
11) 2-Methylnaphthalene-d10	12.120	152	2616	0.36	ng	0.00
14) 2,4,6-Tribromophenol	15.881	330	312	0.31	ng	0.00
15) 2-Fluorobiphenyl	13.001	172	2848	0.36	ng	0.00
27) Fluoranthene-d10	19.168	212	8183	0.35	ng	0.00
31) Terphenyl-d14	19.774	244	6038	0.37	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.295	88	392	0.30	ng	95
3) n-Nitrosodimethylamine	3.746	42	35	0.09	ng	# 1
6) bis(2-Chloroethyl)ether	7.169	93	863	0.38	ng	90
9) Naphthalene	10.568	128	2829	0.36	ng	# 92
10) Hexachlorobutadiene	10.872	225	680	0.36	ng	# 99
12) 2-Methylnaphthalene	12.195	142	2056	0.36	ng	# 92
16) Acenaphthylene	14.105	152	2679	0.34	ng	98
17) Acenaphthene	14.448	154	2109	0.36	ng	99
18) Fluorene	15.437	166	2763	0.35	ng	97
20) 4,6-Dinitro-2-methylph...	15.513	198	185	0.36	ng	# 1
21) 4-Bromophenyl-phenylether	16.325	248	1121	0.35	ng	# 72
22) Hexachlorobenzene	16.447	284	1242	0.36	ng	91
23) Atrazine	16.605	200	627	0.31	ng	# 90
24) Pentachlorophenol	16.788	266	320	0.28	ng	# 40
25) Phenanthrene	17.177	178	5090	0.35	ng	99
26) Anthracene	17.262	178	4042	0.33	ng	99
28) Fluoranthene	19.203	202	6631	0.35	ng	98
30) Pyrene	19.566	202	6576	0.35	ng	99
32) Benzo(a)anthracene	21.314	228	6825	0.34	ng	99
33) Chrysene	21.367	228	7700	0.37	ng	98
34) Bis(2-ethylhexyl)phtha...	21.261	149	1770	0.32	ng	# 81
36) Indeno(1,2,3-cd)pyrene	25.899	276	9752	0.36	ng	# 92
37) Benzo(b)fluoranthene	22.918	252	8130m	0.35	ng	
38) Benzo(k)fluoranthene	22.962	252	8433	0.35	ng	97
39) Benzo(a)pyrene	23.503	252	6763	0.35	ng	# 94
40) Dibenzo(a,h)anthracene	25.913	278	8327	0.36	ng	# 95
41) Benzo(g,h,i)perylene	26.597	276	7752	0.35	ng	# 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051121\
Data File : BN014570.D
Acq On : 11 May 2021 19:55
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM


Quant Time: May 12 09:54:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 12 09:51:41 2021
Response via : Initial Calibration





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.741 min Scan# 616
 Delta R.T. -0.000 min
 Lab File: BN014570.D
 Acq: 11 May 2021 19:55




Instrument :
 BNA_N
 ClientSampled :
 ICVBN051121




Tgt Ion: 152 Resp: 768
 Ion Ratio Lower Upper
 152 100
 150 153.7 123.8 185.8
 115 86.6 47.0 70.4#

Manual Integrations
 APPROVED



mohammad
 5/12/2021 2:05:36 PM




#2
 1,4-Dioxane
 Concen: 0.30 ng
 RT: 3.295 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN014570.D
 Acq: 11 May 2021 19:55



Tgt Ion: 88 Resp: 392
 Ion Ratio Lower Upper
 88 100
 58 52.8 44.4 66.6
 43 16.6 15.9 23.9









#3
n-Nitrosodimethylamine
Concen: 0.09 ng
RT: 3.746 min Scan# 120
Delta R.T. -0.024 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion: 42 Resp: 35
Ion Ratio Lower Upper
42 100
74 22.9 175.1 262.7#
44 31.4 7.5 11.3#

Instrument :
BNA_N
ClientSampled :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM



#4
2-Fluorophenol
Concen: 0.37 ng
RT: 5.333 min Scan# 317
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion: 112 Resp: 748
Ion Ratio Lower Upper
112 100
64 58.2 41.8 62.6
63 31.0 22.0 33.0









#5
Phenol-d6
Concen: 0.38 ng
RT: 6.903 min Scan# 512
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	99	Resp:	1041
Ion	Ratio	Lower	Upper
99	100		
42	12.7	13.2	19.8#
71	43.3	26.2	39.2#

Instrument :
BNA_N
ClientSampled :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM




#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 7.169 min Scan# 545
Delta R.T. -0.008 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	93	Resp:	863
Ion	Ratio	Lower	Upper
93	100		
63	61.0	58.0	87.0
95	33.3	27.0	40.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.530 min Scan# 862
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55





Tgt Ion:	136	Resp:	2978
Ion	Ratio	Lower	Upper
136	100		
137	13.1	8.9	13.3
54	7.1	3.8	5.8#
68	7.0	3.8	5.6#



#8
Nitrobenzene-d5
Concen: 0.35 ng
RT: 8.883 min Scan# 732
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:	82	Resp:	893
Ion	Ratio	Lower	Upper
82	100		
128	33.5	29.5	44.3
54	46.2	36.9	55.3



Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM

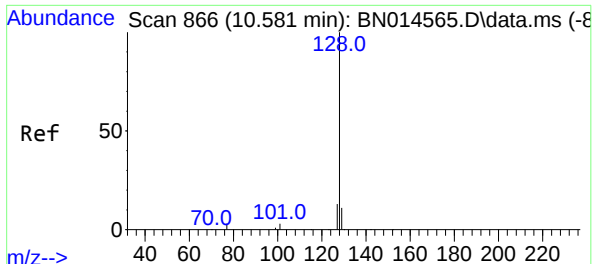





#9
Naphthalene
Concen: 0.36 ng
RT: 10.568 min Scan# 865
Delta R.T. -0.013 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:128 Resp: 2829
Ion Ratio Lower Upper
128 100
129 13.9 9.0 13.4#
127 16.6 10.4 15.6#

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM



#10
Hexachlorobutadiene
Concen: 0.36 ng
RT: 10.872 min Scan# 889
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:225 Resp: 680
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.6 50.9 76.3









#11
2-Methylnaphthalene-d10
Concen: 0.36 ng
RT: 12.120 min Scan# 1077
Delta R.T. -0.005 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:152 Resp: 2616
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.2

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM




#12
2-Methylnaphthalene
Concen: 0.36 ng
RT: 12.195 min Scan# 1094
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:142 Resp: 2056
Ion Ratio Lower Upper
142 100
141 87.7 70.2 105.4
115 49.0 26.7 40.1#






#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.384 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55



Tgt Ion:164 Resp: 2157



Ion	Ratio	Lower	Upper
164	100		
162	101.9	78.6	118.0
160	45.8	35.8	53.8




Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM






#14
2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.881 min Scan# 1430
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55



Tgt Ion:330 Resp: 312

Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	29.2	27.0	40.4









#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 13.001 min Scan# 1203
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	172	Resp:	2848
Ion	Ratio	Lower	Upper
172	100		
171	38.1	27.1	40.7
170	26.2	18.3	27.5

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM




#16
Acenaphthylene
Concen: 0.34 ng
RT: 14.105 min Scan# 1290
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	152	Resp:	2679
Ion	Ratio	Lower	Upper
152	100		
151	20.0	15.6	23.4
153	14.1	10.5	15.7





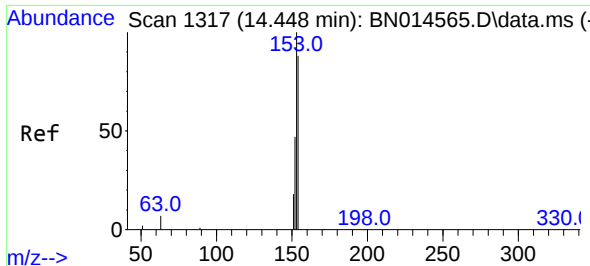


#17
Acenaphthene
Concen: 0.36 ng
RT: 14.448 min Scan# 1317
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:154 Resp: 2109

Ion	Ratio	Lower	Upper
154	100		
153	112.6	90.2	135.4
152	55.4	46.2	69.2





#18
Fluorene
Concen: 0.35 ng
RT: 15.437 min Scan# 1395
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55



Tgt Ion:166 Resp: 2763


Ion	Ratio	Lower	Upper
166	100		
165	100.7	78.4	117.6
167	14.0	10.7	16.1



Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM







#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.128 min Scan# 1532
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:188 Resp: 5273
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.0 5.2 7.8#

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.36 ng
RT: 15.513 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:198 Resp: 185
Ion Ratio Lower Upper
198 100
51 66.7 865.3 1297.9#
105 59.5 93.6 140.4#








#21
4-Bromophenyl-phenylether
Concen: 0.35 ng
RT: 16.325 min Scan# 1466
Delta R.T. -0.012 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion: 248 Resp: 1121

Ion	Ratio	Lower	Upper
248	100		
250	91.2	80.5	120.7
141	92.3	37.2	55.8#





#22
Hexachlorobenzene
Concen: 0.36 ng
RT: 16.447 min Scan# 1476
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55



Tgt Ion: 284 Resp: 1242


Ion	Ratio	Lower	Upper
284	100		
142	27.8	26.6	39.8
249	34.1	23.6	35.4



Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM







#23
Atrazine
Concen: 0.31 ng
RT: 16.605 min Scan# 1489
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	200	Resp:	627
Ion Ratio	Lower	Upper	
200	100		
173	30.3	23.0	34.6
215	58.0	38.6	57.8#

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM



#24
Pentachlorophenol
Concen: 0.28 ng
RT: 16.788 min Scan# 1504
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	266	Resp:	320
Ion Ratio	Lower	Upper	
266	100		
264	59.4	24.2	36.4#
268	67.8	25.2	37.8#



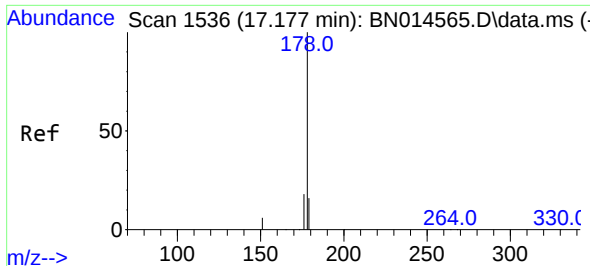





#25
Phenanthrene
Concen: 0.35 ng
RT: 17.177 min Scan# 1536
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	178	Resp:	5090
Ion Ratio	Lower	Upper	
178	100		
176	19.3	15.2	22.8
179	15.2	12.4	18.6

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM



#26
Anthracene
Concen: 0.33 ng
RT: 17.262 min Scan# 1543
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	178	Resp:	4042
Ion Ratio	Lower	Upper	
178	100		
176	18.9	14.8	22.2
179	15.6	12.2	18.2









#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.168 min Scan# 1837
Delta R.T. -0.005 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	212	Resp:	8183
Ion Ratio	Lower	Upper	
212	100		
106	10.1	10.1	15.1
104	6.2	5.4	8.2

Instrument :
BNA_N
ClientSampleId :
ICVBN051121




Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM




#28
Fluoranthene
Concen: 0.35 ng
RT: 19.203 min Scan# 1844
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	202	Resp:	6631
Ion Ratio	Lower	Upper	
202	100		
101	9.4	8.4	12.6
203	17.3	13.5	20.3









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.324 min Scan# 2130
Delta R.T. -0.011 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55





Tgt Ion:240 Resp: 6853
Ion Ratio Lower Upper
240 100
120 11.7 5.8 8.8#
236 28.7 20.6 30.8



#30
Pyrene
Concen: 0.35 ng
RT: 19.566 min Scan# 1917
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:202 Resp: 6576
Ion Ratio Lower Upper
202 100
200 20.8 16.3 24.5
203 18.0 14.0 21.0




Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED


mohammad
5/12/2021 2:05:36 PM



#31
Terphenyl-d14
Concen: 0.37 ng
RT: 19.774 min Scan# 1959
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:244 Resp: 6038
Ion Ratio Lower Upper
244 100
212 8.1 6.0 9.0
122 9.0 9.3 13.9#




Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:36 PM




#32
Benzo(a)anthracene
Concen: 0.34 ng
RT: 21.314 min Scan# 2129
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:228 Resp: 6825
Ion Ratio Lower Upper
228 100
226 27.6 21.7 32.5
229 20.5 15.7 23.5






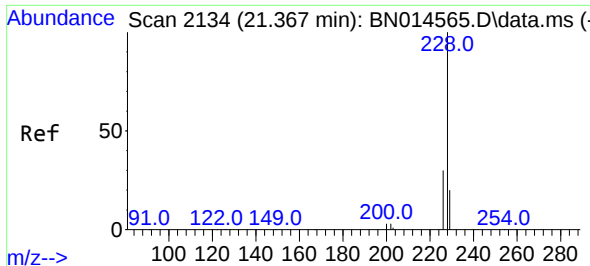


#33
Chrysene
Concen: 0.37 ng
RT: 21.367 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55





Tgt Ion:228 Resp: 7700
Ion Ratio Lower Upper
228 100
226 30.3 23.8 35.6
229 20.6 15.6 23.4



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.32 ng
RT: 21.261 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:149 Resp: 1770
Ion Ratio Lower Upper
149 100
167 36.0 20.5 30.7#
279 7.3 2.9 4.3#




Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:36 PM



#35
Perylene-d12
Concen: 0.40 ng
RT: 23.602 min Scan# 2581
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:264 Resp: 6731
Ion Ratio Lower Upper
264 100
260 25.9 19.5 29.3
265 51.7 35.4 53.0




Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED



mohammad
5/12/2021 2:05:36 PM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.36 ng
RT: 25.899 min Scan# 3252
Delta R.T. -0.003 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55







Tgt Ion:276 Resp: 9752
Ion Ratio Lower Upper
276 100
138 16.8 18.8 28.2#
277 25.8 19.8 29.8








#37
Benzo(b)fluoranthene
Concen: 0.35 ng m
RT: 22.918 min Scan# 2381
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.1	19.6	29.4
125	9.2	10.3	15.5#



#38
Benzo(k)fluoranthene
Concen: 0.35 ng
RT: 22.962 min Scan# 2394
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55


Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.4	19.7	29.5
125	10.4	9.7	14.5




Instrument :
BNA_N
ClientSampled :
ICVBN051121

Manual Integrations
APPROVED




mohammad
5/12/2021 2:05:36 PM




#39
Benzo(a)pyrene
Concen: 0.35 ng
RT: 23.503 min Scan# 2552
Delta R.T. -0.000 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55





Tgt Ion:252 Resp: 6763
Ion Ratio Lower Upper
252 100
253 27.3 21.8 32.6
125 12.3 14.9 22.3#



#40
Dibenzo(a,h)anthracene
Concen: 0.36 ng
RT: 25.913 min Scan# 3256
Delta R.T. -0.004 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55




Tgt Ion:278 Resp: 8327
Ion Ratio Lower Upper
278 100
139 12.1 13.9 20.9#
279 26.1 20.7 31.1



Instrument :
BNA_N
ClientSampleId :
ICVBN051121


Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM



#41
Benzo(g,h,i)perylene
Concen: 0.35 ng
RT: 26.597 min Scan# 3456
Delta R.T. -0.003 min
Lab File: BN014570.D
Acq: 11 May 2021 19:55

Tgt Ion:	276	Resp:	7752
Ion	Ratio	Lower	Upper
276	100		
277	25.8	19.6	29.4
138	14.0	17.5	26.3#



Instrument :
BNA_N
ClientSampleId :
ICVBN051121

Manual Integrations
APPROVED

mohammad
5/12/2021 2:05:36 PM