
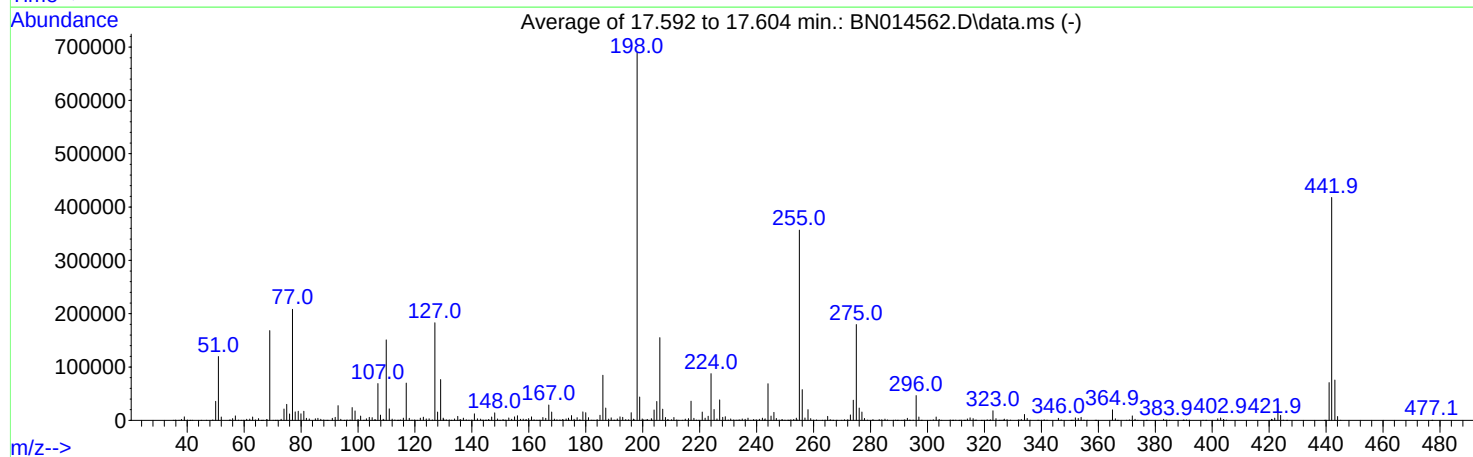


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051121\
 Data File : BN014562.D
 Acq On : 11 May 2021 15:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 12 09:51:41 2021

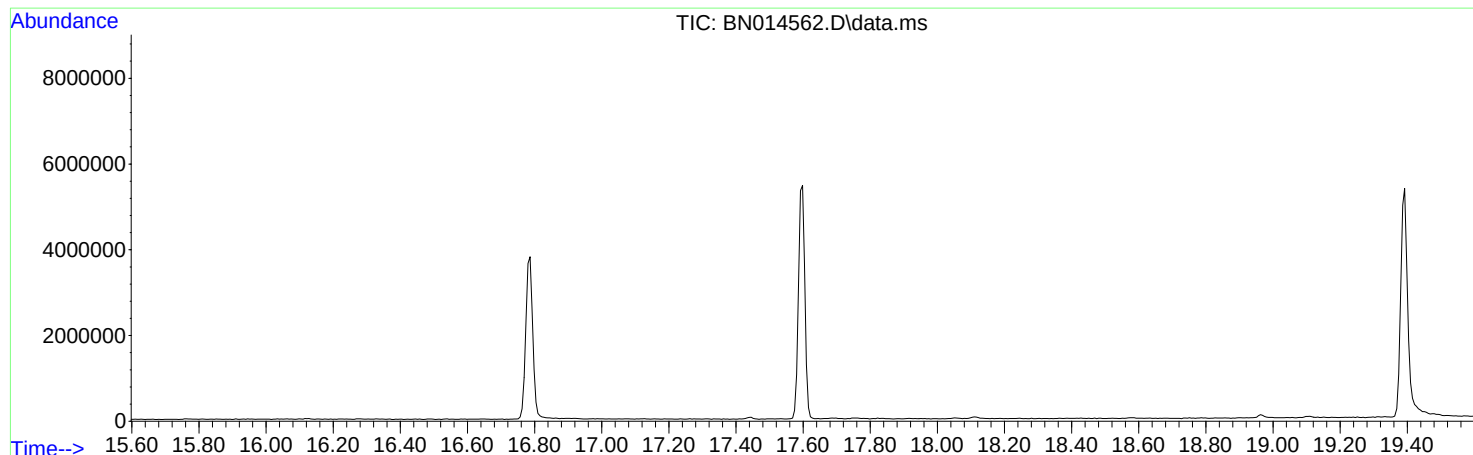




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.3	119618	PASS
68	69	0.00	2	0.9	1571	PASS
69	198	0.00	100	24.4	168203	PASS
70	69	0.00	2	0.1	252	PASS
127	198	10	80	26.5	183125	PASS
197	198	0.00	2	0.4	2433	PASS
198	198	100	100	100.0	689771	PASS
199	198	5	9	6.4	43920	PASS
275	198	10	60	26.1	179883	PASS
365	198	1	100	2.9	19707	PASS
441	198	0.01	100	10.3	70715	PASS
442	442	50	100	100.0	417963	PASS
443	442	15	24	18.1	75773	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BP051121\
Data File : BN014562.D
Acq On : 11 May 2021 15:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 11 16:17:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 08 04:11:21 2021
Response via : Initial Calibration

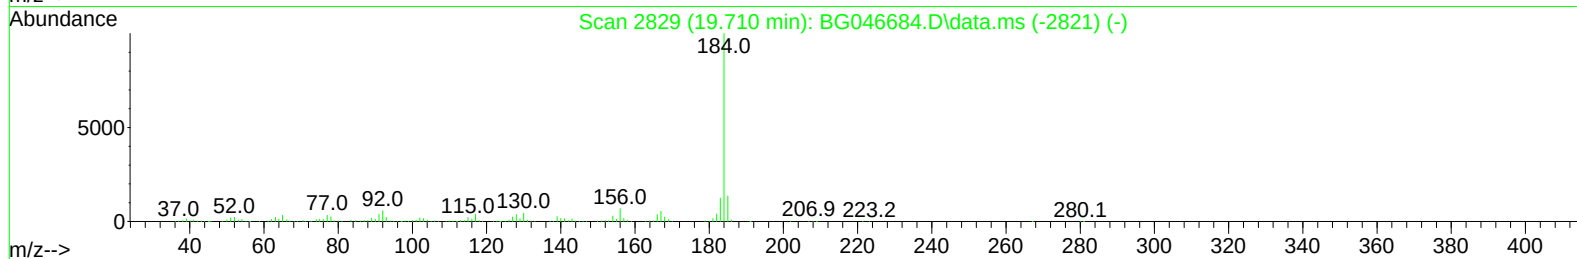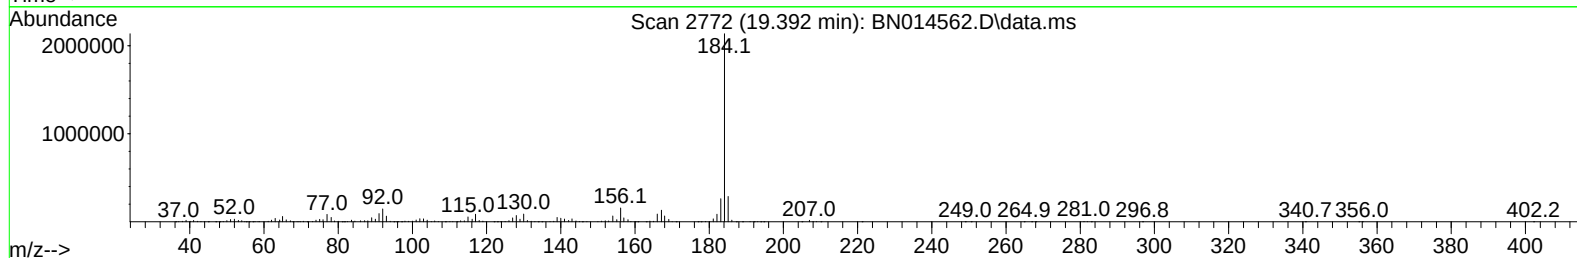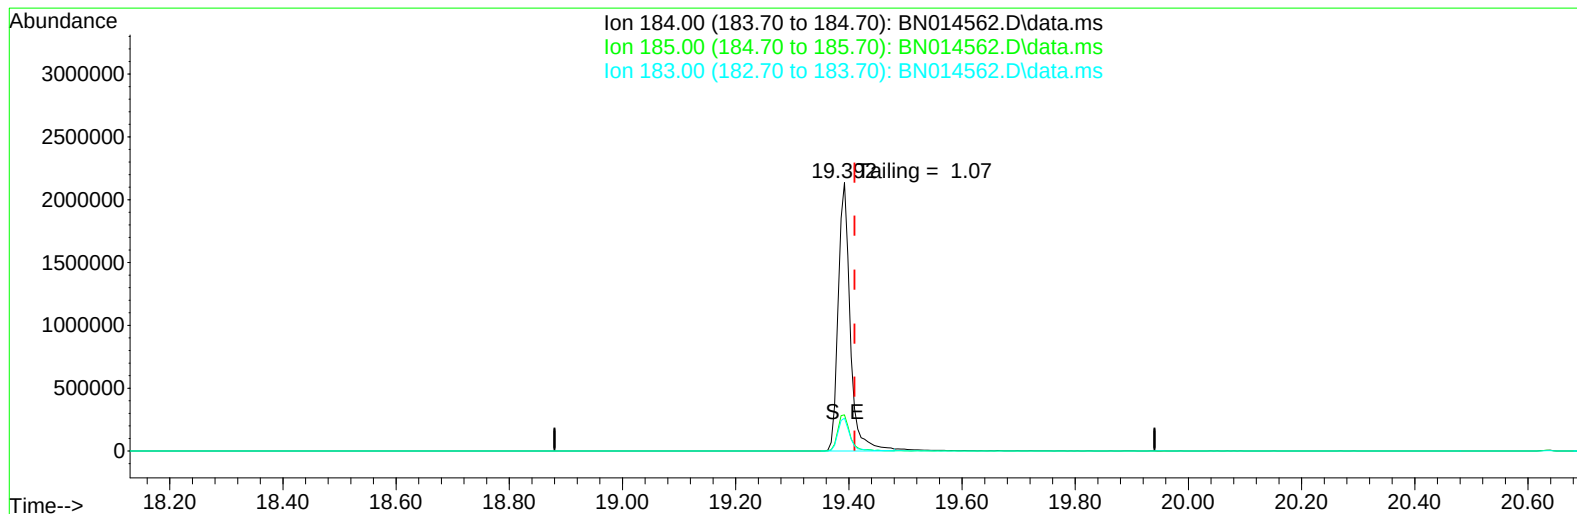

TIC: BN014562.D\data.ms

(77) Benzidine

19.392min (-0.018) 929499.03 ng




response 3180389

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	12.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BP051121\
 Data File : BN014562.D
 Acq On : 11 May 2021 15:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 11 16:17:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

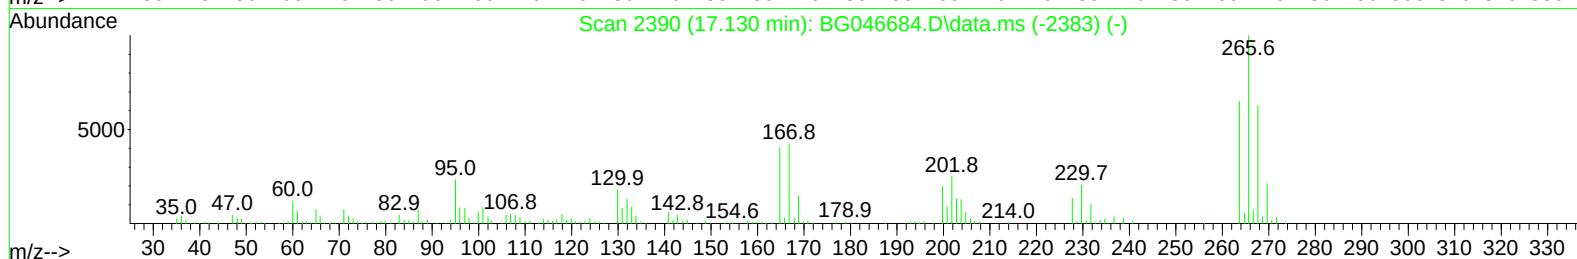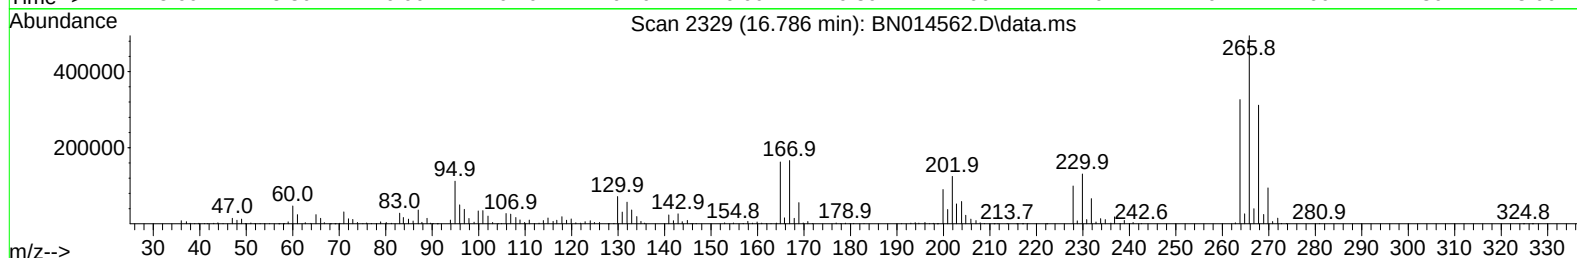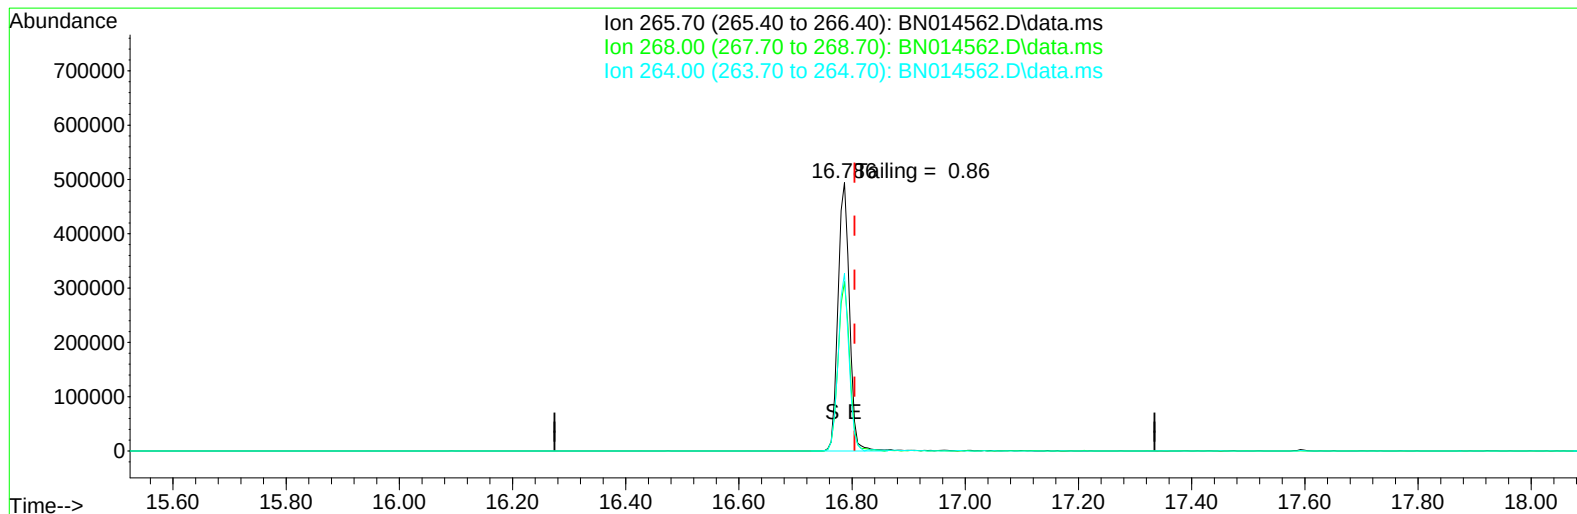

TIC: BN014562.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.018) 22269.12 ng

response 696603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.07
264.00	61.60	66.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2021	BNA_N	<u>BN014562.D</u>
Compound Name	Response	Retention Time
DDT	1986130	20.63
DDD	2899	20.19
DDE	4178	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7077	1993207	0.36