

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019724.D
 Acq On : 11 May 2022 16:16
 Operator : CG/JU
 Sample : PB144864BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 50

Instrument :
 BNA_N
 ClientSampleId :
 PB144864BL

Quant Time: May 12 08:11:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 10 01:35:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.862	152	234331	20.000	ng	0.00
7) Naphthalene-d8	10.648	136	723789	20.000	ng	# 0.00
13) Acenaphthene-d10	14.474	164	428740	20.000	ng	0.00
19) Phenanthrene-d10	17.215	188	921955	20.000	ng	0.00
29) Chrysene-d12	21.404	240	814757	20.000	ng	# 0.00
35) Perylene-d12	23.752	264	779800	20.000	ng	# 0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.442	112	1853718	174.848	ng	0.00
5) Phenol-d6	7.024	99	2337711	175.113	ng	0.00
8) Nitrobenzene-d5	9.003	82	1140235	94.265	ng	0.00
11) 2-Methylnaphthalene-d10	12.246	152	2	0.000	ng	0.01
14) 2,4,6-Tribromophenol	15.964	330	536024	172.149	ng	0.00
15) 2-Fluorobiphenyl	13.105	172	2651545	68.539	ng	0.00
27) Fluoranthene-d10	19.253	212	11	0.000	ng	0.00
31) Terphenyl-d14	19.851	244	2420190	63.902	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
Data File : BN019724.D
Acq On : 11 May 2022 16:16
Operator : CG/JU
Sample : PB144864BL
Misc :
ALS Vial : 4 Sample Multiplier: 50

Instrument :
BNA_N
ClientSampleId :
PB144864BL


Quant Time: May 12 08:11:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 10 01:35:26 2022
Response via : Initial Calibration

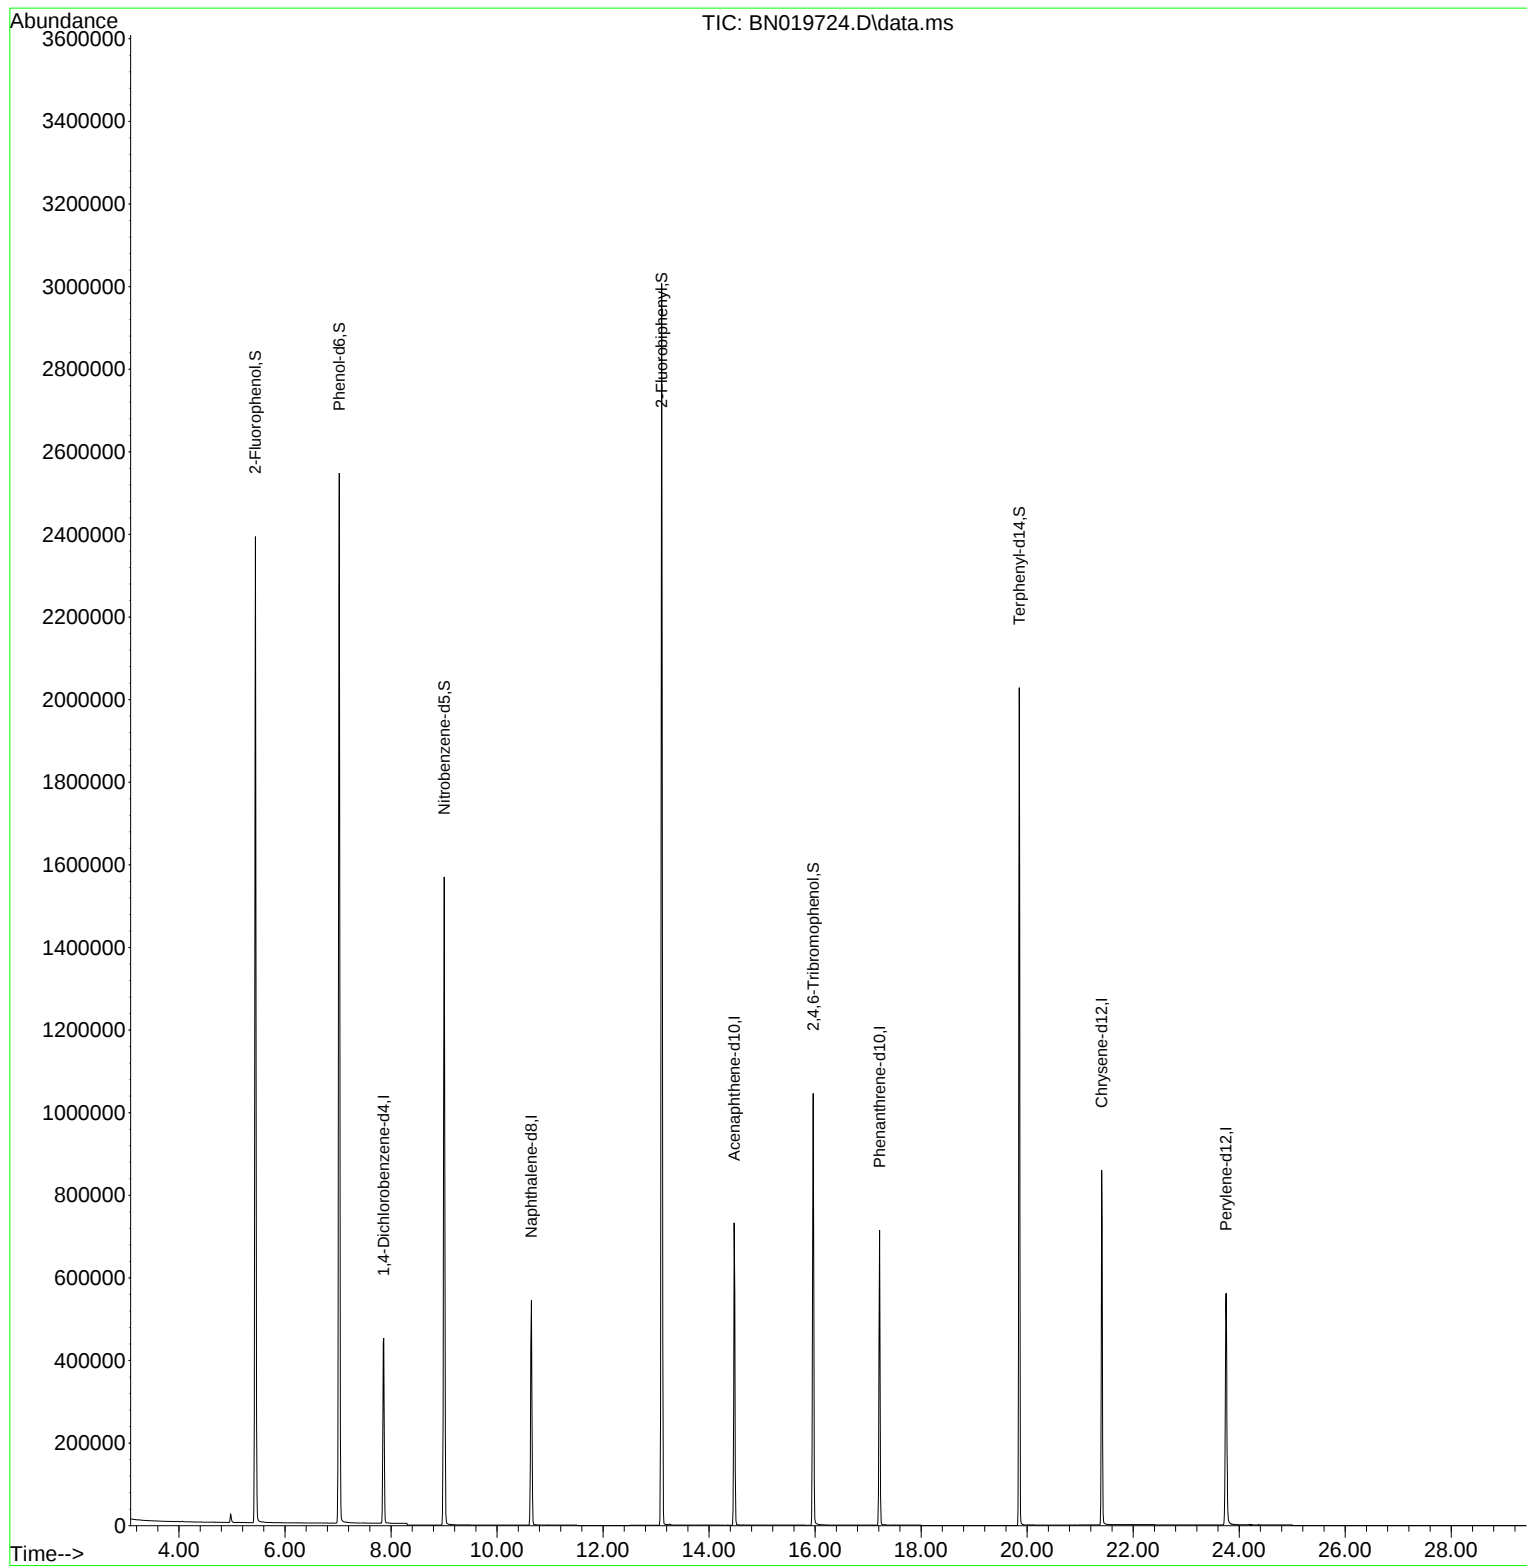






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.862 min Scan# 662
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Instrument :
BNA_N
ClientSampleId :
PB144864BL







Tgt Ion:152 Resp: 234331
Ion Ratio Lower Upper
152 100
150 153.8 125.0 187.4
115 58.8 50.6 76.0

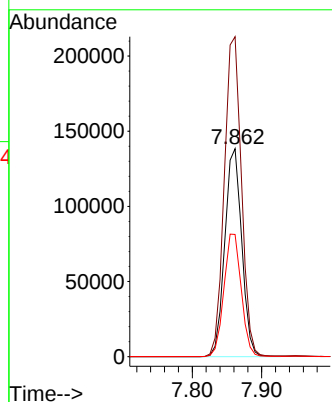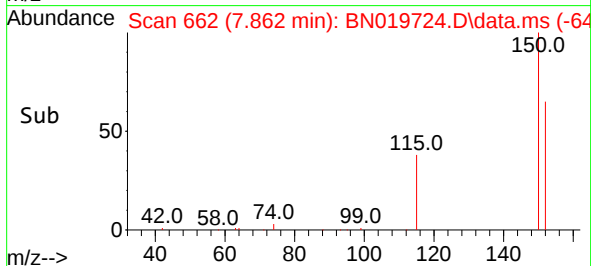

#4
2-Fluorophenol
Concen: 174.848 ng
RT: 5.442 min Scan# 327
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:112 Resp: 1853718
Ion Ratio Lower Upper
112 100
64 61.7 49.1 73.7
63 32.6 26.4 39.6

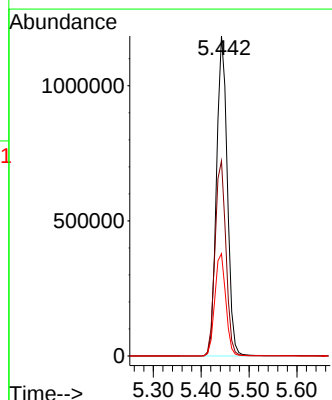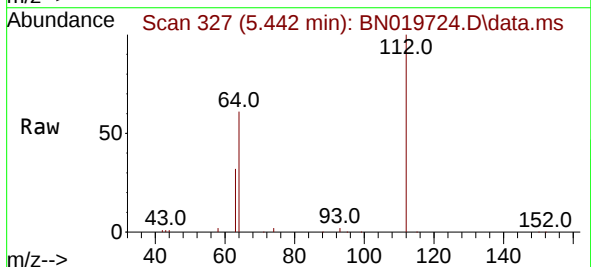







#5
Phenol-d6
Concen: 175.113 ng
RT: 7.024 min Scan# 546
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Instrument :
BNA_N
ClientSampleId :
PB144864BL

Tgt Ion: 99 Resp: 2337711




Ion	Ratio	Lower	Upper
99	100		
42	22.1	19.6	29.4
71	34.7	27.3	40.9

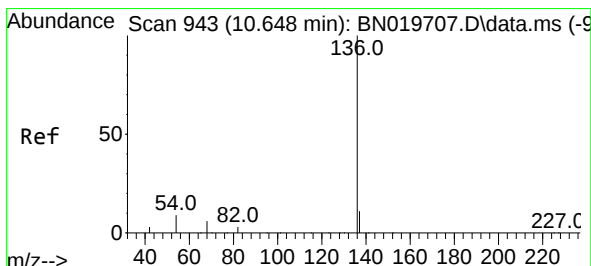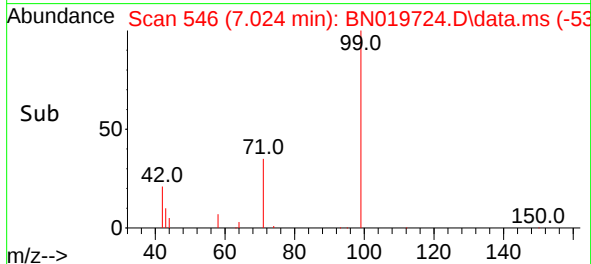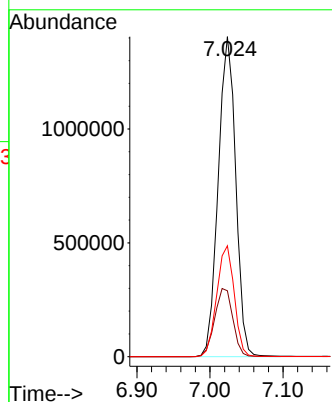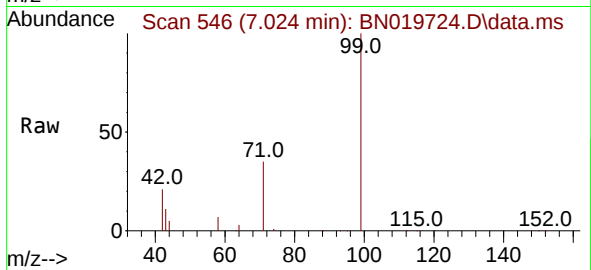


#7
Naphthalene-d8
Concen: 20.000 ng
RT: 10.648 min Scan# 943
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:136 Resp: 723789

Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.1	13.7
54	8.4	8.2	12.4
68	5.4	5.5	8.3


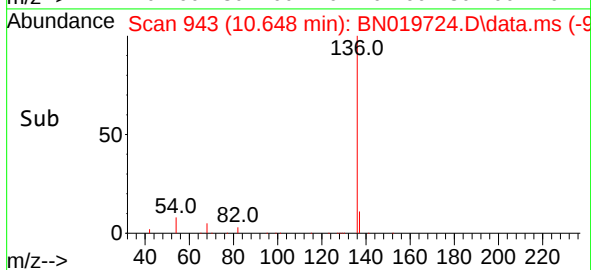
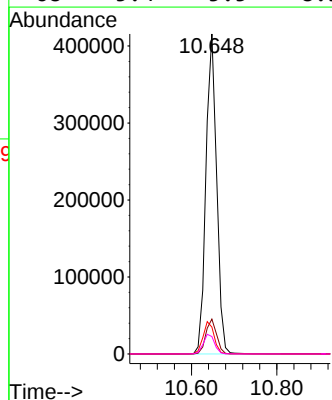
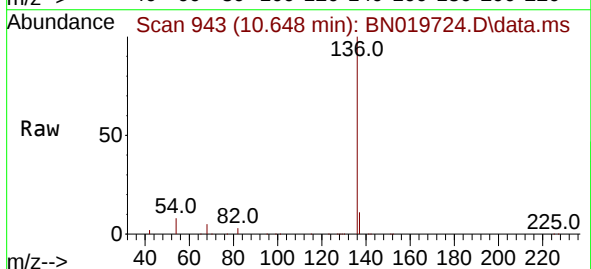


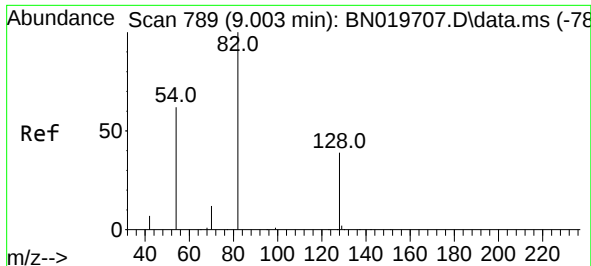

#8
Nitrobenzene-d5
Concen: 94.265 ng
RT: 9.003 min Scan# 789
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16




Instrument :
BNA_N
ClientSampleId :
PB144864BL


Tgt Ion: 82 Resp: 1140235
Ion Ratio Lower Upper
82 100
128 42.8 32.4 48.6
54 59.5 50.7 76.1

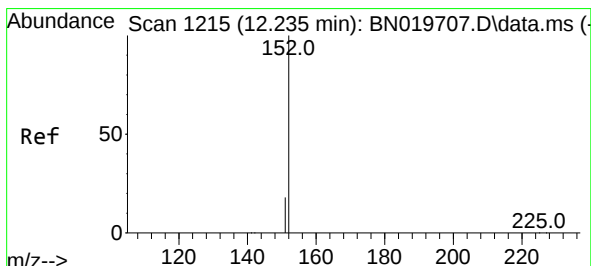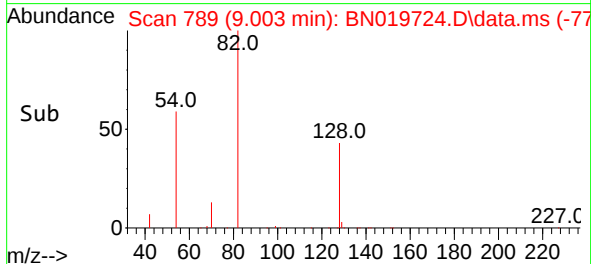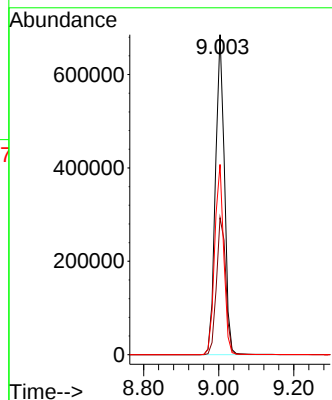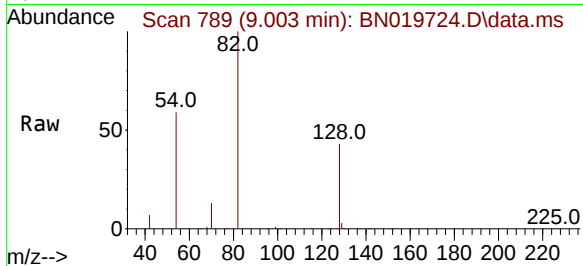

#11
2-Methylnaphthalene-d10
Concen: 0.000 ng
RT: 12.246 min Scan# 1218
Delta R.T. 0.011 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:152 Resp: 2
Ion Ratio Lower Upper
152 100
151 100.0 16.4 24.6#


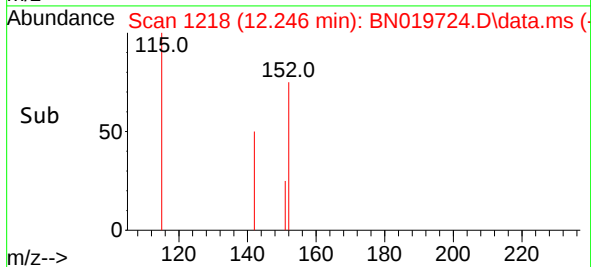
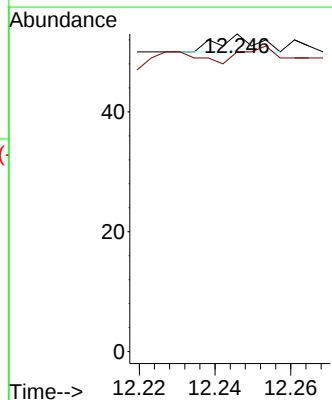
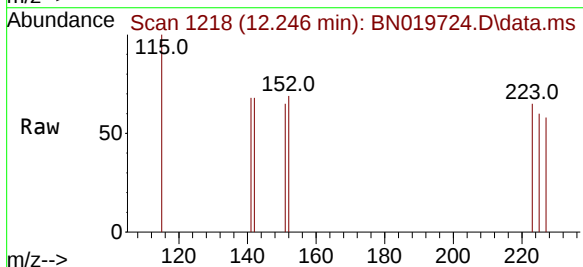




#13
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.474 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16




Instrument :
BNA_N
ClientSampleId :
PB144864BL


Tgt Ion:164 Resp: 428740
Ion Ratio Lower Upper
164 100
162 103.5 84.0 126.0
160 47.6 41.1 61.7

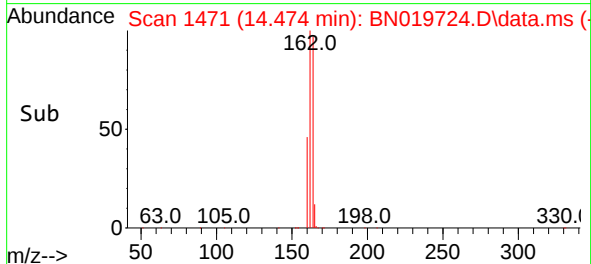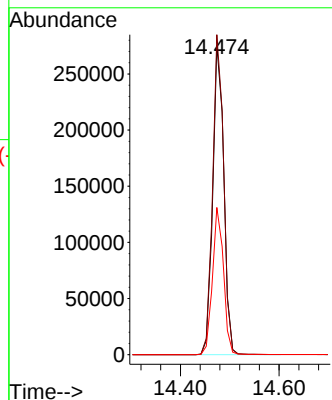

#14
2,4,6-Tribromophenol
Concen: 172.149 ng
RT: 15.964 min Scan# 1611
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:330 Resp: 536024
Ion Ratio Lower Upper
330 100
332 96.1 75.7 113.5
141 51.0 40.2 60.2


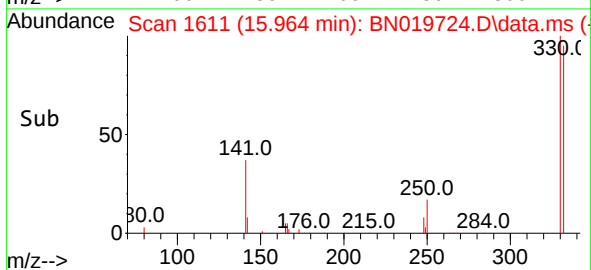
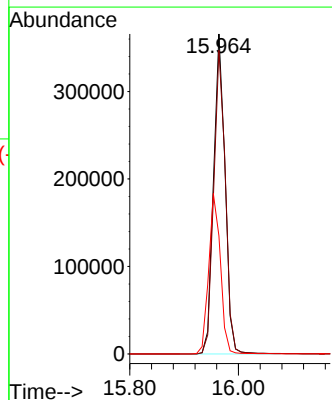
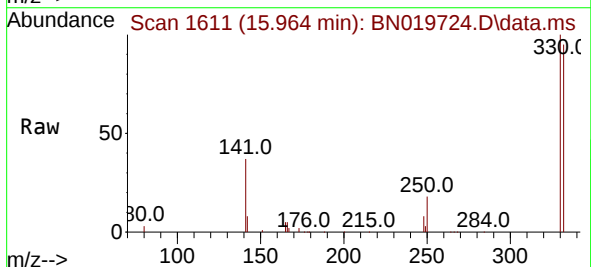


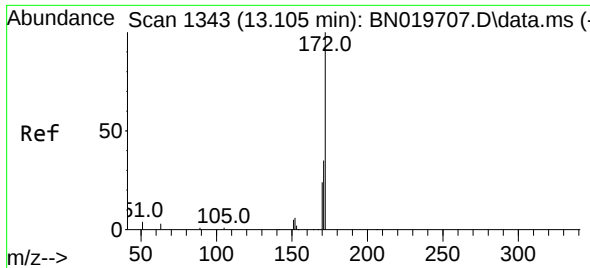

#15
2-Fluorobiphenyl
Concen: 68.539 ng
RT: 13.105 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16




Instrument :
BNA_N
ClientSampleId :
PB144864BL


Tgt Ion:172 Resp: 2651545
Ion Ratio Lower Upper
172 100
171 34.7 28.5 42.7
170 23.1 19.4 29.2

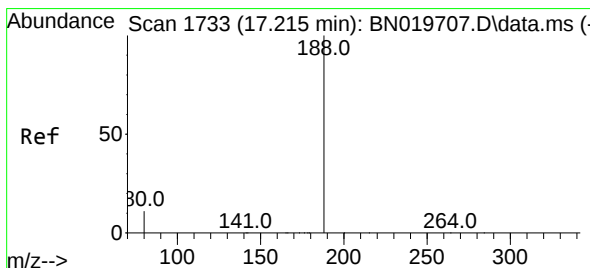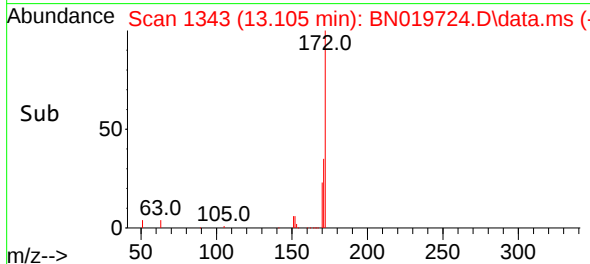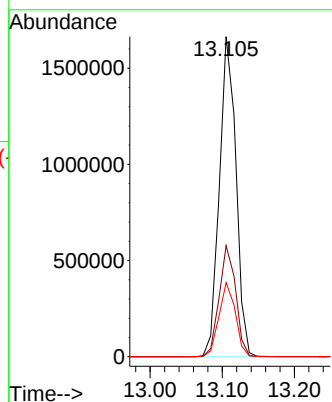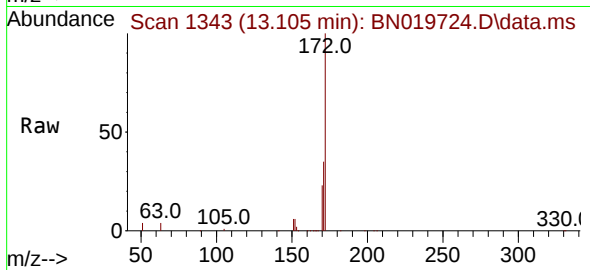

#19
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.215 min Scan# 1733
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:188 Resp: 921955
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 9.6 14.4


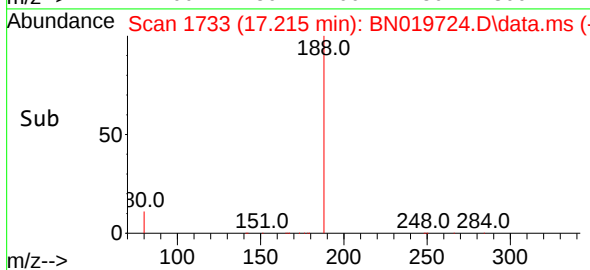
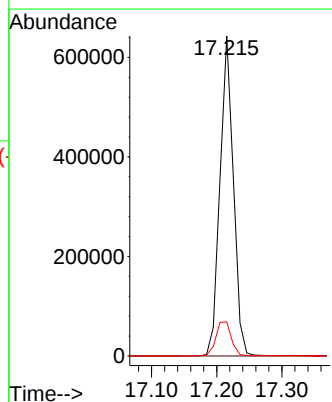
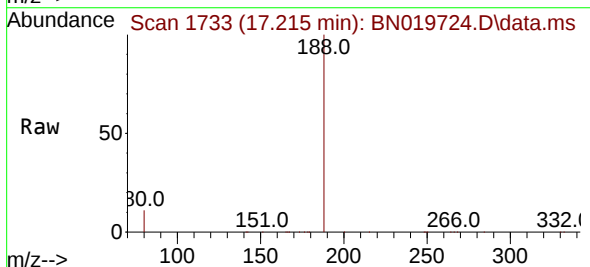




#27
Fluoranthene-d10
Concen: 0.000 ng
RT: 19.253 min Scan# 2106
Delta R.T. 0.004 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16




Instrument :
BNA_N
ClientSampleId :
PB144864BL


Tgt Ion:212 Resp: 11
Ion Ratio Lower Upper
212 100
106 18.2 13.0 19.4
104 27.3 7.3 10.9#

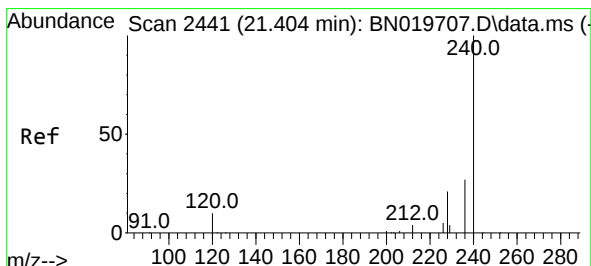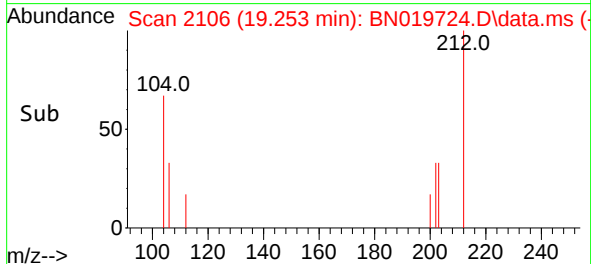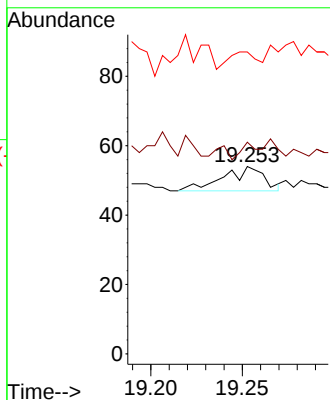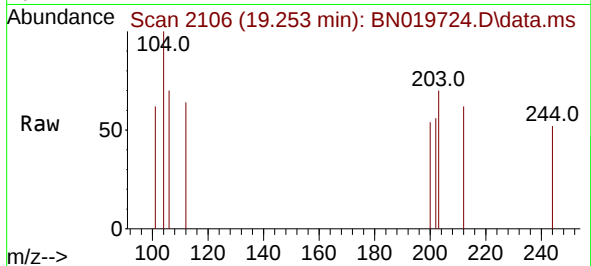

#29
Chrysene-d12
Concen: 20.000 ng
RT: 21.404 min Scan# 2441
Delta R.T. -0.000 min
Lab File: BN019724.D
Acq: 11 May 2022 16:16

Tgt Ion:240 Resp: 814757
Ion Ratio Lower Upper
240 100
120 17.1 9.0 13.6#
236 27.7 22.0 33.0


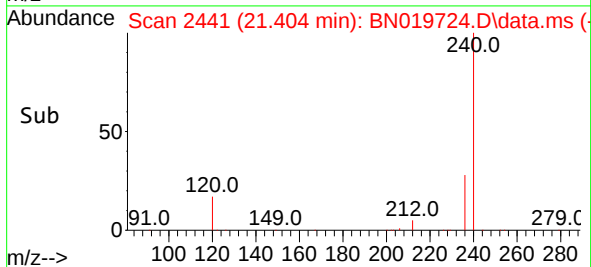
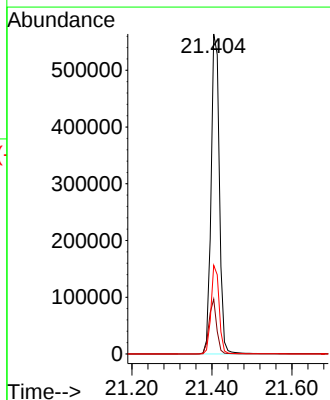
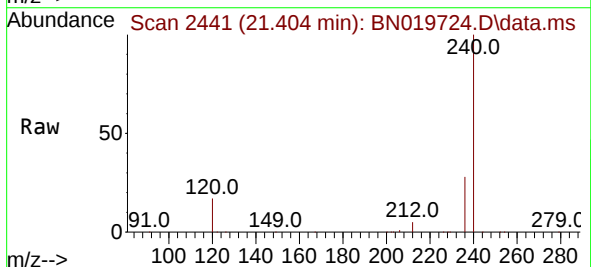


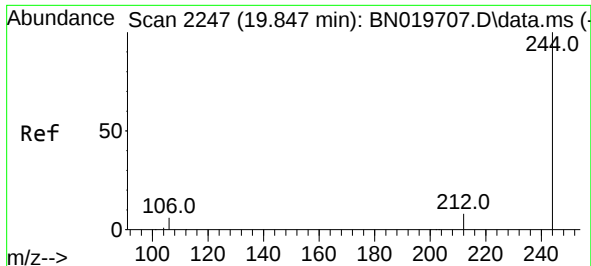

#31
 Terphenyl-d14
 Concen: 63.902 ng
 RT: 19.851 min Scan# 21
 Delta R.T. 0.004 min
 Lab File: BN019724.D
 Acq: 11 May 2022 16:16

Instrument :
 BNA_N
 ClientSampleId :
 PB144864BL

Tgt Ion:244 Resp: 2420190
 Ion Ratio Lower Upper
 244 100
 212 9.7 7.0 10.6
 122 0.0 0.0 0.0

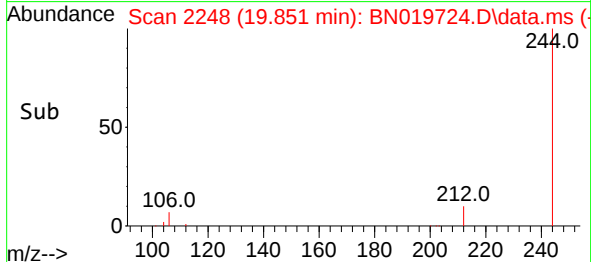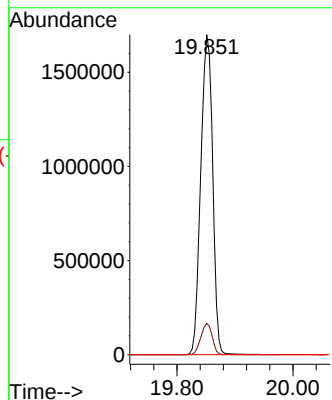

#35
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.752 min Scan# 3013
 Delta R.T. 0.012 min
 Lab File: BN019724.D
 Acq: 11 May 2022 16:16

Tgt Ion:264 Resp: 779800
 Ion Ratio Lower Upper
 264 100
 260 25.6 20.8 31.2
 265 21.5 35.6 53.4#

