
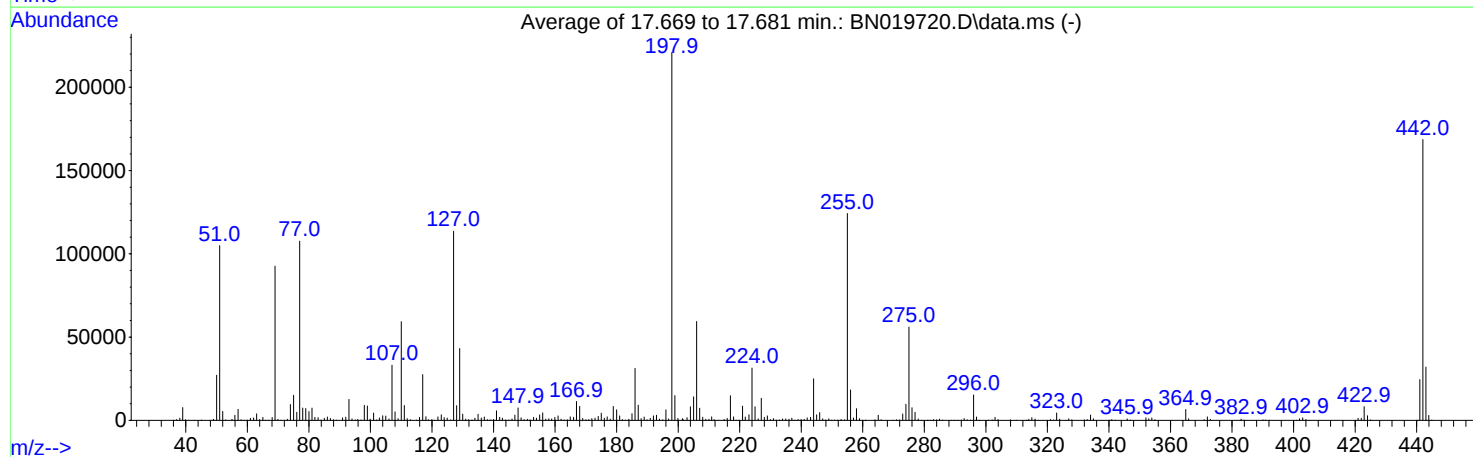


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019720.D
 Acq On : 11 May 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 10 01:35:26 2022

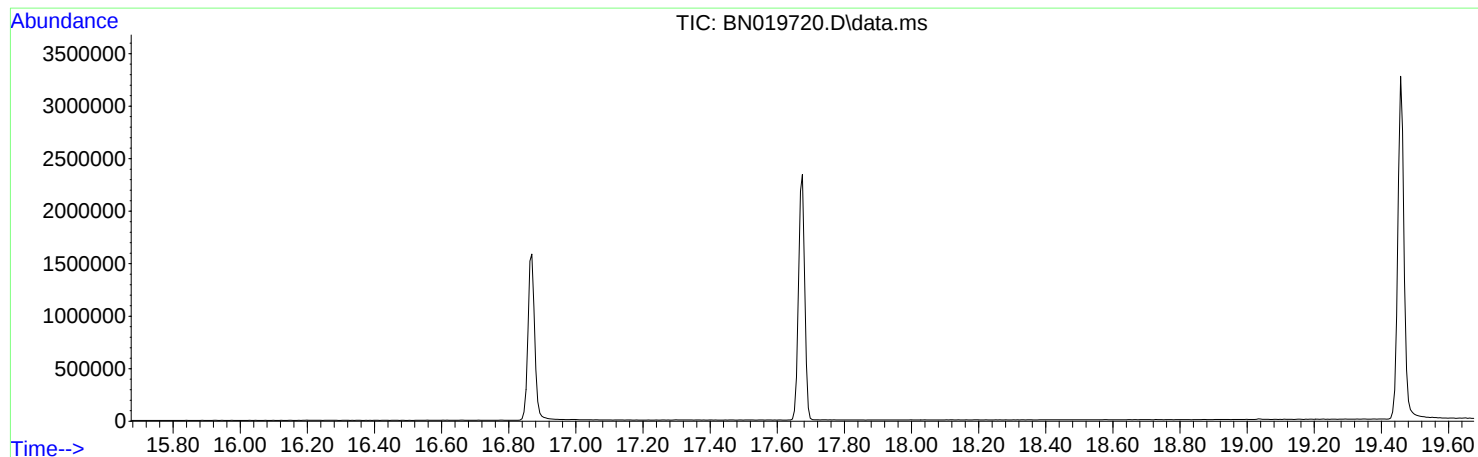




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	104940	PASS
68	69	0.00	2	1.9	1719	PASS
69	198	0.00	100	41.9	92616	PASS
70	69	0.00	2	0.6	583	PASS
127	198	10	80	51.4	113573	PASS
197	198	0.00	2	0.4	899	PASS
198	198	100	100	100.0	220885	PASS
199	198	5	9	6.7	14850	PASS
275	198	10	60	25.4	56000	PASS
365	198	1	100	2.9	6504	PASS
441	198	0.01	100	11.1	24509	PASS
442	442	50	100	100.0	168619	PASS
443	442	15	24	19.0	32021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019720.D
 Acq On : 11 May 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 12 09:55:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

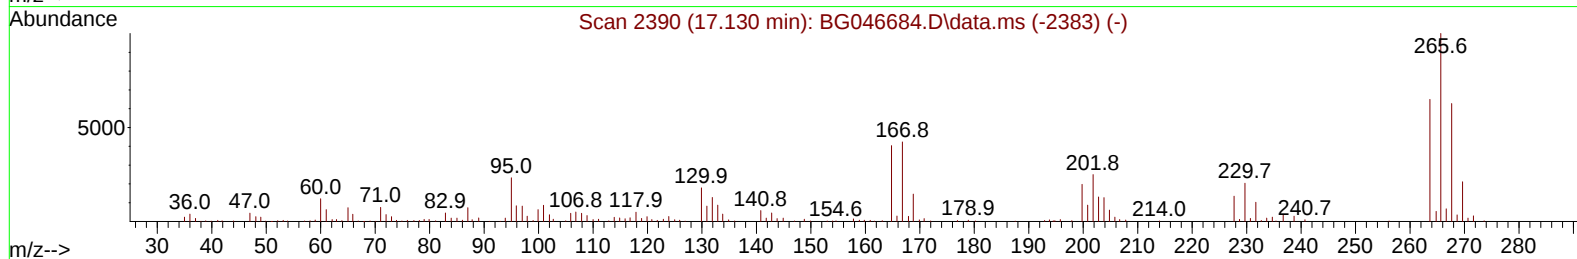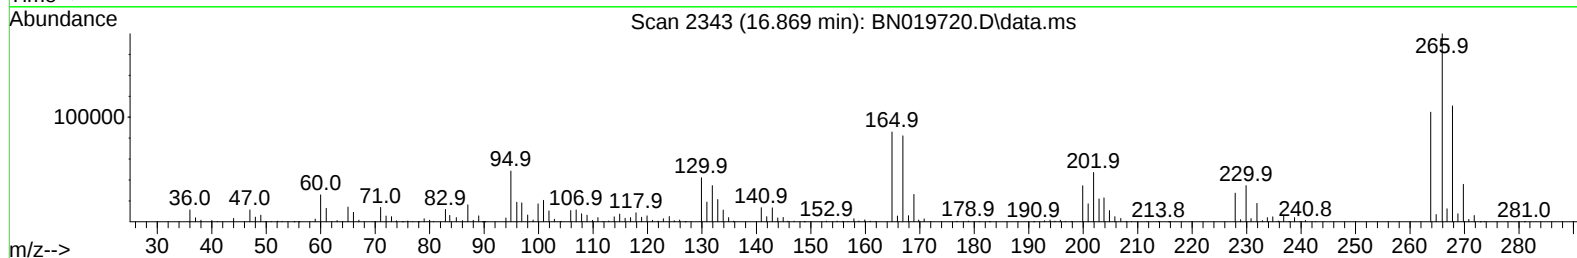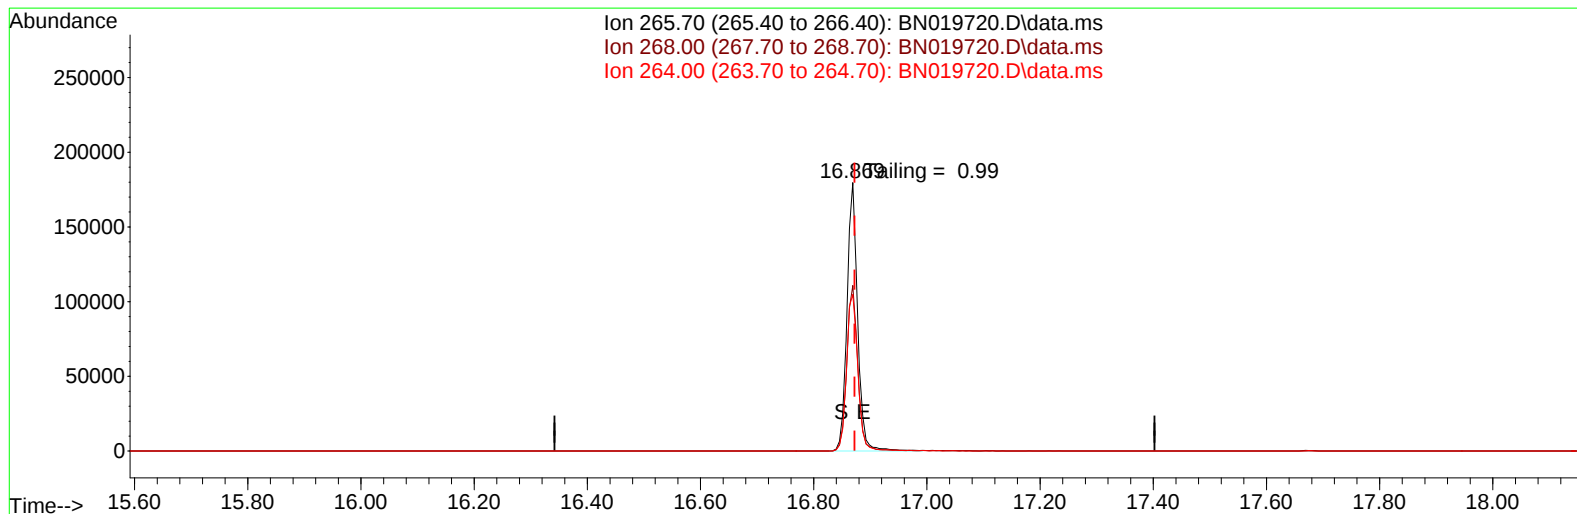

TIC: BN019720.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 19362.70 ng




response 235832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.64
264.00	61.60	58.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
Data File : BN019720.D
Acq On : 11 May 2022 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 09:55:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

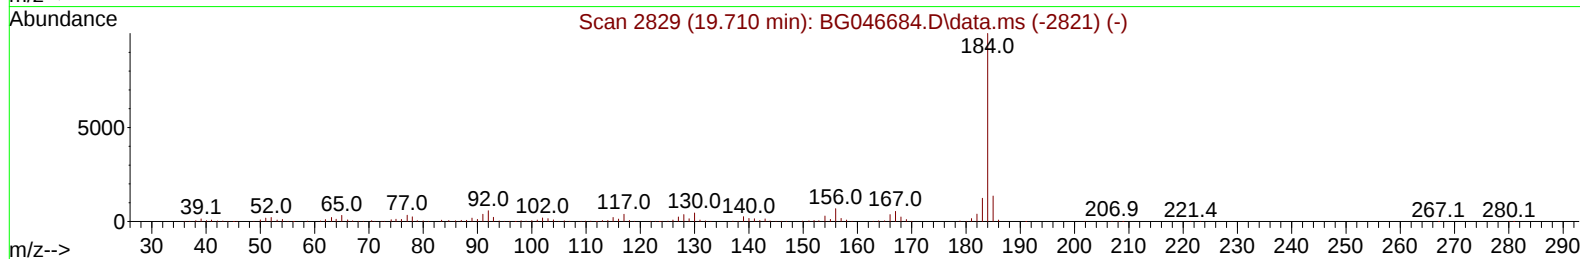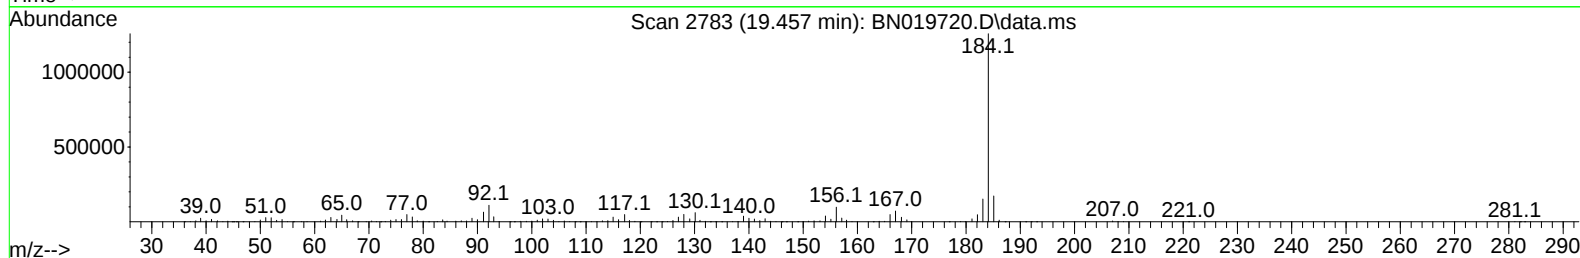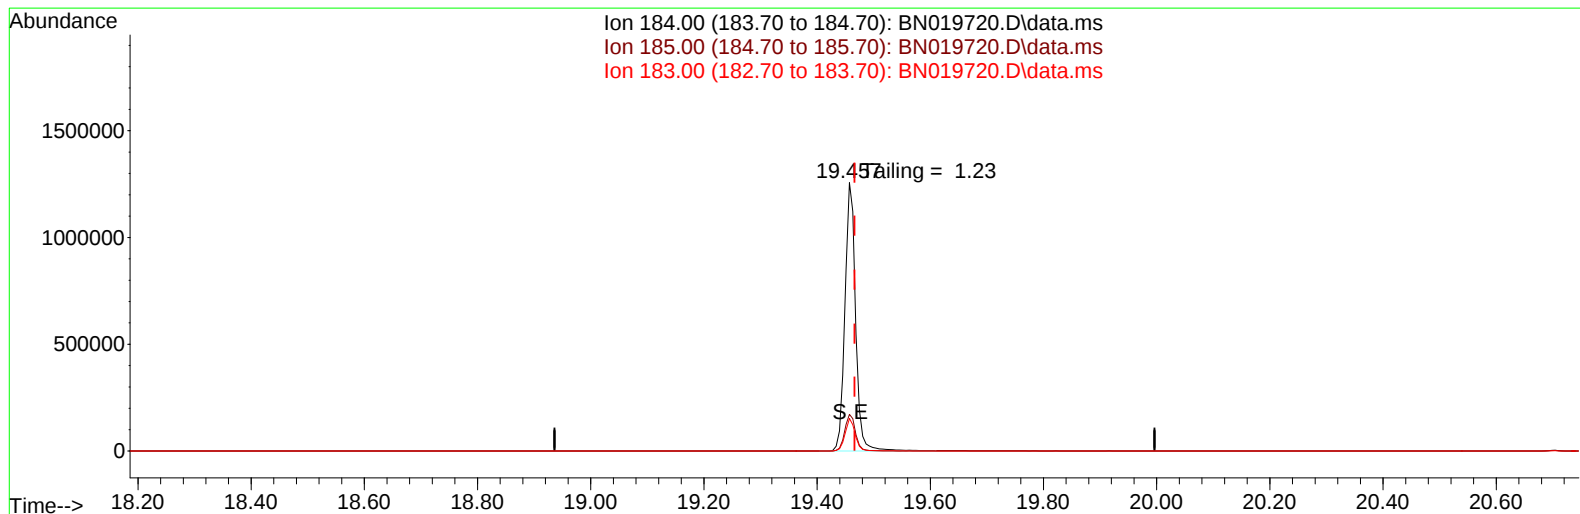

TIC: BN019720.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1655980

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.68
183.00	13.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2022	BNA_N	<u>BN019720.D</u>
Compound Name	Response	Retention Time
DDT	739575	20.704
DDD	5297	20.257
DDE	154	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5451	745026	0.73

Instrument :
BNA_N
ClientSampleId :
DFTPP