


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019732.D
 Acq On : 11 May 2022 21:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 10 01:35:26 2022

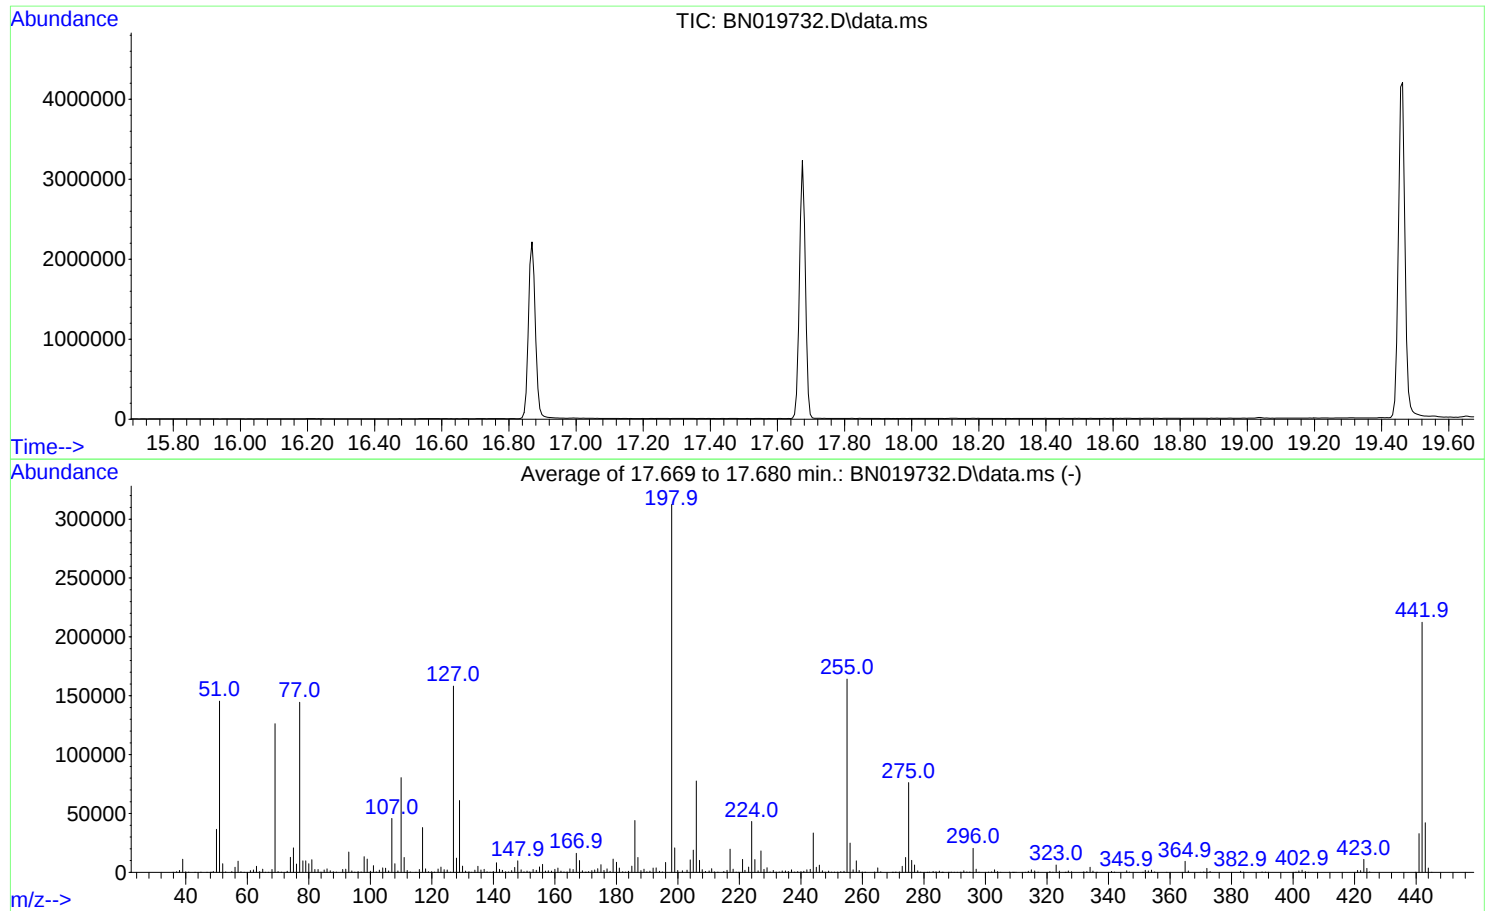




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	145455	PASS
68	69	0.00	2	1.9	2447	PASS
69	198	0.00	100	40.4	126224	PASS
70	69	0.00	2	0.6	742	PASS
127	198	10	80	50.6	158251	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	312448	PASS
199	198	5	9	6.7	20795	PASS
275	198	10	60	24.4	76299	PASS
365	198	1	100	3.0	9374	PASS
441	198	0.01	100	10.5	32917	PASS
442	442	50	100	100.0	212416	PASS
443	442	15	24	19.8	42152	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019732.D
 Acq On : 11 May 2022 21:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 12 10:00:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

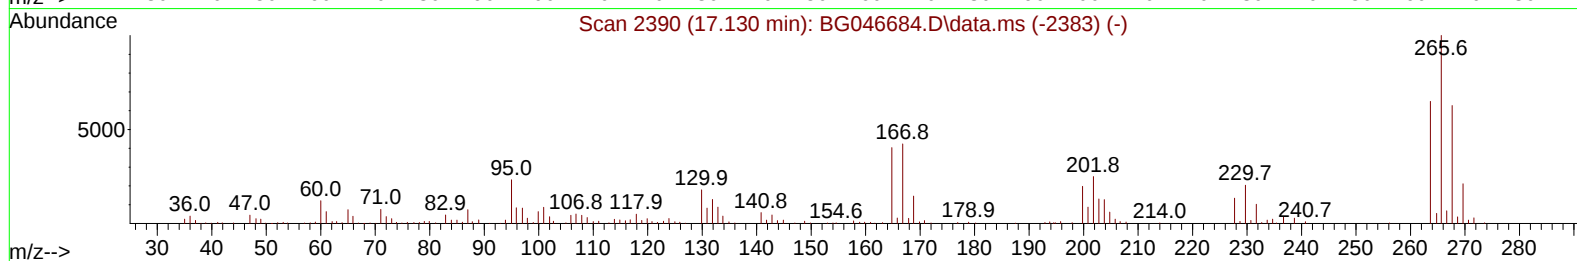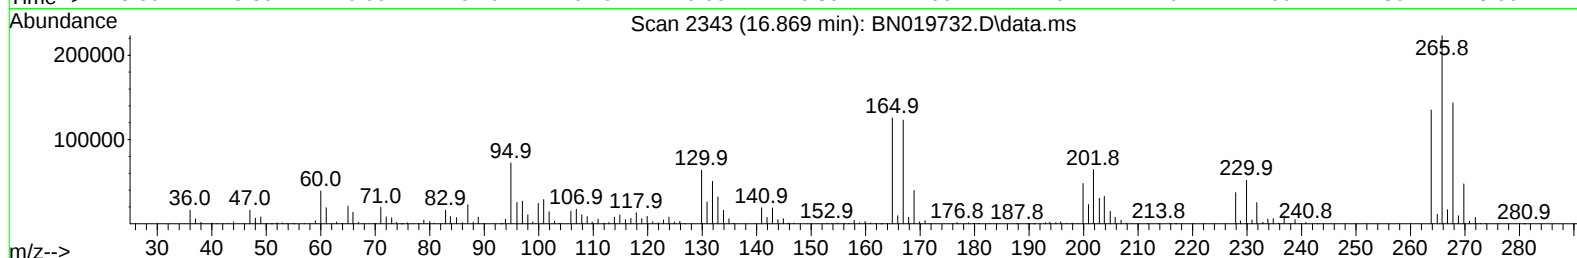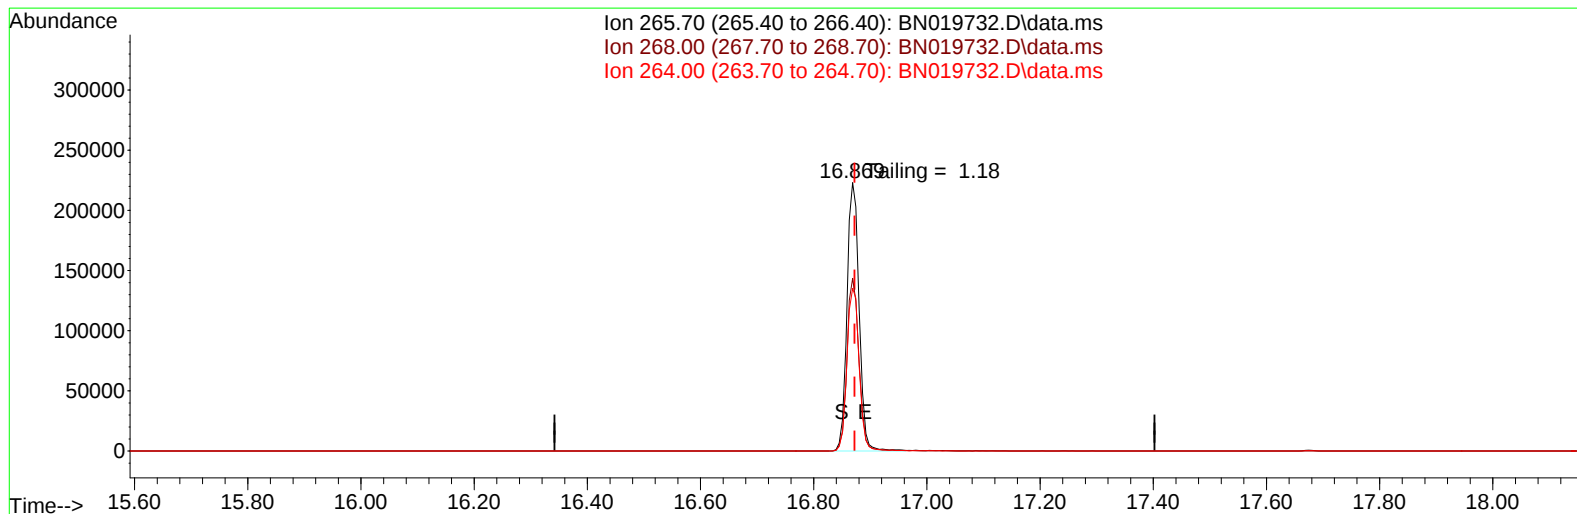

TIC: BN019732.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 19194.90 ng




response 330497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.31
264.00	61.60	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051122\
 Data File : BN019732.D
 Acq On : 11 May 2022 21:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 12 10:00:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

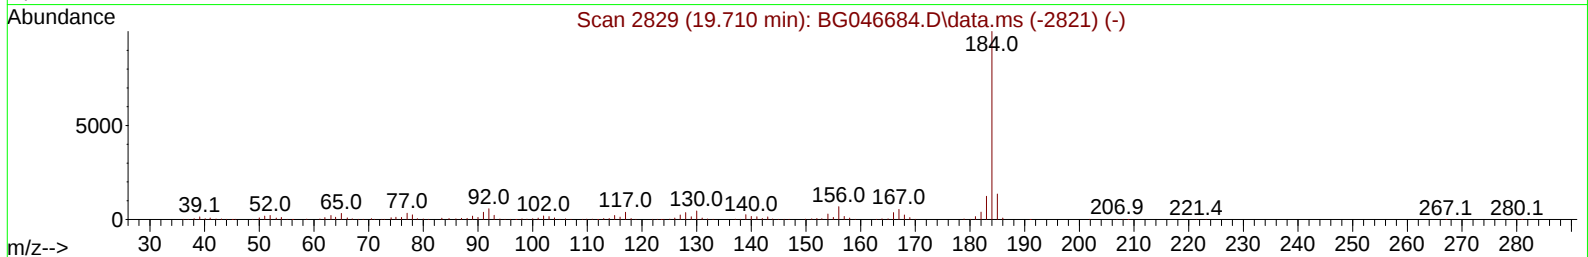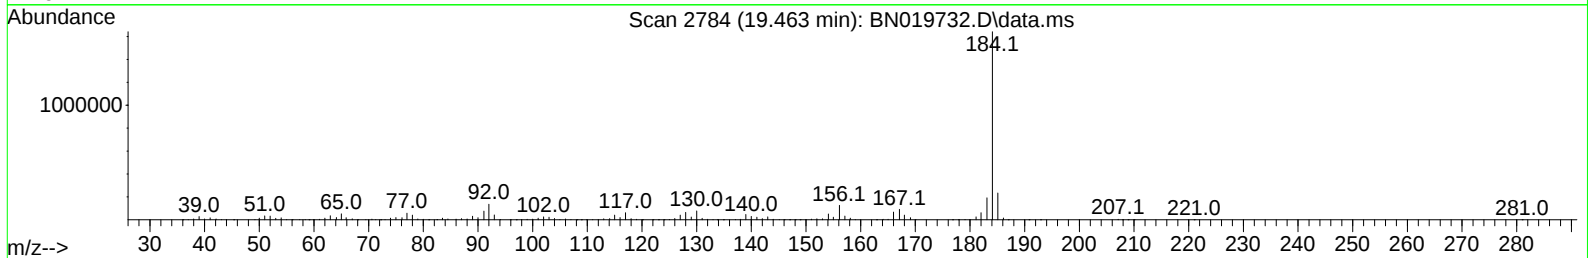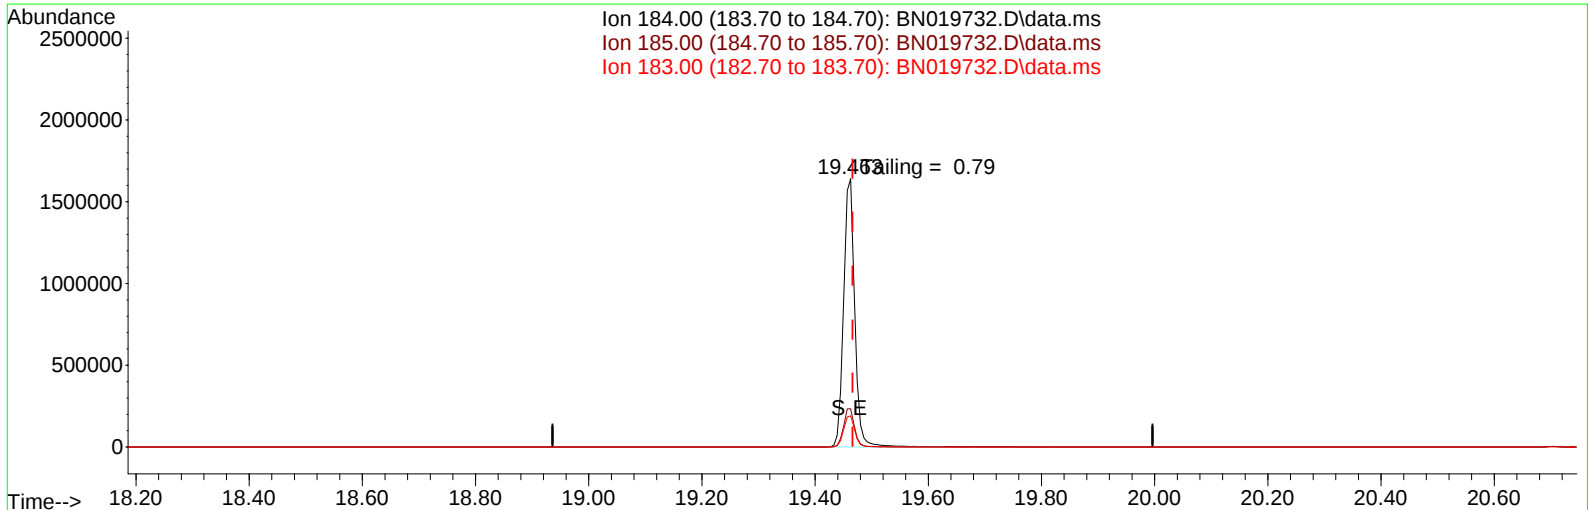

TIC: BN019732.D\data.ms

(77) Benzidine

19.463min (-0.003) 0.00 ng

response 2245970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2022	BNA_N	<u>BN019732.D</u>
Compound Name	Response	Retention Time
DDT	979415	20.704
DDD	10085	20.262
DDE	327	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10412	989827	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP