
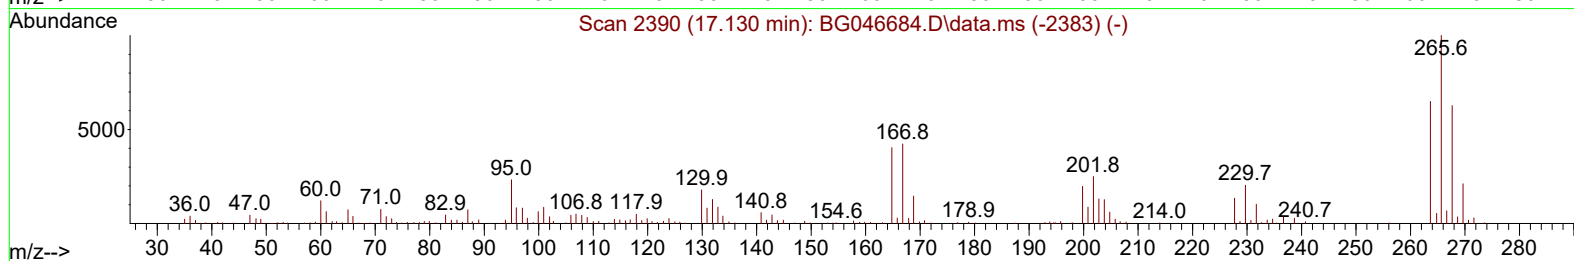
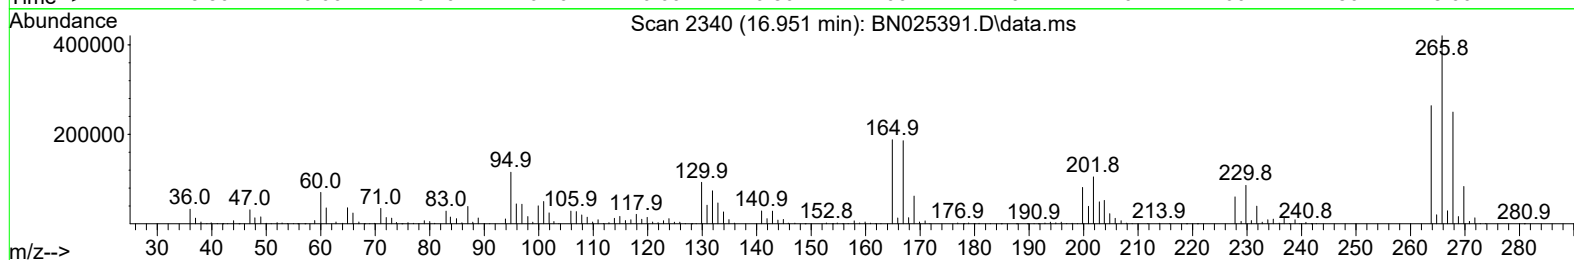


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025391.D
Acq On : 11 May 2023 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:09:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

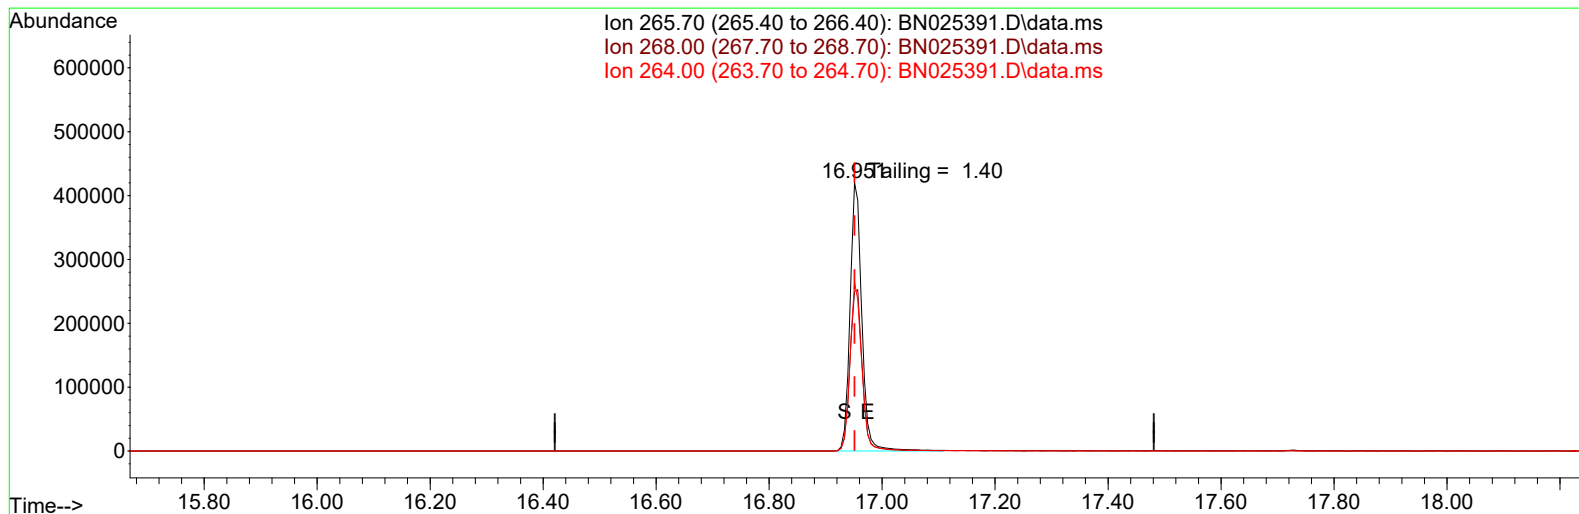

TIC: BN025391.D\data.ms

(70) Pentachlorophenol (C)




16.951min (0.000) 23752.72 ng

response 613833

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.46
264.00	61.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025391.D
Acq On : 11 May 2023 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:09:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

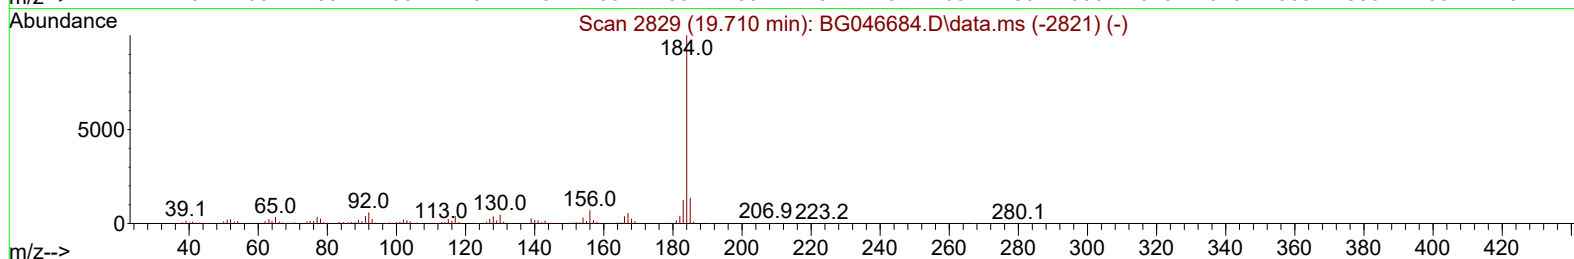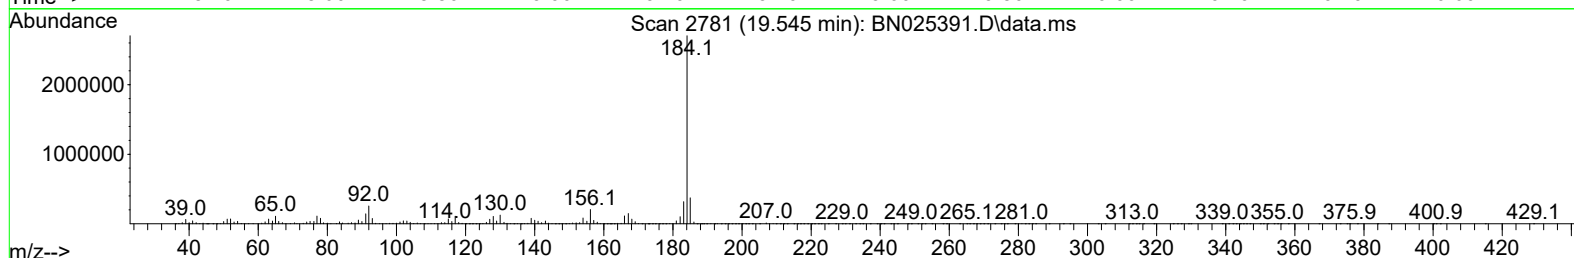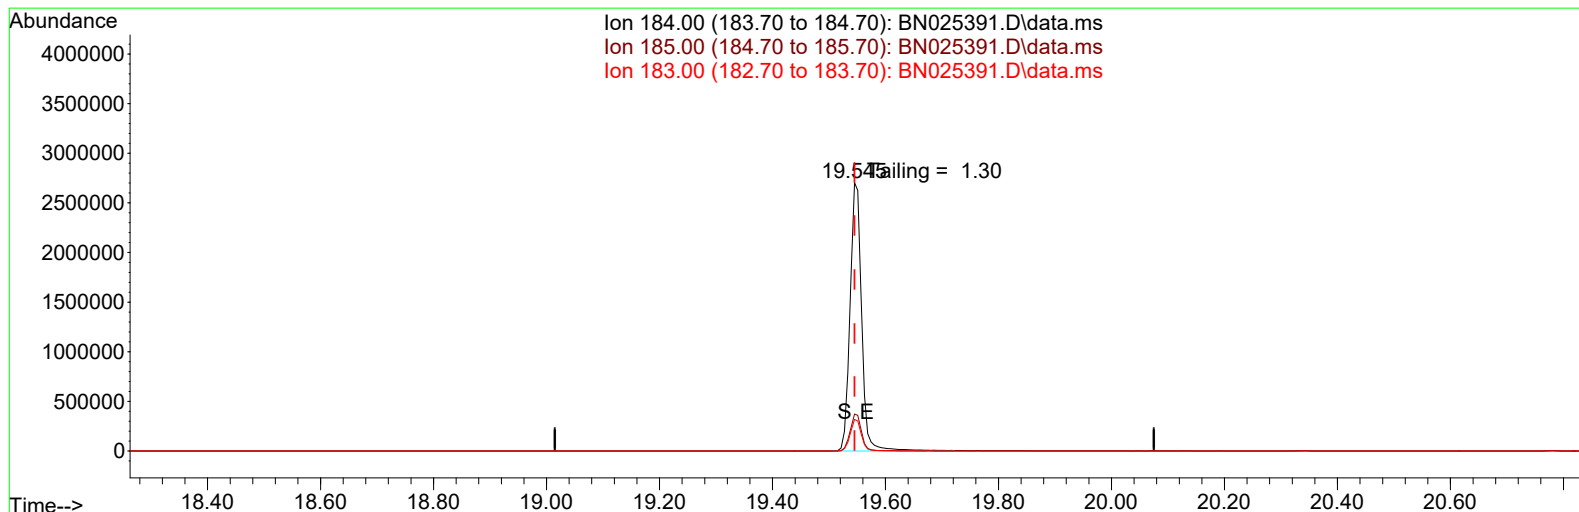

TIC: BN025391.D\data.ms

(77) Benzidine**19.545min (0.000) 208760.05 ng****response 3880369**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.75
0.00	0.00	0.00