
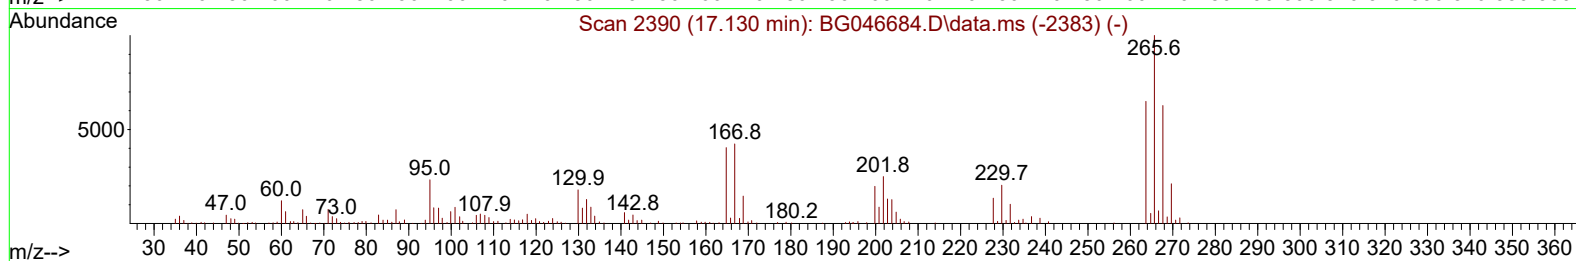
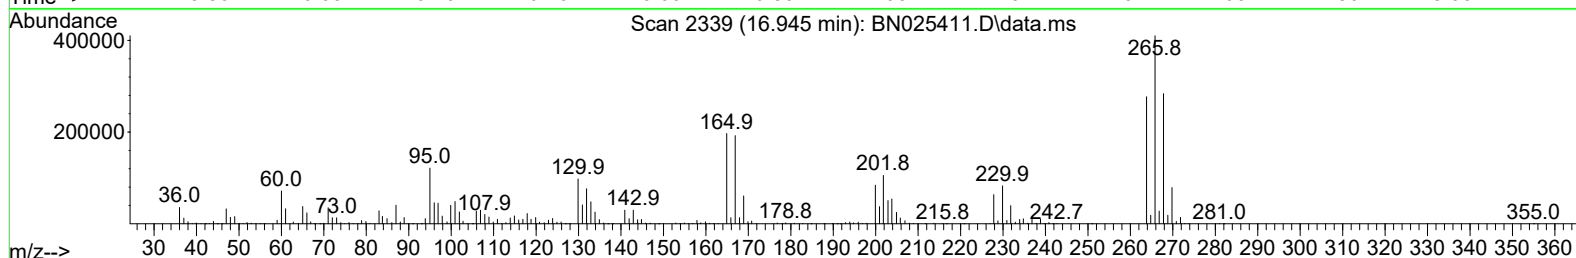


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
 Data File : BN025411.D
 Acq On : 11 May 2023 21:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:11:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 06:09:14 2023
 Response via : Initial Calibration

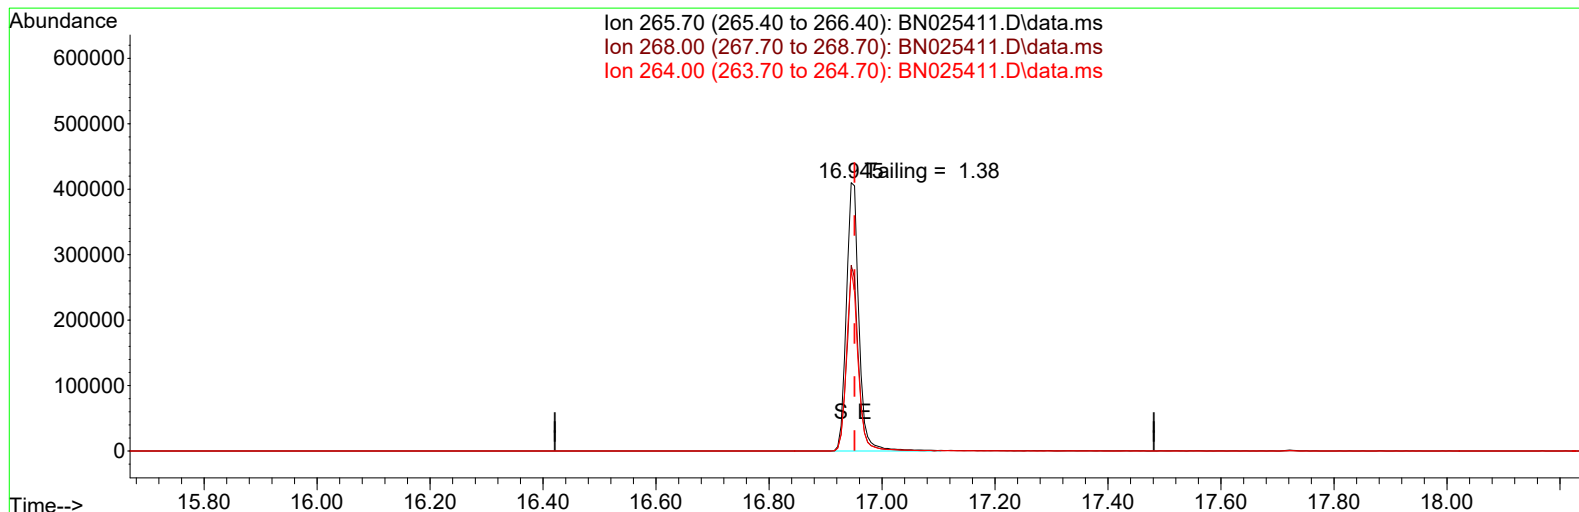

TIC: BN025411.D\data.ms

(70) Pentachlorophenol (C)




16.945min (-0.006) 25019.44 ng

response 632235

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.19
264.00	61.60	67.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025411.D
Acq On : 11 May 2023 21:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:11:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

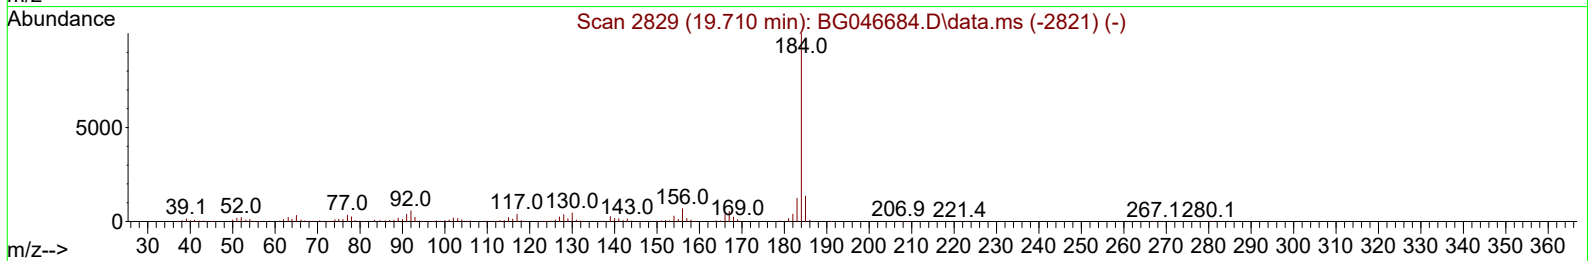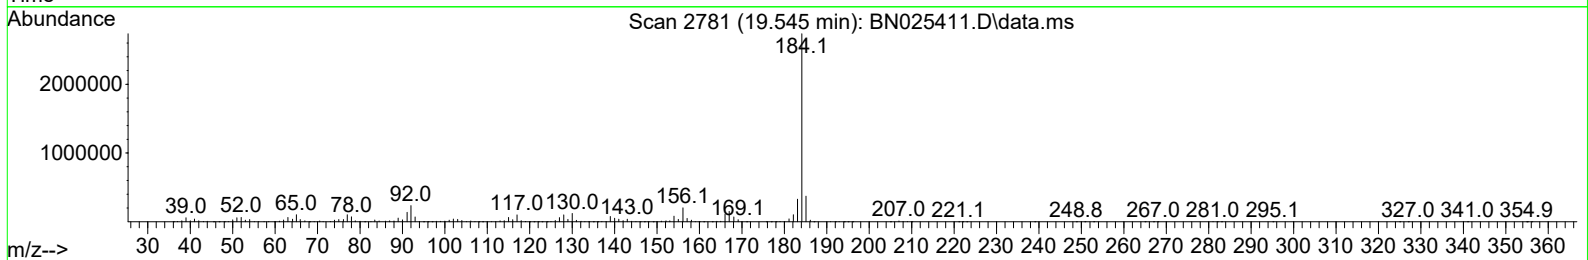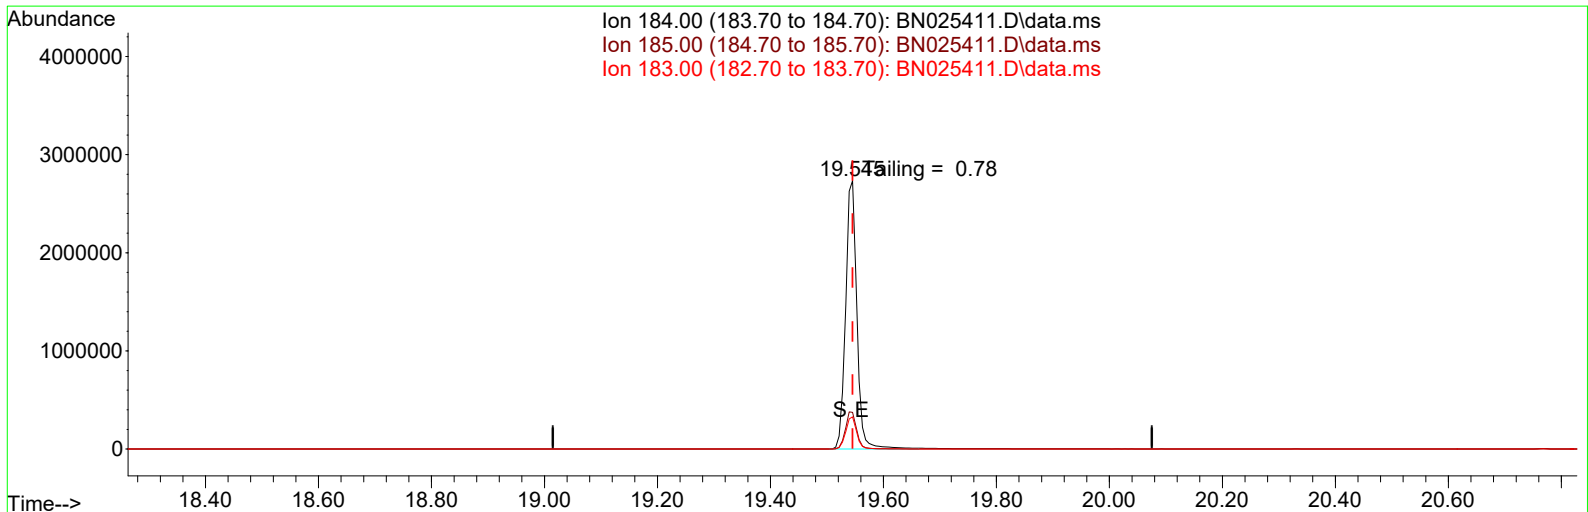

TIC: BN025411.D\data.ms

(77) Benzidine

19.545min (+ 0.000) 625498.16 ng

response 3798399

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	12.02
0.00	0.00	0.00