

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
 Data File : BN025407.D
 Acq On : 11 May 2023 18:55
 Operator : CG/JU
 Sample : 02723-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB-14-G1-SO-7.5-050923

Quant Time: May 12 04:01:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 00:57:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	7078	0.400	ng	0.00
7) Naphthalene-d8	10.718	136	21050	0.400	ng	0.01
13) Acenaphthene-d10	14.544	164	12786	0.400	ng	0.00
19) Phenanthrene-d10	17.298	188	27411	0.400	ng	0.00
29) Chrysene-d12	21.491	240	20250	0.400	ng	# 0.00
35) Perylene-d12	23.916	264	19078	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.463	112	4675	0.285	ng	0.00
5) Phenol-d6	7.088	99	4992	0.224	ng	0.00
8) Nitrobenzene-d5	9.105	82	3273	0.192	ng	0.02
11) 2-Methylnaphthalene-d10	12.317	152	6979	0.251	ng	0.01
14) 2,4,6-Tribromophenol	16.057	330	350	0.051	ng	0.00
15) 2-Fluorobiphenyl	13.176	172	9889	0.223	ng	0.00
27) Fluoranthene-d10	19.329	212	14846	0.237	ng	0.00
31) Terphenyl-d14	19.920	244	11413	0.234	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.383	149	4072	0.061	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025407.D
Acq On : 11 May 2023 18:55
Operator : CG/JU
Sample : 02723-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB-14-G1-SO-7.5-050923


Quant Time: May 12 04:01:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 00:57:16 2023
Response via : Initial Calibration

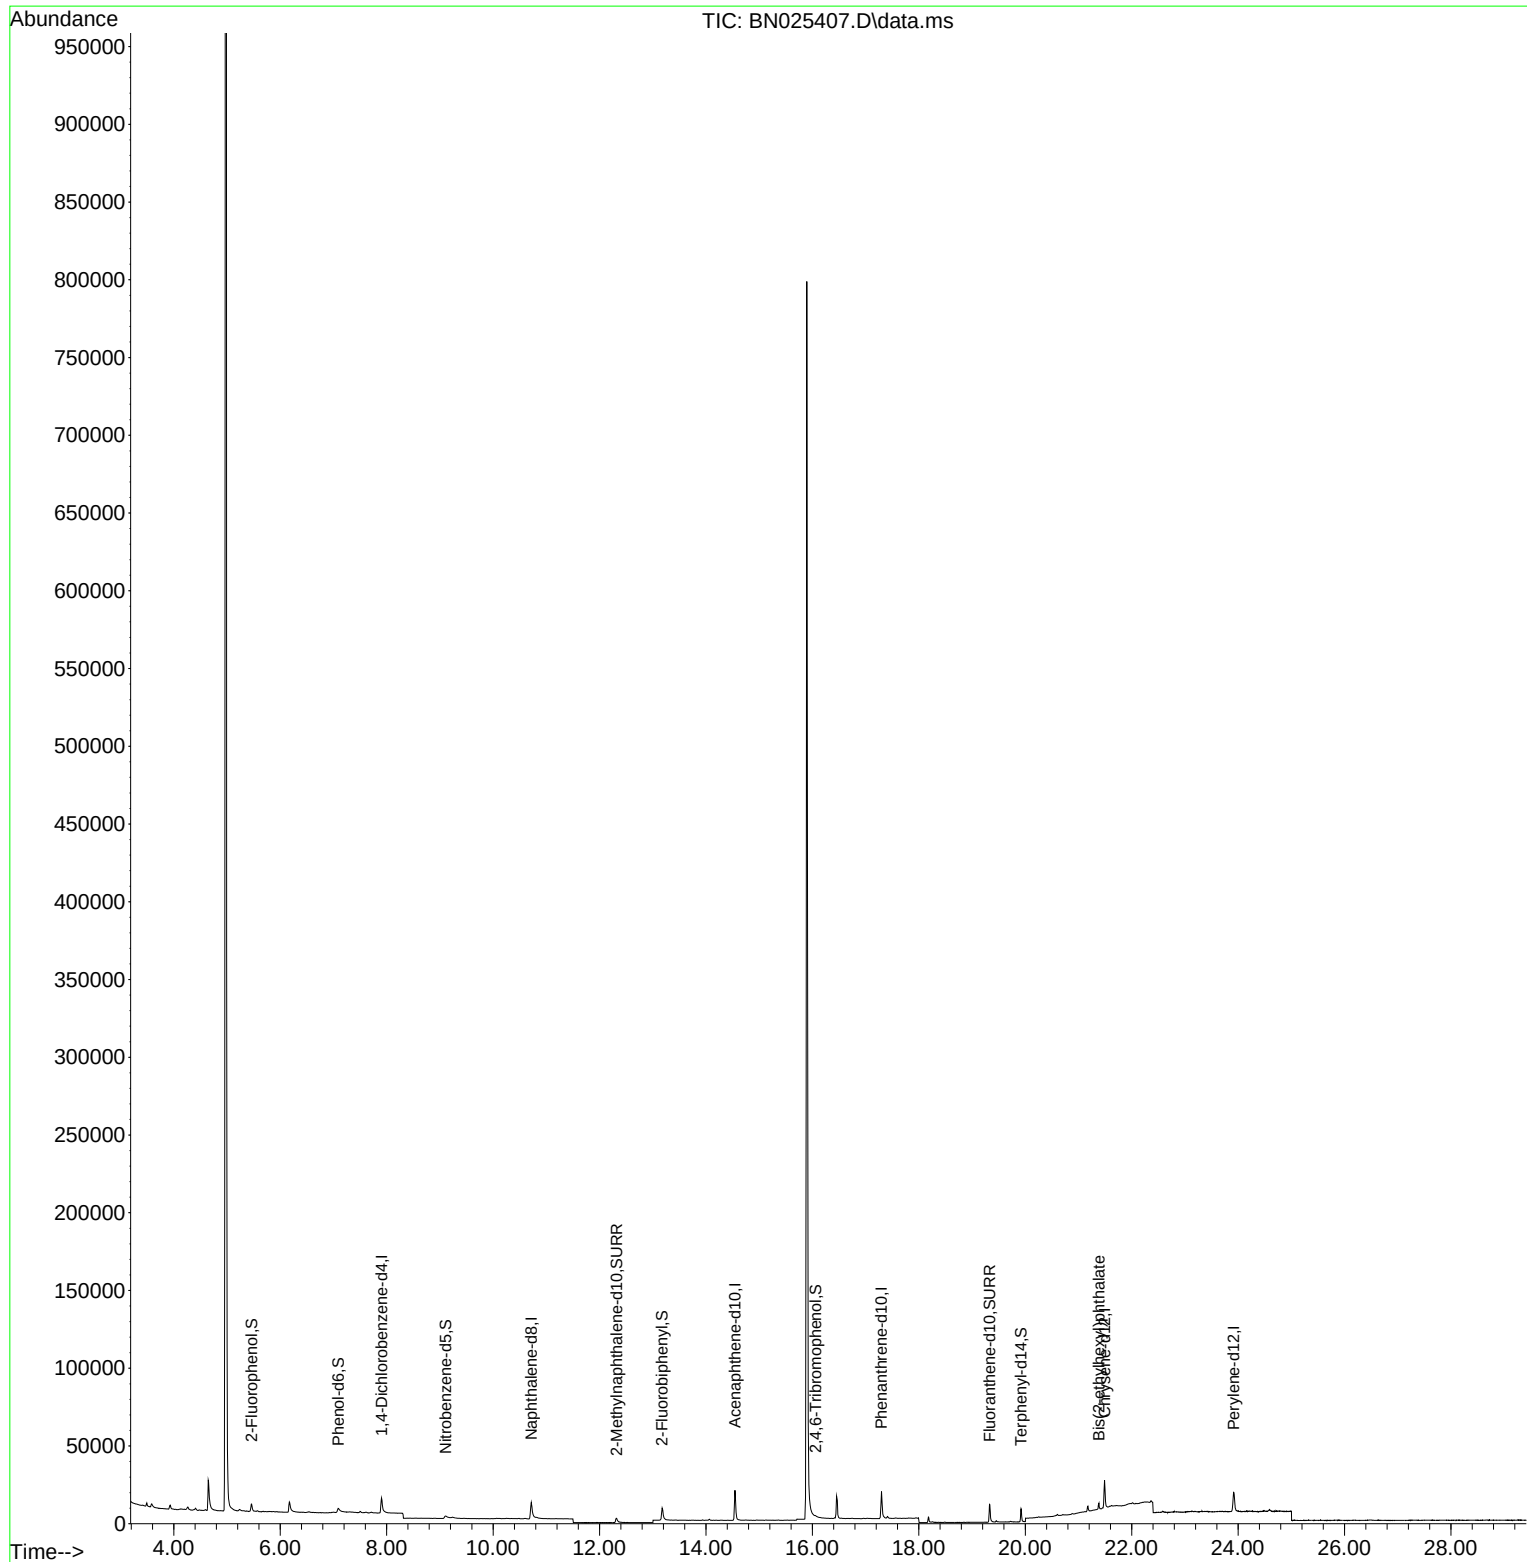

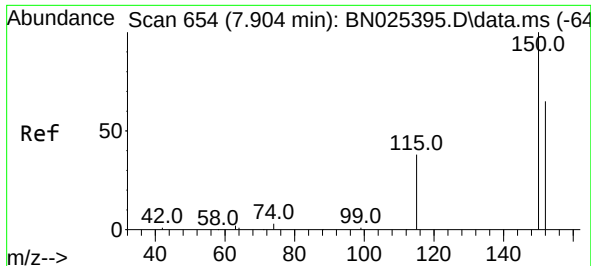




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.904 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN025407.D
 Acq: 11 May 2023 18:55

Instrument :
 BNA_N
 ClientSampleId :
 CB-14-G1-SO-7.5-050923

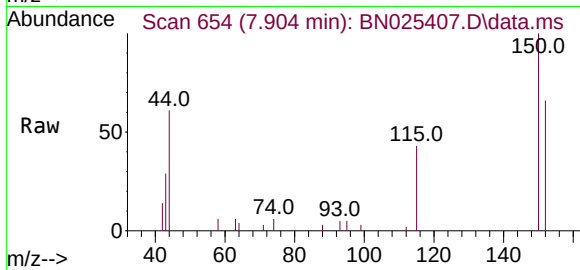

Tgt Ion:152 Resp: 7078




Ion	Ratio	Lower	Upper
152	100		
150	151.2	121.4	182.2
115	65.0	50.6	76.0

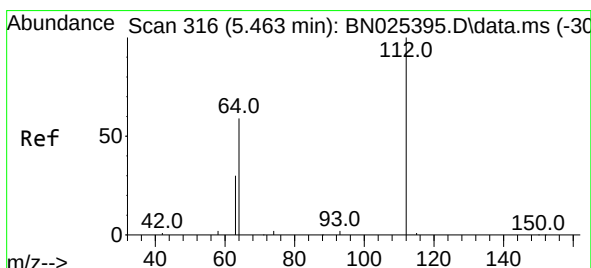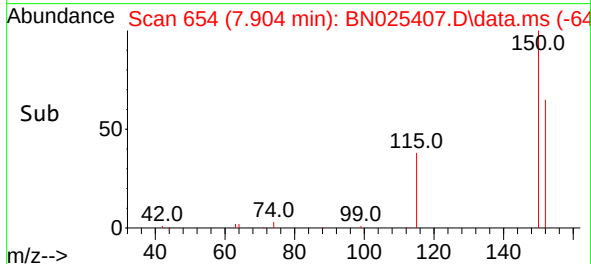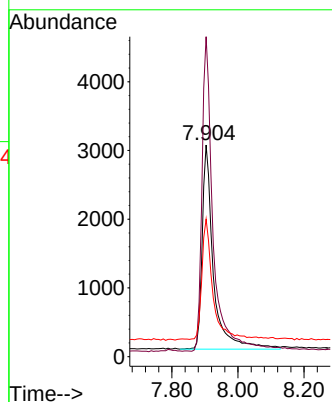


#4
 2-Fluorophenol
 Concen: 0.285 ng
 RT: 5.463 min Scan# 316
 Delta R.T. 0.000 min
 Lab File: BN025407.D
 Acq: 11 May 2023 18:55

Tgt Ion:112 Resp: 4675

Ion	Ratio	Lower	Upper
112	100		
64	64.4	51.9	77.9
63	35.4	27.4	41.2

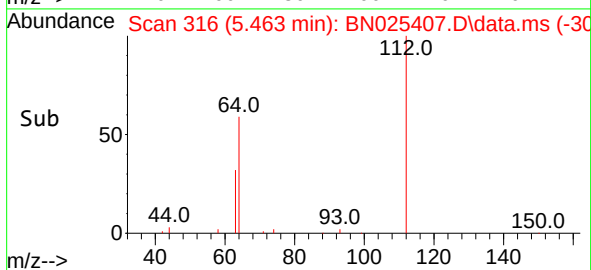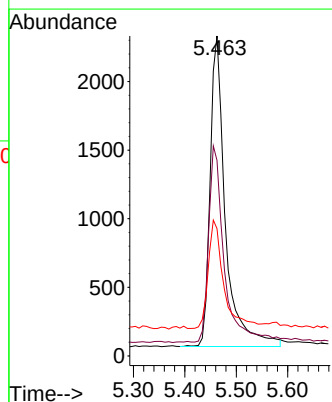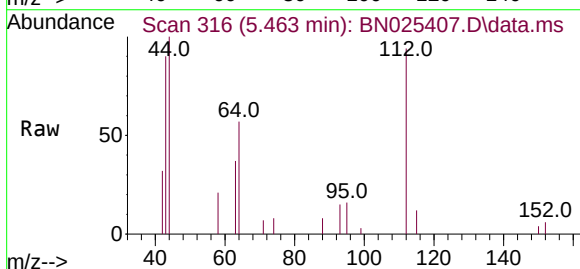

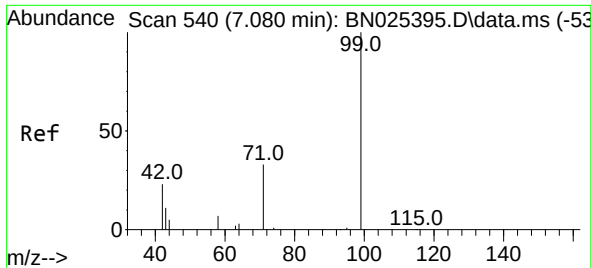

#5

Phenol-d6

Concen: 0.224 ng

RT: 7.088 min Scan# 541

Delta R.T. 0.007 min

Lab File: BN025407.D


Acq: 11 May 2023 18:55

Instrument :




BNA_N

ClientSampleId :

CB-14-G1-SO-7.5-050923

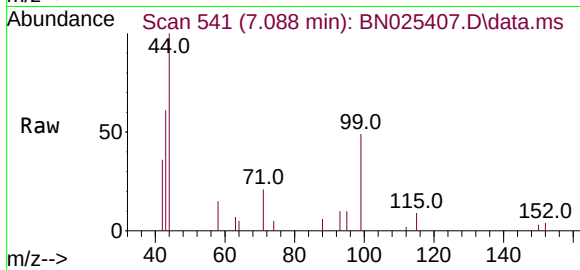

Tgt Ion:	99	Resp:	4992
Ion Ratio	100		
Lower	23.5		
Upper	35.3		
42	22.4	23.5	35.3
71	32.9	28.1	42.1

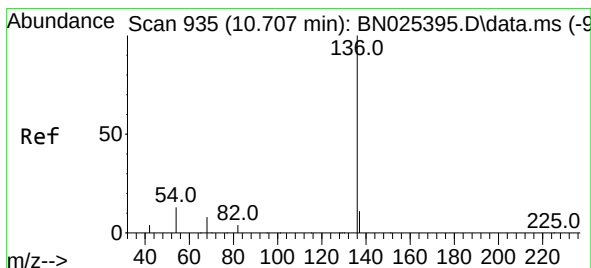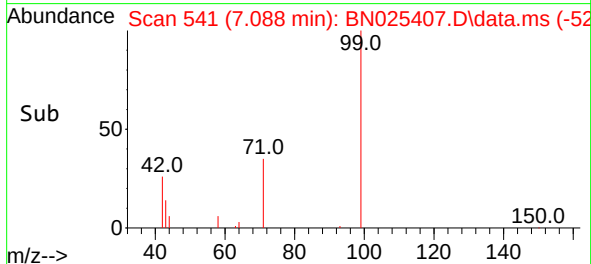

#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.718 min Scan# 936


Delta R.T. 0.011 min

Lab File: BN025407.D

Acq: 11 May 2023 18:55

Tgt Ion:	136	Resp:	21050
Ion Ratio	100		
Lower	9.1		
Upper	13.7		
137	11.8	9.1	13.7
54	12.8	11.2	16.8
68	8.7	7.4	11.0


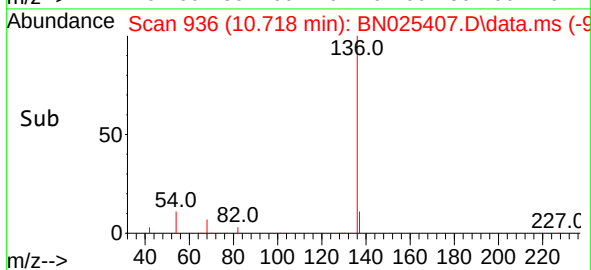

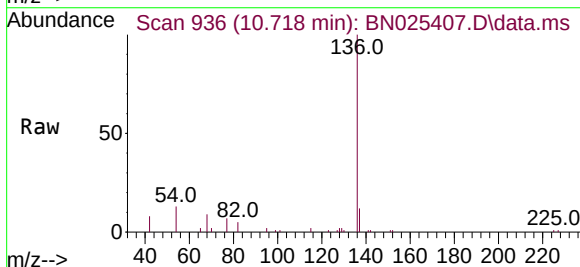


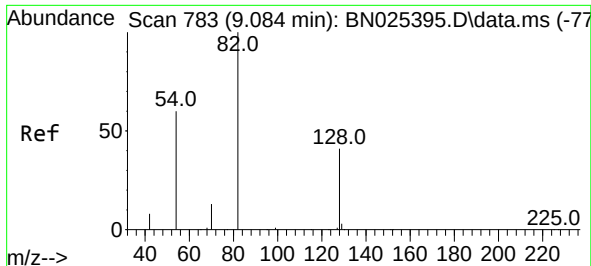

#8
Nitrobenzene-d5
Concen: 0.192 ng
RT: 9.105 min Scan# 783
Delta R.T. 0.021 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55




Instrument :
BNA_N
ClientSampleId :
CB-14-G1-SO-7.5-050923


Tgt Ion: 82 Resp: 3273
Ion Ratio Lower Upper
82 100
128 51.6 35.8 53.8
54 74.7 50.4 75.6

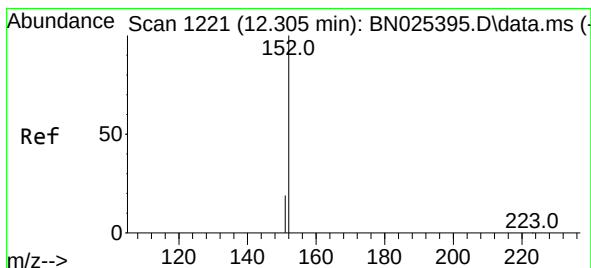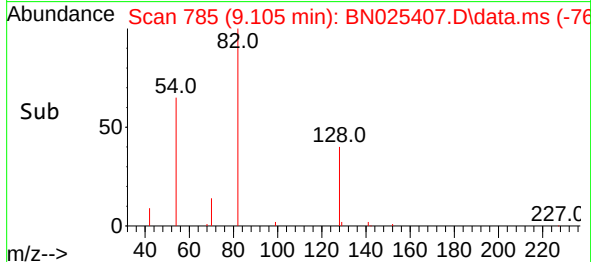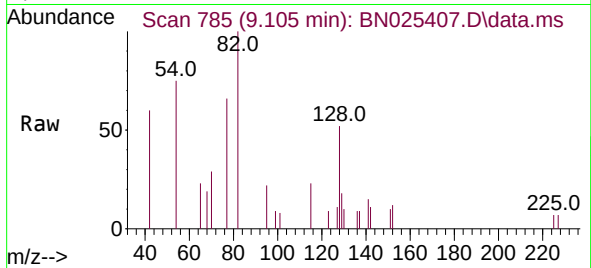

#11
2-Methylnaphthalene-d10
Concen: 0.251 ng
RT: 12.317 min Scan# 1224
Delta R.T. 0.011 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55

Tgt Ion: 152 Resp: 6979
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1


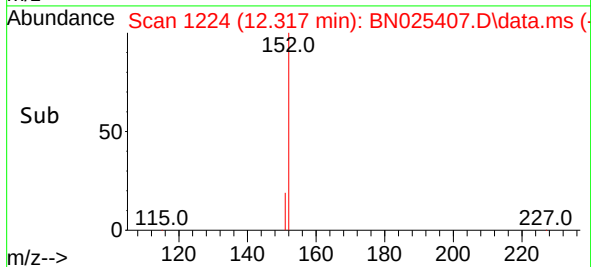

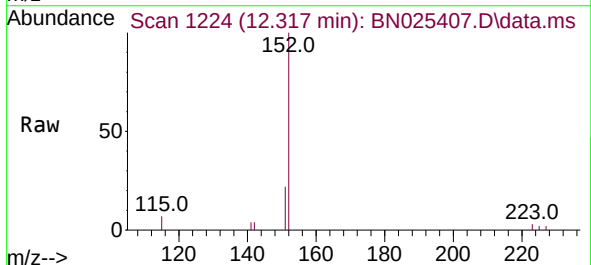


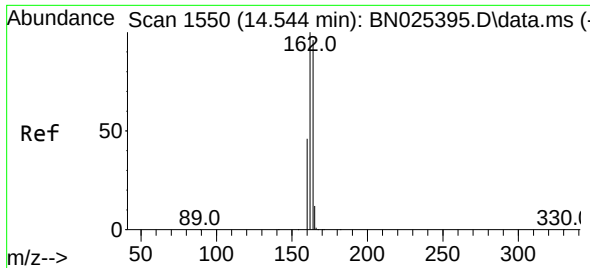

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.544 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55




Instrument :
BNA_N
ClientSampleId :
CB-14-G1-SO-7.5-050923


Tgt Ion:164 Resp: 12786
Ion Ratio Lower Upper
164 100
162 105.1 83.2 124.8
160 49.4 38.8 58.2

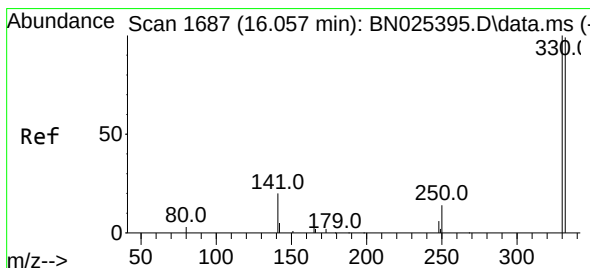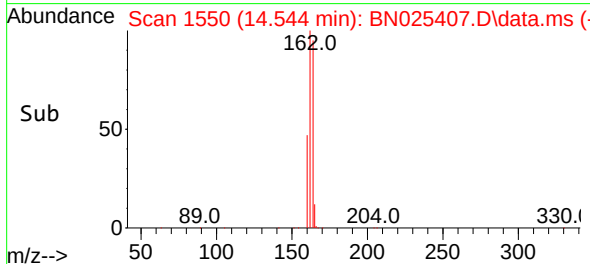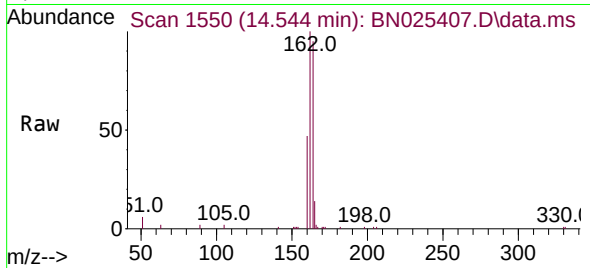

#14
2,4,6-Tribromophenol
Concen: 0.051 ng
RT: 16.057 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55

Tgt Ion:330 Resp: 350
Ion Ratio Lower Upper
330 100
332 102.3 78.0 117.0
141 52.9 30.2 45.2#


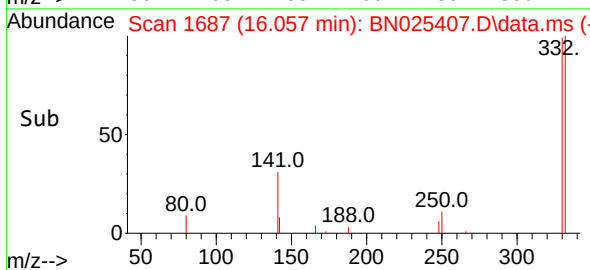

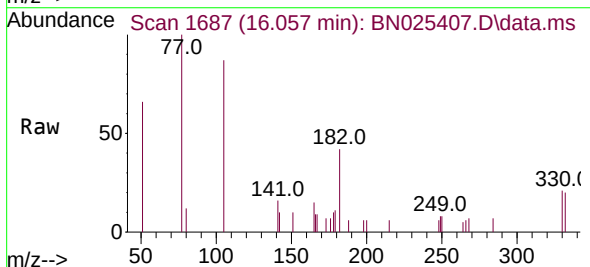


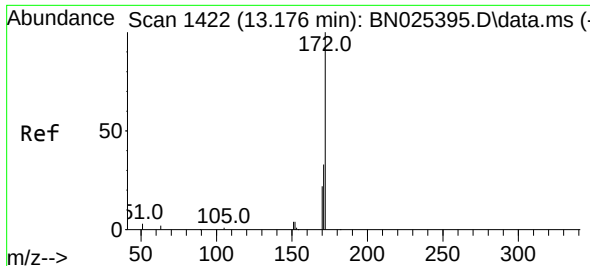

#15
2-Fluorobiphenyl
Concen: 0.223 ng
RT: 13.176 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55




Instrument :
BNA_N
ClientSampleId :
CB-14-G1-SO-7.5-050923


Tgt Ion:	172	Resp:	9889
Ion	Ratio	Lower	Upper
172	100		
171	35.7	26.7	40.1
170	24.4	17.8	26.8

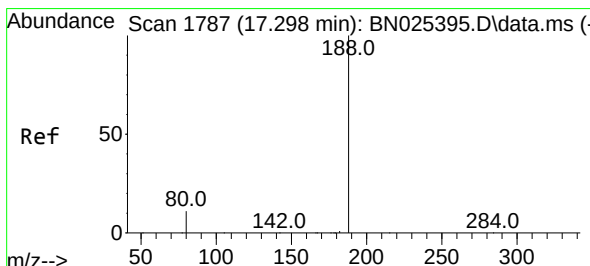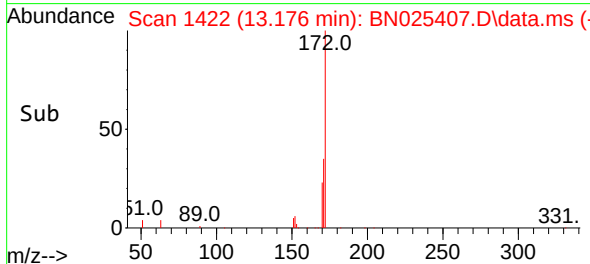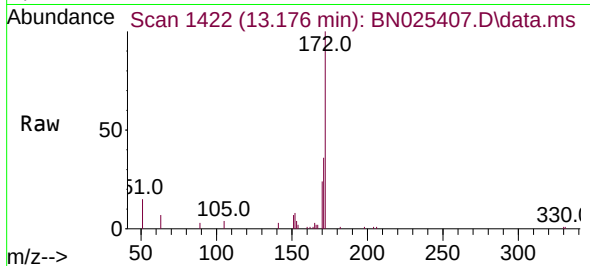

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.298 min Scan# 1787
Delta R.T. 0.000 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55

Tgt Ion:	188	Resp:	27411
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.8	9.4	14.2


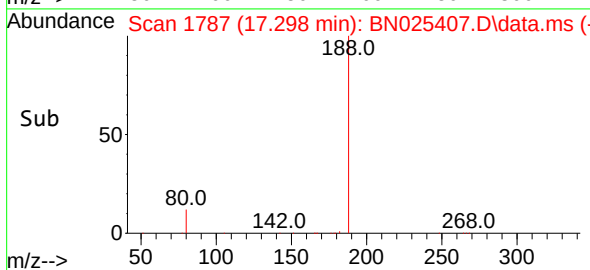

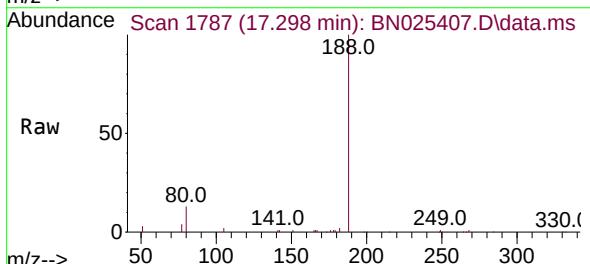


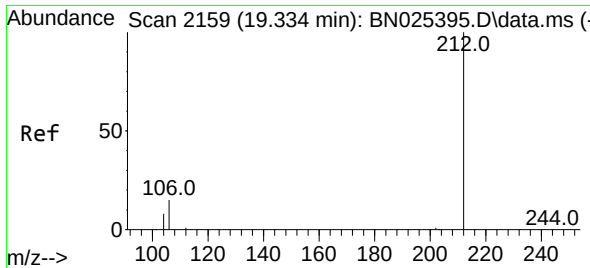

#27
Fluoranthene-d10
Concen: 0.237 ng
RT: 19.329 min Scan# 2158
Delta R.T. -0.004 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55




Instrument :
BNA_N
ClientSampleId :
CB-14-G1-SO-7.5-050923


Tgt Ion:212 Resp: 14846
Ion Ratio Lower Upper
212 100
106 16.5 12.6 19.0
104 10.0 7.0 10.4

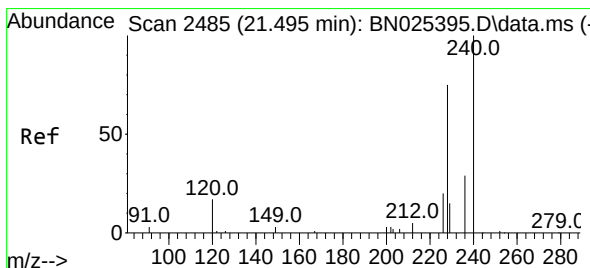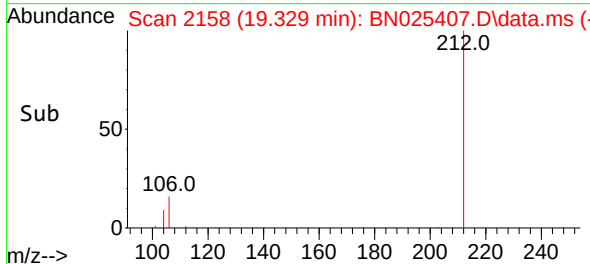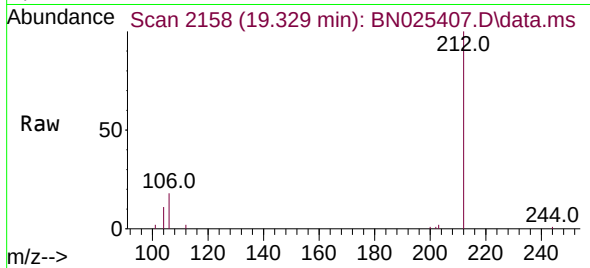

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.491 min Scan# 2484
Delta R.T. -0.004 min
Lab File: BN025407.D
Acq: 11 May 2023 18:55

Tgt Ion:240 Resp: 20250
Ion Ratio Lower Upper
240 100
120 17.5 19.0 28.6#
236 29.1 25.0 37.6


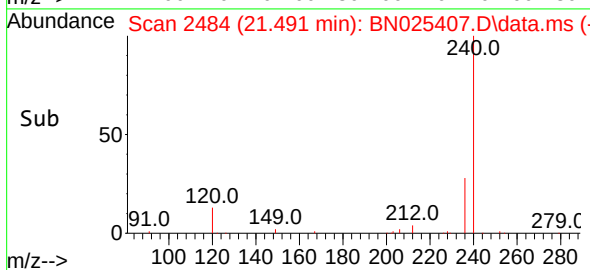

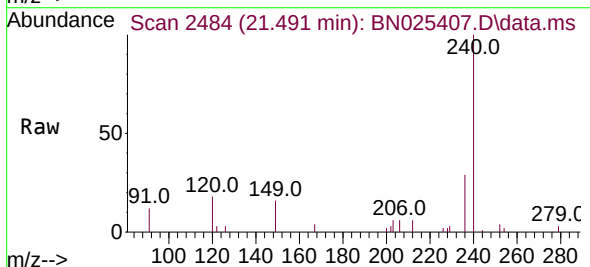


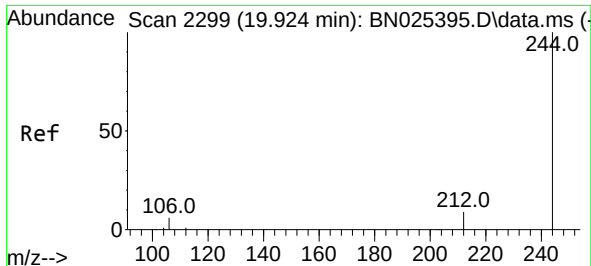

#31
 Terphenyl-d14
 Concen: 0.234 ng
 RT: 19.920 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN025407.D
 Acq: 11 May 2023 18:55




Instrument :
 BNA_N
 ClientSampleId :
 CB-14-G1-SO-7.5-050923


Tgt Ion:244 Resp: 11413
 Ion Ratio Lower Upper
 244 100
 212 9.8 7.5 11.3
 122 0.0 0.0 0.0

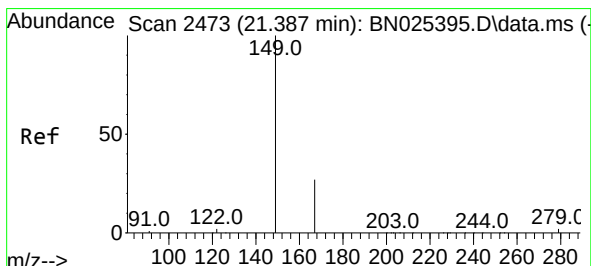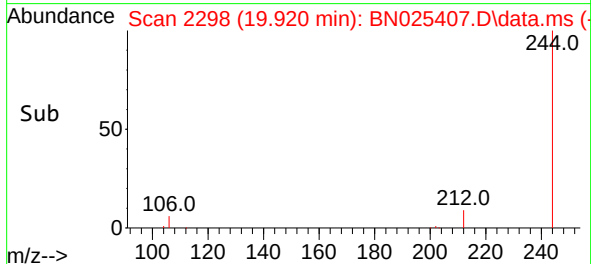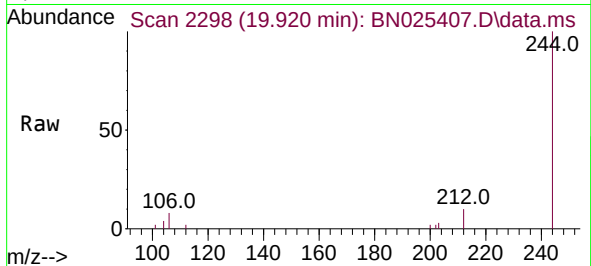

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.061 ng
 RT: 21.383 min Scan# 2472
 Delta R.T. -0.004 min
 Lab File: BN025407.D
 Acq: 11 May 2023 18:55


Tgt Ion:149 Resp: 4072
 Ion Ratio Lower Upper
 149 100
 167 26.2 21.7 32.5
 279 5.2 3.0 4.4#

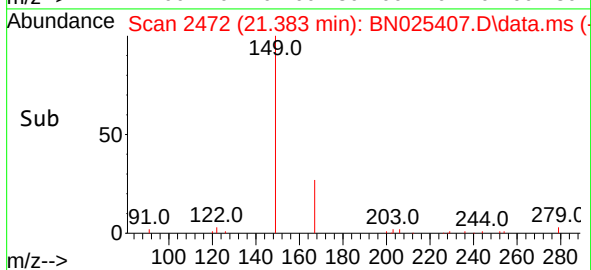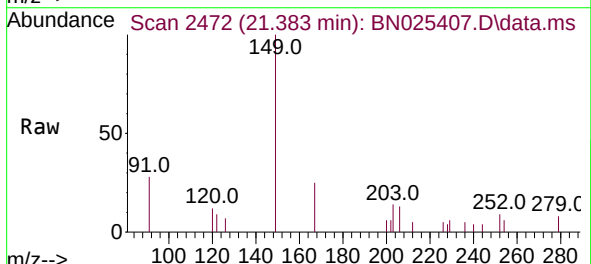

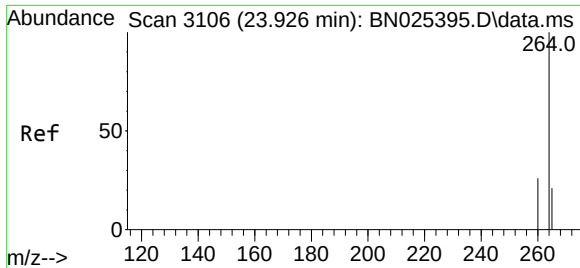

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.916 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: BN025407.D
 Acq: 11 May 2023 18:55

Instrument :
 BNA_N
 ClientSampleId :
 CB-14-G1-SO-7.5-050923

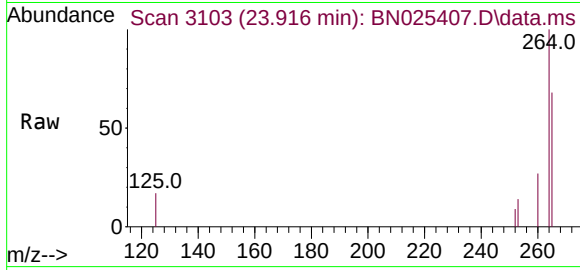

Tgt Ion:264 Resp: 19078

Ion	Ratio	Lower	Upper
264	100		
260	27.0	23.5	35.3
265	68.2	50.9	76.3

