
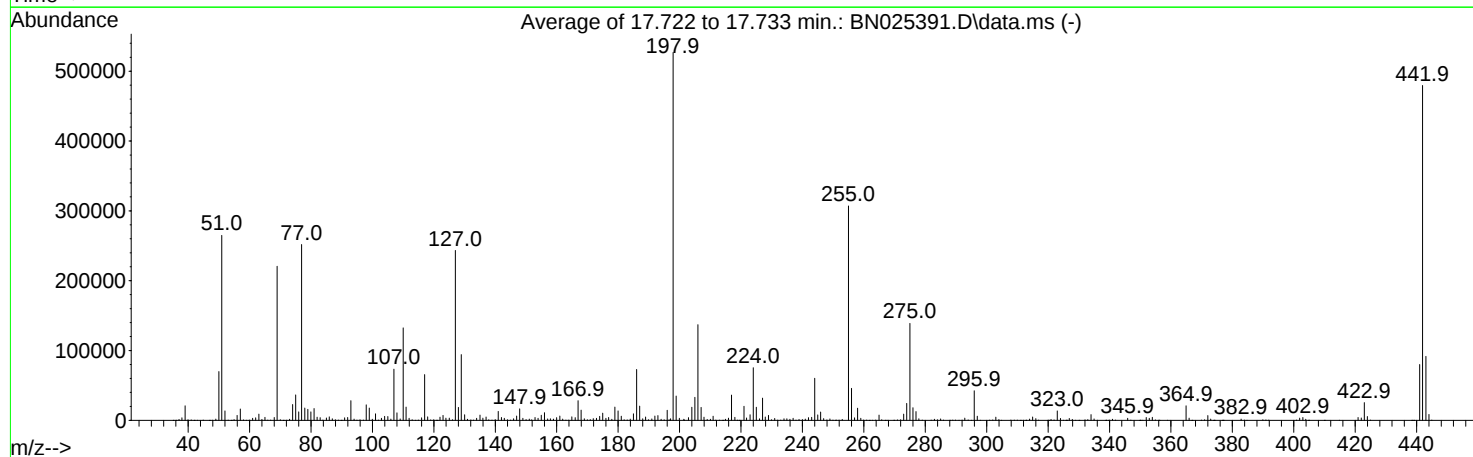


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025391.D
Acq On : 11 May 2023 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 00:57:16 2023

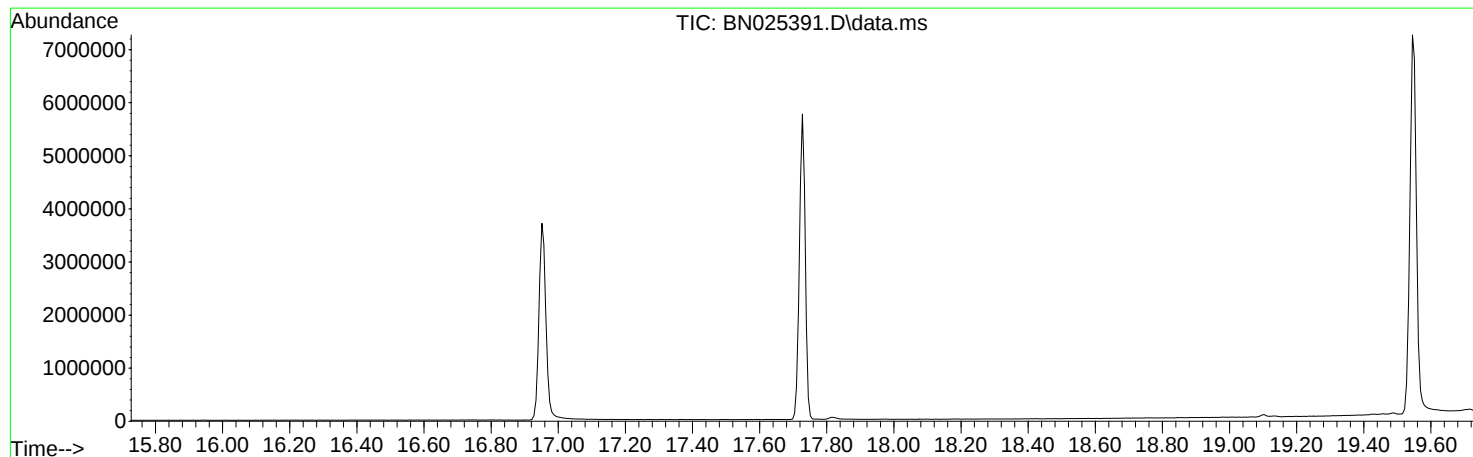

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	264954	PASS
68	69	0.00	2	1.8	4061	PASS
69	198	0.00	100	41.9	220772	PASS
70	69	0.00	2	0.5	999	PASS
127	198	10	80	46.2	243328	PASS
197	198	0.00	2	0.4	2233	PASS
198	198	100	100	100.0	526805	PASS
199	198	5	9	6.6	34760	PASS
275	198	10	60	26.4	138885	PASS
365	198	1	100	4.0	20812	PASS
441	198	0.01	100	15.2	79955	PASS
442	442	50	100	100.0	479595	PASS
443	442	15	24	19.1	91579	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/11/2023	BNA_N	<u>BN025391.D</u>
Compound Name	Response	Retention Time
DDT	709725	20.78
DDD	840724	20.3339
DDE	2404	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
843128	1552853	54.30

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025391.D
Acq On : 11 May 2023 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 06:09:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

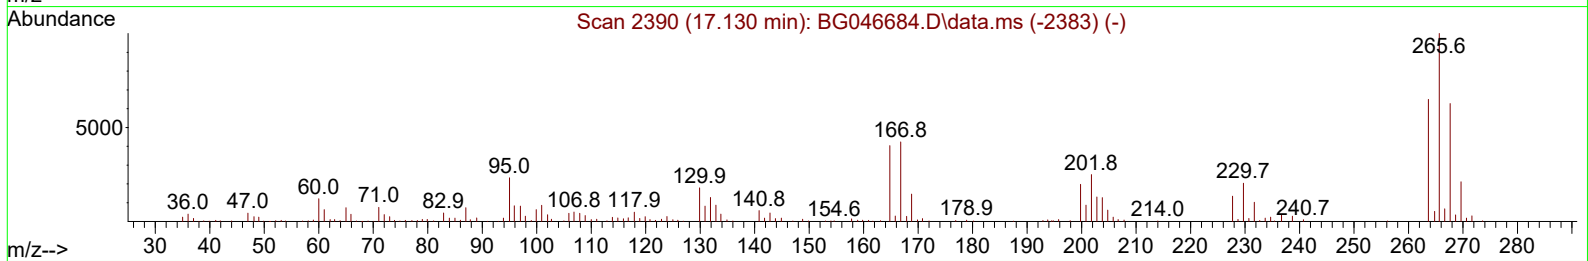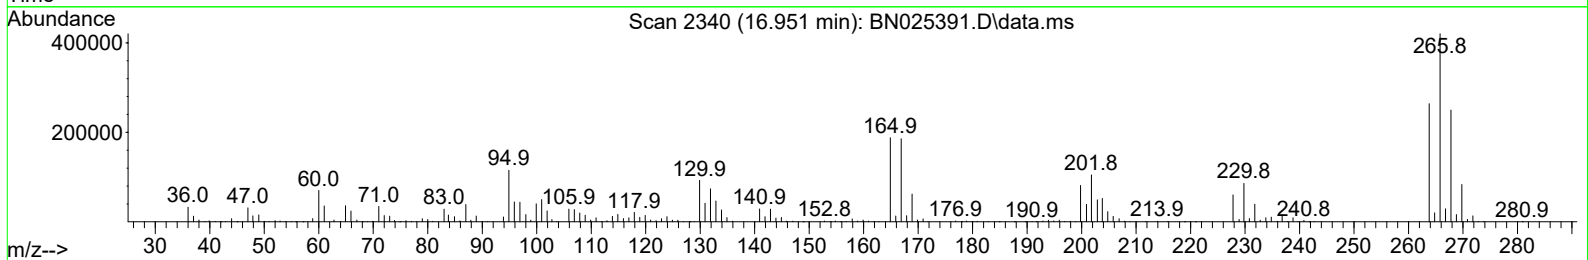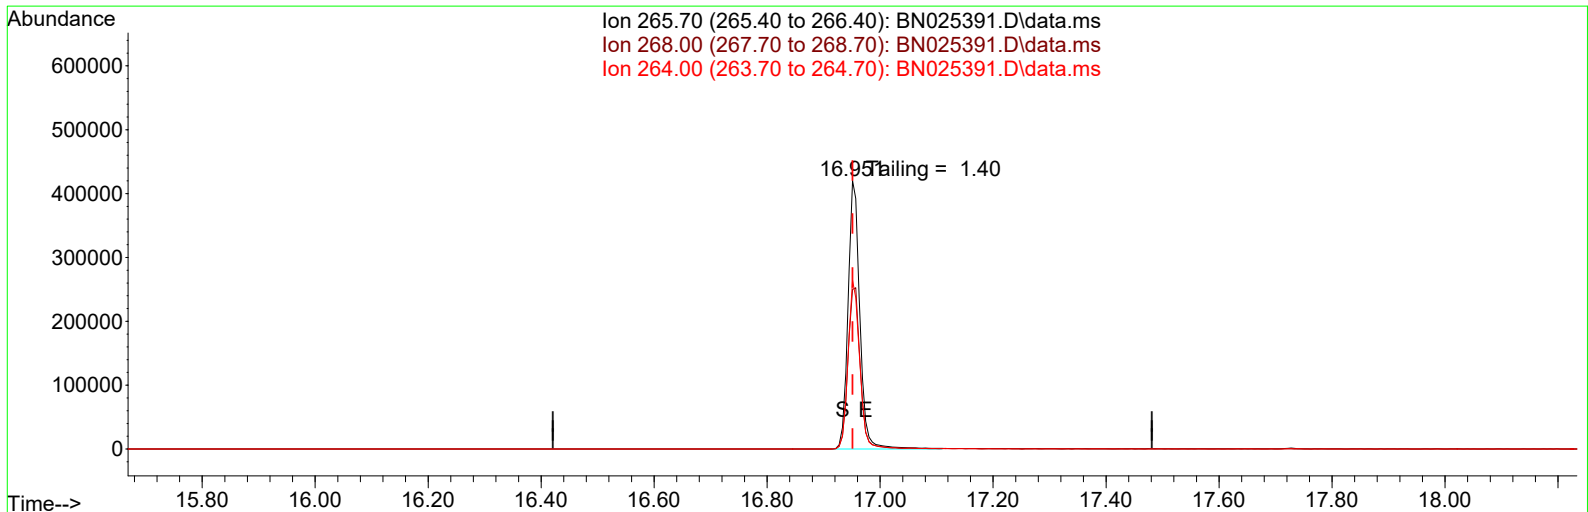

TIC: BN025391.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 23752.72 ng




response 613833

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.46
264.00	61.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025391.D
Acq On : 11 May 2023 09:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 06:09:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

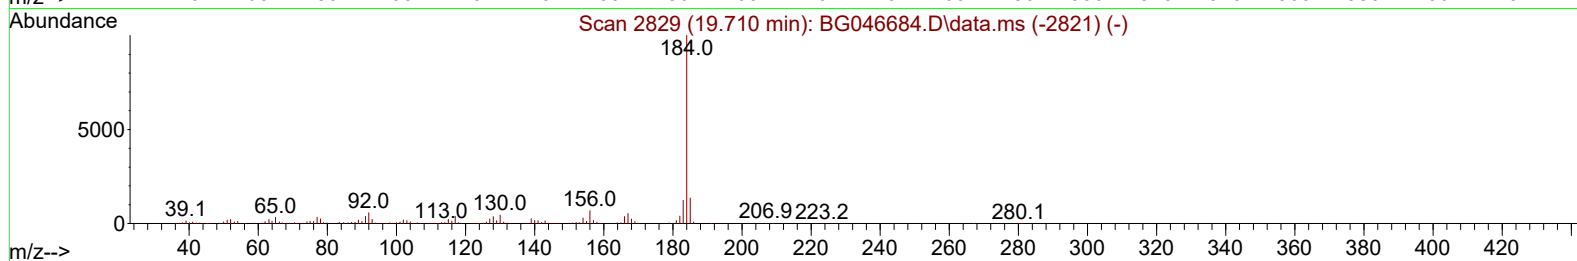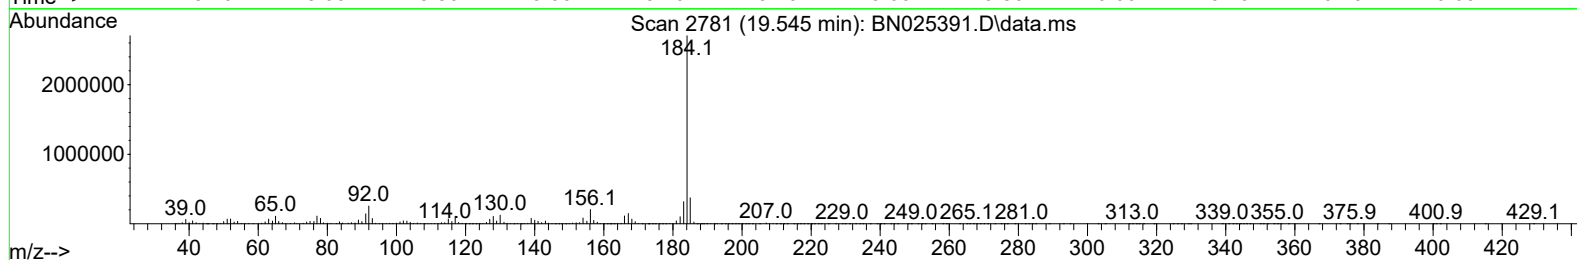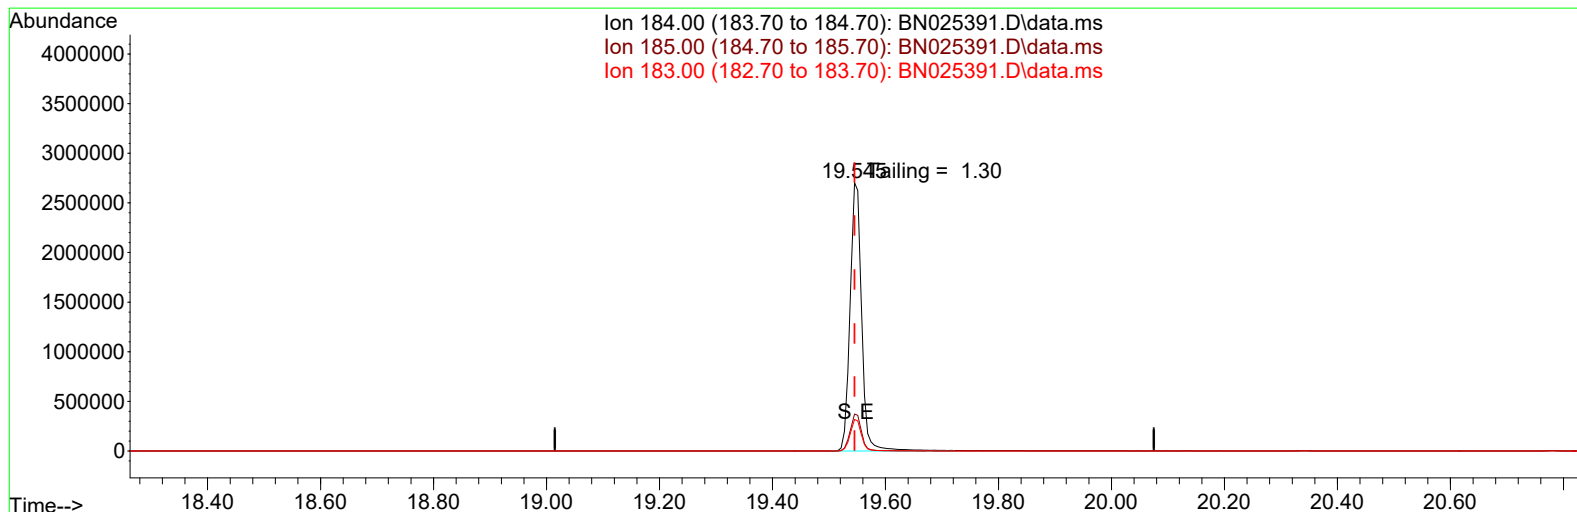

TIC: BN025391.D\data.ms

(77) Benzidine

19.545min (0.000) 208760.05 ng

response 3880369

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.75
0.00	0.00	0.00