
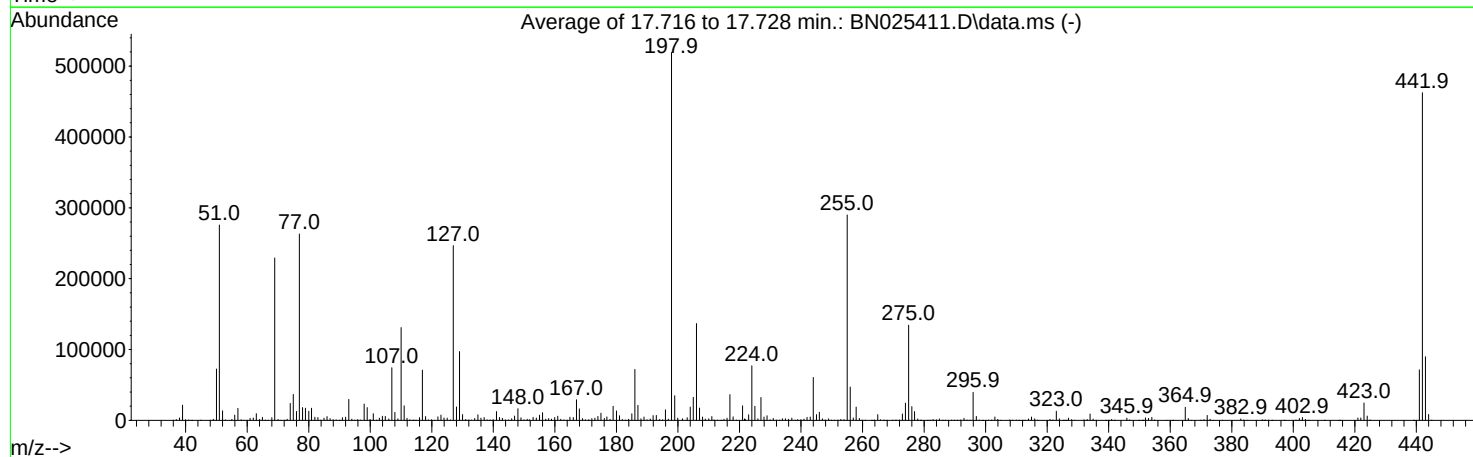


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025411.D
Acq On : 11 May 2023 21:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 00:57:16 2023

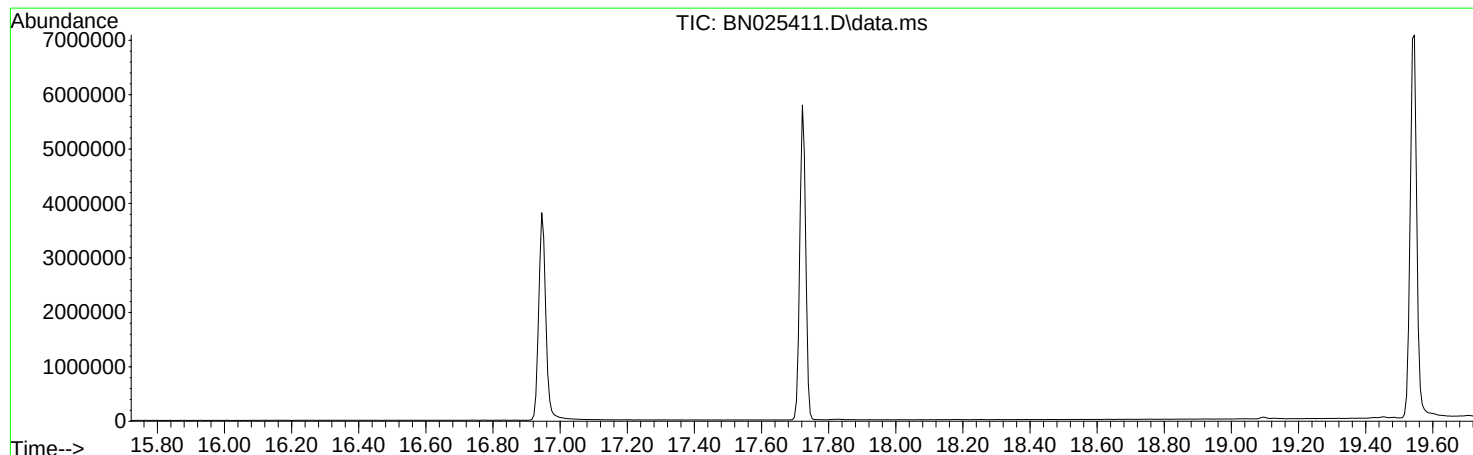

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	275696	PASS
68	69	0.00	2	1.6	3767	PASS
69	198	0.00	100	44.2	229314	PASS
70	69	0.00	2	0.6	1335	PASS
127	198	10	80	47.5	246720	PASS
197	198	0.00	2	0.4	1859	PASS
198	198	100	100	100.0	519211	PASS
199	198	5	9	6.7	34867	PASS
275	198	10	60	25.9	134333	PASS
365	198	1	100	3.6	18533	PASS
441	198	0.01	100	13.8	71397	PASS
442	442	50	100	100.0	462528	PASS
443	442	15	24	19.4	89816	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/11/2023	BNA_N	<u>BN025411.D</u>
Compound Name	Response	Retention Time
DDT	1064820	20.769
DDD	545283	20.333
DDE	2380	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
547663	1612483	33.96

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
 Data File : BN025411.D
 Acq On : 11 May 2023 21:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 12 06:11:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 06:09:14 2023
 Response via : Initial Calibration

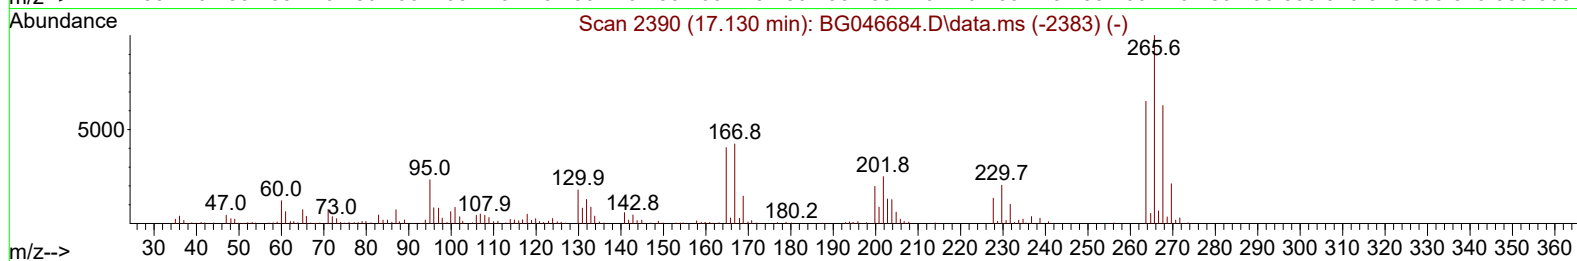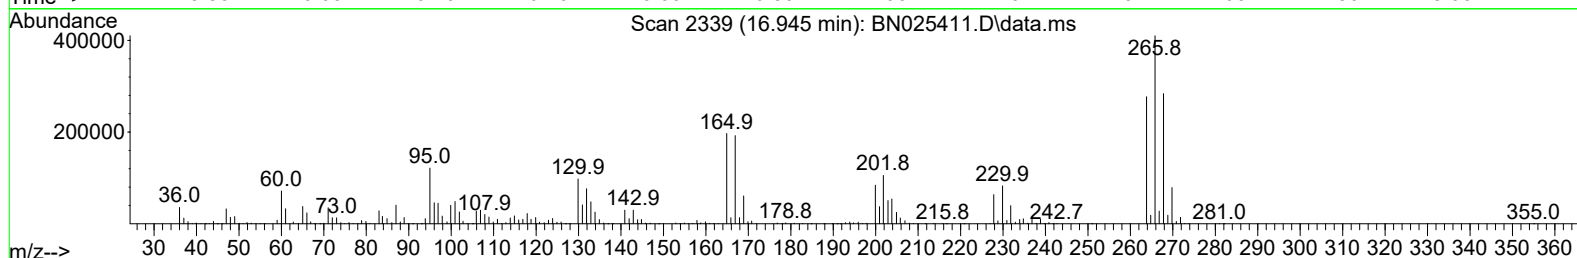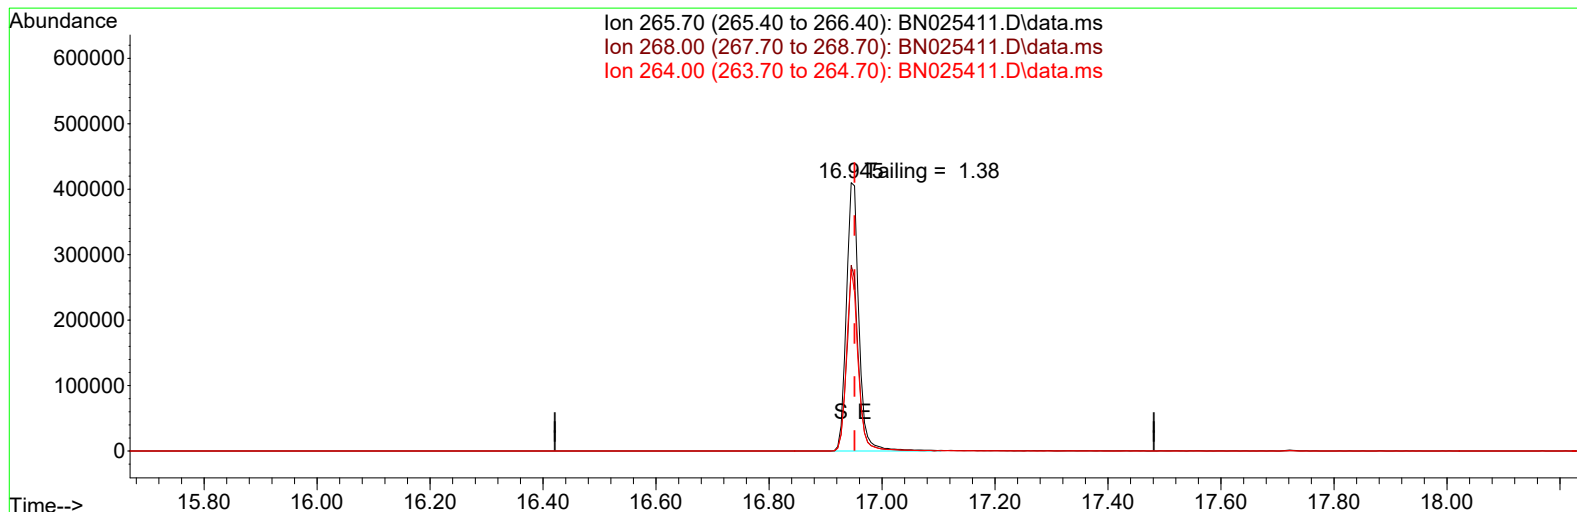

TIC: BN025411.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.006) 25019.44 ng




response 632235

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.19
264.00	61.60	67.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051123\
Data File : BN025411.D
Acq On : 11 May 2023 21:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 06:11:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 06:09:14 2023
Response via : Initial Calibration

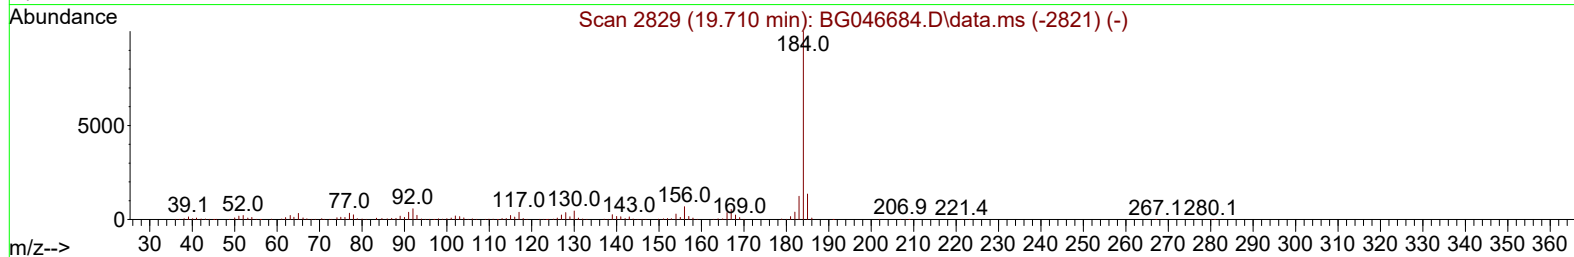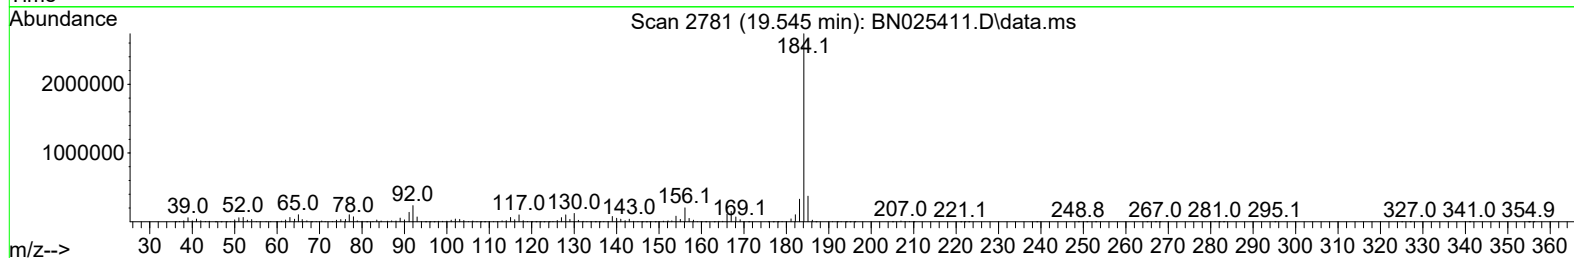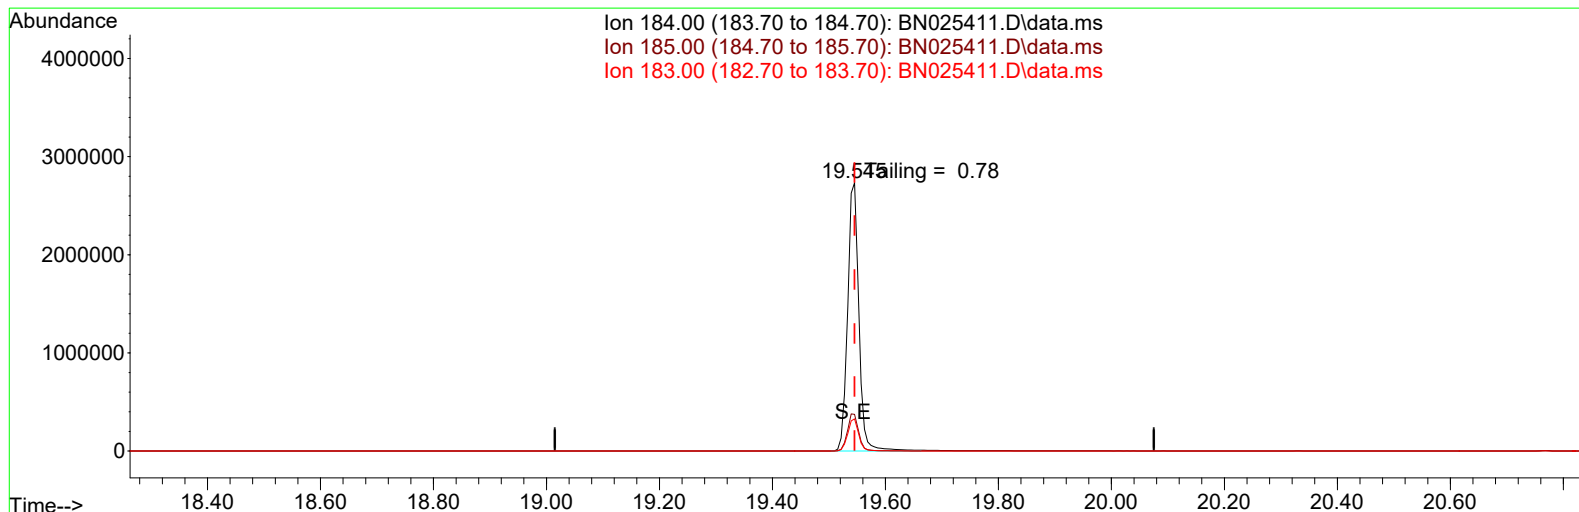

TIC: BN025411.D\data.ms

(77) Benzidine

19.545min (+ 0.000) 625498.16 ng

response 3798399

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	12.02
0.00	0.00	0.00