


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051220\
 Data File : BN010692.D
 Acq On : 12 May 2020 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 12 10:58:34 2020

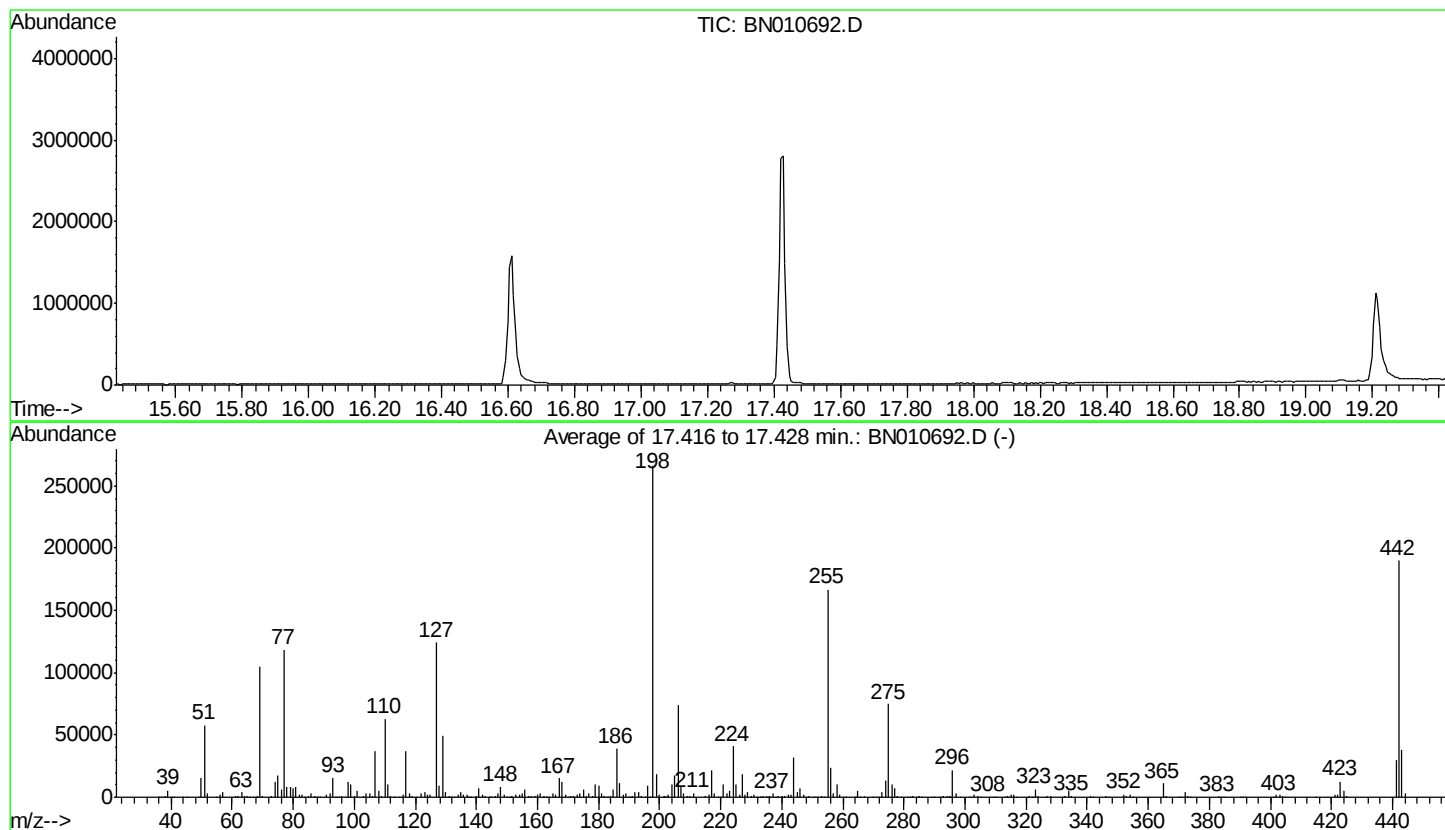

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	58072	PASS
68	69	0.00	2	0.6	660	PASS
69	198	0.00	100	39.5	105090	PASS
70	69	0.00	2	0.7	697	PASS
127	198	10	80	46.5	123920	PASS
197	198	0.00	2	0.2	444	PASS
198	198	100	100	100.0	266325	PASS
199	198	5	9	7.0	18714	PASS
275	198	10	60	28.1	74810	PASS
365	198	1	100	4.1	10869	PASS
441	198	0.01	100	11.1	29487	PASS
442	198	50	100	71.4	190170	PASS
443	442	15	24	19.8	37621	PASS