

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051221\
 Data File : BN014578.D
 Acq On : 12 May 2021 14:05
 Operator : CG/JU
 Sample : SSTD3.2006
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2006

Quant Time: May 12 14:36:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 12 12:52:43 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	596	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	1992	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1359	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.14	188	3277	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	4127	0.40	ng/ul	0.00
23) Perylene-d12	23.60	264	3139	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	1901	2.92	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
18) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
2) 1,4-Dioxane	3.29	88	2058	3.110	ng/ul#	78
14) Pentachlorophenol	16.78	266	2191	2.066	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051221\
Data File : BN014578.D
Acq On : 12 May 2021 14:05
Operator : CG/JU
Sample : SSTD3.206
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTD3.2006

Quant Time: May 12 14:36:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 12 12:52:43 2021
Response via : Initial Calibration

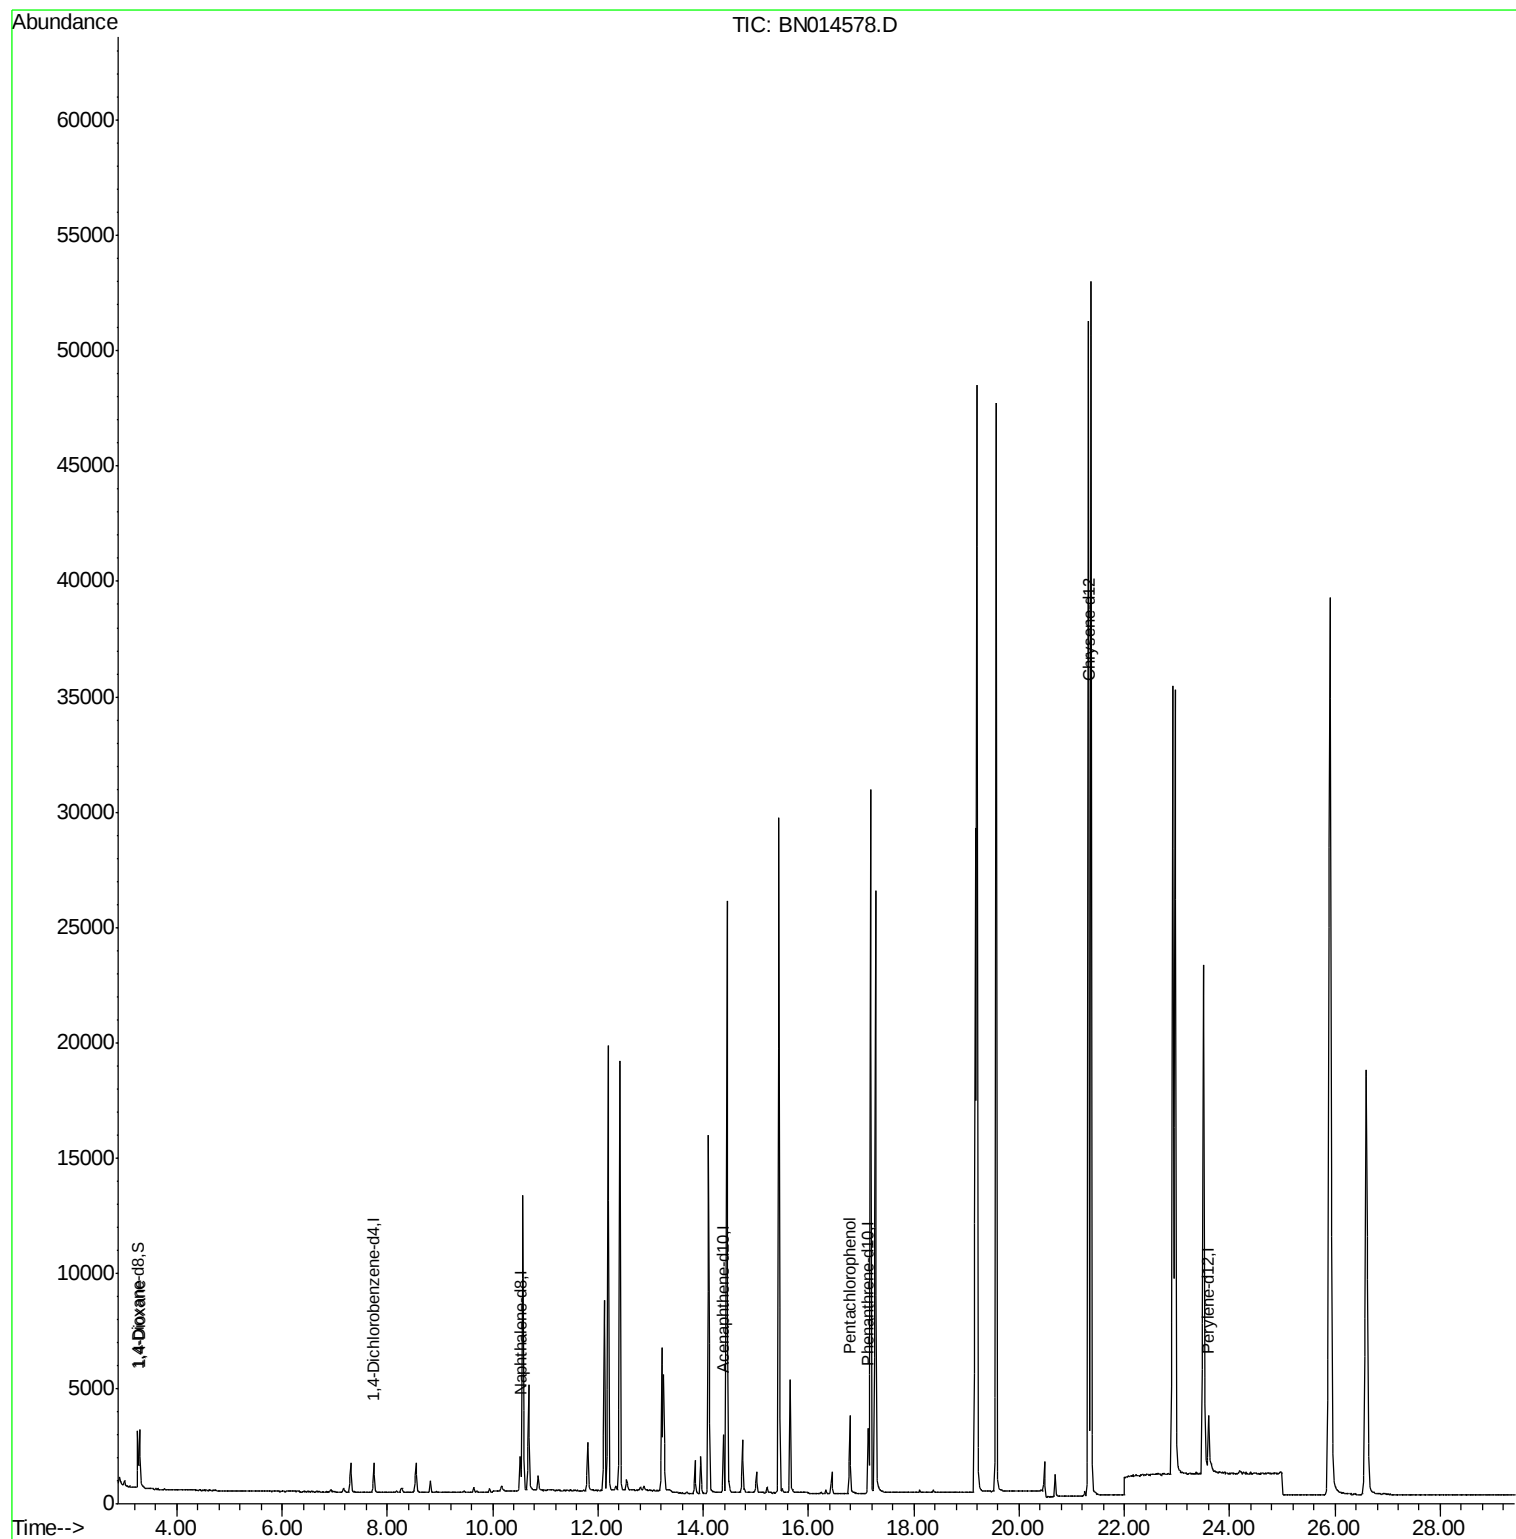

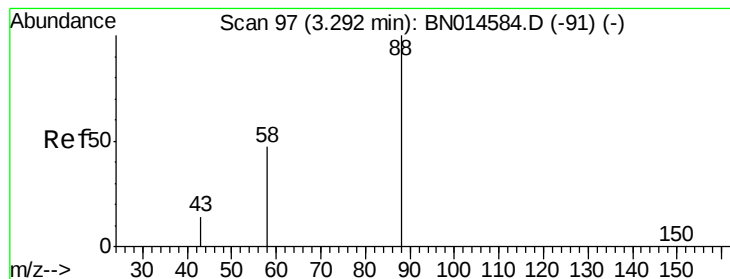

#2

1,4-Dioxane

Concen: 3.110 ng/ul

RT: 3.29 min Scan# 97

Delta R.T. -0.01 min

Lab File: BN014578.D

Acq: 12 May 2021 14:05

Instrument :

BNA_N

ClientSampleId :

SSTD3.2006


Tot Ion: 88 Resp: 2058

Ion Ratio Lower Upper

88 100

43 16.7 15.7 23.5




58 47.0 23.8 35.6#

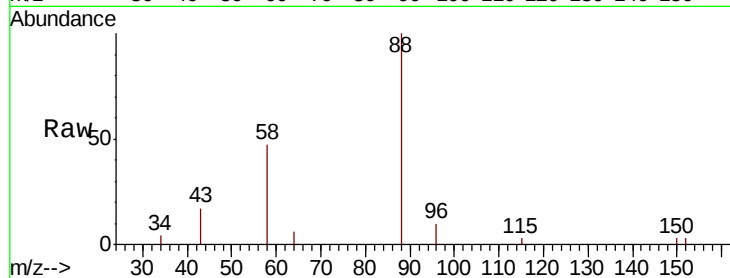

Abundance Ion 88.00 (87.70 to 88.70): BN014578.D (-87) (-)

Ion 43.00 (42.70 to 43.70): BN014578.D (-87) (-)

Ion 58.00 (57.70 to 58.70): BN014578.D (-87) (-)

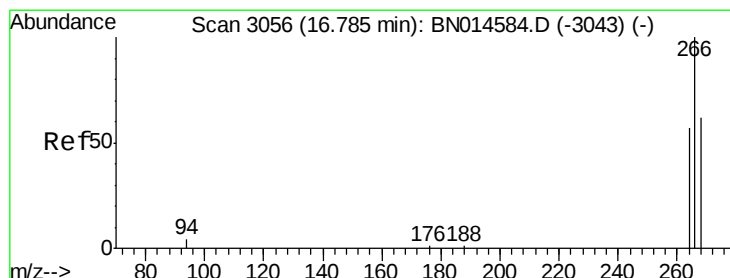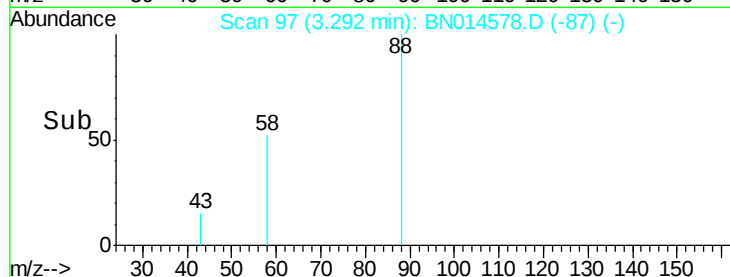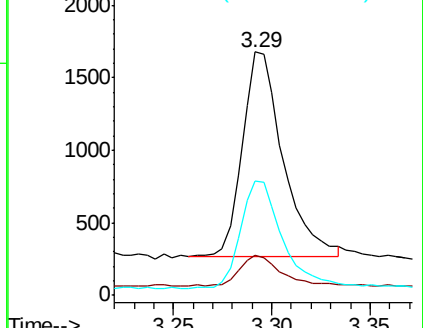

#14

Pentachlorophenol

Concen: 2.066 ng/ul

RT: 16.78 min Scan# 3056

Delta R.T. -0.00 min

Lab File: BN014578.D

Acq: 12 May 2021 14:05


Tgt Ion: 266 Resp: 2191

Ion Ratio Lower Upper

266 100

264 61.8 49.4 74.2

268 63.5 49.1 73.7

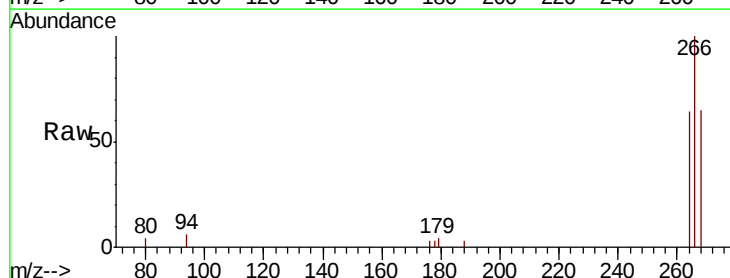

Abundance Ion 266.00 (265.70 to 266.70): BN014578.D (-3032) (-)

Ion 264.00 (263.70 to 264.70): BN014578.D (-3032) (-)

Ion 268.00 (267.70 to 268.70): BN014578.D (-3032) (-)

