
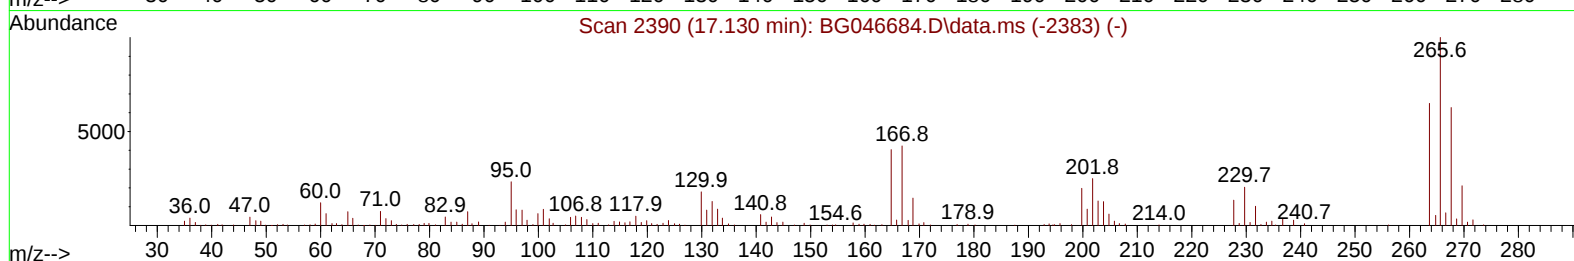
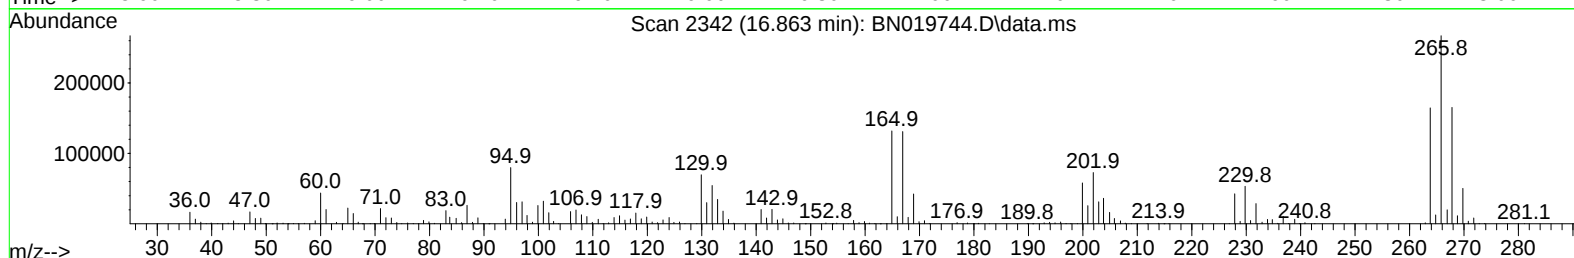


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051222\
Data File : BN019744.D
Acq On : 12 May 2022 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:17:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

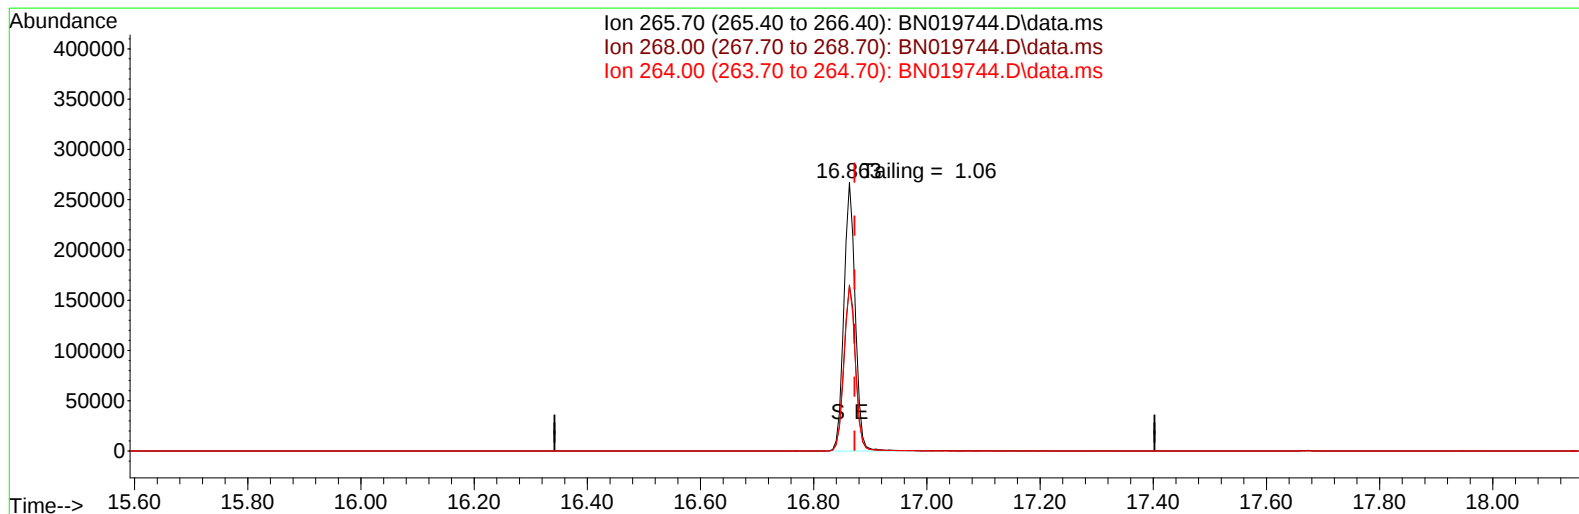

TIC: BN019744.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.009) 23452.32 ng

response 372881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.88
264.00	61.60	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051222\
Data File : BN019744.D
Acq On : 12 May 2022 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:17:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

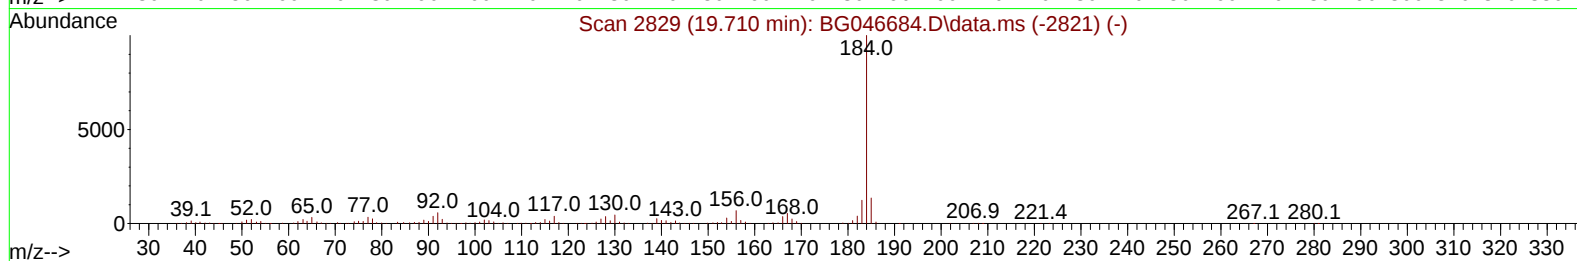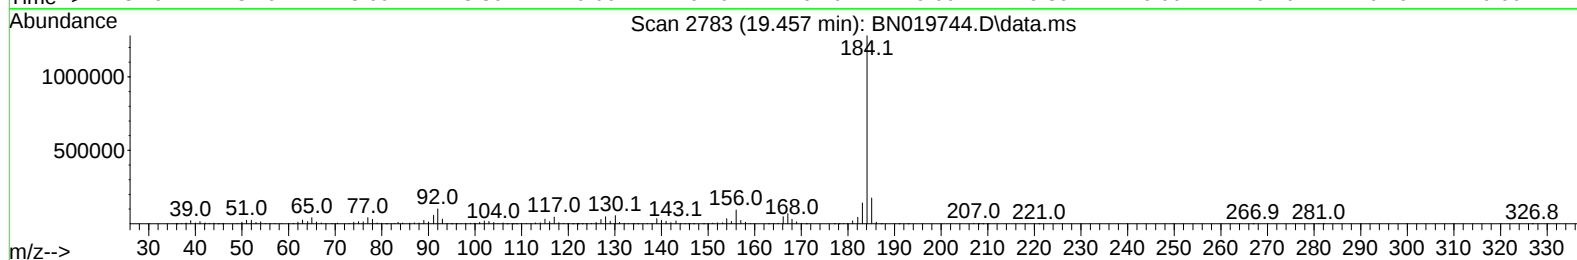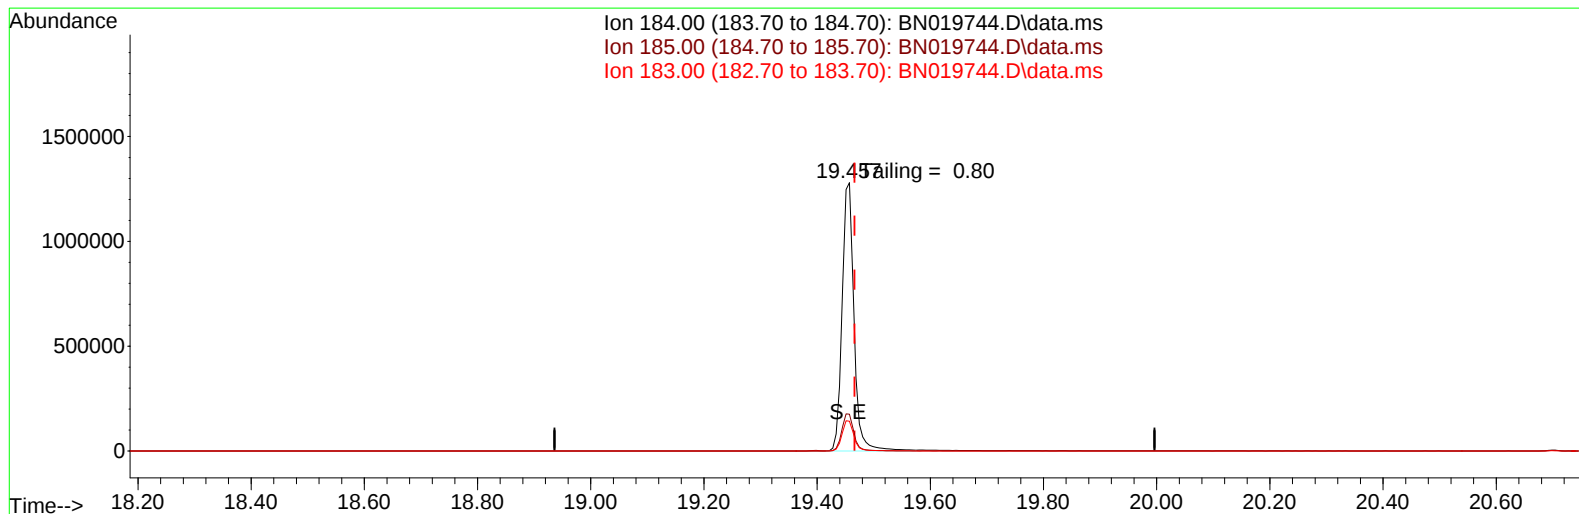

TIC: BN019744.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1871927

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.11
0.00	0.00	0.00