
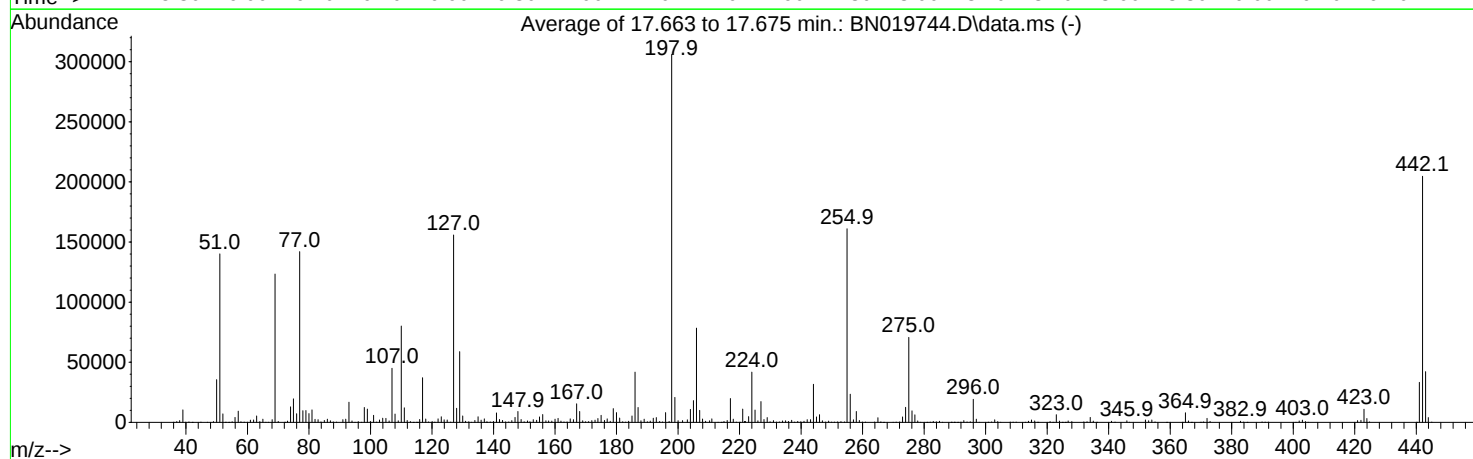


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051222\
 Data File : BN019744.D
 Acq On : 12 May 2022 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 10 01:35:26 2022

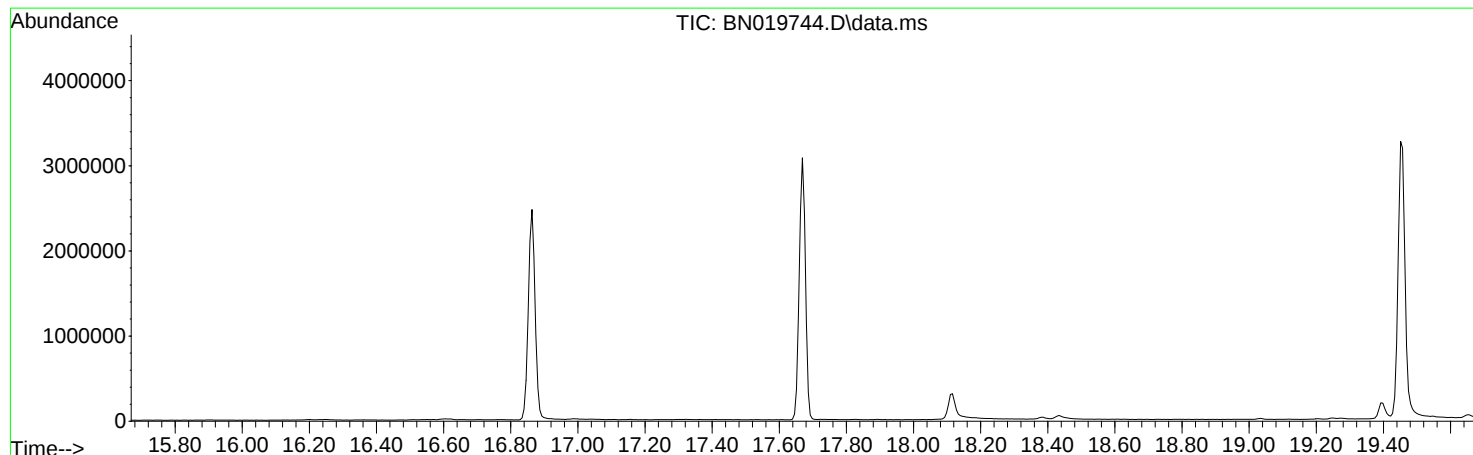

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	140106	PASS
68	69	0.00	2	1.8	2214	PASS
69	198	0.00	100	40.3	123377	PASS
70	69	0.00	2	0.7	828	PASS
127	198	10	80	50.9	155819	PASS
197	198	0.00	2	0.3	821	PASS
198	198	100	100	100.0	305984	PASS
199	198	5	9	6.8	20840	PASS
275	198	10	60	23.1	70699	PASS
365	198	1	100	2.6	8005	PASS
441	198	0.01	100	10.9	33235	PASS
442	442	50	100	100.0	204693	PASS
443	442	15	24	20.6	42160	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2022	BNA_N	<u>BN019744.D</u>
Compound Name	Response	Retention Time
DDT	1008084	20.704
DDD	11318	20.257
DDE	123	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11441	1019525	1.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051222\
Data File : BN019744.D
Acq On : 12 May 2022 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 07:17:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

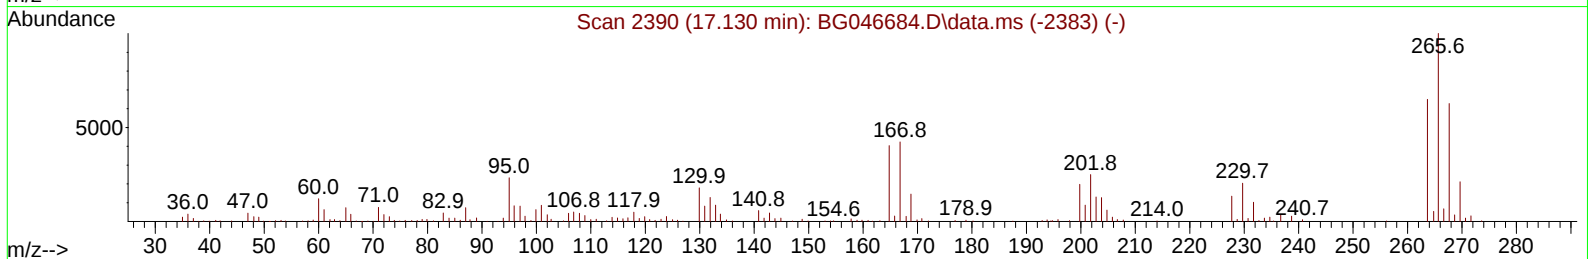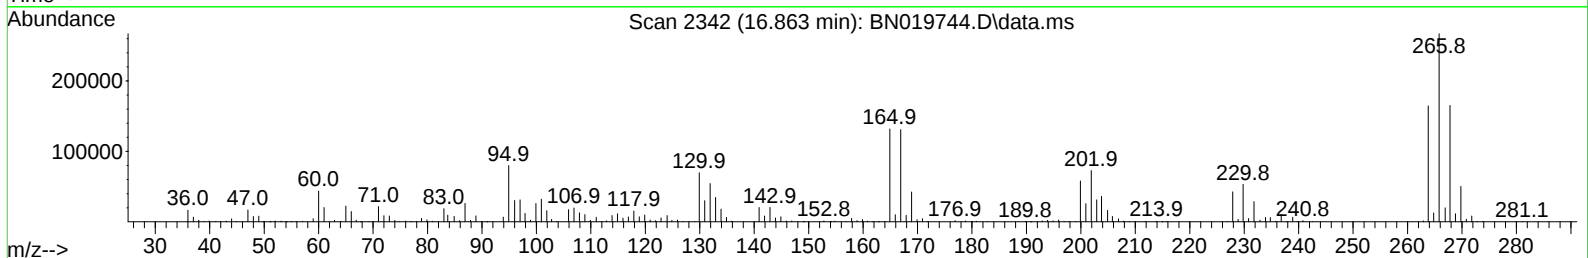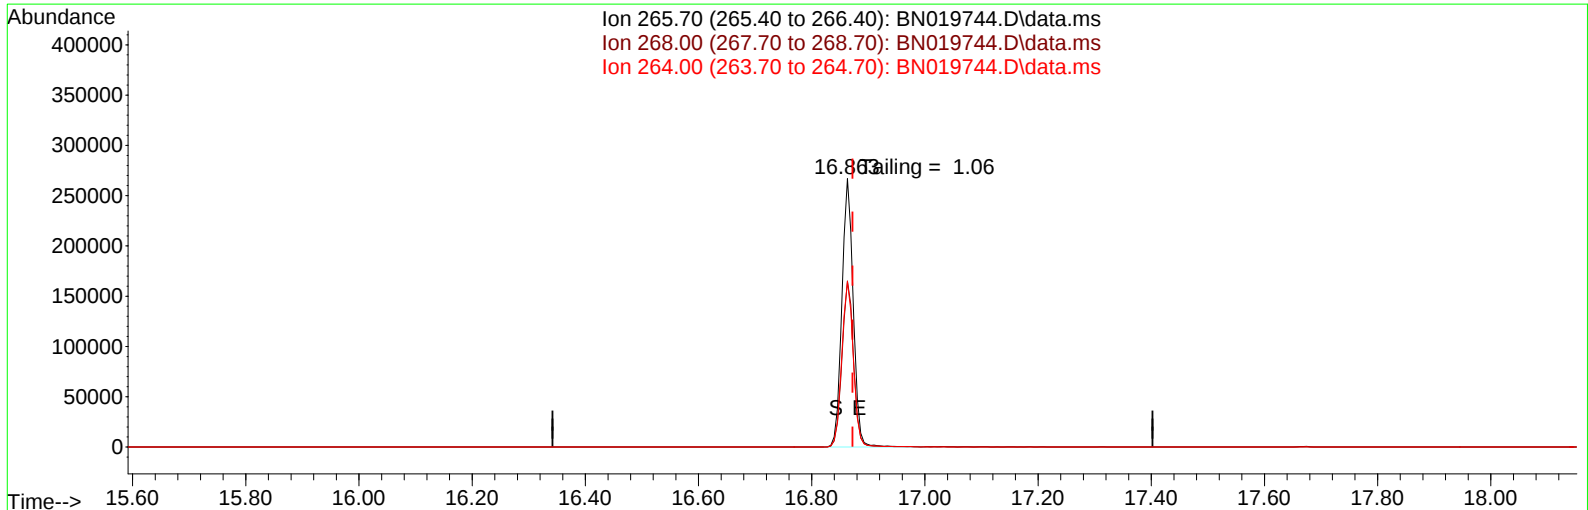

TIC: BN019744.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 23452.32 ng




response 372881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.88
264.00	61.60	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051222\
Data File : BN019744.D
Acq On : 12 May 2022 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 07:17:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

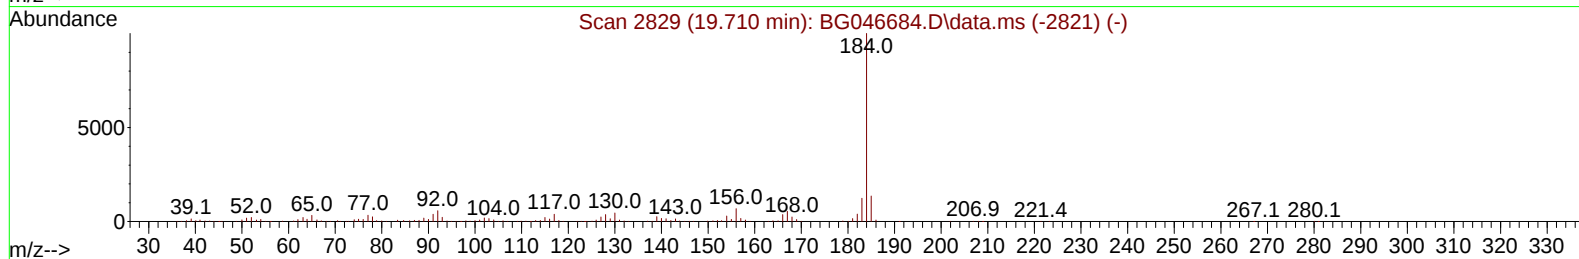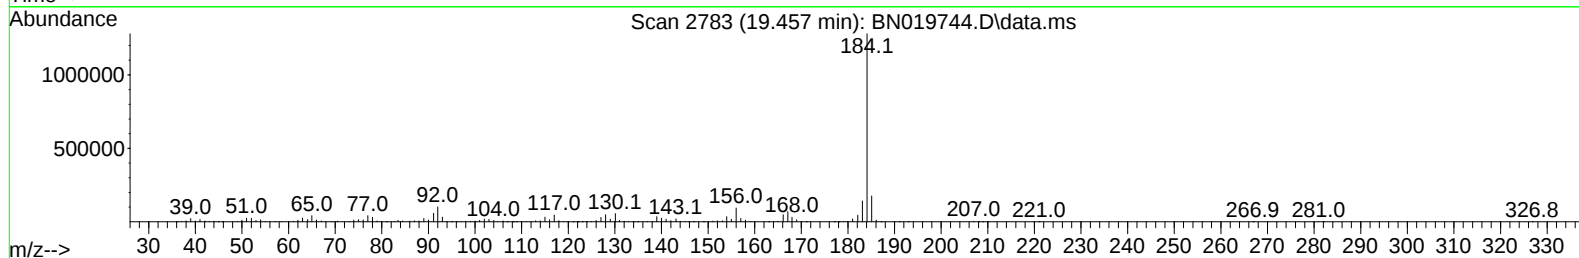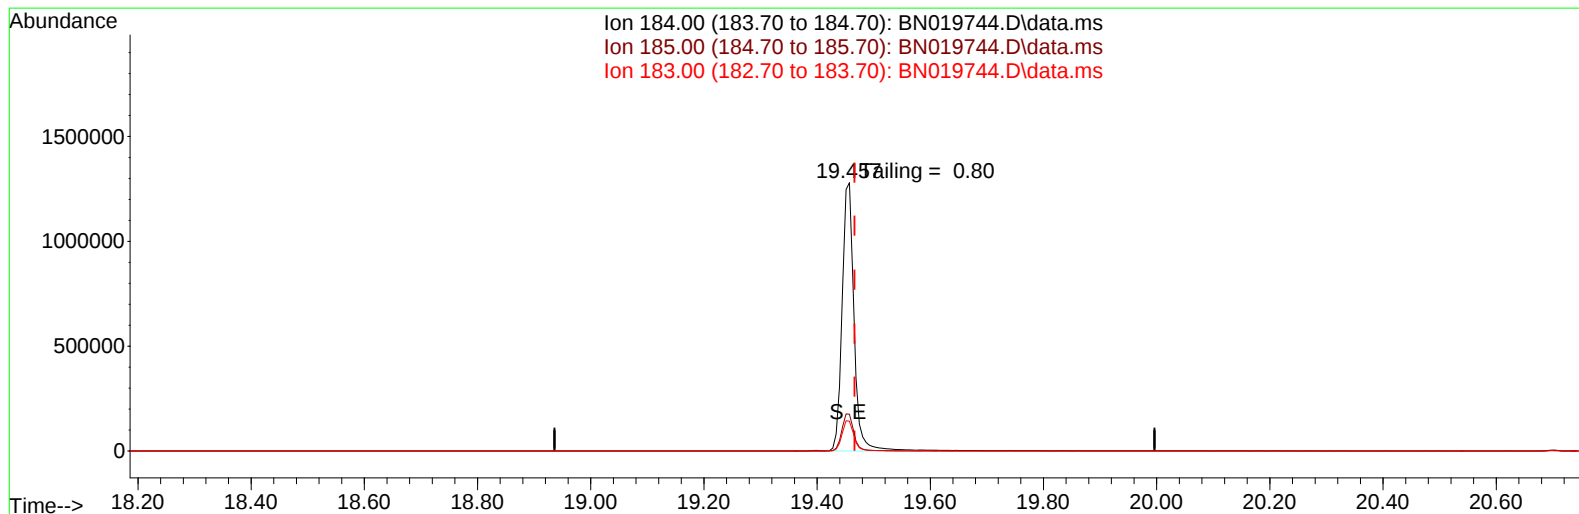

TIC: BN019744.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1871927

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	11.11
0.00	0.00	0.00