
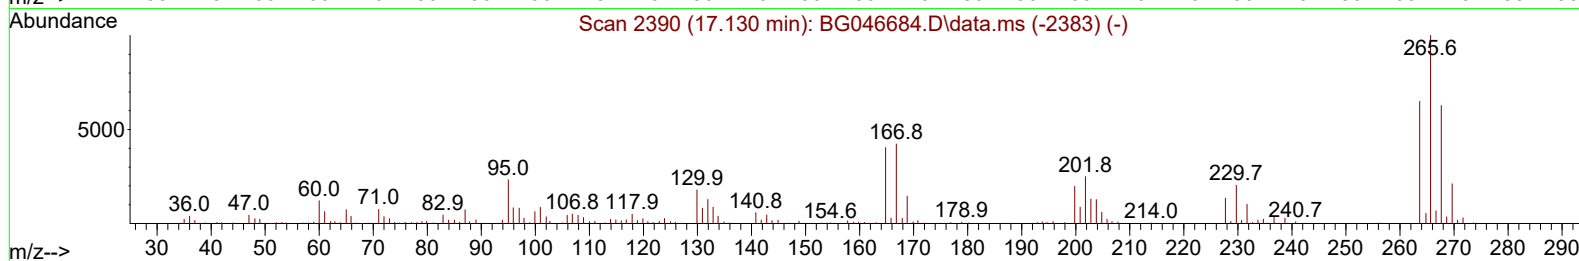
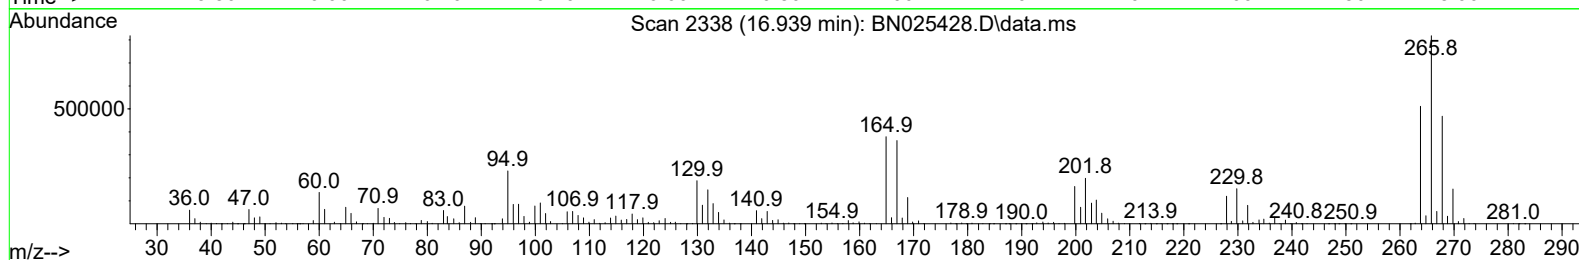


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051223\  
Data File : BN025428.D  
Acq On : 12 May 2023 09:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:28:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 13 04:28:53 2023  
Response via : Initial Calibration

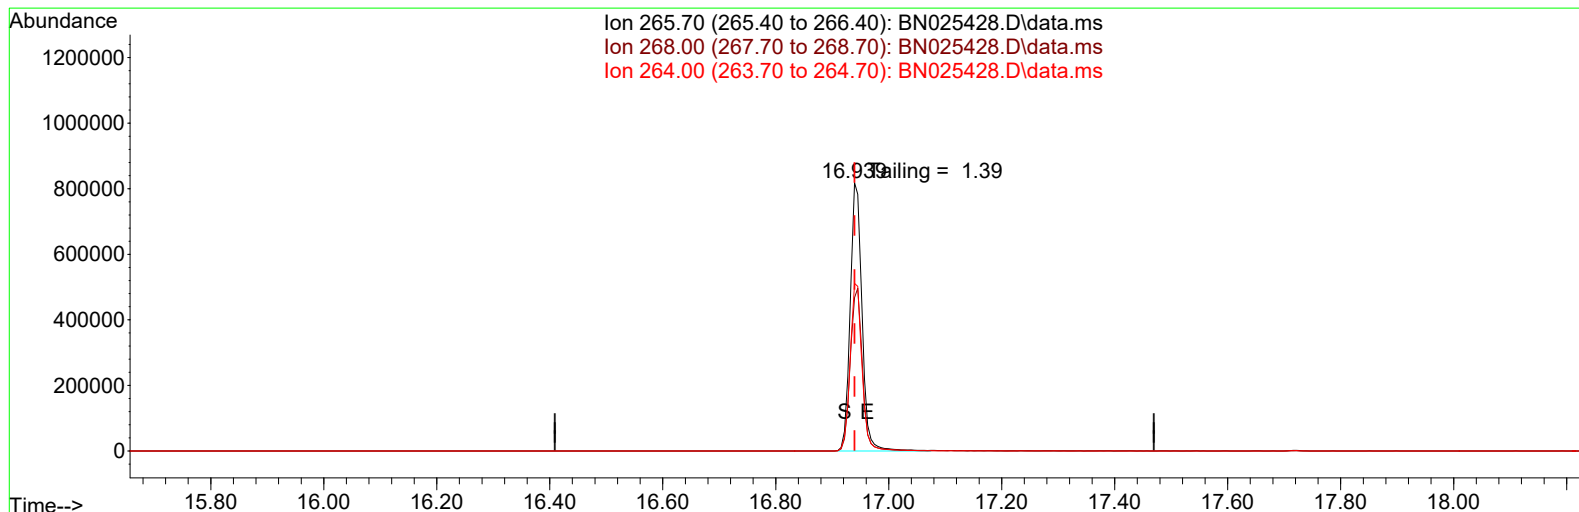

TIC: BN025428.D\data.ms

(70) Pentachlorophenol (C)

16.939min ( 0.000) 25313.08 ng

**response**      **1194089**

| Ion | Exp% | Act% |
|-----|------|------|
|-----|------|------|

|        |        |        |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
|--------|--------|--------|




|        |       |       |
|--------|-------|-------|
| 268.00 | 62.20 | 57.19 |
|--------|-------|-------|

|        |       |       |
|--------|-------|-------|
| 264.00 | 61.60 | 62.45 |
|--------|-------|-------|

0.00                      0.00                      0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN051223\  
Data File : BN025428.D  
Acq On : 12 May 2023 09:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:28:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 13 04:28:53 2023  
Response via : Initial Calibration

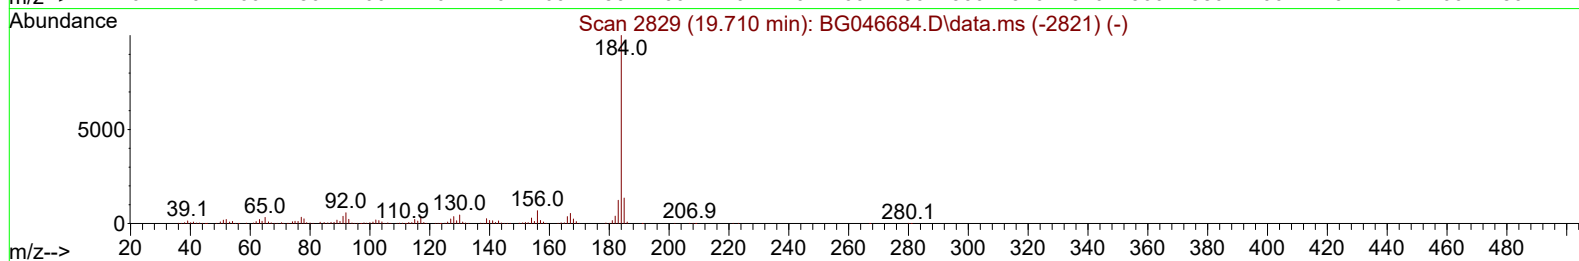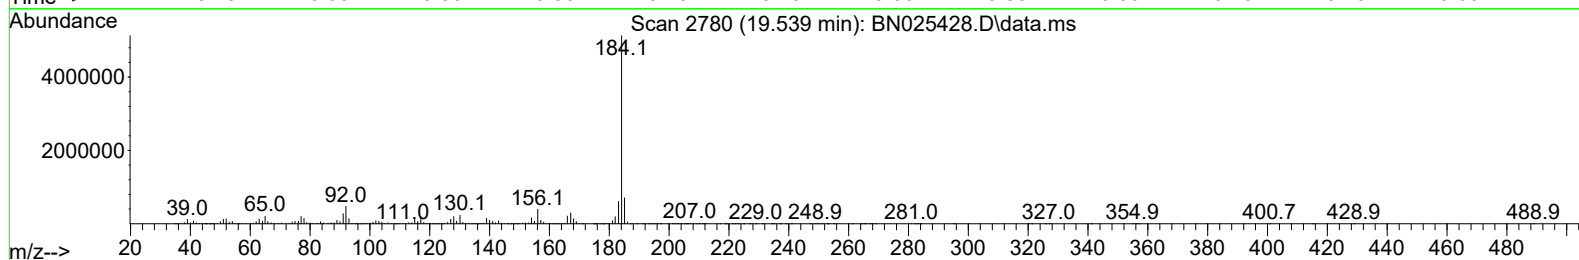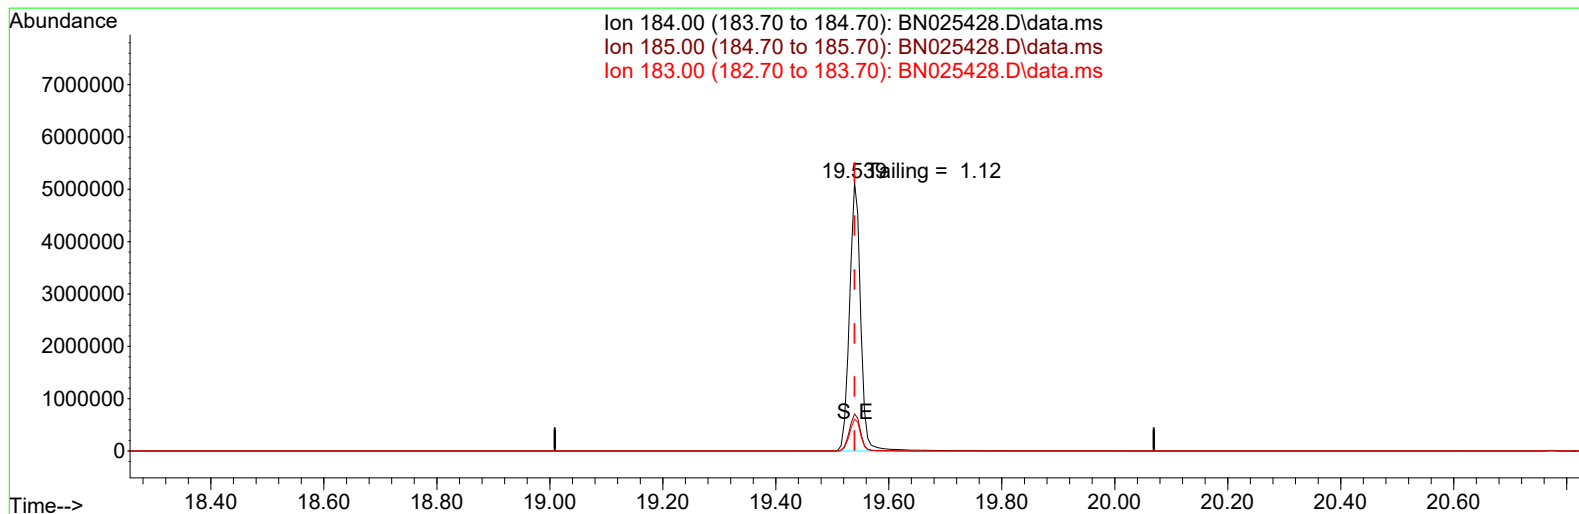

TIC: BN025428.D\data.ms

**(77) Benzidine****19.539min ( 0.000) 1332549.05 ng****response 7065127**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.83  |
| 183.00 | 13.20  | 11.92  |
| 0.00   | 0.00   | 0.00   |