
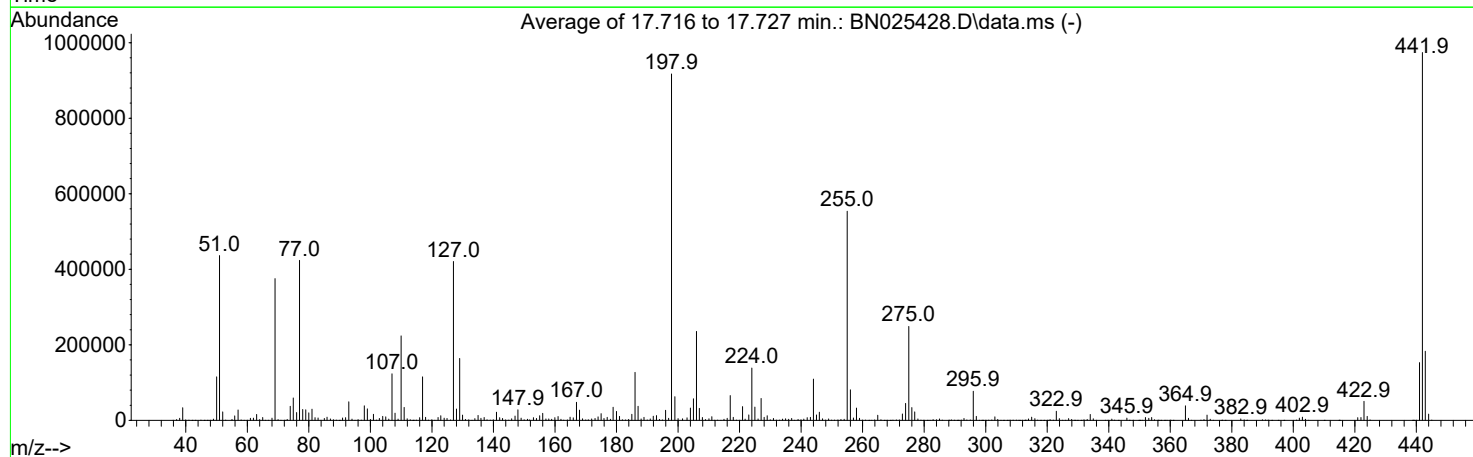


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051223\
 Data File : BN025428.D
 Acq On : 12 May 2023 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 12 00:57:16 2023

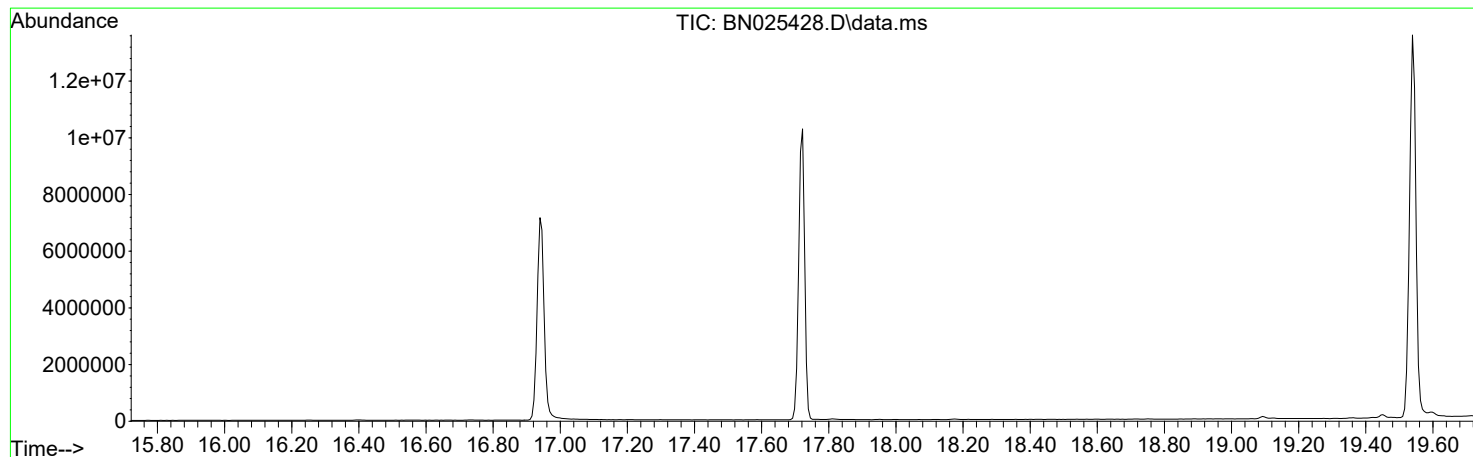

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	436581	PASS
68	69	0.00	2	1.6	6123	PASS
69	198	0.00	100	40.9	375293	PASS
70	69	0.00	2	0.6	2163	PASS
127	198	10	80	45.9	420629	PASS
197	198	0.00	2	0.6	5630	PASS
198	198	100	100	100.0	917141	PASS
199	198	5	9	6.8	62664	PASS
275	198	10	60	27.1	248875	PASS
365	198	1	100	4.2	38768	PASS
441	198	0.01	100	16.7	152981	PASS
442	442	50	100	100.0	973995	PASS
443	442	15	24	18.8	183125	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2023	BNA_N	<u>BN025428.D</u>
Compound Name	Response	Retention Time
DDT	2188758	20.774
DDD	894827	20.333
DDE	6345	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
901172	3089930	29.16

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051223\
 Data File : BN025428.D
 Acq On : 12 May 2023 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 13 04:28:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 13 04:28:53 2023
 Response via : Initial Calibration

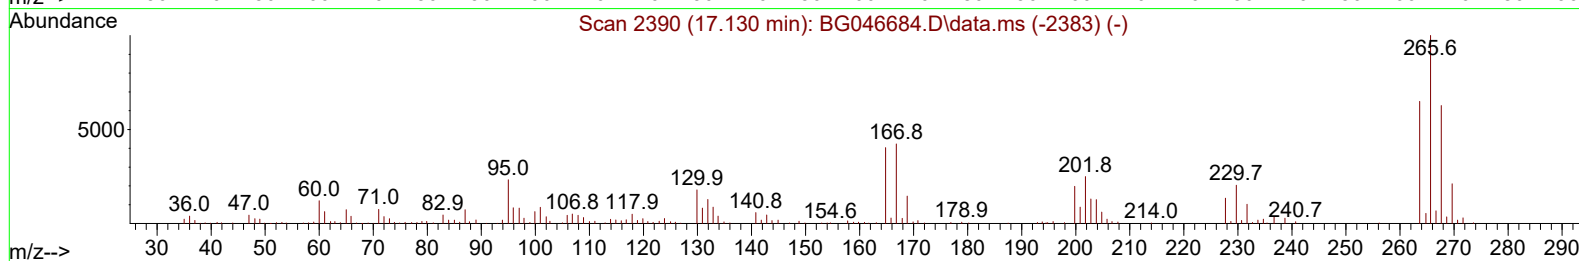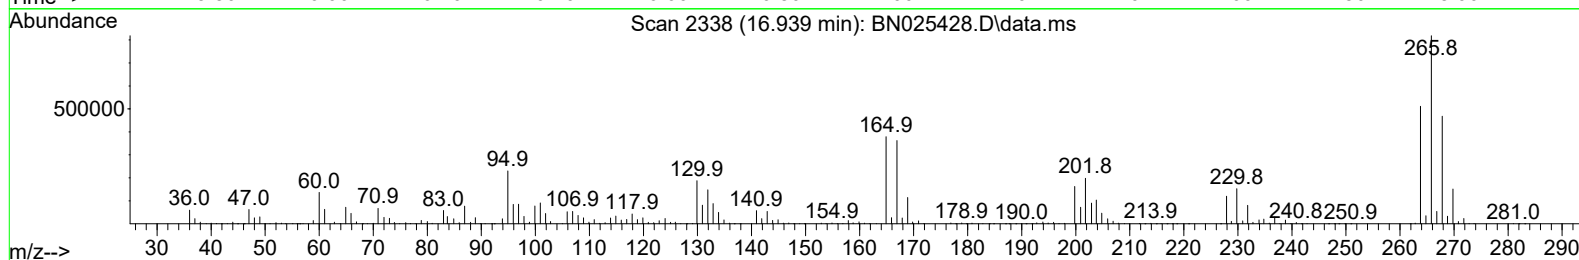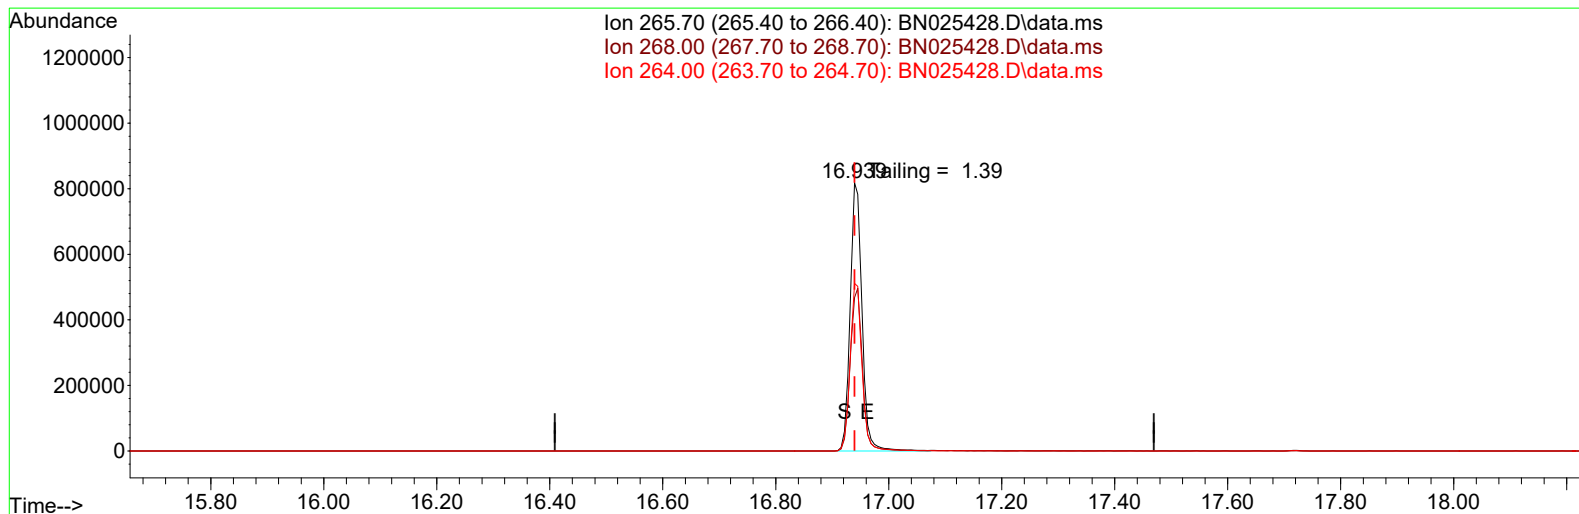

TIC: BN025428.D\data.ms

(70) Pentachlorophenol (C)

16.939min (0.000) 25313.08 ng




response 1194089

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.19
264.00	61.60	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051223\
Data File : BN025428.D
Acq On : 12 May 2023 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 04:28:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 13 04:28:53 2023
Response via : Initial Calibration

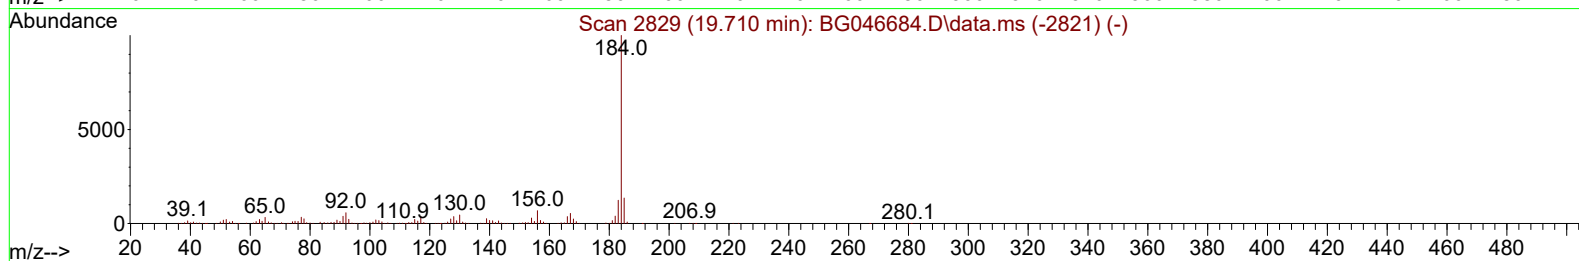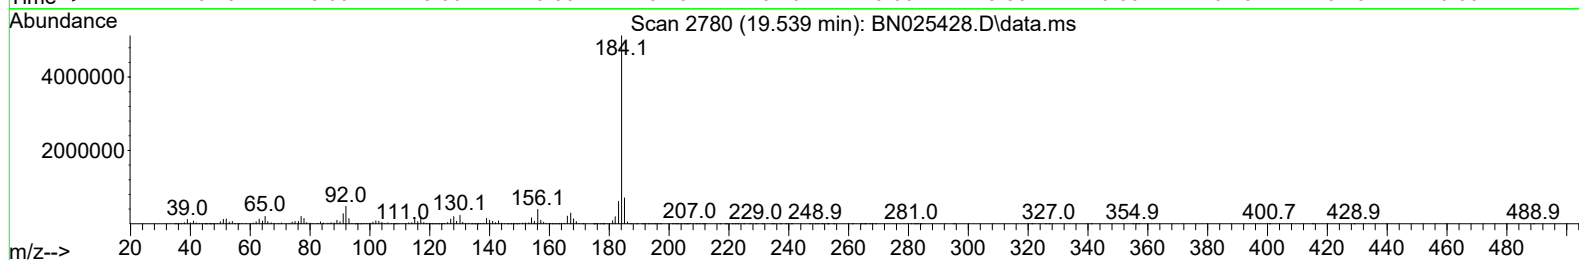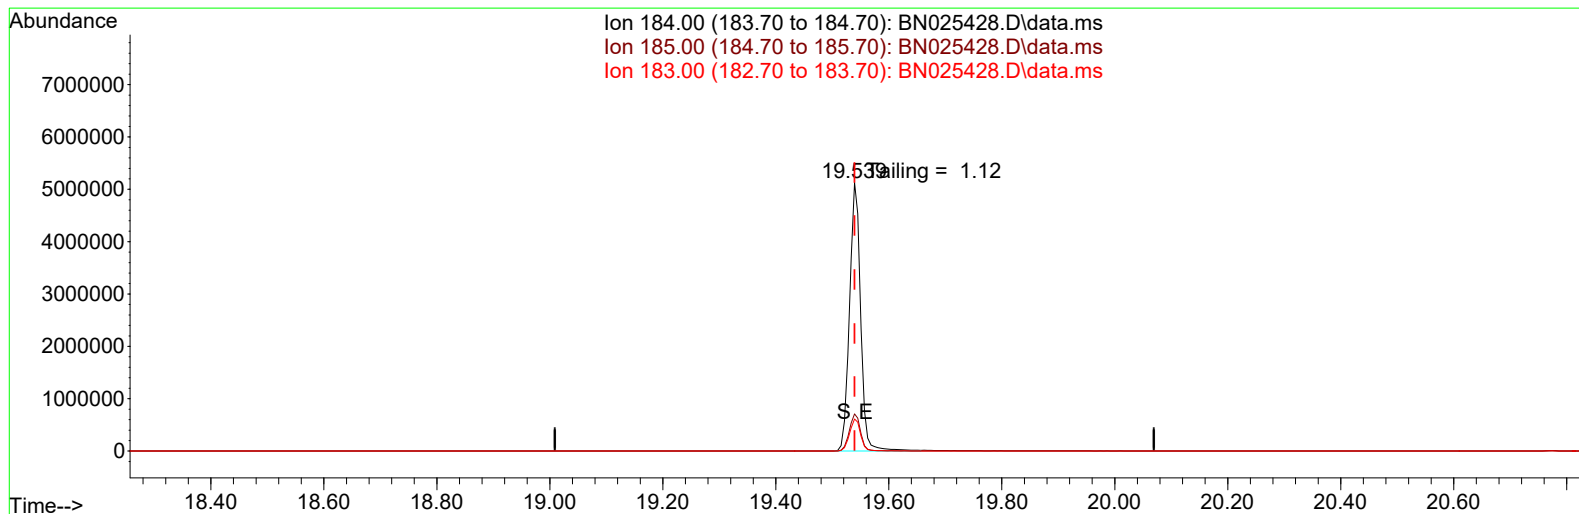

TIC: BN025428.D\data.ms

(77) Benzidine

19.539min (0.000) 1332549.05 ng

response 7065127

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.83
183.00	13.20	11.92
0.00	0.00	0.00