


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
Data File : BN014600.D
Acq On : 13 May 2021 21:44
Operator : CG/JU
Sample : M2197-17
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARS0

Manual Integrations
APPROVED

mohammad
5/14/2021 12:51:02 PM

Quant Time: May 14 01:40:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 01:34:46 2021
Response via : Initial Calibration

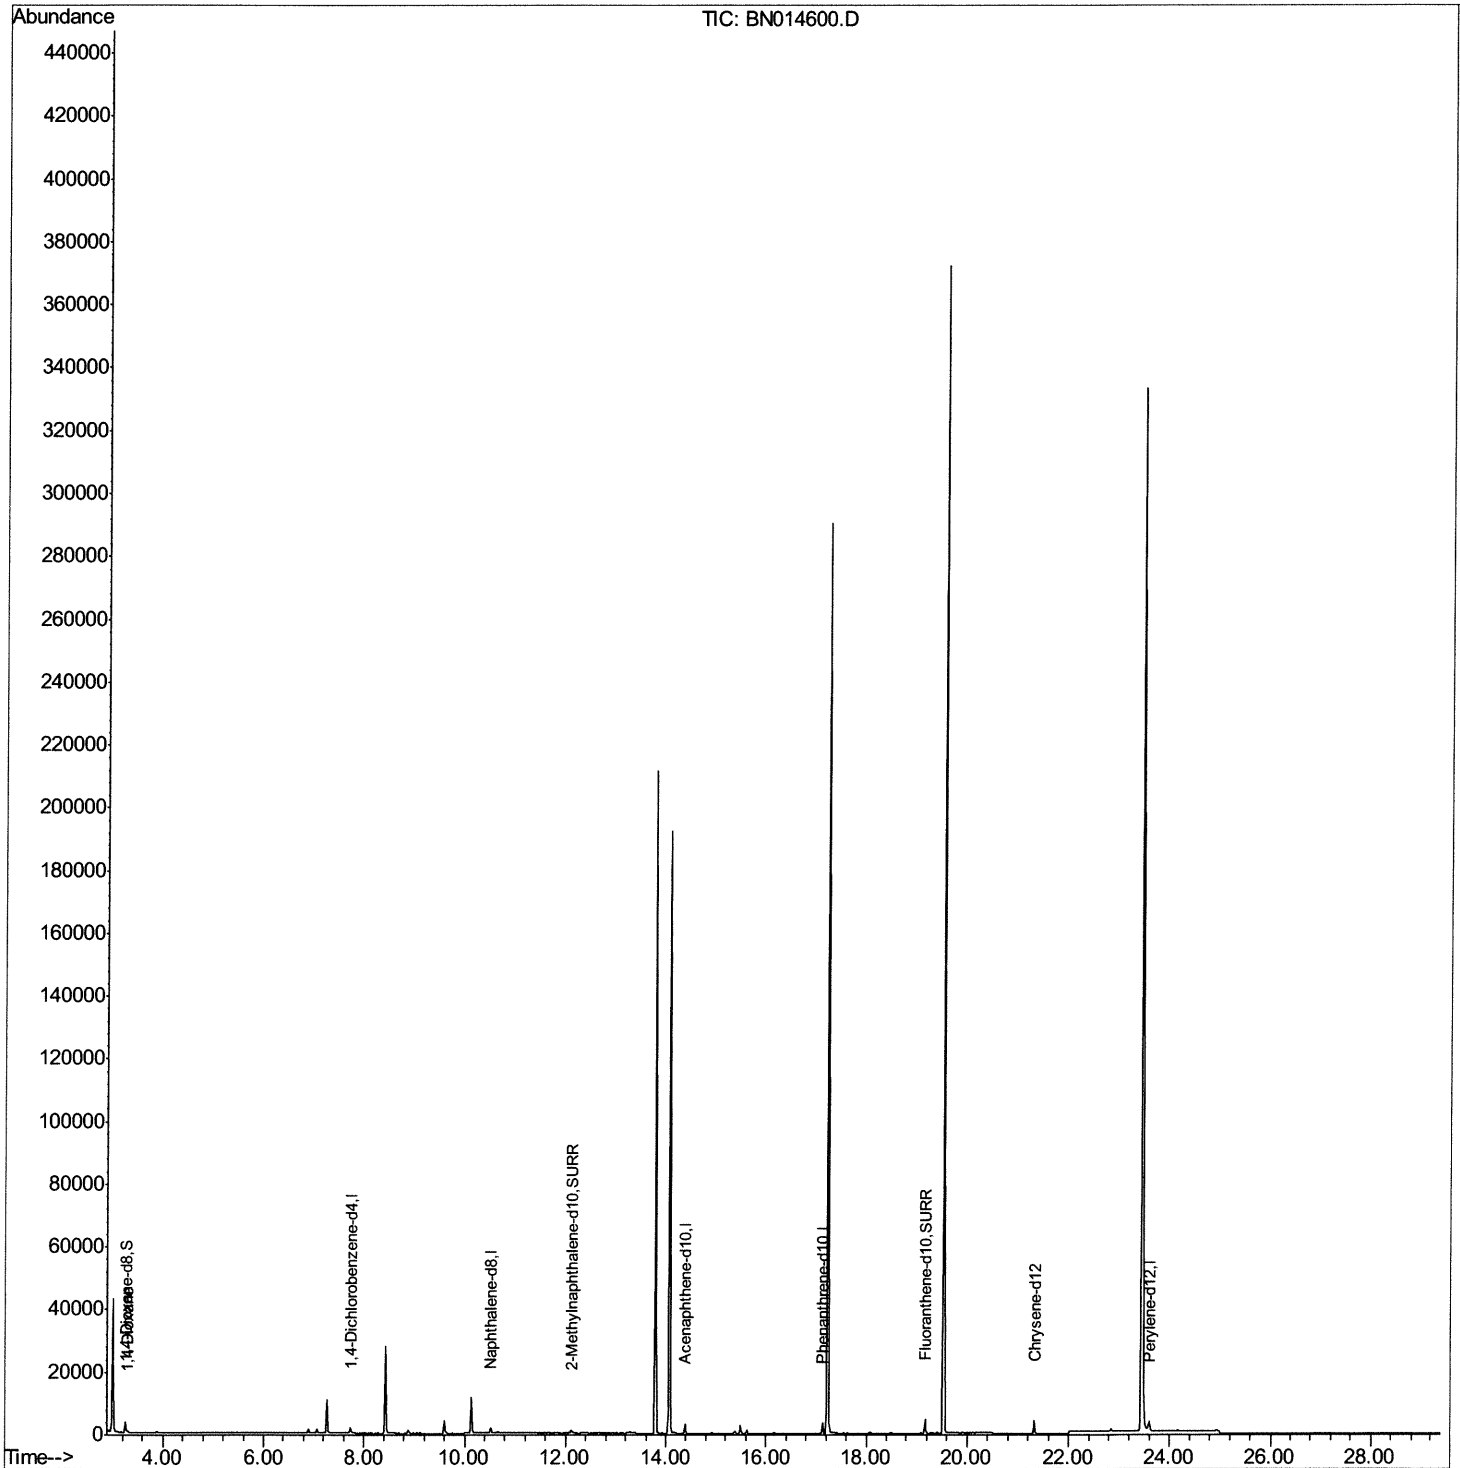

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
 Data File : BN014600.D
 Acq On : 13 May 2021 21:44
 Operator : CG/JU
 Sample : M2197-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARS0

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:02 PM

Quant Time: May 14 01:38:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 01:34:46 2021
 Response via : Initial Calibration

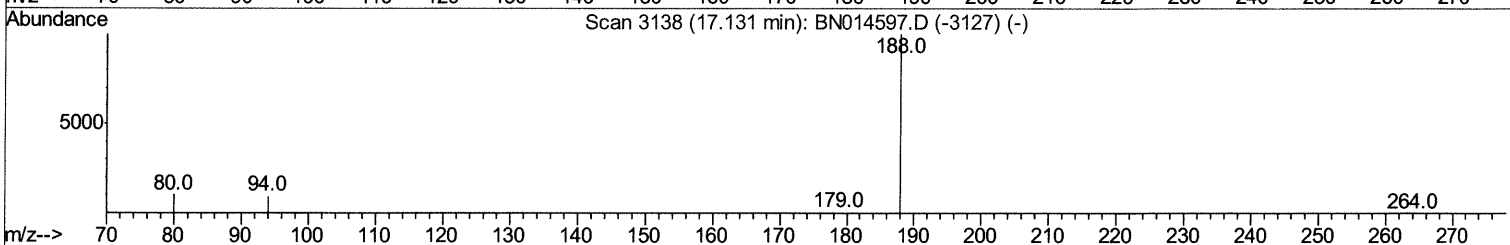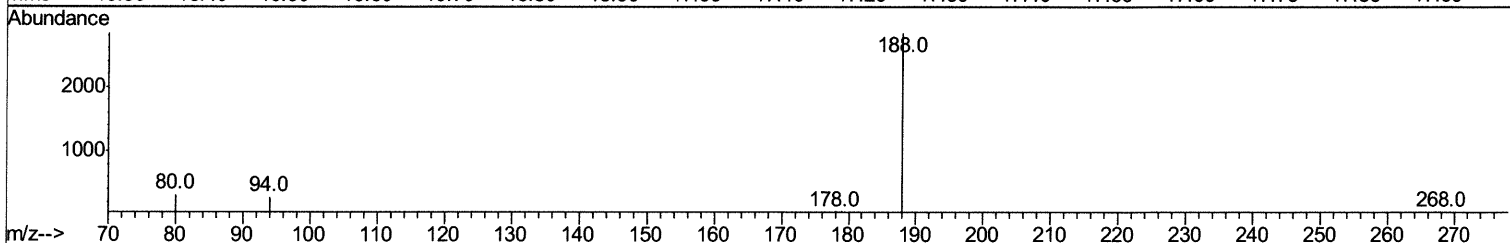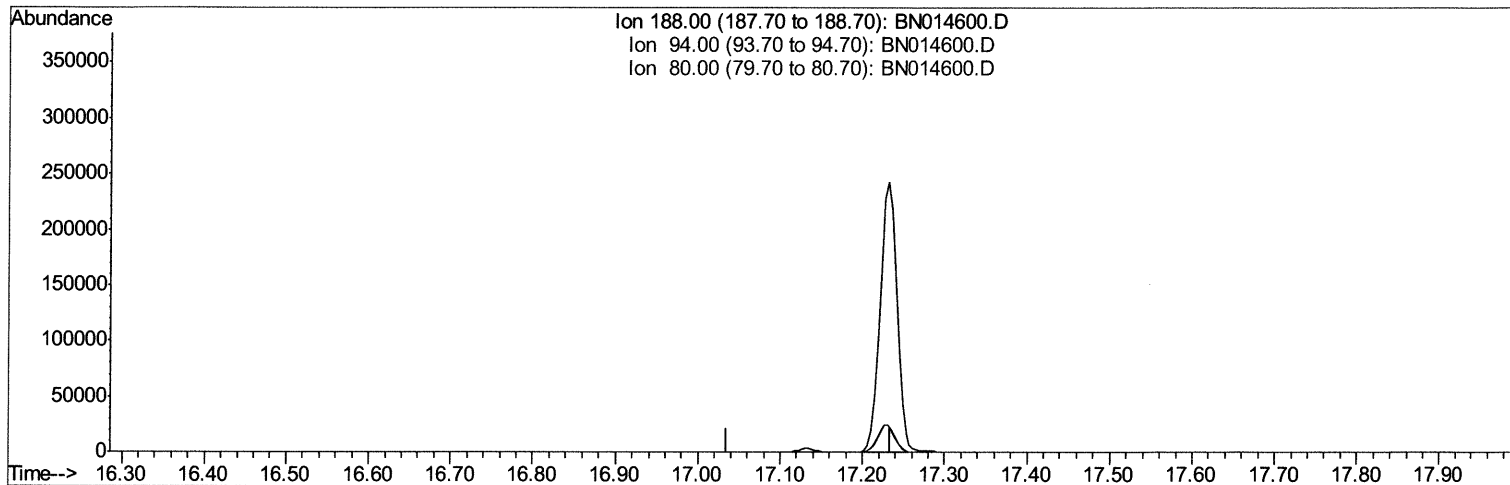

TIC: BN014600.D

(13) Phenanthrene-d10 (I)

17.135min (-17.135) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.70	0.00#
80.00	12.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
 Data File : BN014600.D
 Acq On : 13 May 2021 21:44
 Operator : CG/JU
 Sample : M2197-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARS0

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:02 PM

Quant Time: May 14 01:38:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 01:34:46 2021
 Response via : Initial Calibration

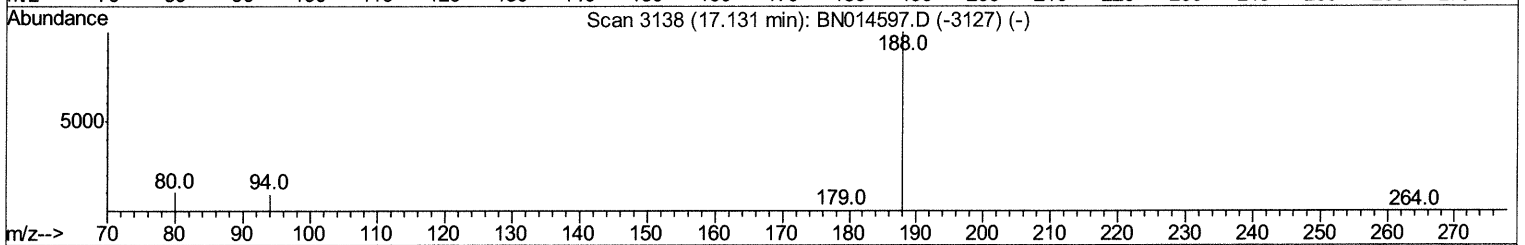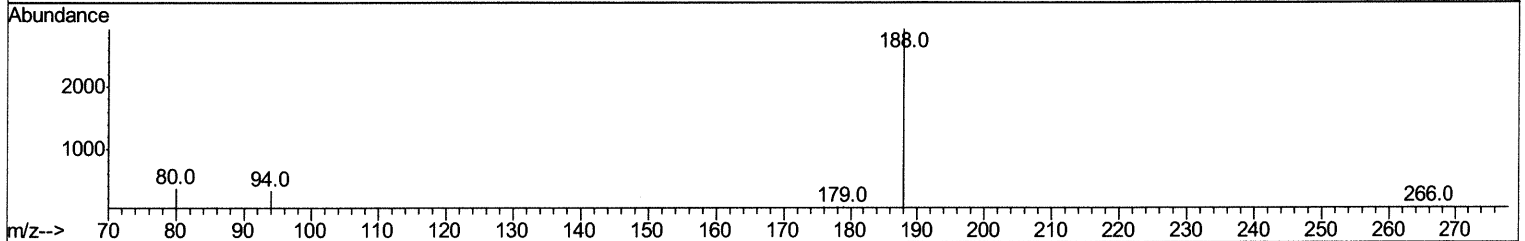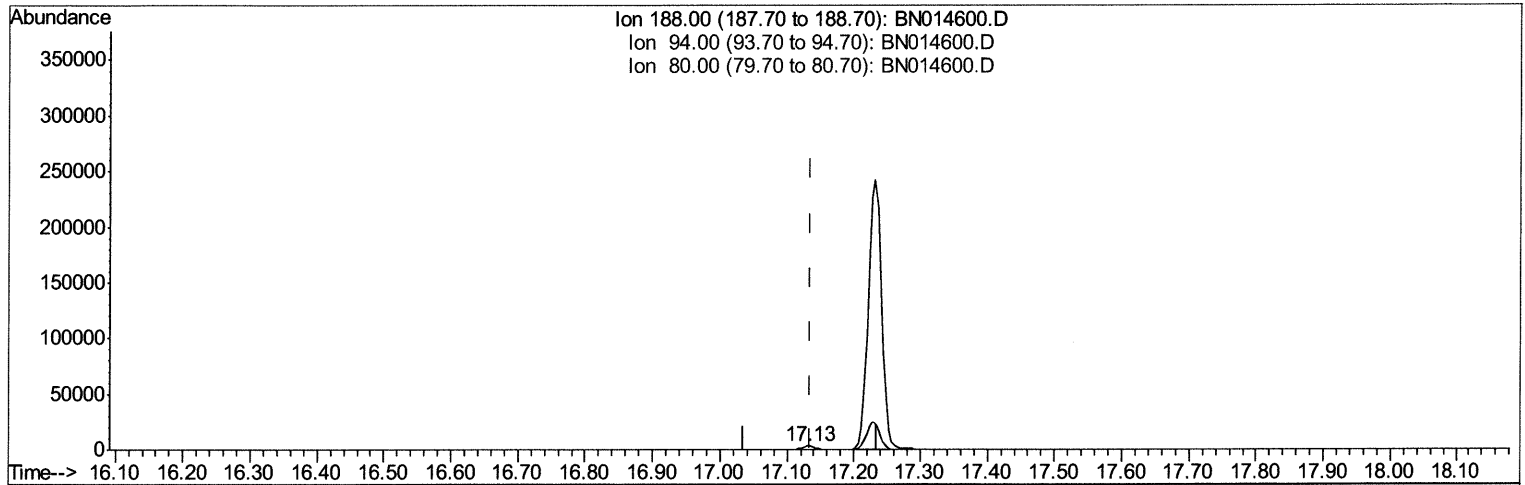

TIC: BN014600.D

(13) Phenanthrene-d10 (I)

17.130min (-0.005) 0.40ng/ul m 05/17/21 JU

response 4022

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	10.69
80.00	12.20	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
 Data File : BN014600.D
 Acq On : 13 May 2021 21:44
 Operator : CG/JU
 Sample : M2197-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARS0

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:02 PM

Quant Time: May 14 01:40:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 01:34:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	661	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	2466	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1801	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	4022m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.33	240	4006	0.40	ng/ul	0.00
23) Perylene-d12	23.60	264	4001	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	2407	3.52	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	1512	0.36	ng/ul	0.00
18) Fluoranthene-d10	19.17	212	4992	0.46	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.29	88	84	0.111	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed