


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
Data File : BN014616.D
Acq On : 14 May 2021 07:46
Operator : CG/JU
Sample : M2197-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARR9

Manual Integrations
APPROVED

mohammad
5/14/2021 12:51:29 PM

Quant Time: May 14 08:17:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 01:39:05 2021
Response via : Initial Calibration

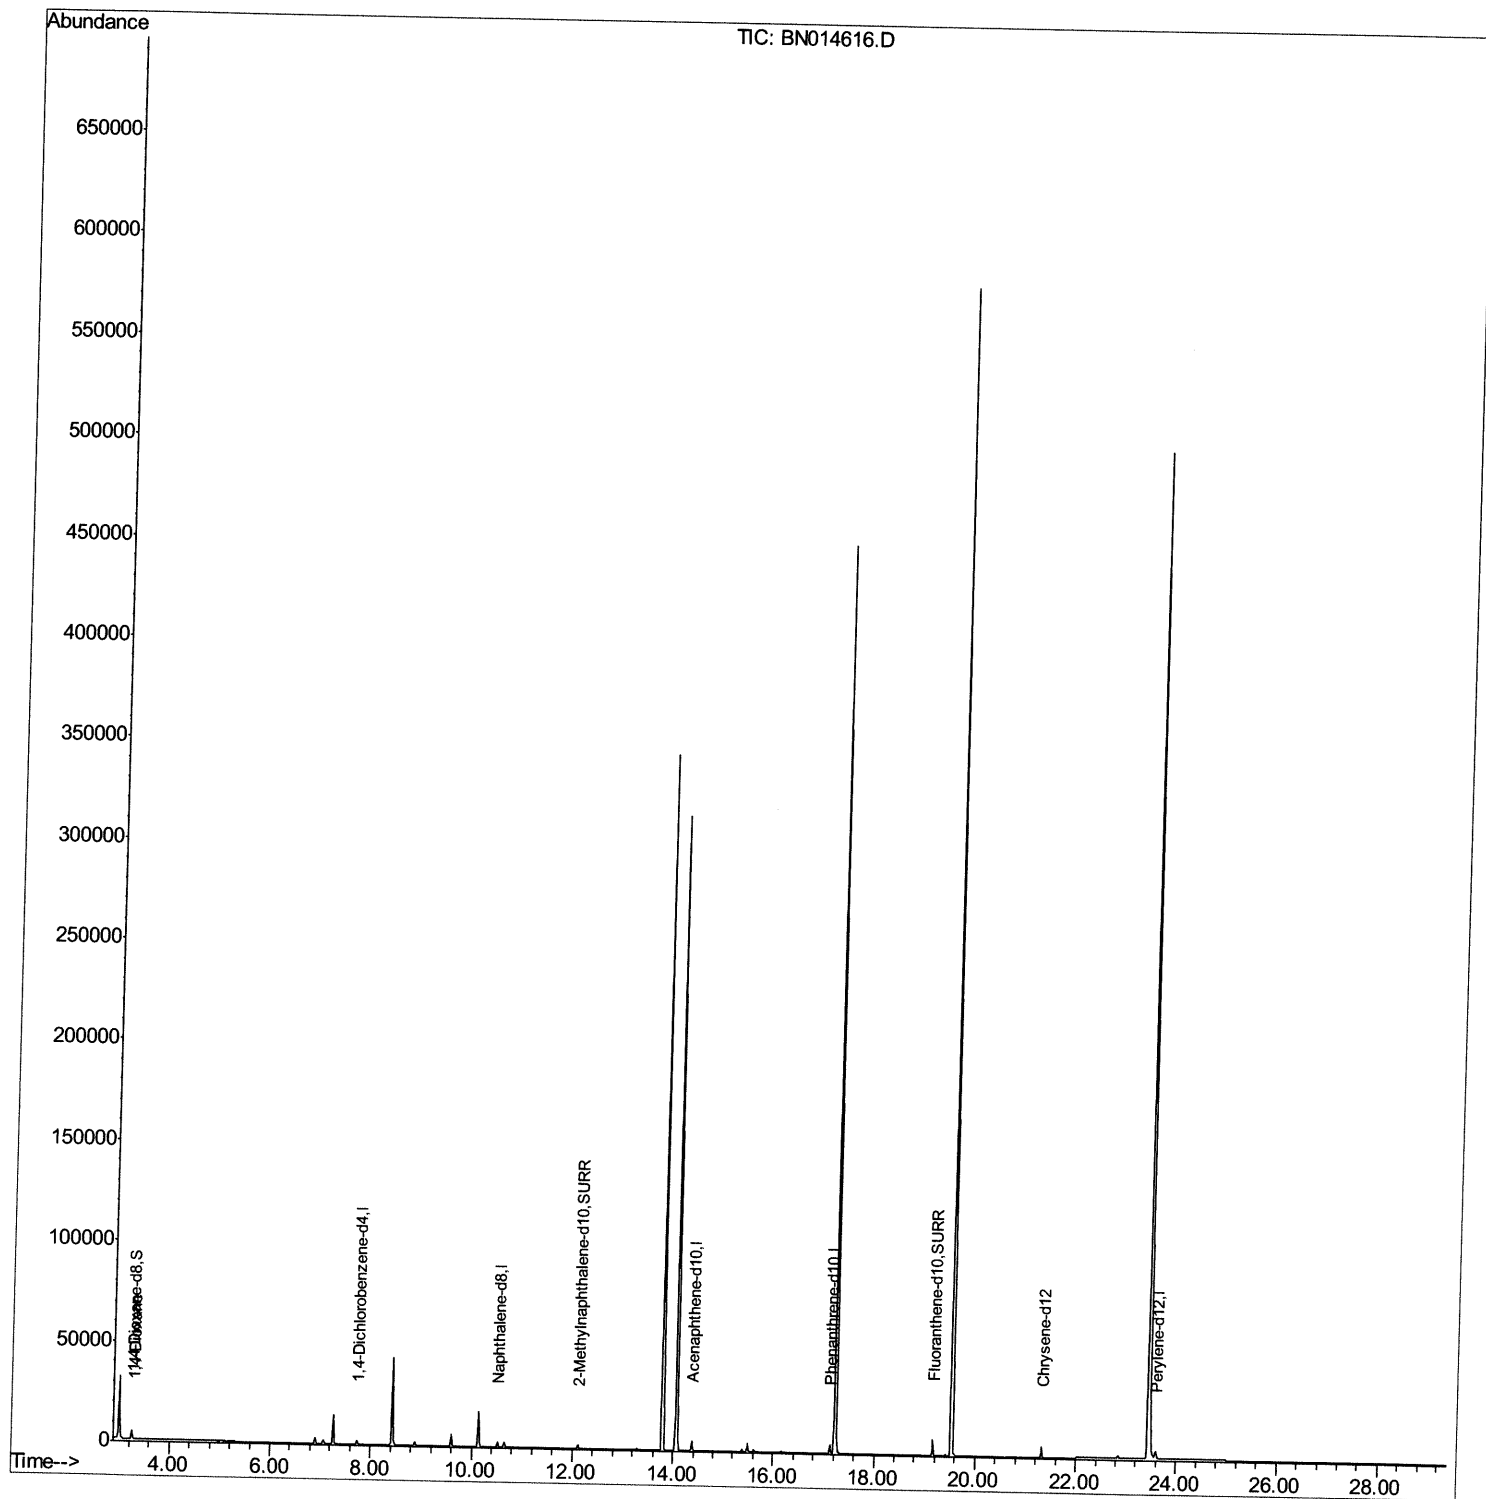

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
Data File : BN014616.D
Acq On : 14 May 2021 07:46
Operator : CG/JU
Sample : M2197-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARR9

Manual Integrations
APPROVED

mohammad
5/14/2021 12:51:29 PM

Quant Time: May 14 08:15:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 01:39:05 2021
Response via : Initial Calibration

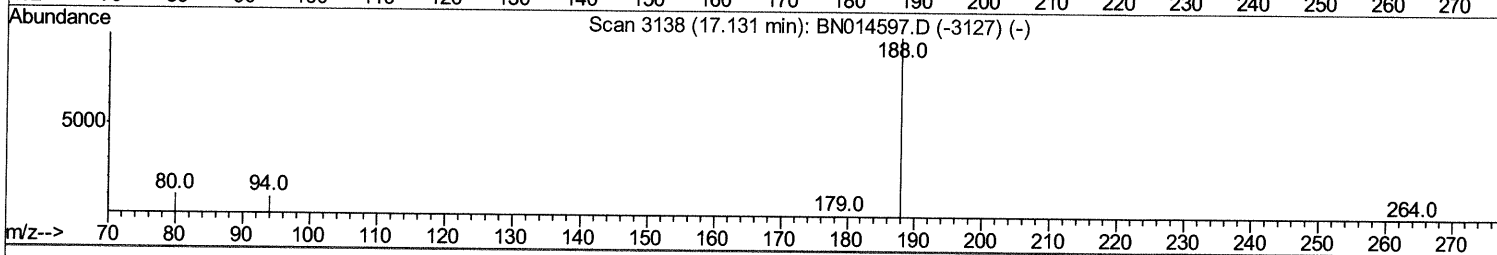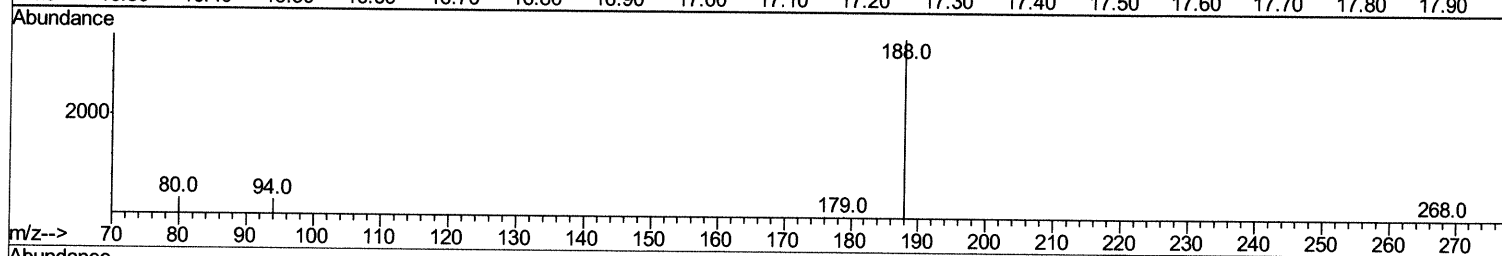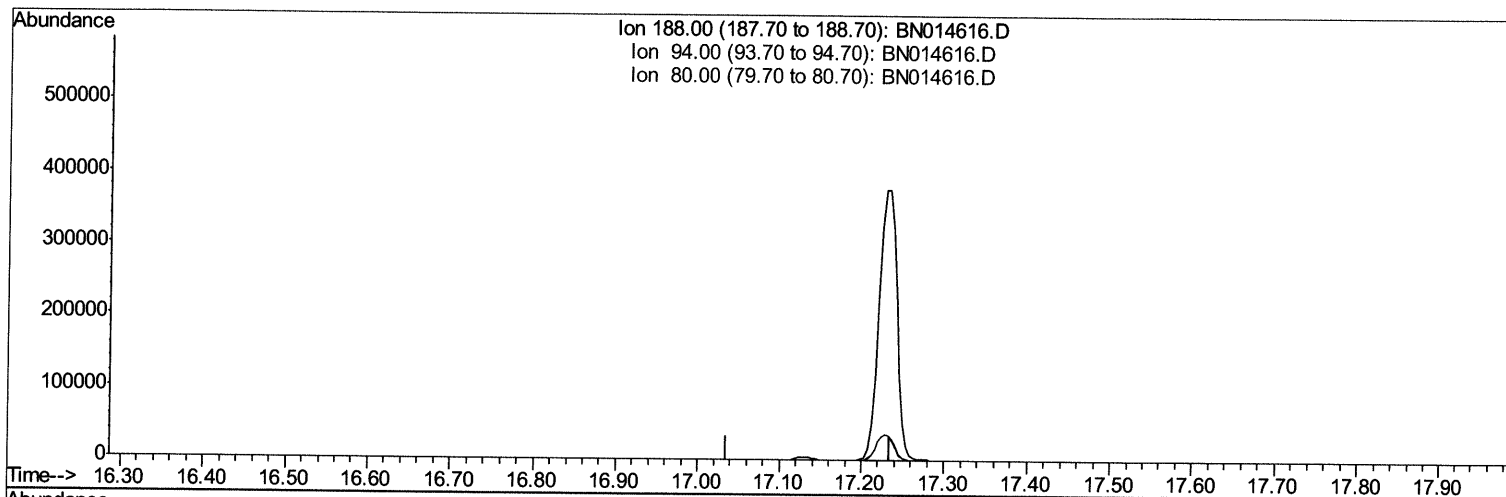

TIC: BN014616.D

(13) Phenanthrene-d10 (I)

17.135min (-17.135) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.70	0.00#
80.00	12.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
Data File : BN014616.D
Acq On : 14 May 2021 07:46
Operator : CG/JU
Sample : M2197-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARR9

Manual Integrations
APPROVED

mohammad
5/14/2021 12:51:29 PM

Quant Time: May 14 08:15:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 01:39:05 2021
Response via : Initial Calibration

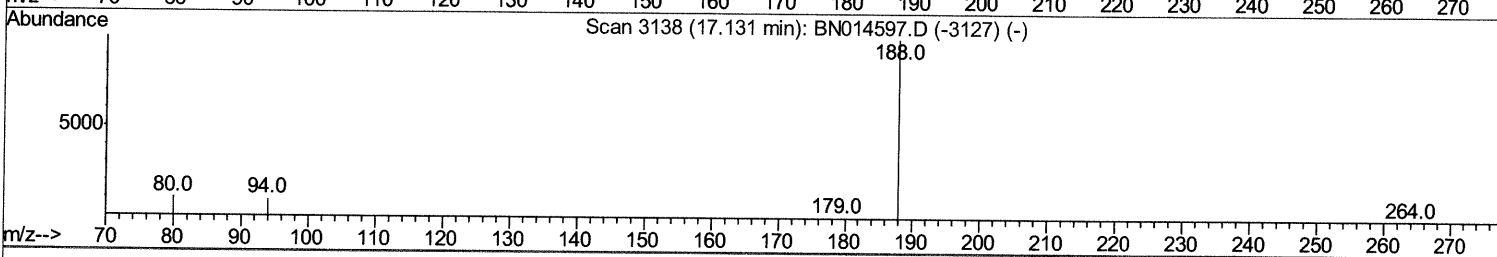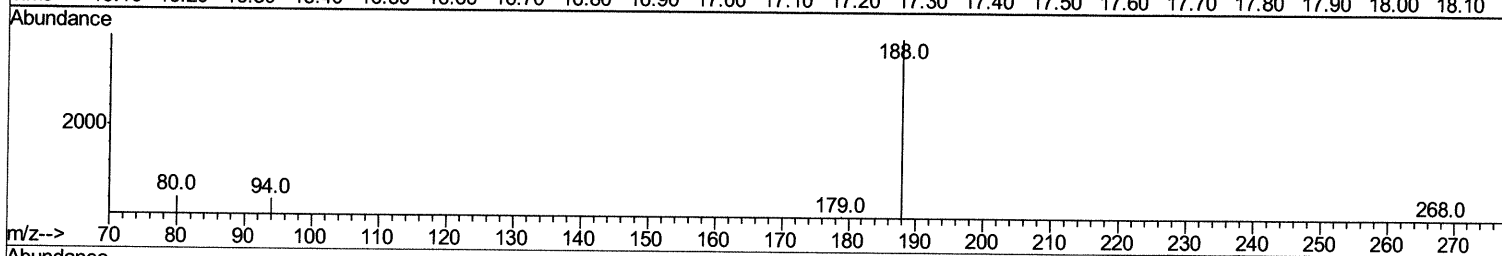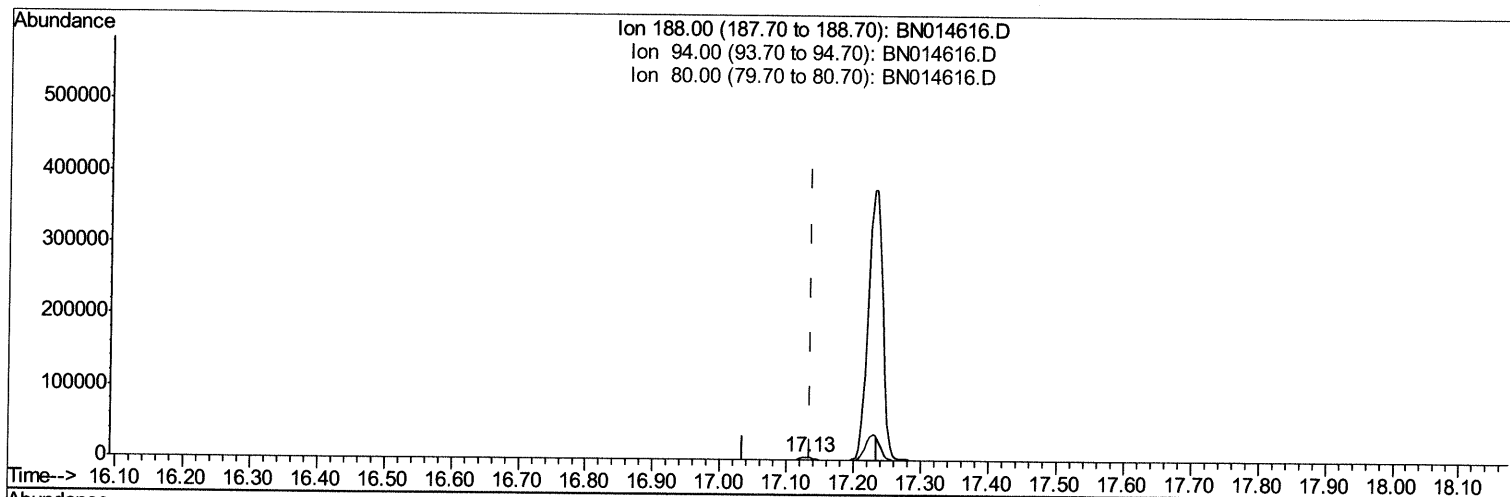

TIC: BN014616.D

(13) Phenanthrene-d10 (I)

17.131min (-0.004) 0.40ng/ul m 0.517/2120

response 5591

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	9.93
80.00	12.20	10.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN051321\
 Data File : BN014616.D
 Acq On : 14 May 2021 07:46
 Operator : CG/JU
 Sample : M2197-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 YARR9

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:29 PM

Quant Time: May 14 08:17:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 01:39:05 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	780	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	3372	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	2531	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	5591m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.33	240	5286	0.40	ng/ul	0.00
23) Perylene-d12	23.59	264	5237	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	2582	3.20	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.12	152	2472	0.43	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	8404	0.59	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.29	88	64	0.072	ng/ul#	Ovalue 26

(#) = qualifier out of range (m) = manual integration (+) = signals summed