

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051321\
 Data File : BN014600.D
 Acq On : 13 May 2021 21:44
 Operator : CG/JU
 Sample : M2197-17
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARS0

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:02 PM

Quant Time: May 14 01:40:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 01:34:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	661	0.40	ng/ul	0.00
4) Naphthalene-d8	10.52	136	2466	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.38	164	1801	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	4022m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	4006	0.40	ng/ul	0.00
23) Perylene-d12	23.60	264	4001	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	2407	3.52	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	1512	0.36	ng/ul	0.00
18) Fluoranthene-d10	19.17	212	4992	0.46	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.29	88	84	0.111	ng/ul#	Ovalue 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN051321\
Data File : BN014600.D
Acq On : 13 May 2021 21:44
Operator : CG/JU
Sample : M2197-17
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YARS0

Manual Integrations
APPROVED

mohammad
5/14/2021 12:51:02 PM

Quant Time: May 14 01:40:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 01:34:46 2021
Response via : Initial Calibration

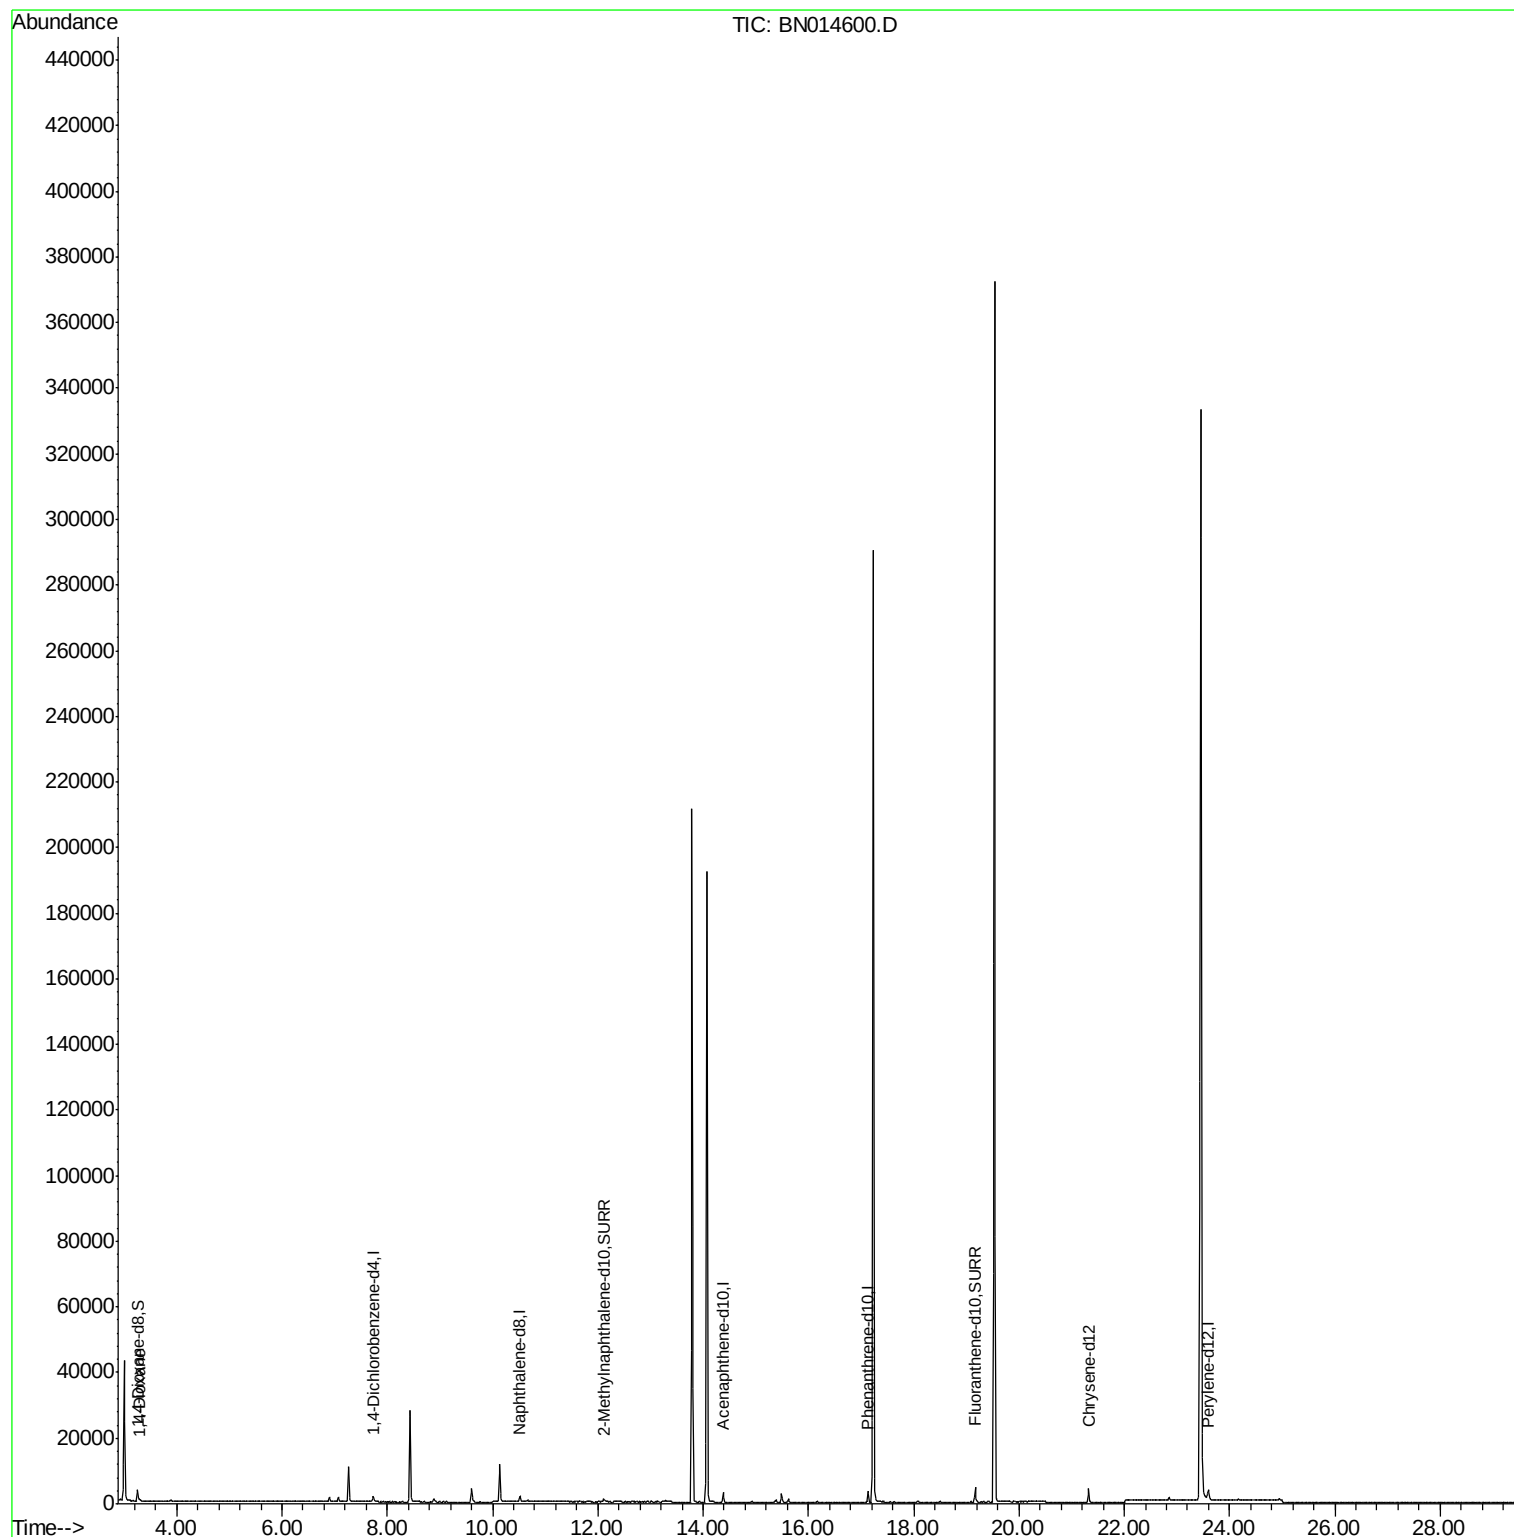

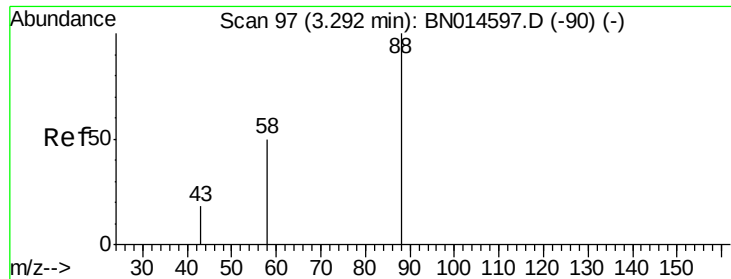

#2
 1,4-Dioxane
 Concen: 0.111 ng/ul
 RT: 3.29 min Scan# 97
 Delta R.T. -0.00 min
 Lab File: BN014600.D
 Acq: 13 May 2021 21:44

Instrument :
 BNA_N
 ClientSampleId :
 YARS0

Tot Ion:	88	Resp:	84
Ion	Ratio	Lower	Upper
88	100		
43	46.1	15.7	23.5#
58	36.5	23.8	35.6#

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:51:02 PM

