
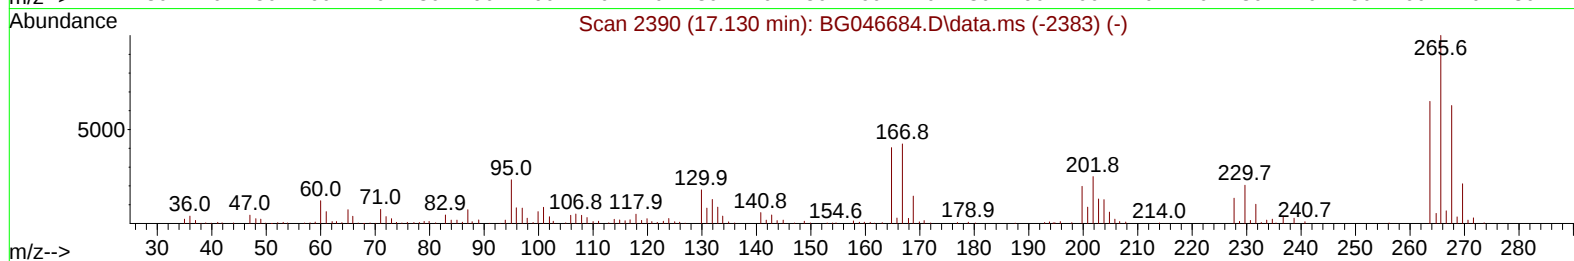
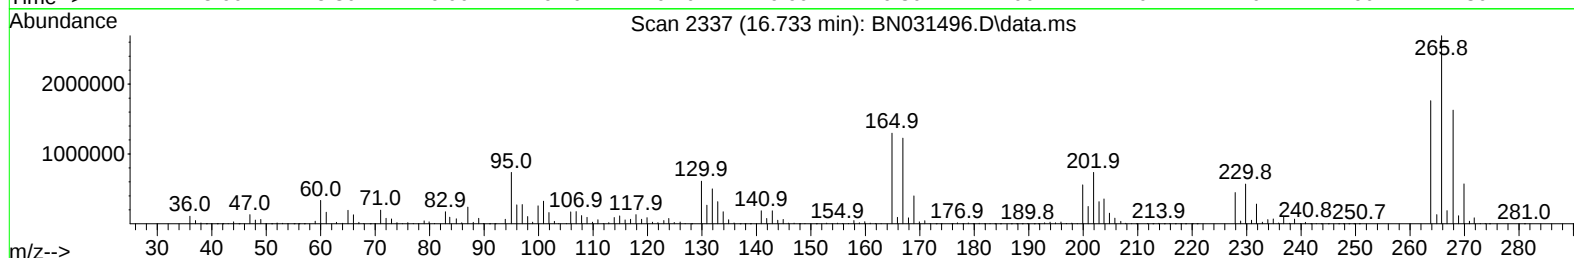


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031496.D
Acq On : 13 May 2024 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 12:50:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

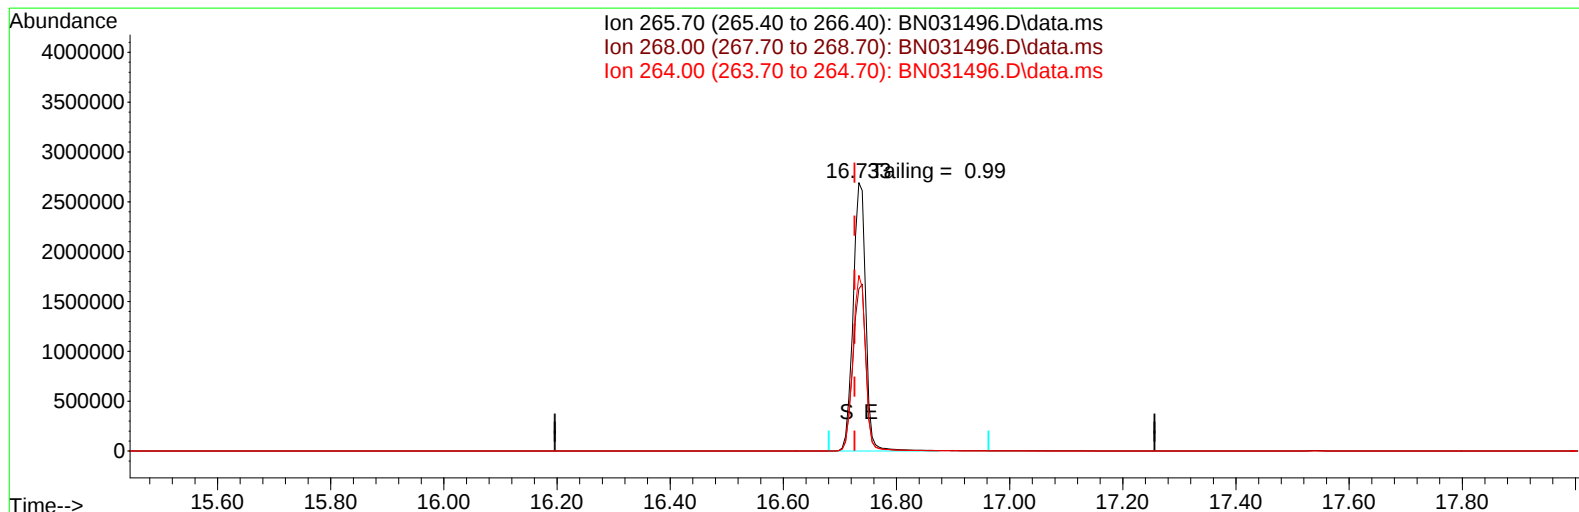

TIC: BN031496.D\data.ms

(70) Pentachlorophenol (C)




16.733min (+ 0.007) 35588.00 ng

response 4204087

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.39
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031496.D
Acq On : 13 May 2024 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 12:50:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

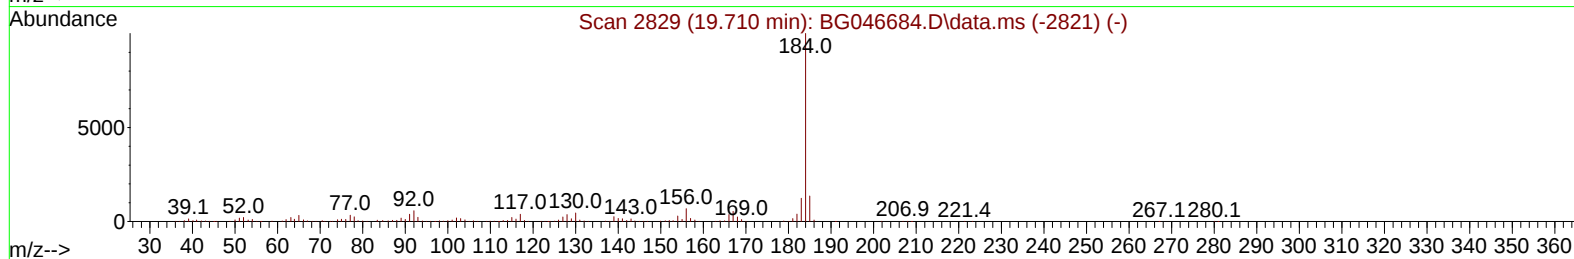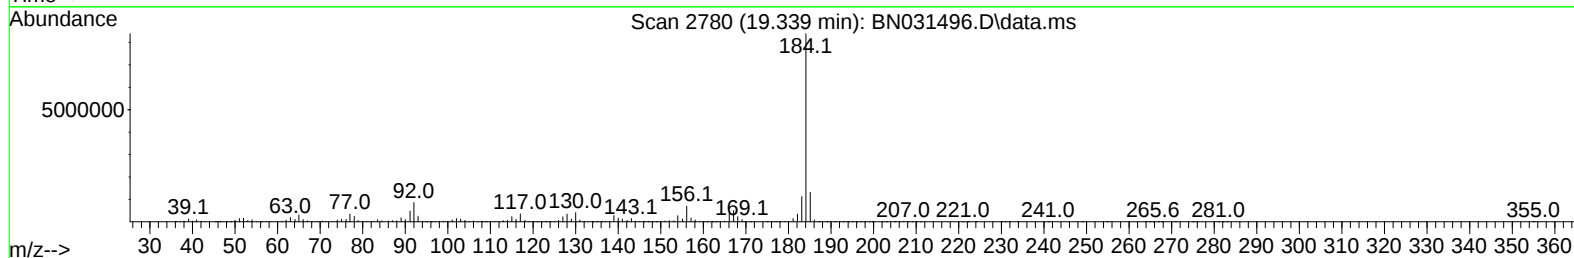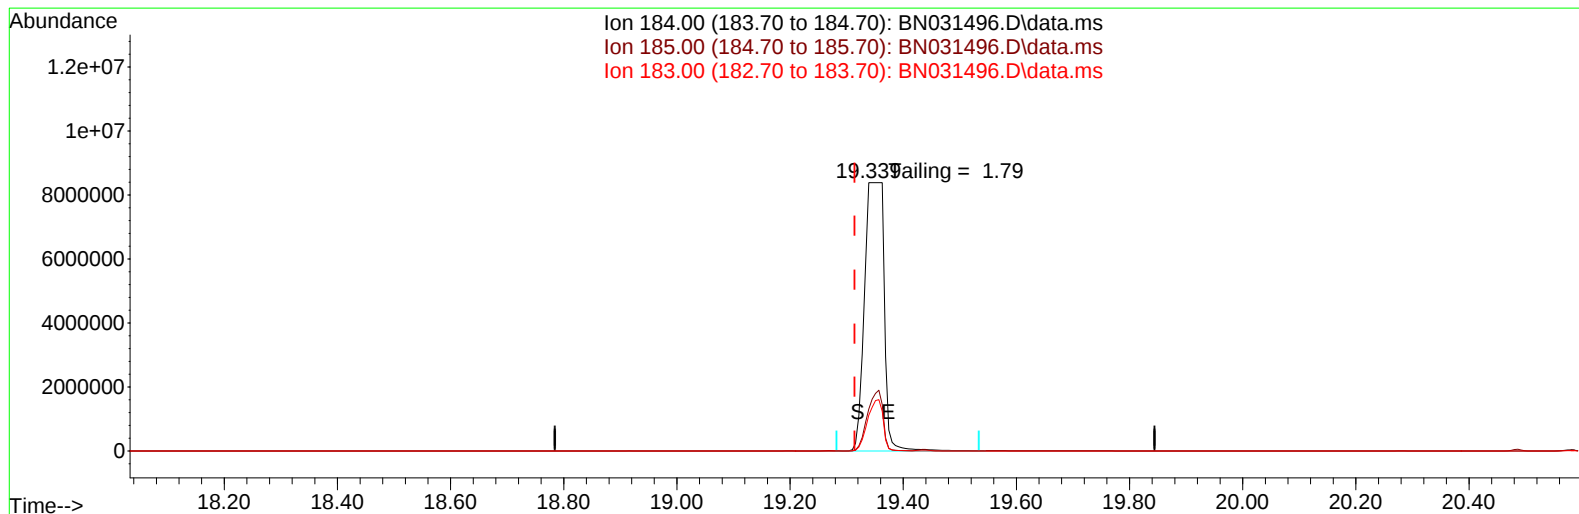

TIC: BN031496.D\data.ms

(77) Benzidine

19.339min (+ 0.025) 3395914.49 ng m

response 20203303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.65
183.00	13.20	13.40
0.00	0.00	0.00