
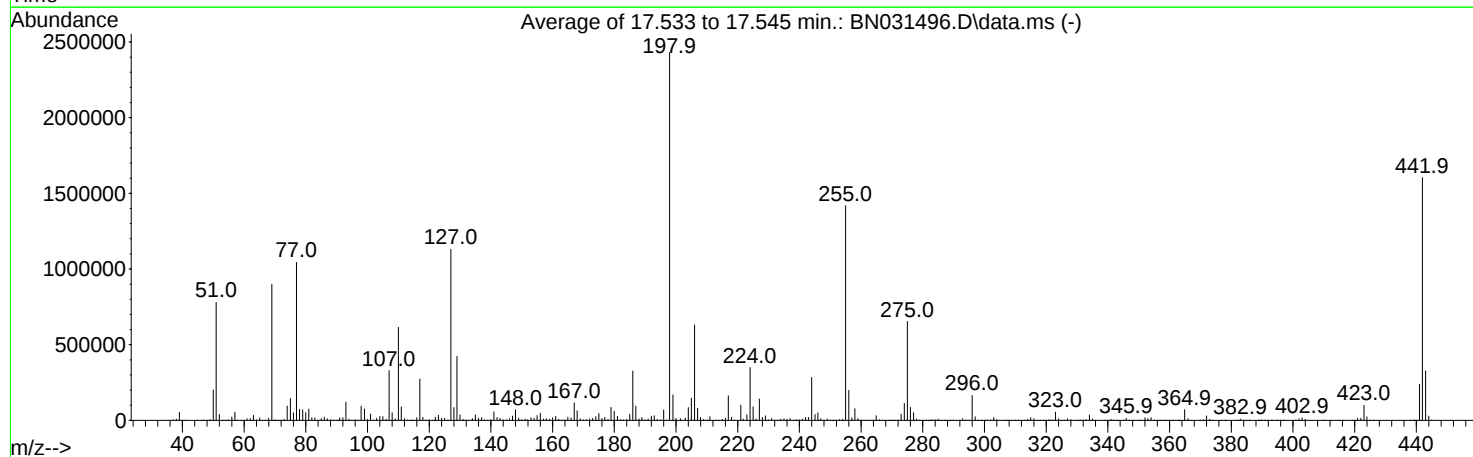


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031496.D
Acq On : 13 May 2024 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

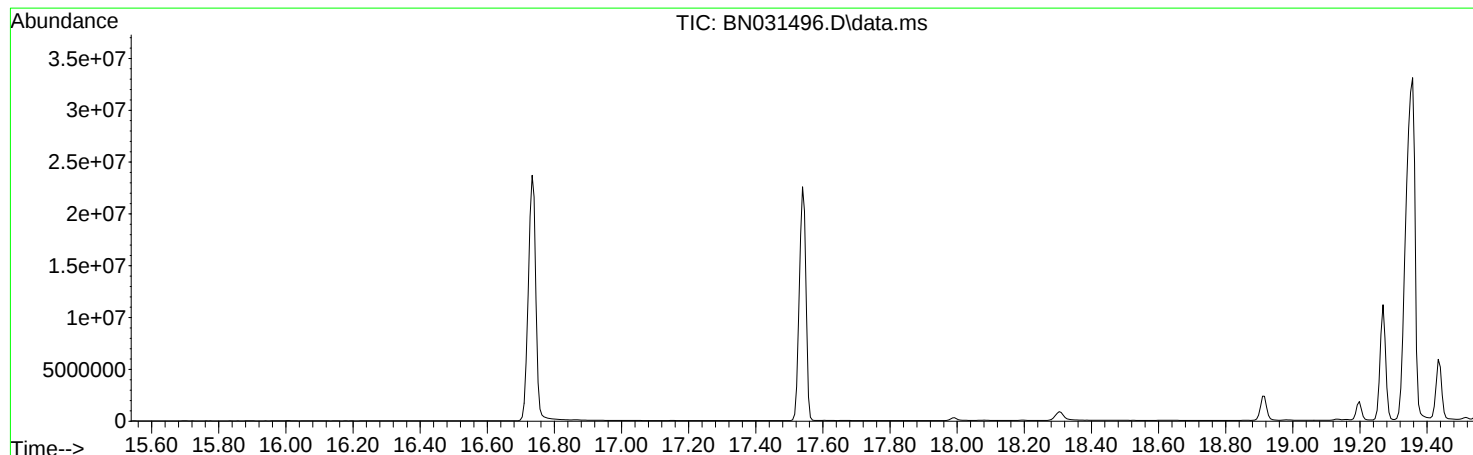

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2465

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	32.1	779730	PASS
68	69	0.00	2	1.6	14310	PASS
69	198	0.00	100	37.0	899484	PASS
70	69	0.00	2	0.5	4465	PASS
127	198	10	80	46.5	1130325	PASS
197	198	0.00	2	0.2	3828	PASS
198	198	100	100	100.0	2430464	PASS
199	198	5	9	6.9	167979	PASS
275	198	10	60	26.9	653419	PASS
365	198	1	100	2.9	70763	PASS
441	198	0.01	100	9.8	238379	PASS
442	442	50	100	100.0	1604267	PASS
443	442	15	24	20.4	327403	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2024	BNA_N	<u>BN031496.D</u>
Compound Name	Response	Retention Time
DDT	9997916	20.58
DDD	320328	20.133
DDE	4147	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
324475	10322391	3.14

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031496.D
Acq On : 13 May 2024 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 12:50:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

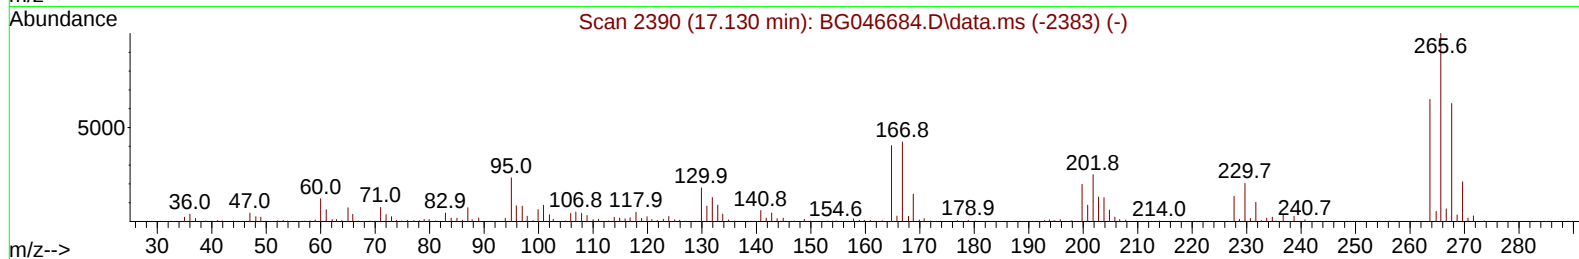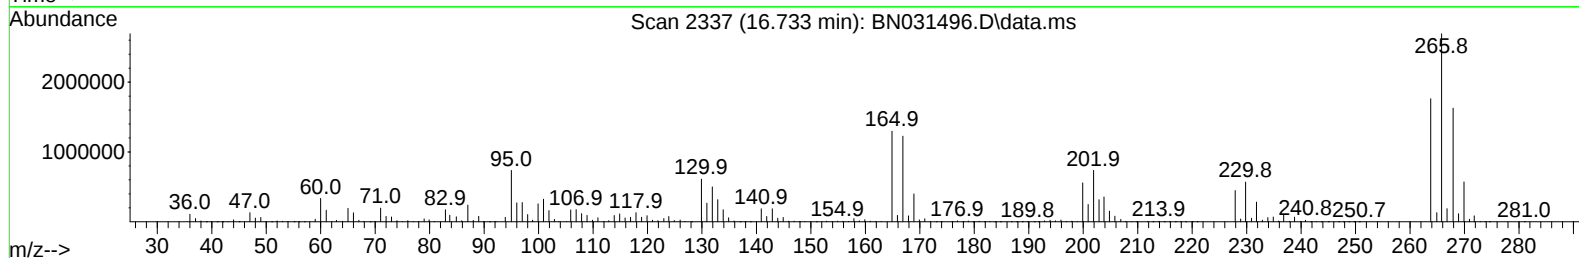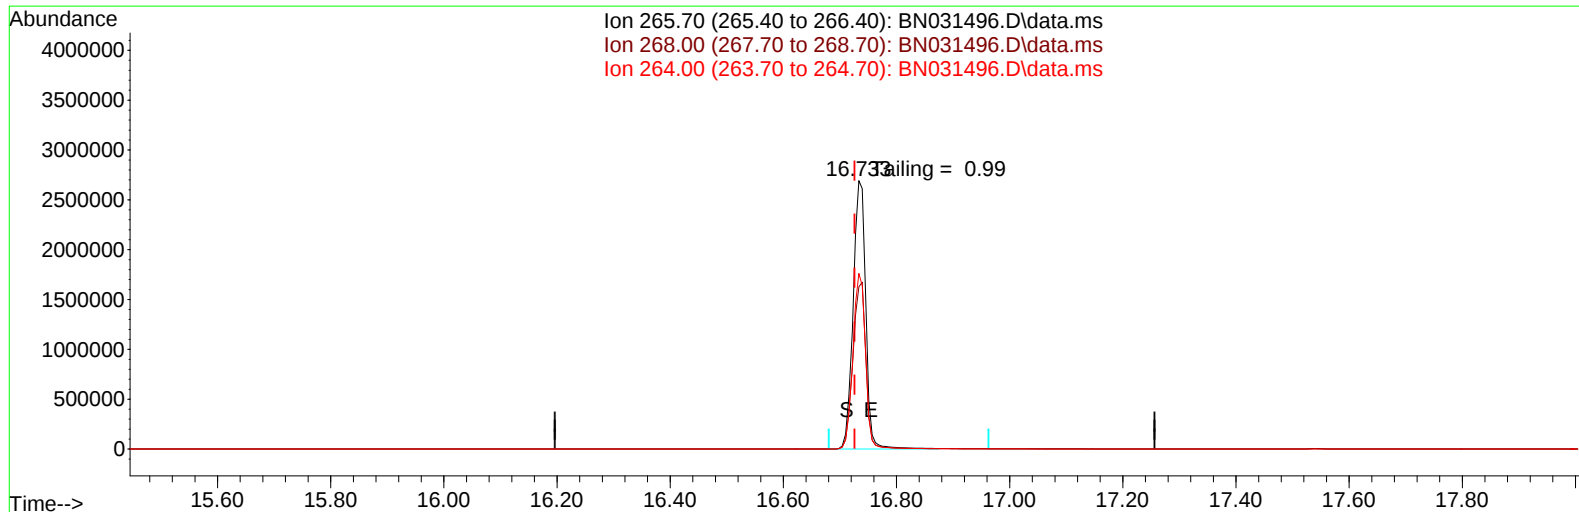

TIC: BN031496.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.007) 35588.00 ng




response 4204087

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.39
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051324\
Data File : BN031496.D
Acq On : 13 May 2024 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 12:50:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

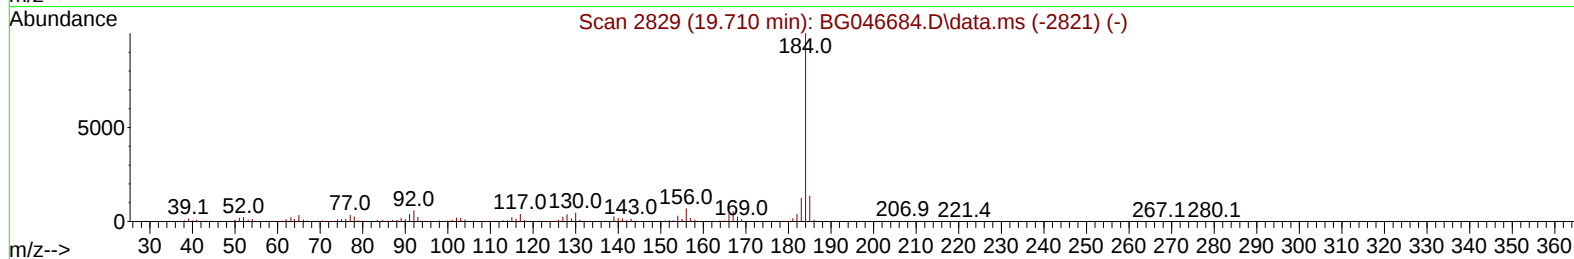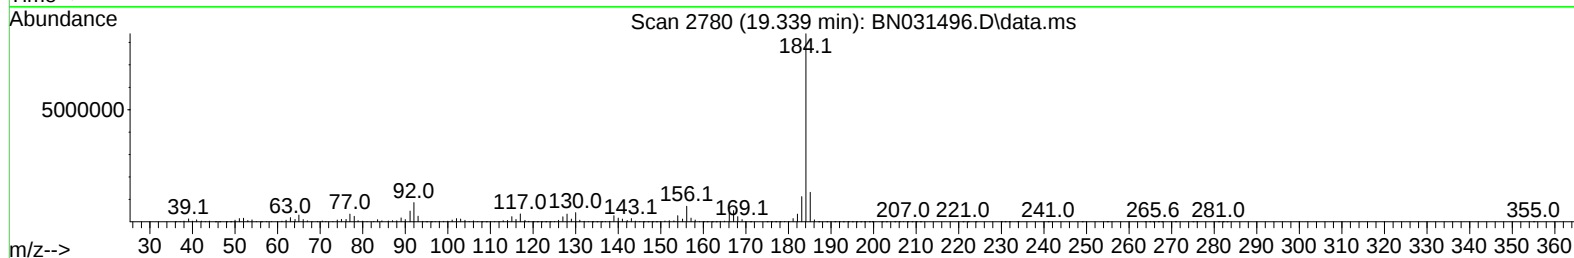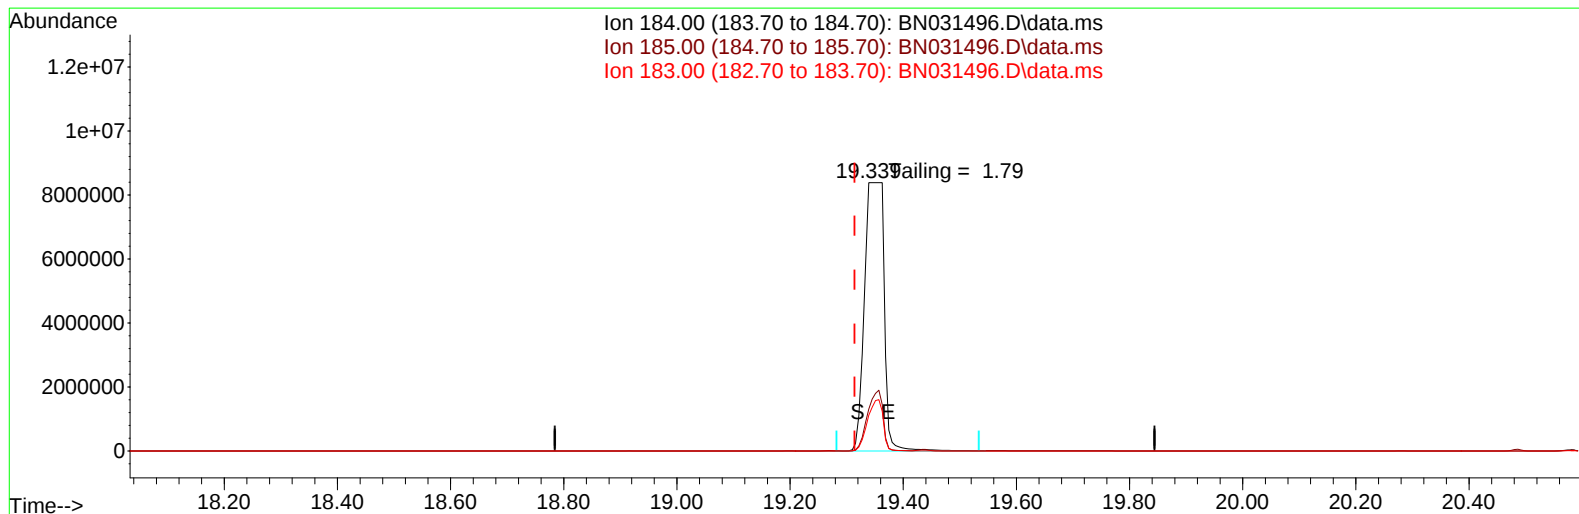

TIC: BN031496.D\data.ms

(77) Benzidine

19.339min (+ 0.025) 3395914.49 ng m

response 20203303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.65
183.00	13.20	13.40
0.00	0.00	0.00